

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP042977.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2022 13:05
 Operator : AJ\MA
 Sample : N1167-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MR-PIPE-C

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 16:37:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.878	4.044	643144	700393	27.181	28.043
2) SA Decachlor...	10.818	9.384	433332	594071	29.643	30.455
Target Compounds						
16) L4 AR-1242-1	6.183	5.309	15912	21064	26.857	26.284
17) L4 AR-1242-2	6.205	5.330	43443	36602	48.693	32.325 #
18) L4 AR-1242-3	6.277	5.525	19676	24806	35.461m	38.904
19) L4 AR-1242-4	6.374	5.618	13289	46552	29.208m	75.786 #
20) L4 AR-1242-5	7.157	6.187	40202	62703	89.624	87.140

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP042977.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2022 13:05
Operator : AJ\MA
Sample : N1167-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MR-PIPE-C


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 16:37:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

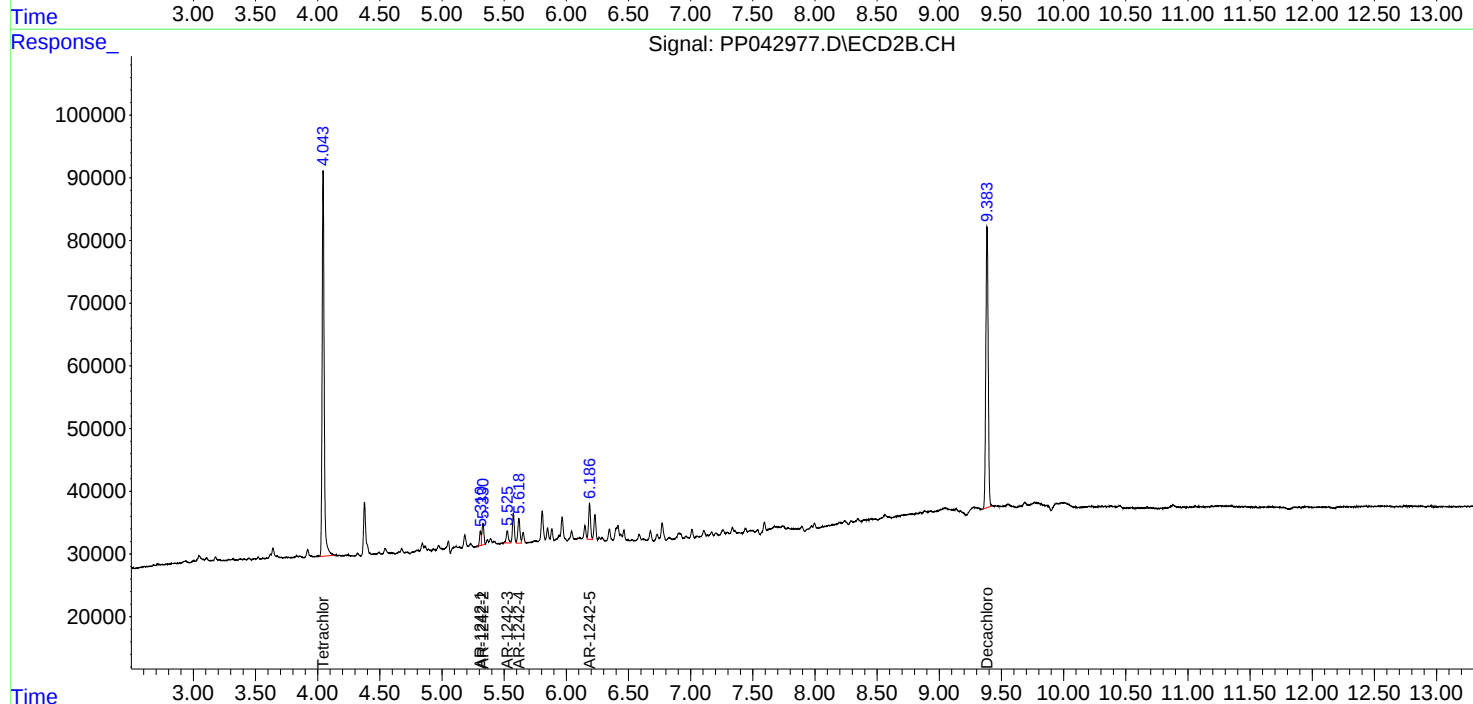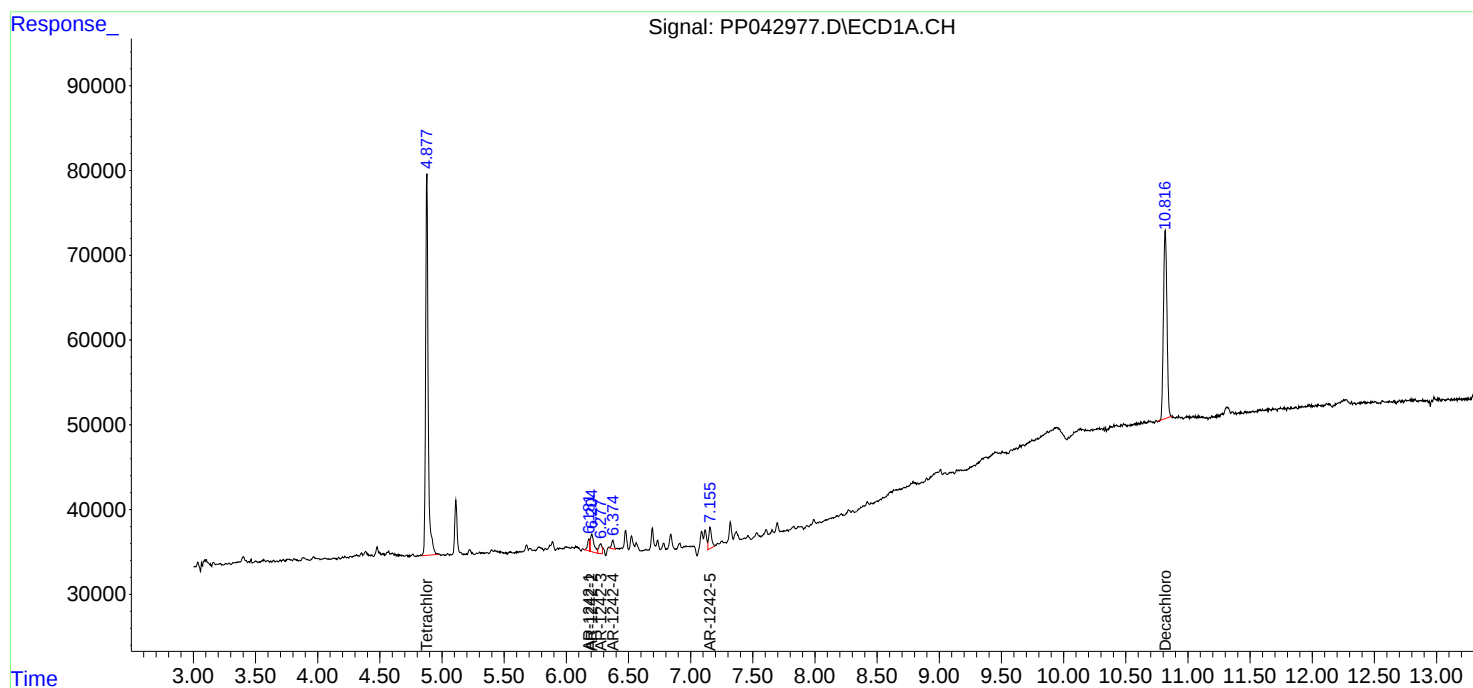

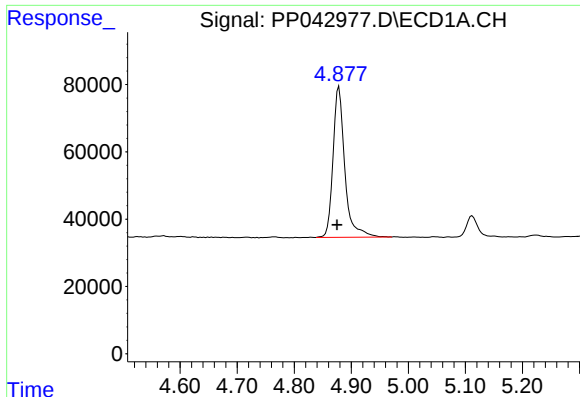


#1 Tetrachloro-m-xylene

R.T.: 4.878 min
Delta R.T.: 0.003 min
Response: 643144
Conc: 27.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-C


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

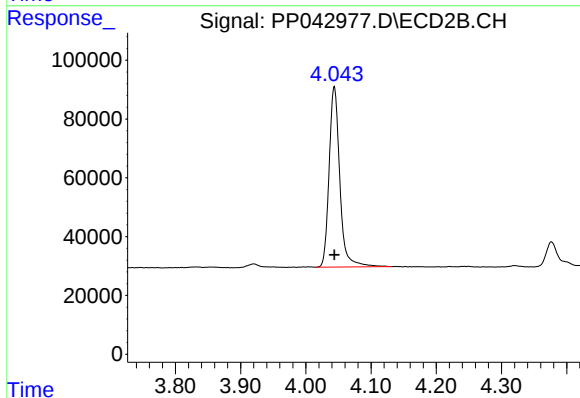


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 700393
Conc: 28.04 ng/ml

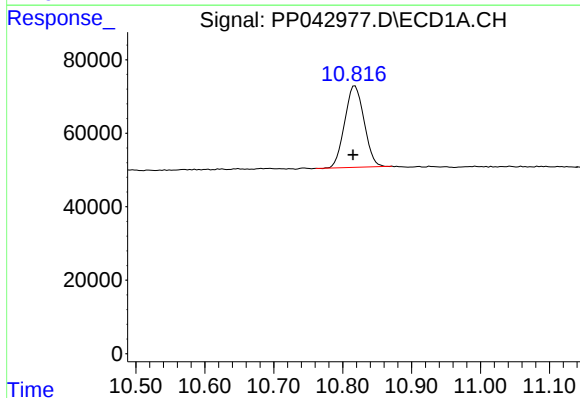


#2 Decachlorobiphenyl

R.T.: 10.818 min
Delta R.T.: 0.003 min
Response: 433332
Conc: 29.64 ng/ml

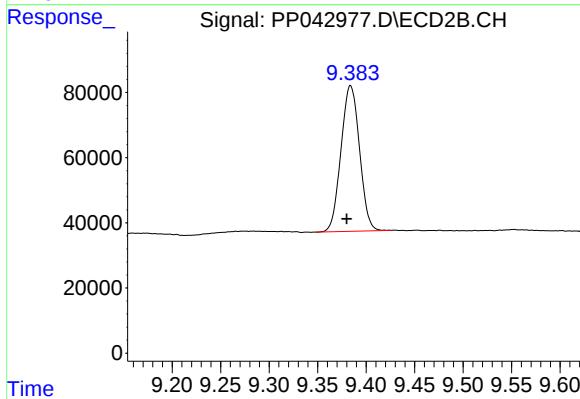

#2 Decachlorobiphenyl

R.T.: 9.384 min
Delta R.T.: 0.004 min
Response: 594071
Conc: 30.45 ng/ml

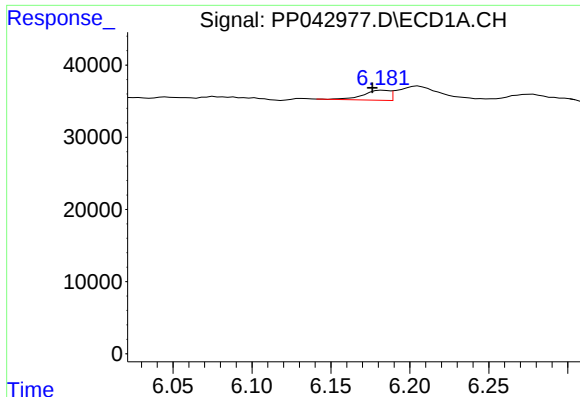


#16 AR-1242-1

R.T.: 6.183 min
Delta R.T.: 0.007 min
Response: 15912
Conc: 26.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-C


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

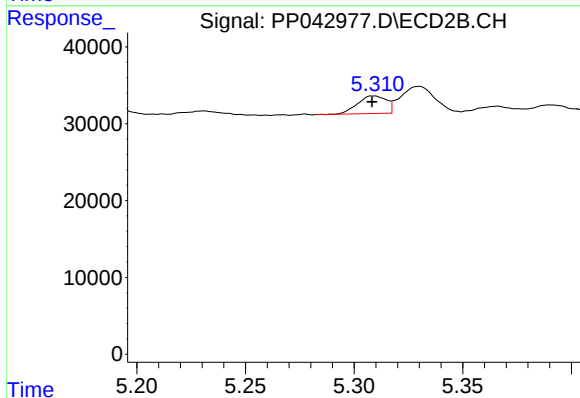


#16 AR-1242-1

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 21064
Conc: 26.28 ng/ml

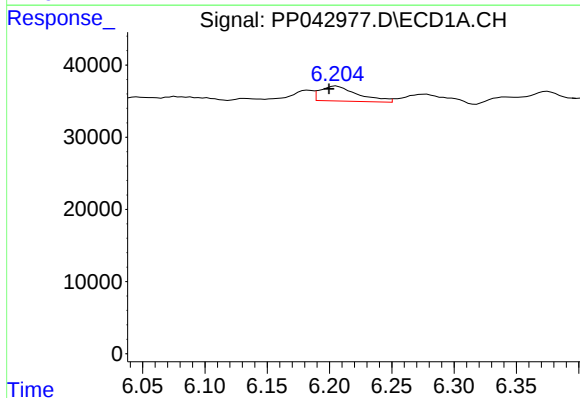


#17 AR-1242-2

R.T.: 6.205 min
Delta R.T.: 0.006 min
Response: 43443
Conc: 48.69 ng/ml

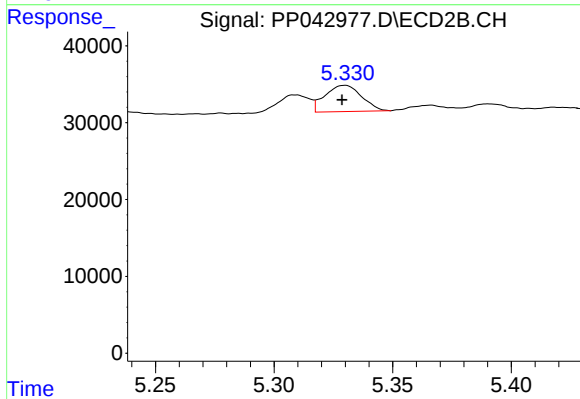

#17 AR-1242-2

R.T.: 5.330 min
Delta R.T.: 0.001 min
Response: 36602
Conc: 32.33 ng/ml

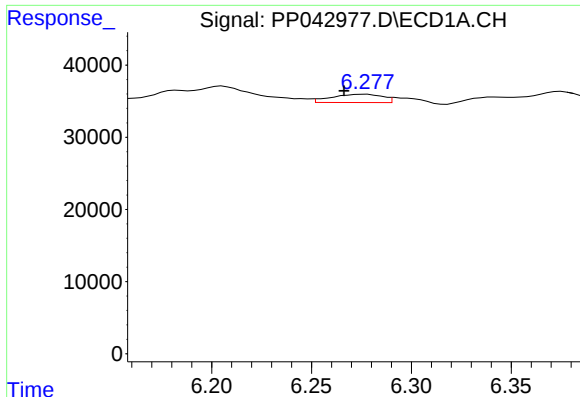


#18 AR-1242-3

R.T.: 6.277 min
Delta R.T.: 0.011 min
Response: 19676
Conc: 35.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-C


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

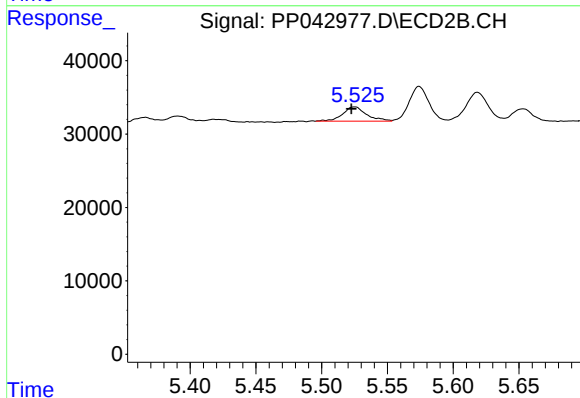


#18 AR-1242-3

R.T.: 5.525 min
Delta R.T.: 0.003 min
Response: 24806
Conc: 38.90 ng/ml

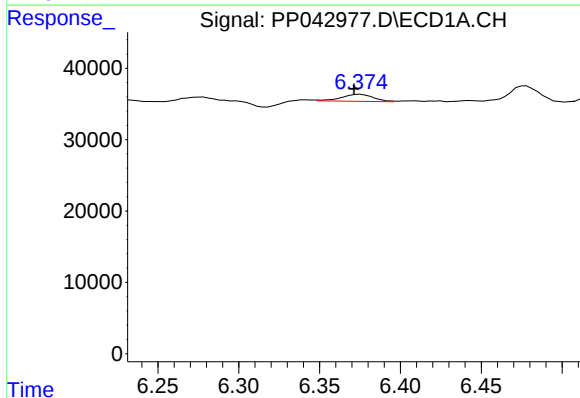


#19 AR-1242-4

R.T.: 6.374 min
Delta R.T.: 0.003 min
Response: 13289
Conc: 29.21 ng/ml m

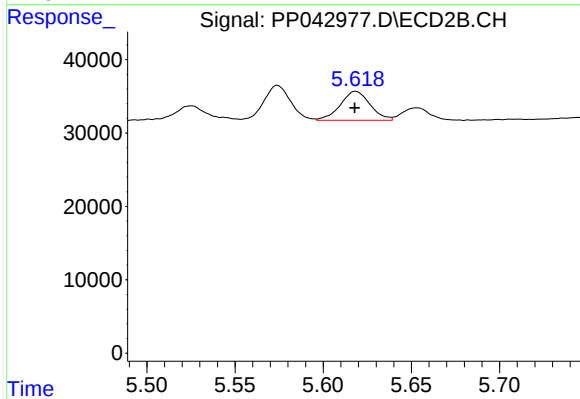

#19 AR-1242-4

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 46552
Conc: 75.79 ng/ml

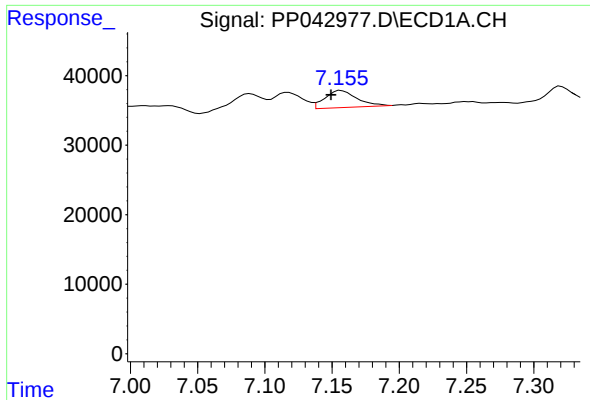


#20 AR-1242-5

R.T.: 7.157 min
Delta R.T.: 0.008 min
Response: 40202
Conc: 89.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-C

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

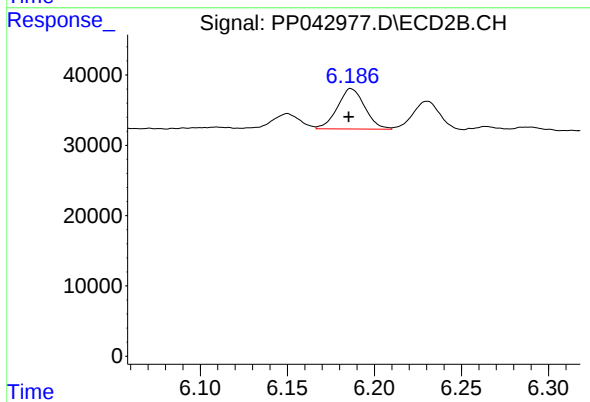

#20 AR-1242-5

R.T.: 6.187 min
Delta R.T.: 0.001 min
Response: 62703
Conc: 87.14 ng/ml