

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP043031.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 5:50
 Operator : AJ\MA
 Sample : N1162-02 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MMO-01-2022-B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 07:12:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.879	4.043	34883	43987	1.474	1.761m
2) SA Decachlor...	10.813	9.381	34083	39371	2.332m	2.018m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP043031.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 5:50
Operator : AJ\MA
Sample : N1162-02 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MMO-01-2022-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 07:12:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

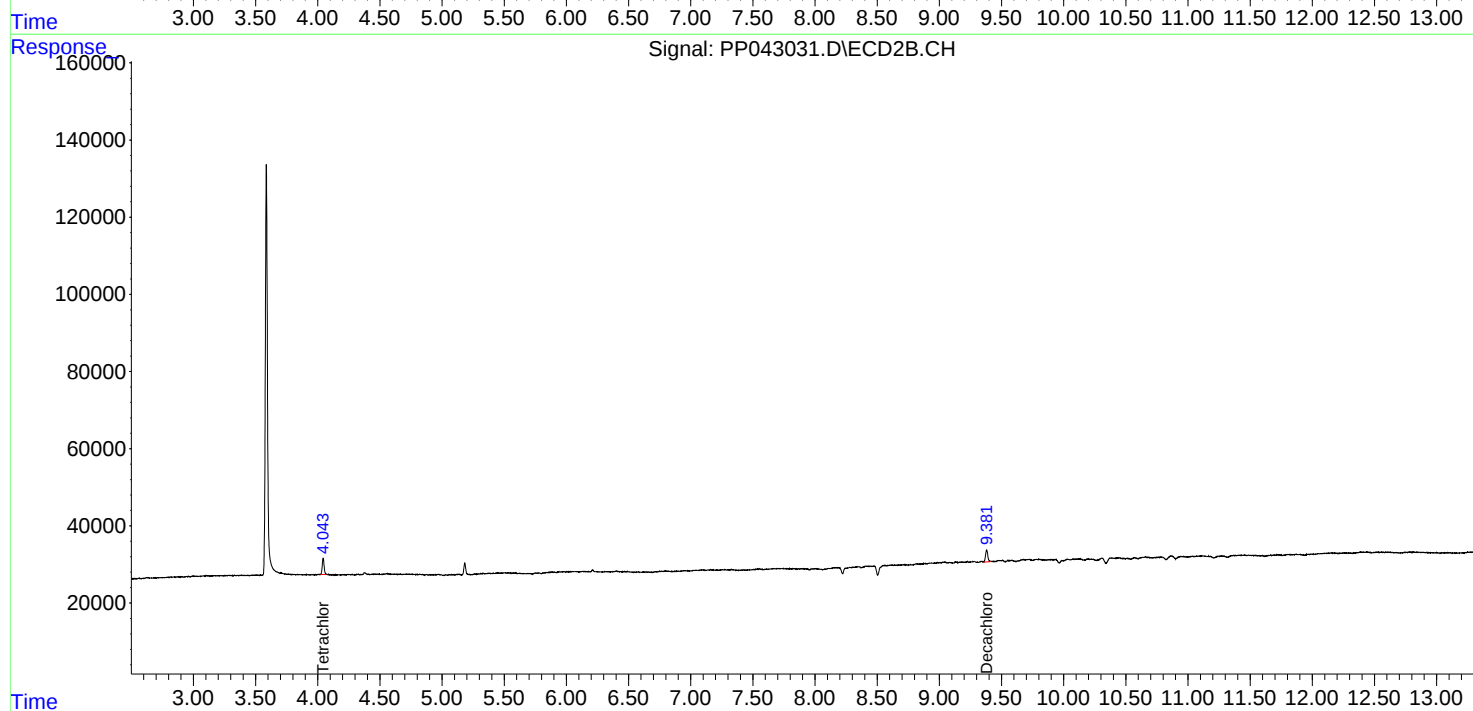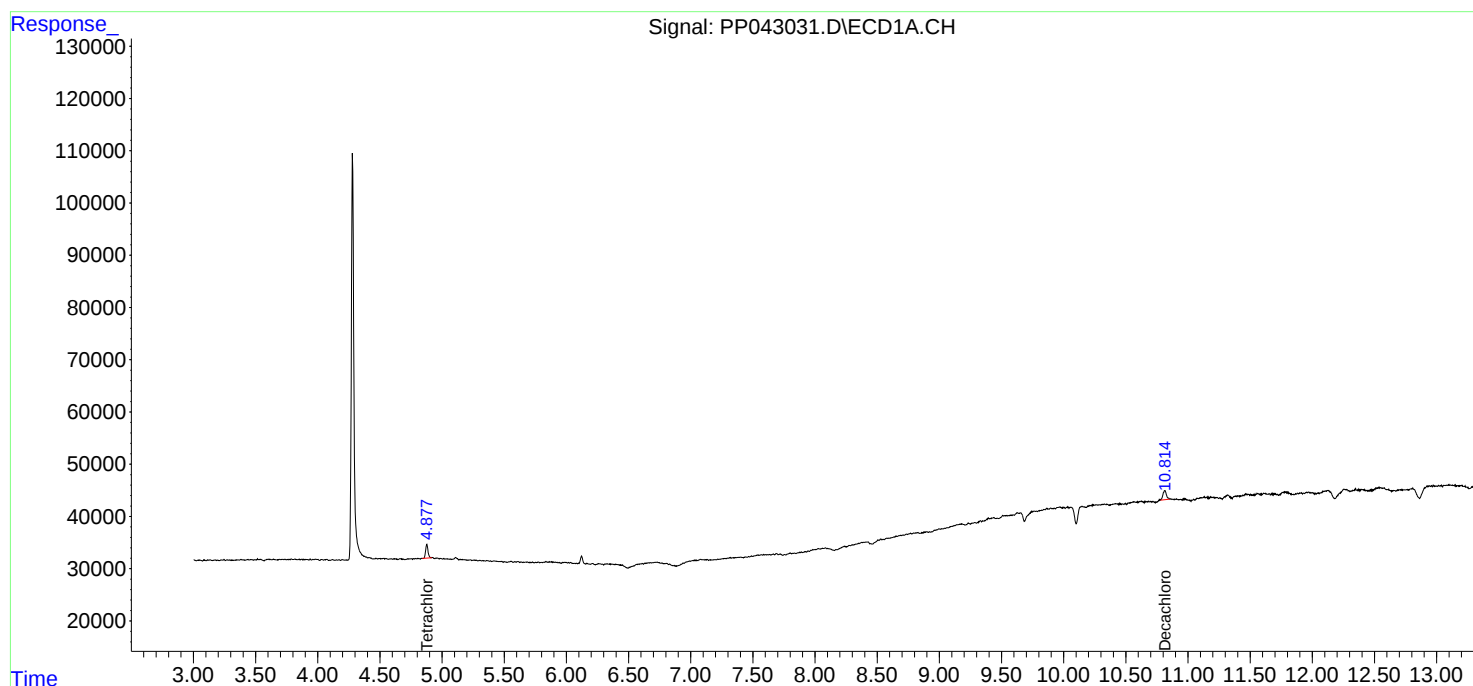

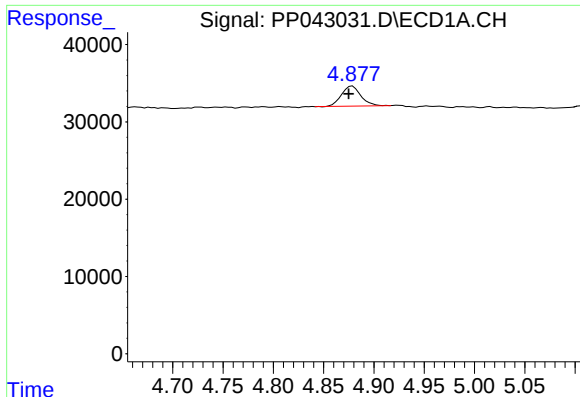


#1 Tetrachloro-m-xylene

R.T.: 4.879 min
Delta R.T.: 0.004 min
Response: 34883
Conc: 1.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MMO-01-2022-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

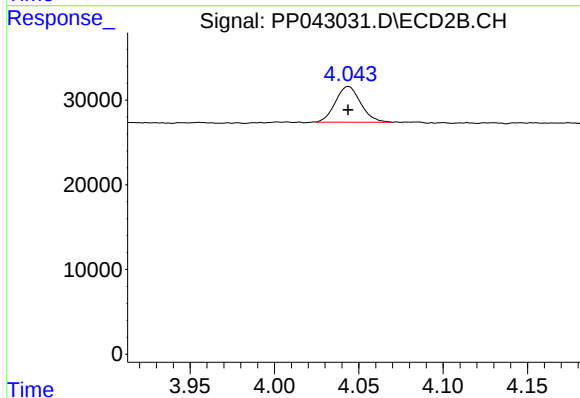


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 43987
Conc: 1.76 ng/ml m

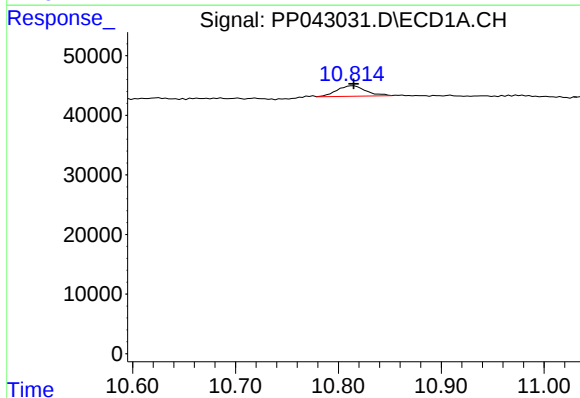

#2 Decachlorobiphenyl

R.T.: 10.813 min
Delta R.T.: -0.002 min
Response: 34083
Conc: 2.33 ng/ml m

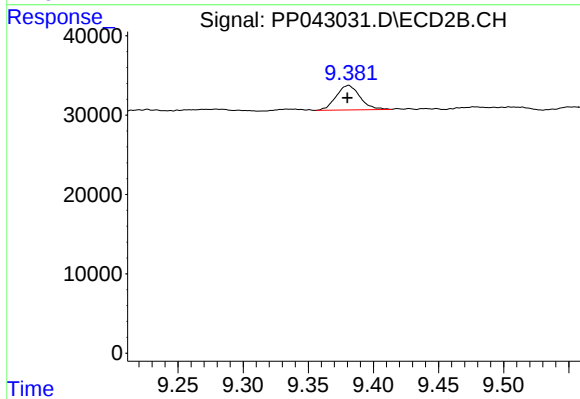

#2 Decachlorobiphenyl

R.T.: 9.381 min
Delta R.T.: 0.000 min
Response: 39371
Conc: 2.02 ng/ml m