

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011725\
 Data File : PP069205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2025 19:33
 Operator : YP\AJ
 Sample : Q1118-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-01-1-16-2025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2025
 Supervised By :Ankita Jodhani 01/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 01:06:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.670	3.980	31935607	20085025	22.954	20.575m
2) SA Decachlor...	10.513	9.100	24331223	22273500	21.793	18.541

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011725\
Data File : PP069205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2025 19:33
Operator : YP\AJ
Sample : Q1118-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OK-01-1-16-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2025
Supervised By :Ankita Jodhani 01/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 01:06:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

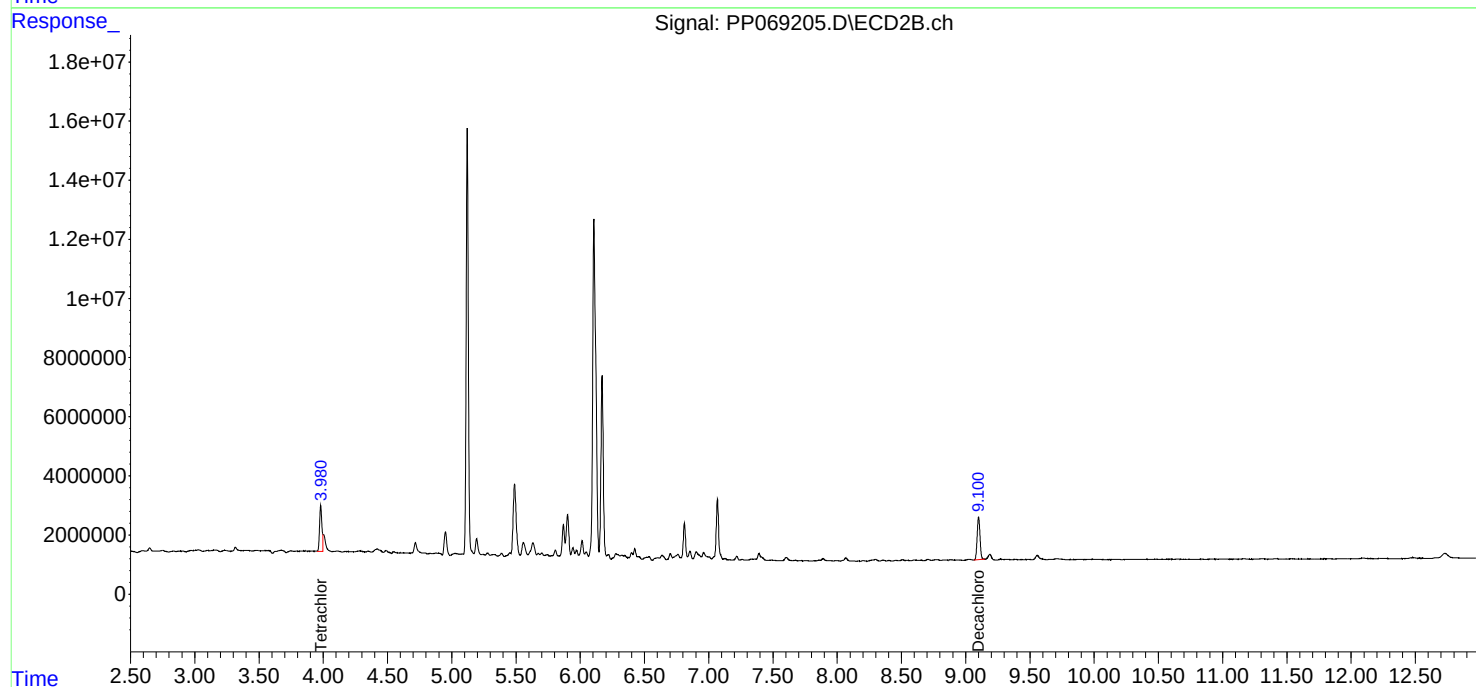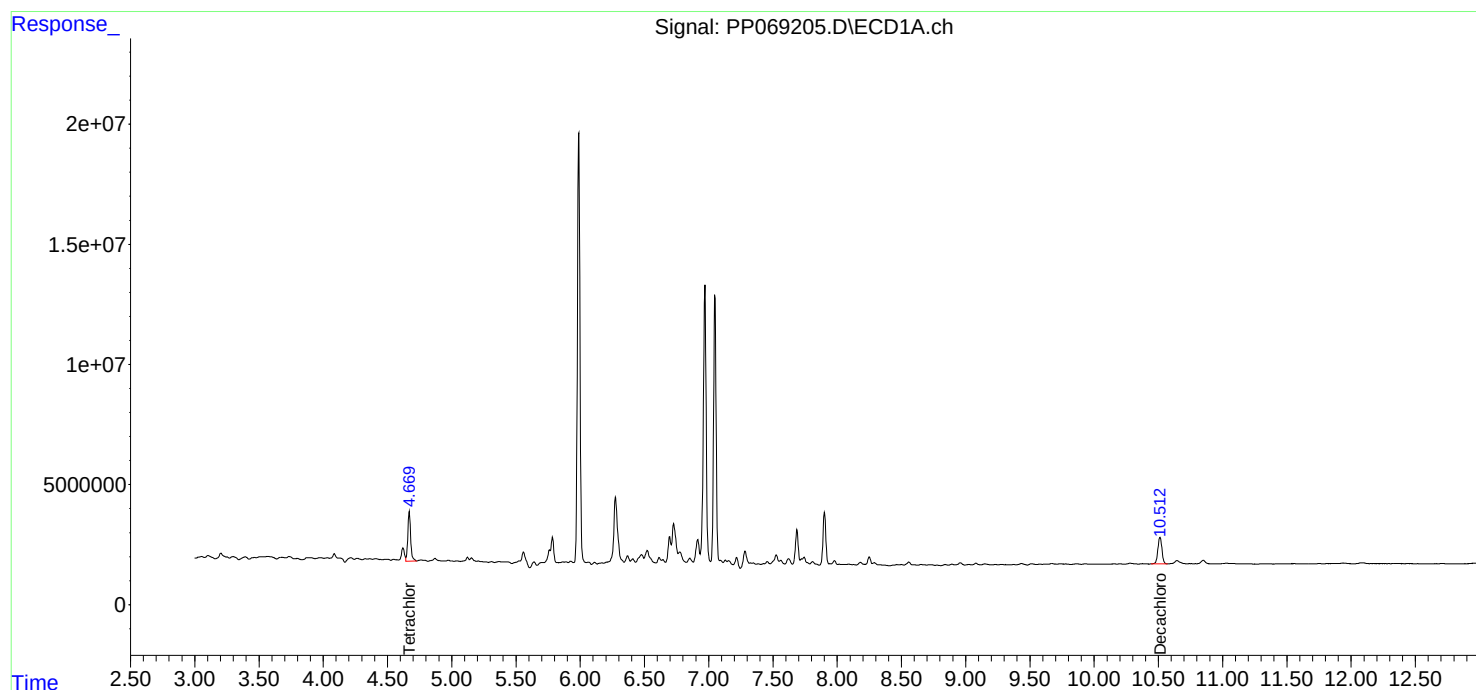

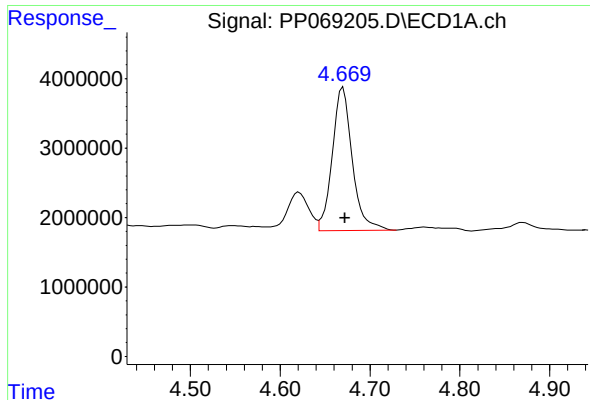


#1 Tetrachloro-m-xylene

R.T.: 4.670 min
Delta R.T.: -0.002 min
Response: 31935607
Conc: 22.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-01-1-16-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2025
Supervised By :Ankita Jodhani 01/21/2025

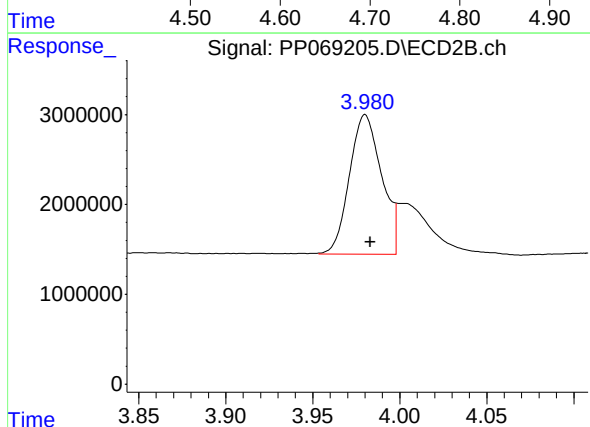


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.003 min
Response: 20085025
Conc: 20.58 ng/ml

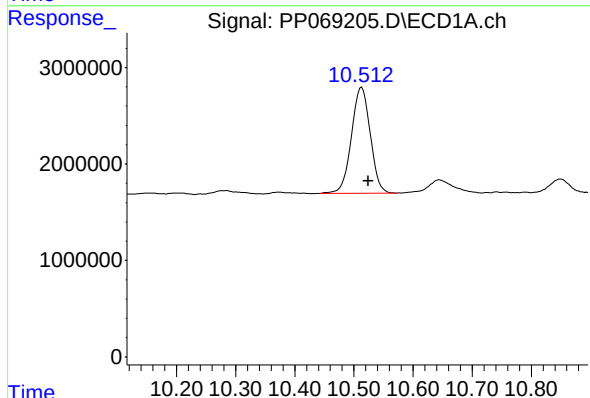

#2 Decachlorobiphenyl

R.T.: 10.513 min
Delta R.T.: -0.011 min
Response: 24331223
Conc: 21.79 ng/ml

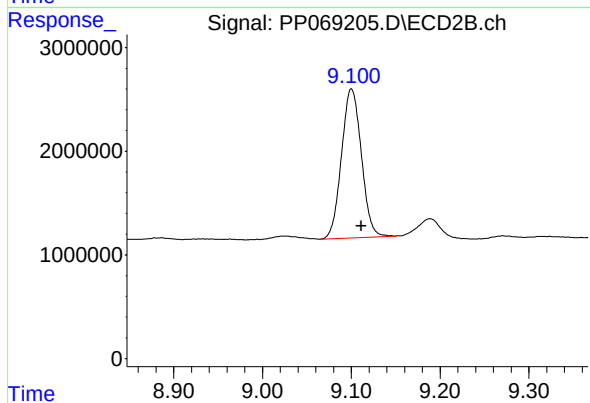

#2 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.011 min
Response: 22273500
Conc: 18.54 ng/ml