

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
 Data File : PP032796.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 16:16
 Operator : DD\AJ
 Sample : M1082-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BACKFILL-ASHCROFT-02

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:04:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:28:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.752	4.012	1707546	1150918	29.400	24.467
2) SA Decachlor...	10.594f	9.297	1166899	999255	29.577m	26.674

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
Data File : PP032796.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 16:16
Operator : DD\AJ
Sample : M1082-03
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-02


Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:28:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

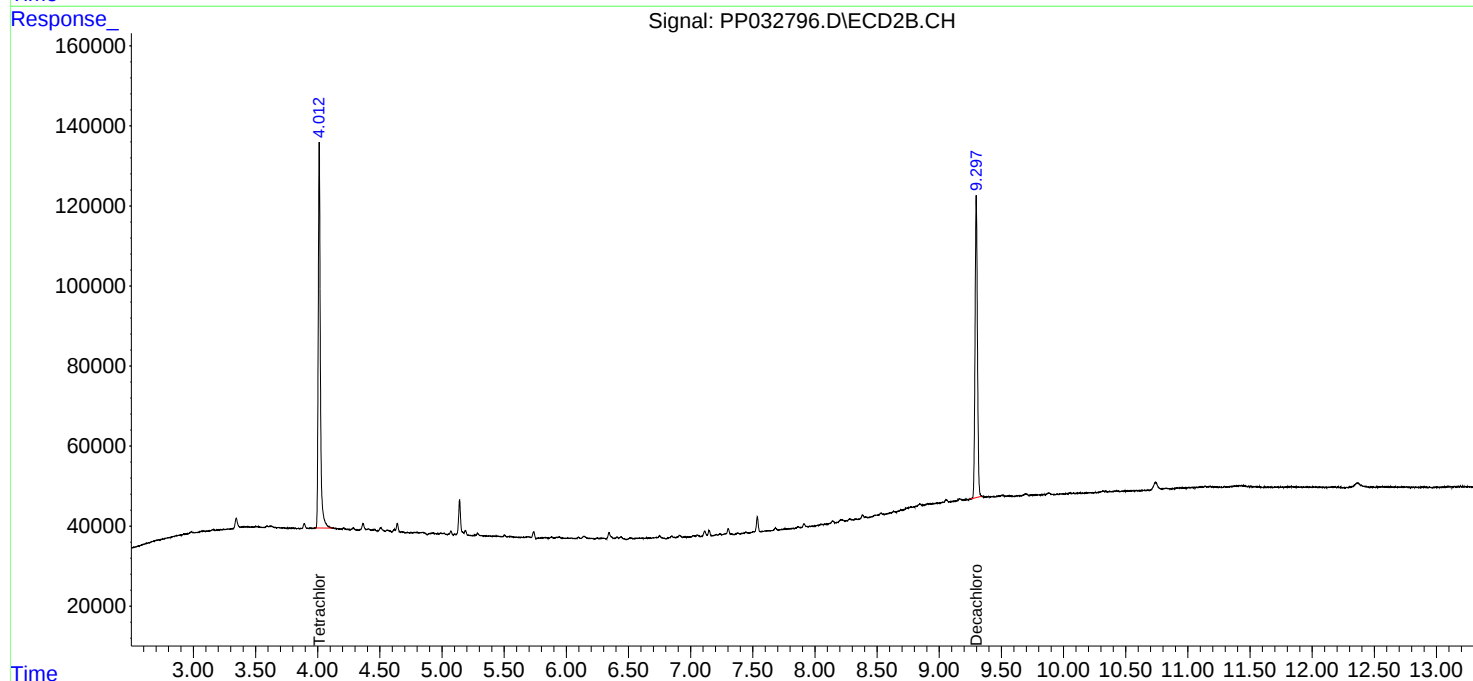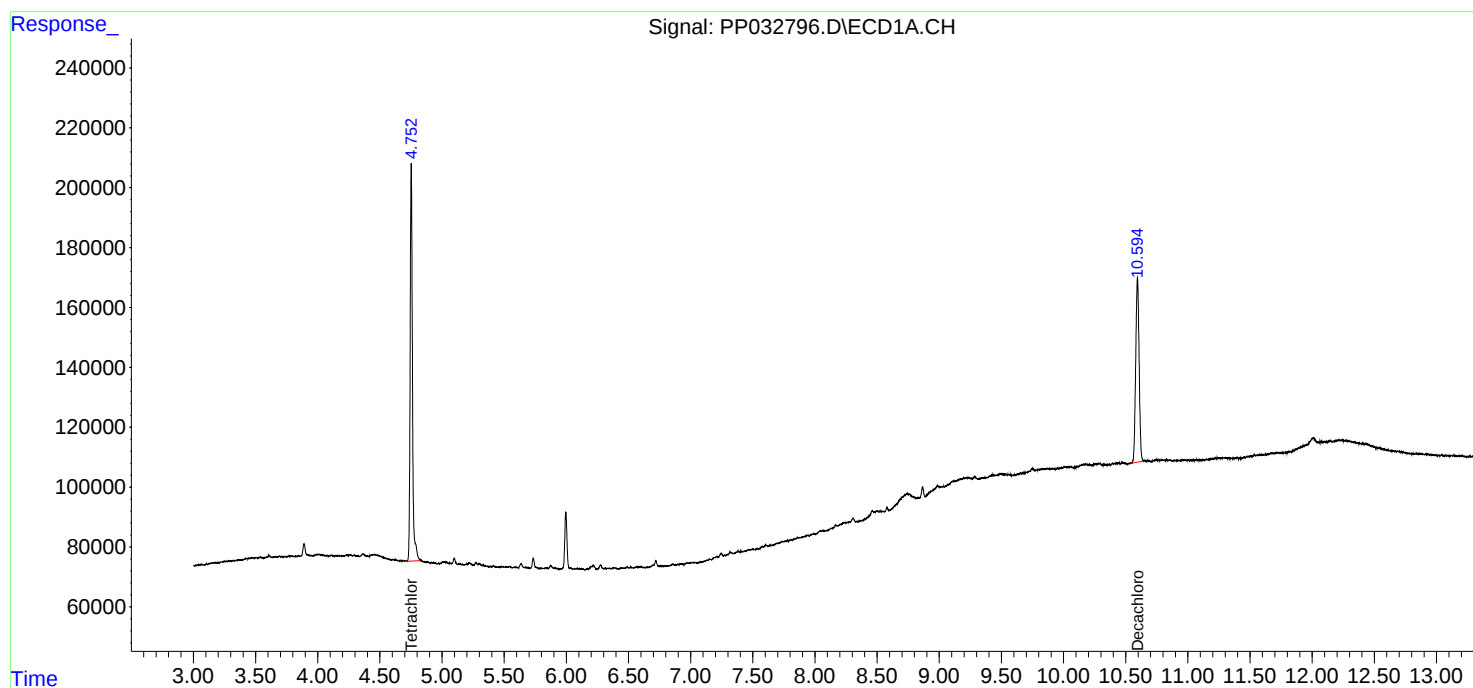

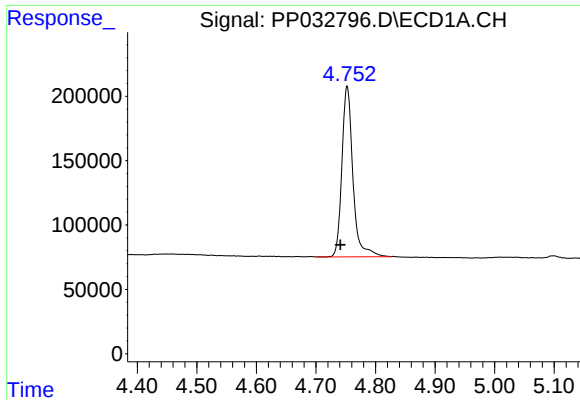


#1 Tetrachloro-m-xylene

R.T.: 4.752 min
Delta R.T.: 0.011 min
Response: 1707546
Conc: 29.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-02


Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:43 AM

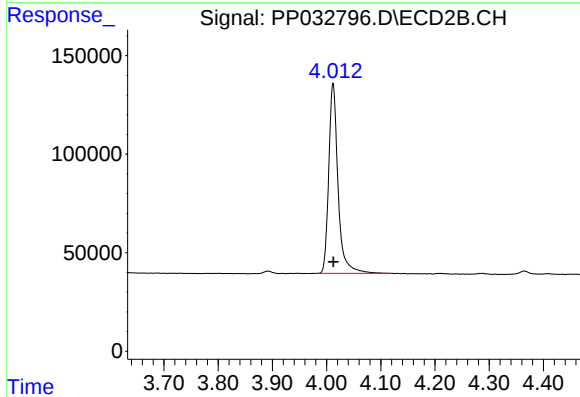


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 1150918
Conc: 24.47 ng/ml

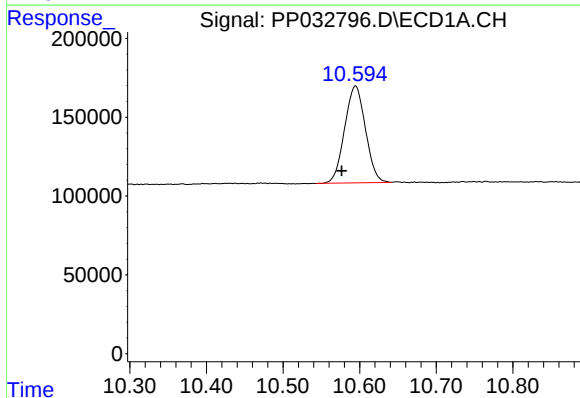

#2 Decachlorobiphenyl

R.T.: 10.594 min
Delta R.T.: 0.017 min
Response: 1166899
Conc: 29.58 ng/ml m

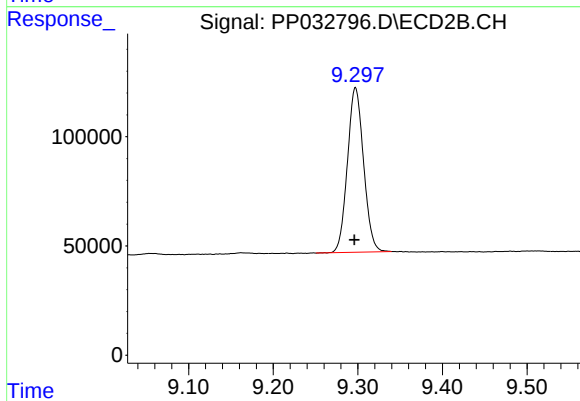

#2 Decachlorobiphenyl

R.T.: 9.297 min
Delta R.T.: 0.001 min
Response: 999255
Conc: 26.67 ng/ml