

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
 Data File : PP032798.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 16:49
 Operator : DD\AJ
 Sample : M1160-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BASIN-4

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:04:44 AM

1/19/2021 10:04:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:29:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.739	4.012	1292745	1011363	22.258m	21.500
2) SA Decachlor...	10.576	9.292	924399	736548	23.430	19.661

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
Data File : PP032798.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 16:49
Operator : DD\AJ
Sample : M1160-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BASIN-4


Manual Integrations
APPROVED


Ankita
1/19/2021 10:04:44 AM

1/19/2021 10:04:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:29:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

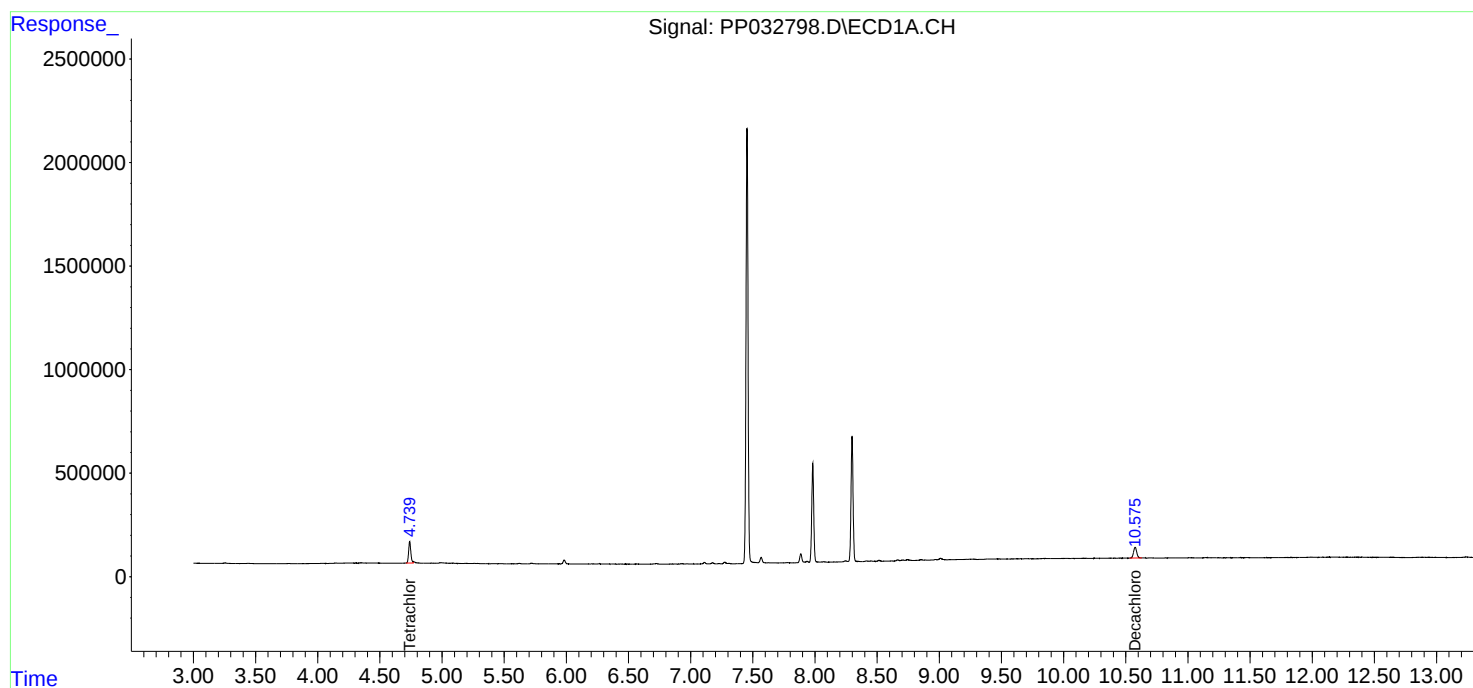

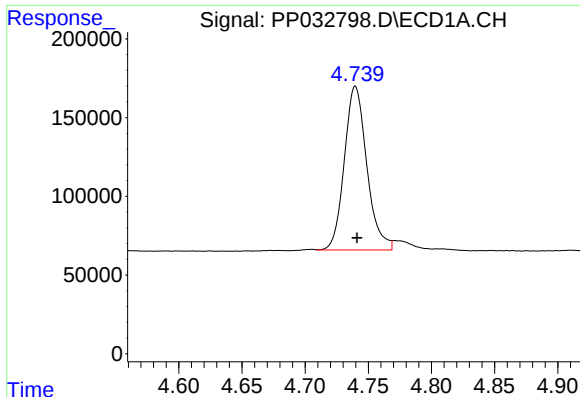

#1 Tetrachloro-m-xylene


R.T.: 4.739 min
Delta R.T.: -0.002 min
Response: 1292745
Conc: 22.26 ng/ml m

Instrument :
ECD_P
ClientSampleId :
BASIN-4

Manual Integrations
APPROVED


Ankita
1/19/2021 10:04:44 AM

1/19/2021 10:04:44 AM

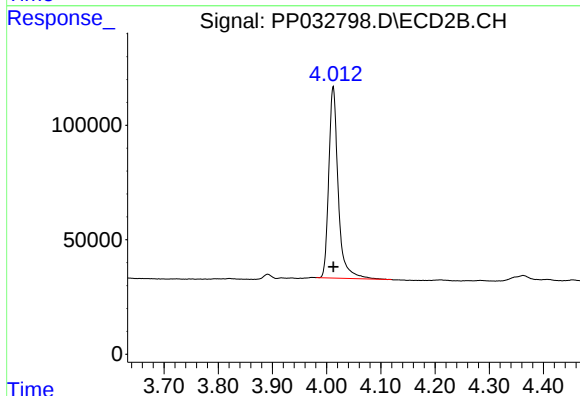


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 1011363
Conc: 21.50 ng/ml

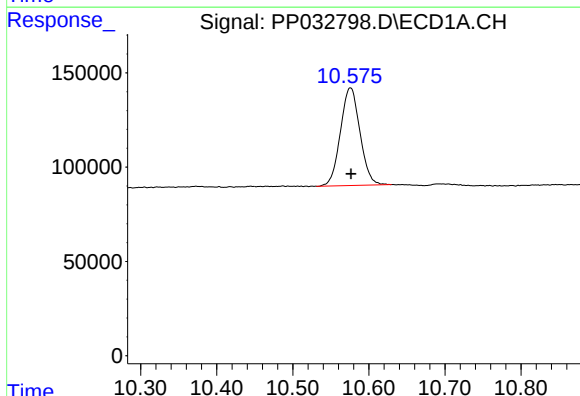

#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: 0.000 min
Response: 924399
Conc: 23.43 ng/ml

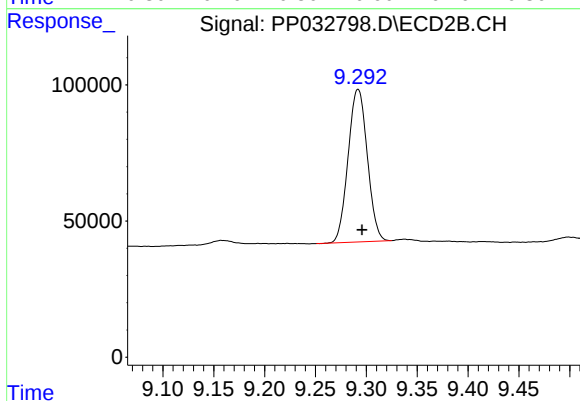

#2 Decachlorobiphenyl

R.T.: 9.292 min
Delta R.T.: -0.004 min
Response: 736548
Conc: 19.66 ng/ml