

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
 Data File : PP032812.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 20:59
 Operator : DD\AJ
 Sample : M1106-06 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6-01-C

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:04:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:33:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.739	4.012	320484	243066	5.518	5.167
2) SA Decachlor...	10.574	9.291	220428	211099	5.587	5.635
Target Compounds						
41) L9 AR-1268-1	9.182	8.209	154998	133324	23.412	23.645
42) L9 AR-1268-2	9.272	8.275	112226	98202	18.630	18.115
43) L9 AR-1268-3	9.482	8.478	122048	102688	22.800	21.627m
44) L9 AR-1268-4	9.885	8.771	34660	26826	16.901m	14.832m
45) L9 AR-1268-5	10.268	9.051	334540	303494	22.131	20.962

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
Data File : PP032812.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 20:59
Operator : DD\AJ
Sample : M1106-06 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
S6-01-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:33:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

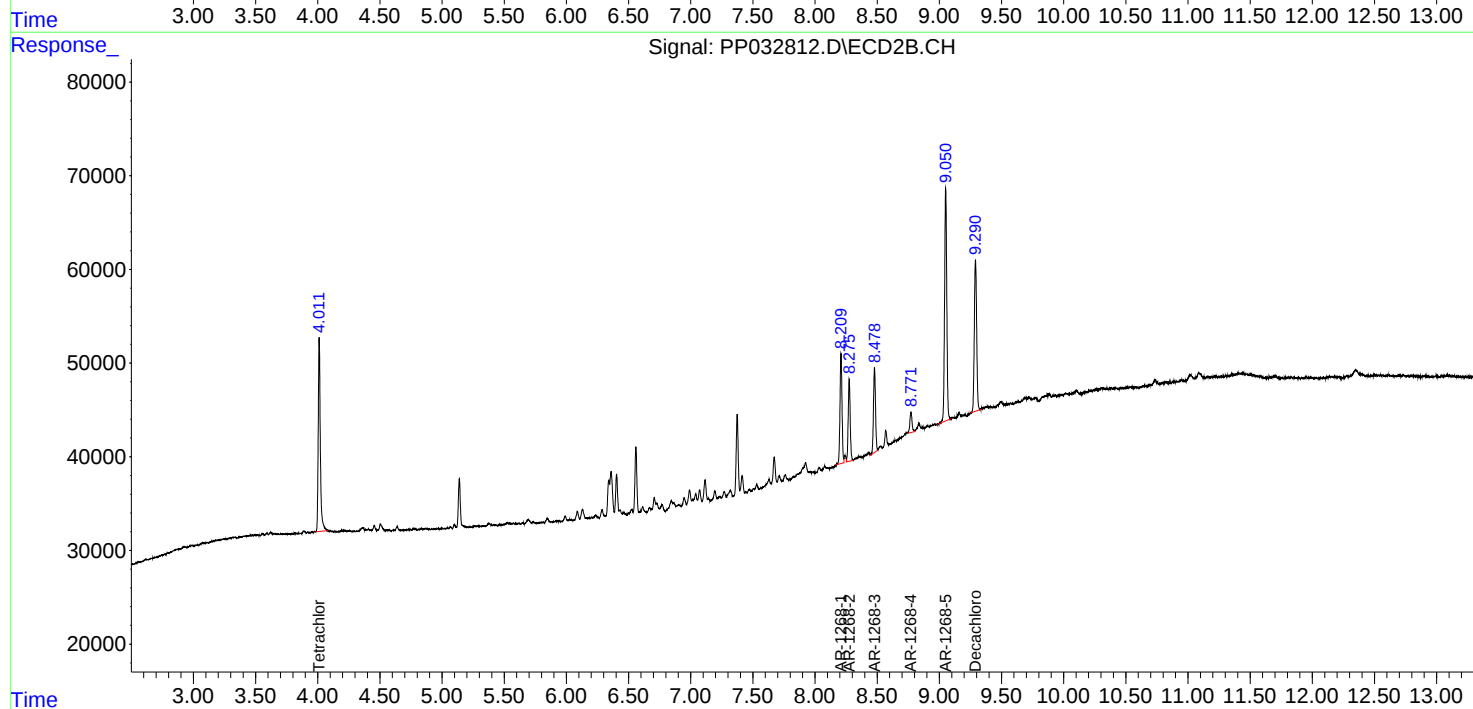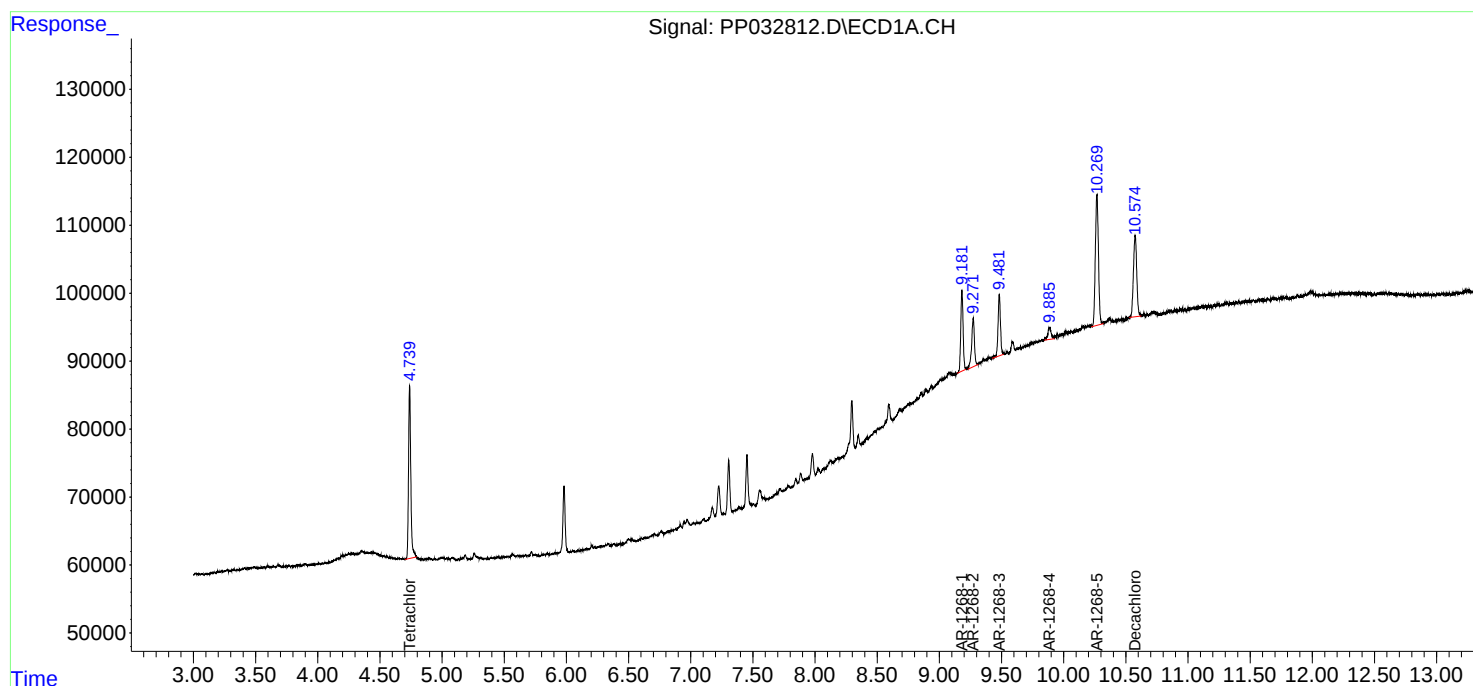

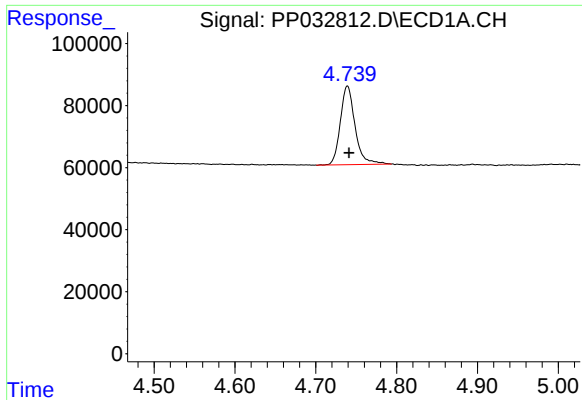


#1 Tetrachloro-m-xylene

R.T.: 4.739 min
Delta R.T.: -0.002 min
Response: 320484
Conc: 5.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-01-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:57 AM

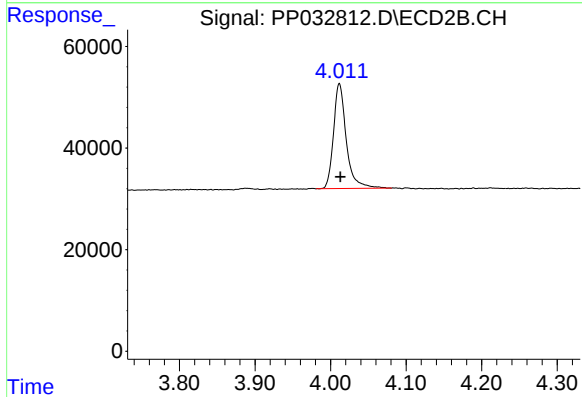


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: -0.001 min
Response: 243066
Conc: 5.17 ng/ml

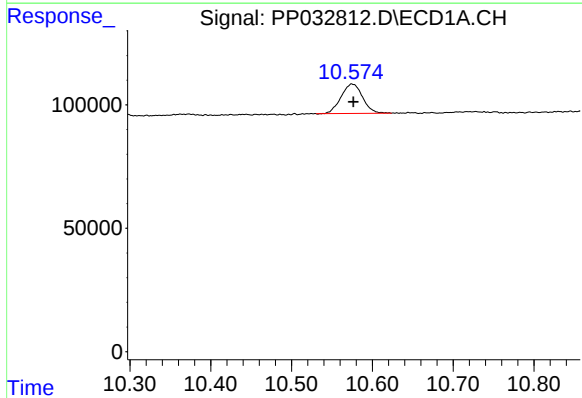


#2 Decachlorobiphenyl

R.T.: 10.574 min
Delta R.T.: -0.002 min
Response: 220428
Conc: 5.59 ng/ml

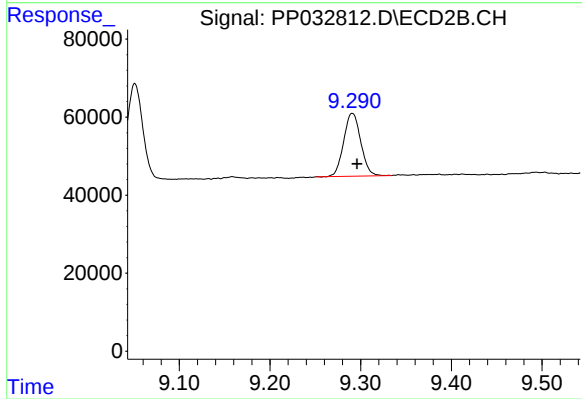

#2 Decachlorobiphenyl

R.T.: 9.291 min
Delta R.T.: -0.005 min
Response: 211099
Conc: 5.63 ng/ml

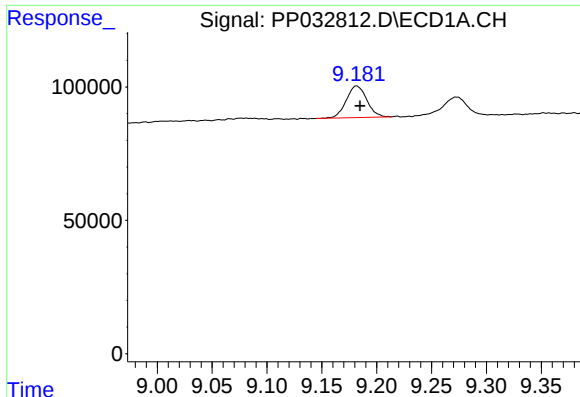


#41 AR-1268-1

R.T.: 9.182 min
Delta R.T.: -0.003 min
Response: 154998
Conc: 23.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-01-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:57 AM

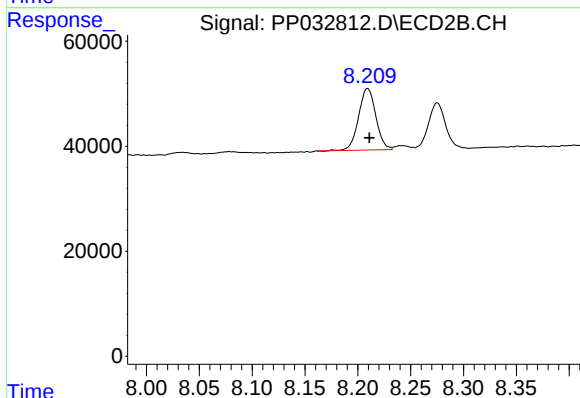


#41 AR-1268-1

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 133324
Conc: 23.65 ng/ml

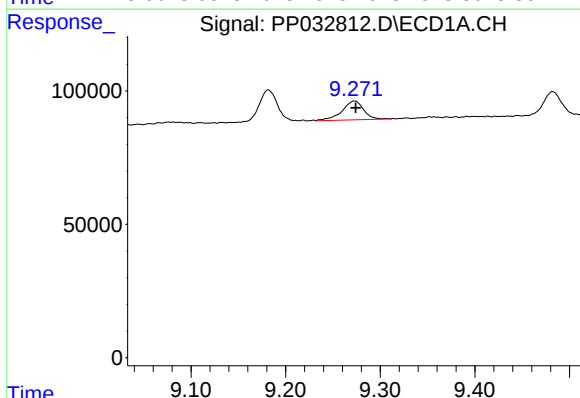


#42 AR-1268-2

R.T.: 9.272 min
Delta R.T.: -0.002 min
Response: 112226
Conc: 18.63 ng/ml

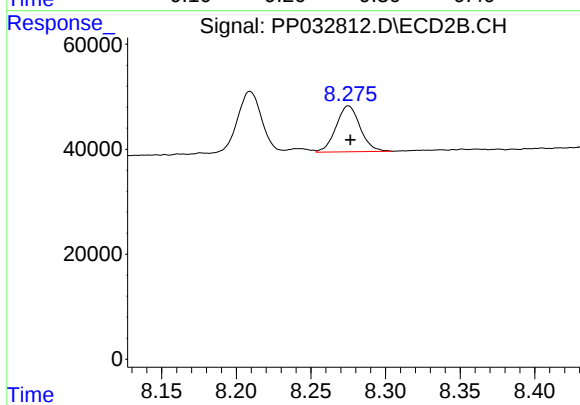

#42 AR-1268-2

R.T.: 8.275 min
Delta R.T.: -0.001 min
Response: 98202
Conc: 18.11 ng/ml

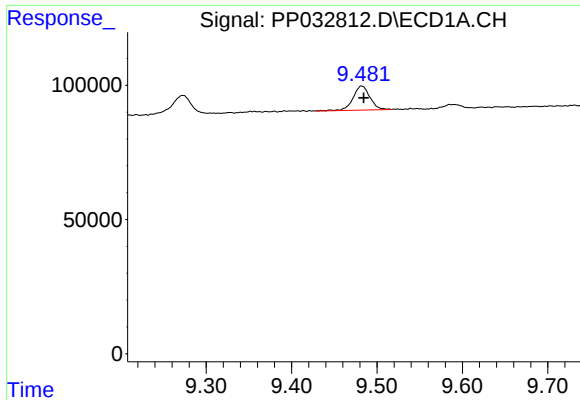


#43 AR-1268-3

R.T.: 9.482 min
Delta R.T.: -0.003 min
Response: 122048
Conc: 22.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-01-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:57 AM

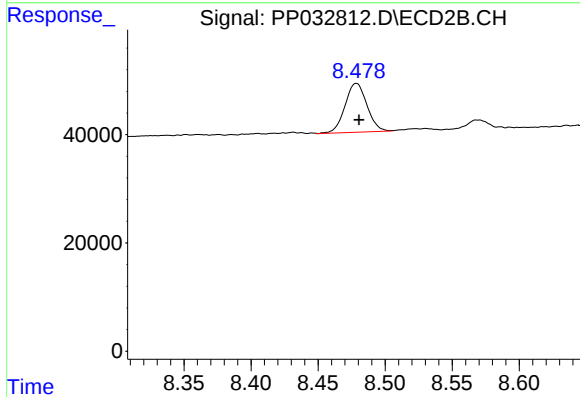


#43 AR-1268-3

R.T.: 8.478 min
Delta R.T.: -0.002 min
Response: 102688
Conc: 21.63 ng/ml m

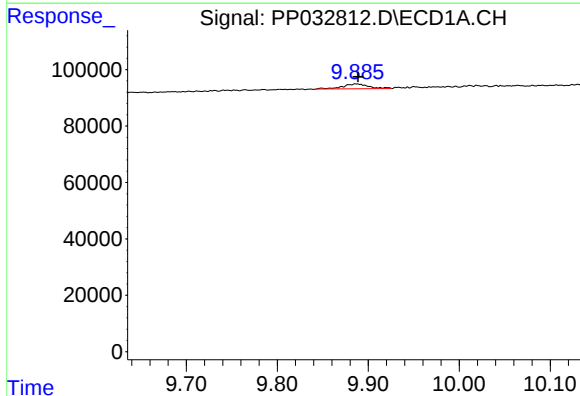


#44 AR-1268-4

R.T.: 9.885 min
Delta R.T.: -0.004 min
Response: 34660
Conc: 16.90 ng/ml m

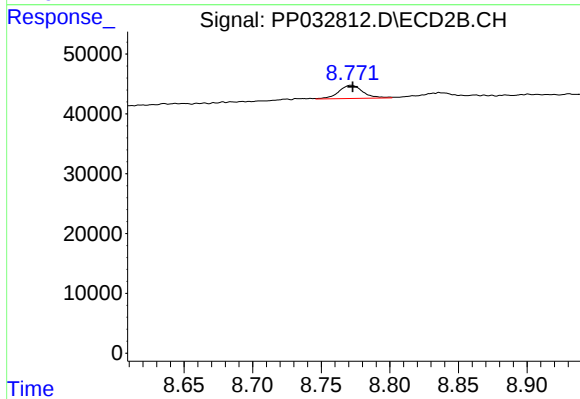

#44 AR-1268-4

R.T.: 8.771 min
Delta R.T.: -0.002 min
Response: 26826
Conc: 14.83 ng/ml m

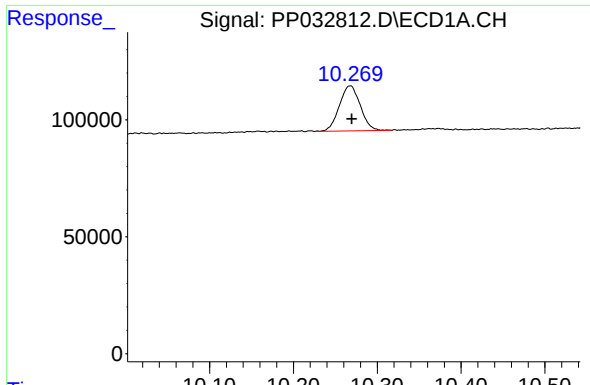


#45 AR-1268-5

R.T.: 10.268 min
Delta R.T.: -0.001 min
Response: 334540
Conc: 22.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-01-C

Manual Integrations
APPROVED

Ankita
1/19/2021 10:04:57 AM

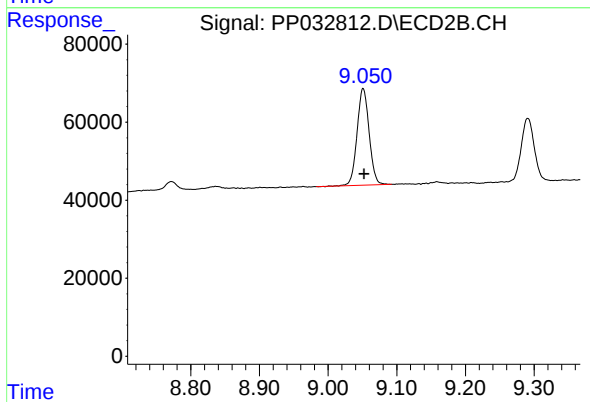

#45 AR-1268-5

R.T.: 9.051 min
Delta R.T.: -0.001 min
Response: 303494
Conc: 20.96 ng/ml