

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
 Data File : PP032816.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 22:06
 Operator : DD\AJ
 Sample : M1106-10 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6-05-C

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:05:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:34:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.739	4.012	262077	200877	4.512	4.270
2) SA Decachlor...	10.573	9.291	185707	172284	4.707	4.599
Target Compounds						
41) L9 AR-1268-1	9.182	8.210	135658	117651	20.491	20.865
42) L9 AR-1268-2	9.271	8.275	89071	72356	14.786	13.347
43) L9 AR-1268-3	9.482	8.479	125478	100937	23.441	21.258
44) L9 AR-1268-4	9.891	8.769	25719	20465	12.541m	11.315m
45) L9 AR-1268-5	10.266	9.050	309482	280353	20.473	19.364m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011821\
Data File : PP032816.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 22:06
Operator : DD\AJ
Sample : M1106-10 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
S6-05-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:34:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

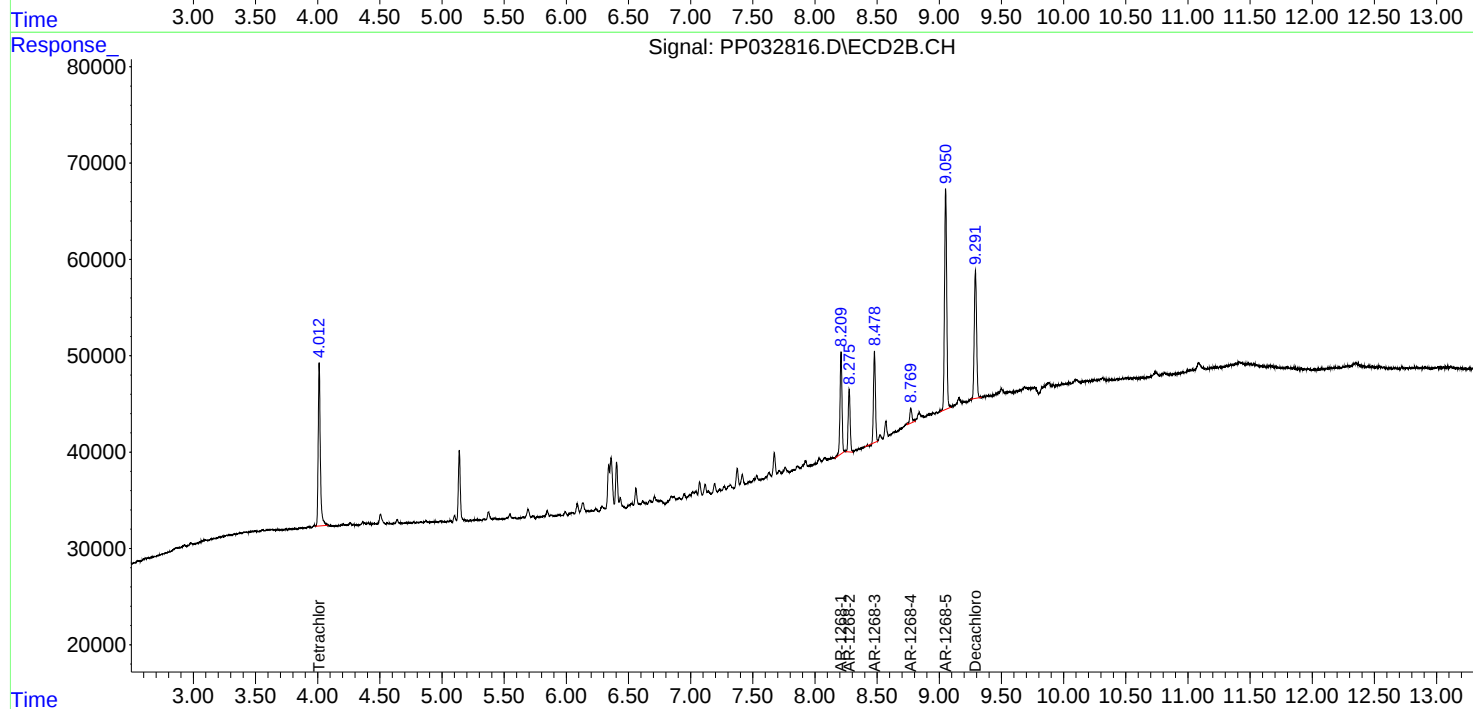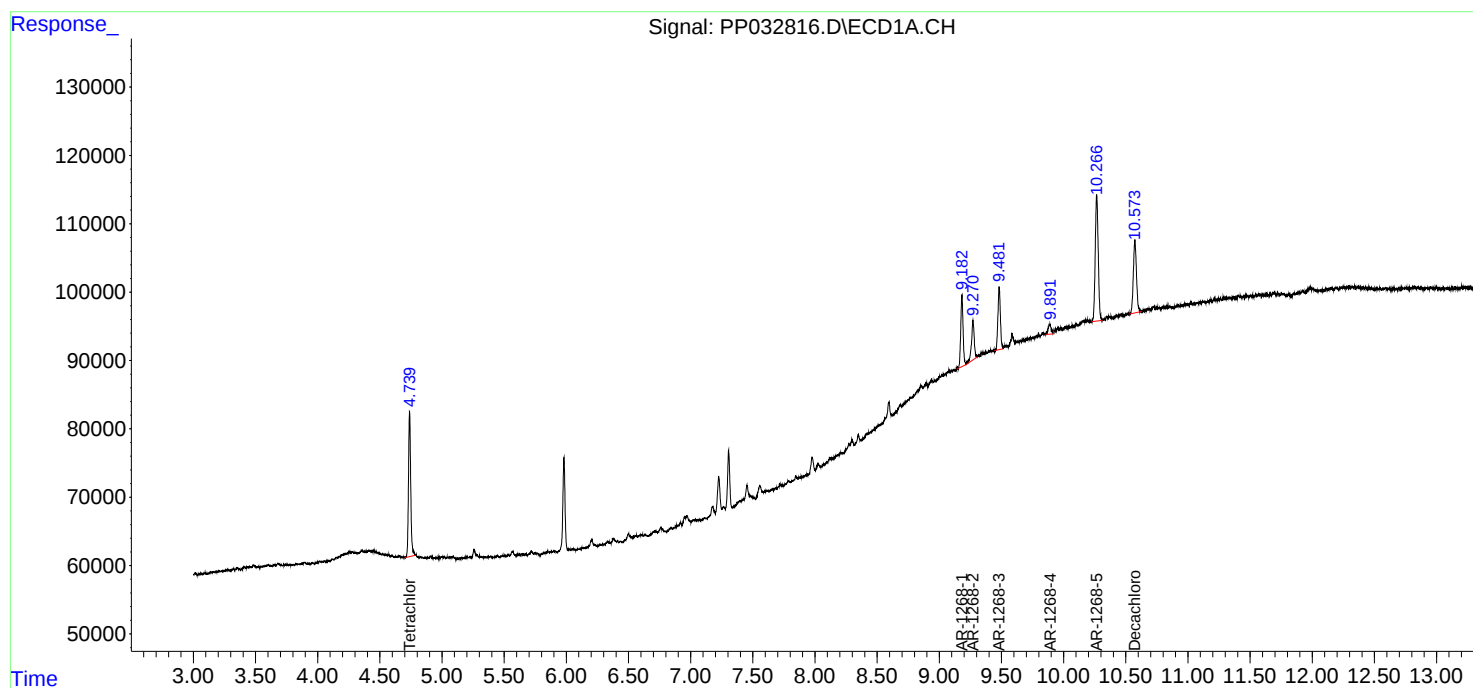

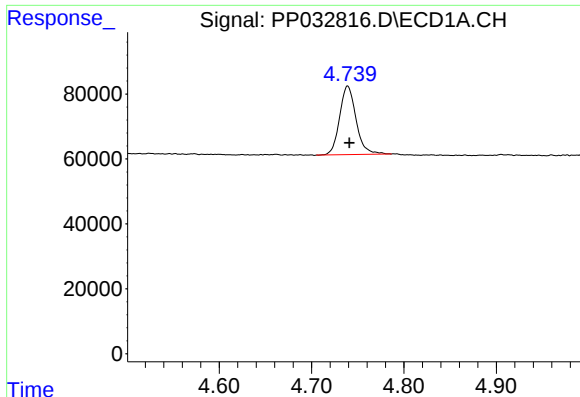


#1 Tetrachloro-m-xylene

R.T.: 4.739 min
Delta R.T.: -0.002 min
Response: 262077
Conc: 4.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-05-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:01 AM

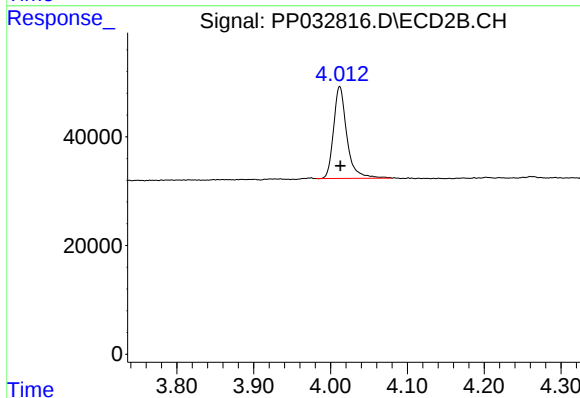


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 200877
Conc: 4.27 ng/ml

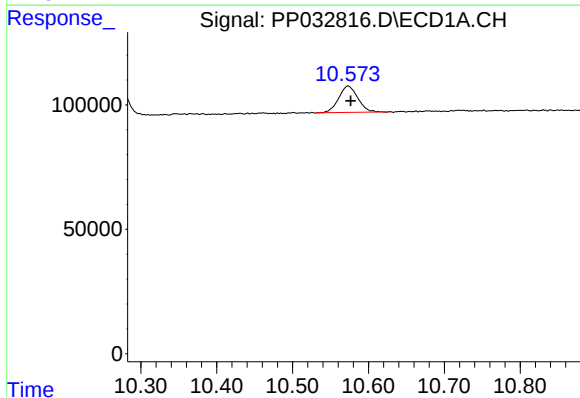


#2 Decachlorobiphenyl

R.T.: 10.573 min
Delta R.T.: -0.003 min
Response: 185707
Conc: 4.71 ng/ml

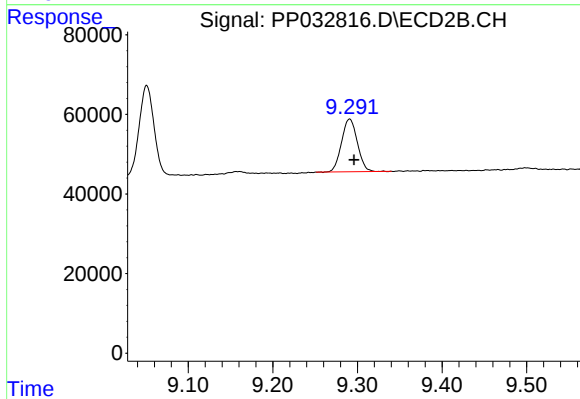

#2 Decachlorobiphenyl

R.T.: 9.291 min
Delta R.T.: -0.005 min
Response: 172284
Conc: 4.60 ng/ml

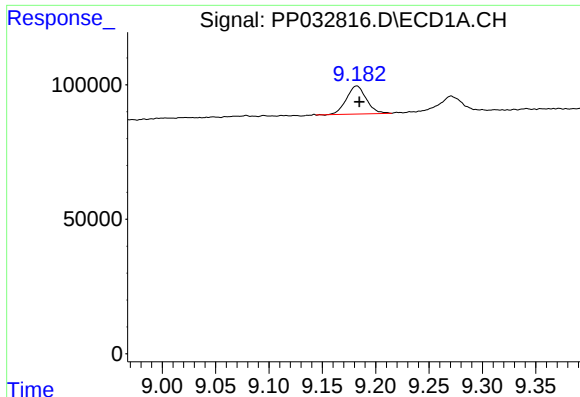


#41 AR-1268-1

R.T.: 9.182 min
Delta R.T.: -0.002 min
Response: 135658
Conc: 20.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-05-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:01 AM

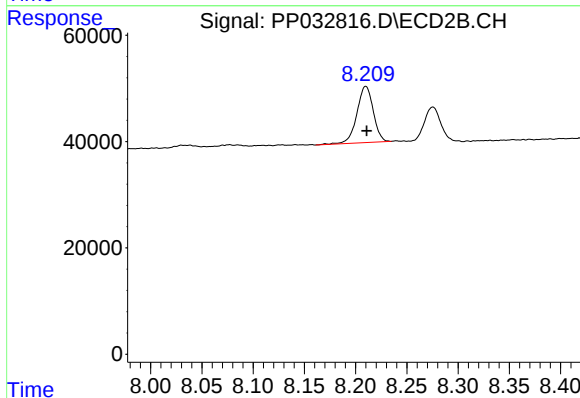


#41 AR-1268-1

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 117651
Conc: 20.87 ng/ml

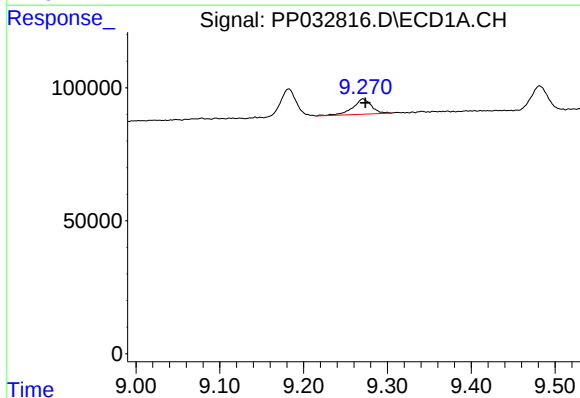


#42 AR-1268-2

R.T.: 9.271 min
Delta R.T.: -0.003 min
Response: 89071
Conc: 14.79 ng/ml

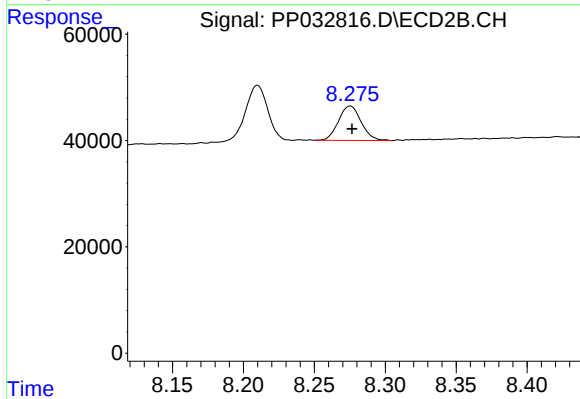

#42 AR-1268-2

R.T.: 8.275 min
Delta R.T.: -0.001 min
Response: 72356
Conc: 13.35 ng/ml

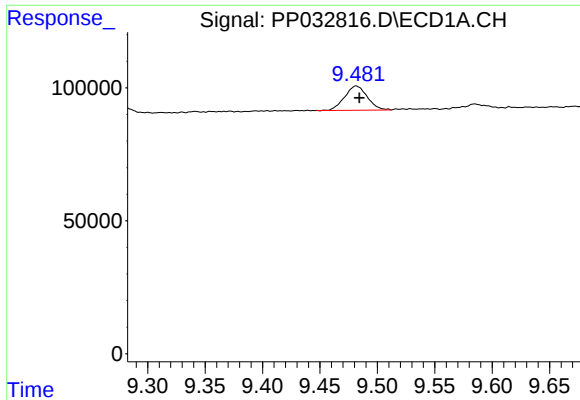


#43 AR-1268-3

R.T.: 9.482 min
Delta R.T.: -0.003 min
Response: 125478
Conc: 23.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-05-C


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:01 AM

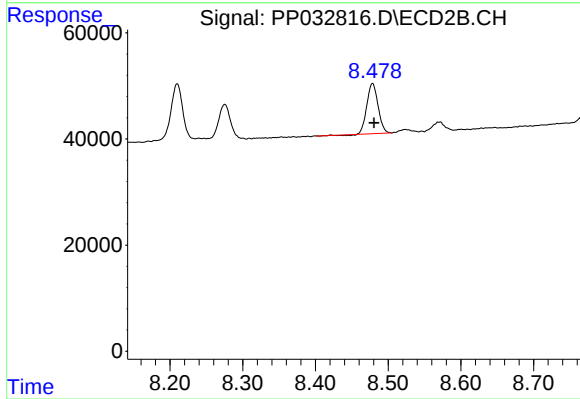


#43 AR-1268-3

R.T.: 8.479 min
Delta R.T.: -0.002 min
Response: 100937
Conc: 21.26 ng/ml

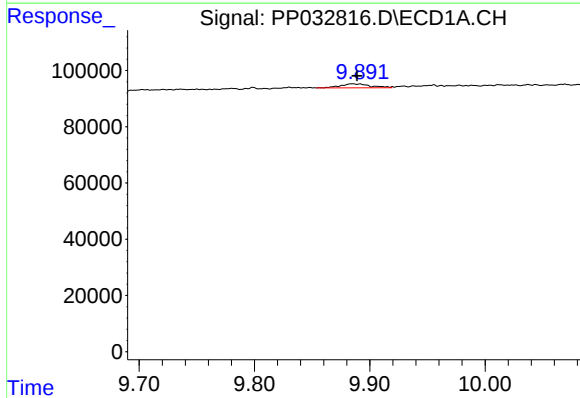


#44 AR-1268-4

R.T.: 9.891 min
Delta R.T.: 0.002 min
Response: 25719
Conc: 12.54 ng/ml m

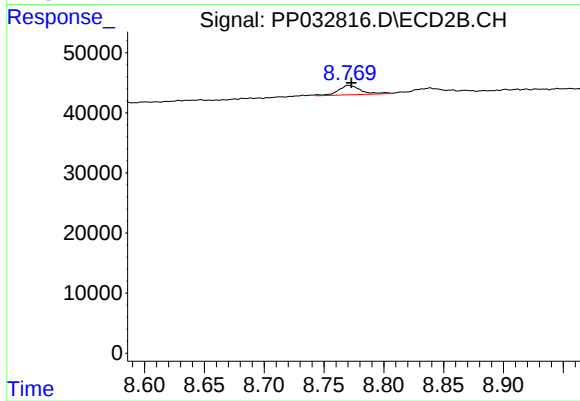

#44 AR-1268-4

R.T.: 8.769 min
Delta R.T.: -0.004 min
Response: 20465
Conc: 11.31 ng/ml m

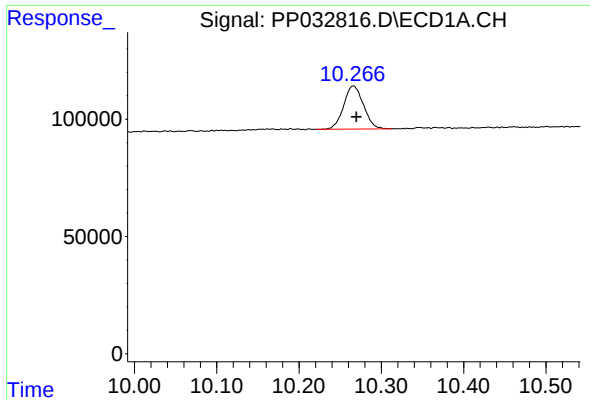


#45 AR-1268-5

R.T.: 10.266 min
Delta R.T.: -0.004 min
Response: 309482
Conc: 20.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-05-C

Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:01 AM

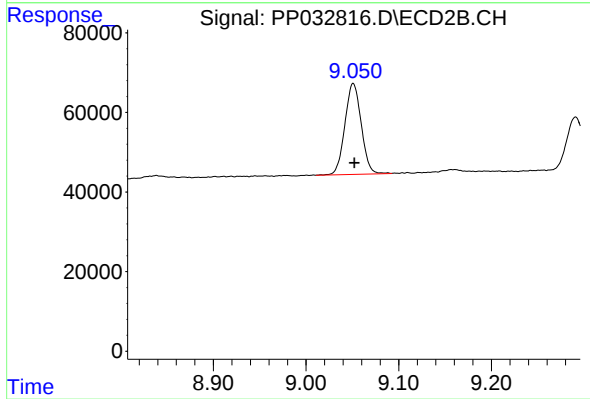

#45 AR-1268-5

R.T.: 9.050 min
Delta R.T.: -0.002 min
Response: 280353
Conc: 19.36 ng/ml m