

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
 Data File : PP043045.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 10:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:17:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.876	4.041	486369	542574	20.555	21.724
2) SA Decachlor...	10.805	9.375	363800	453240	24.886	23.235
Target Compounds						
20) L4 AR-1242-5	0.000	6.208f	0	28582	N.D.	39.721 #
25) L5 AR-1248-5	0.000	6.208f	0	28582	N.D.	29.939 #
26) L6 AR-1254-1	0.000	6.208f	0	28582	N.D.	18.432 #
28) L6 AR-1254-3	0.000	6.786f	0	1897	N.D.	0.887 #
30) L6 AR-1254-5	8.402	0.000	23316	0	24.886	N.D. #
33) L7 AR-1260-3	8.491	0.000	7371	0	9.770	N.D. #
36) L8 AR-1262-1	8.491	0.000	7371	0	6.981	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
Data File : PP043045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 10:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:17:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

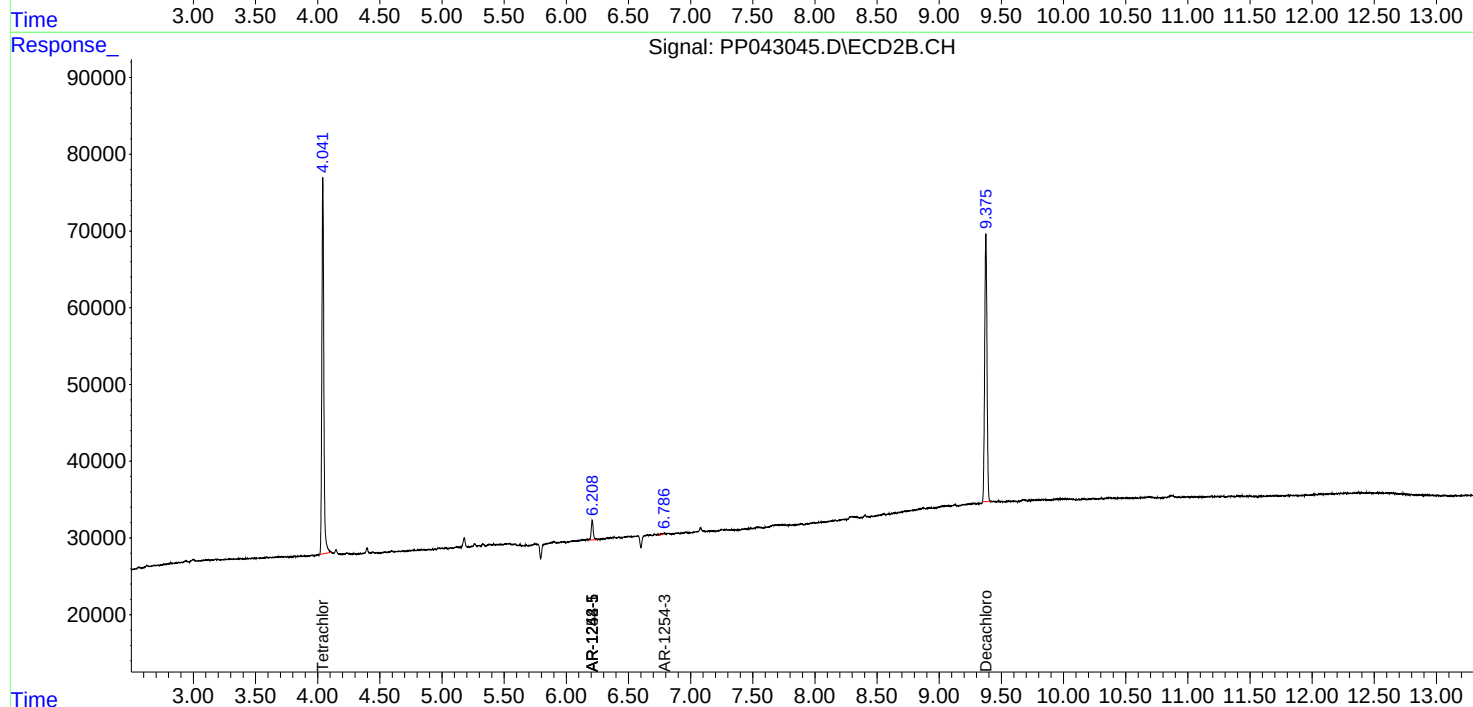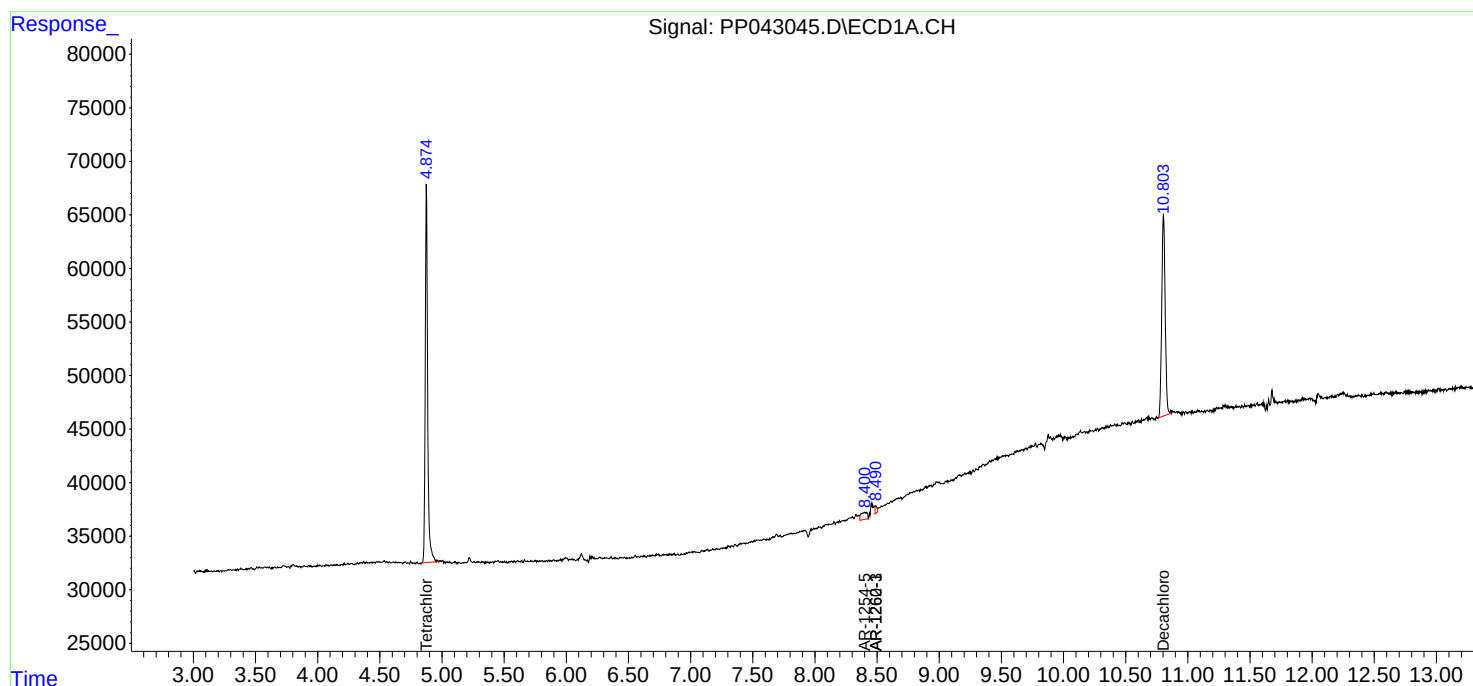


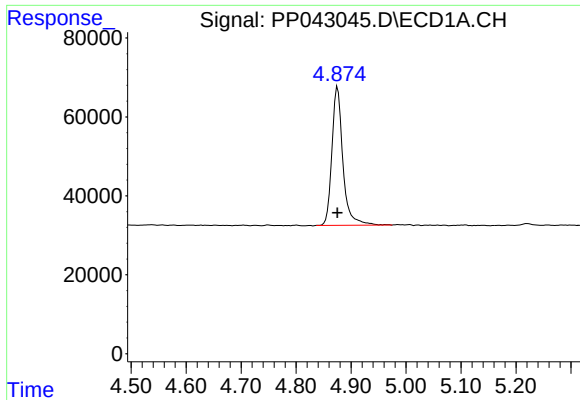

#1 Tetrachloro-m-xylene


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 486369
Conc: 20.56 ng/ml

Instrument :
ECD_P
ClientSampleId :

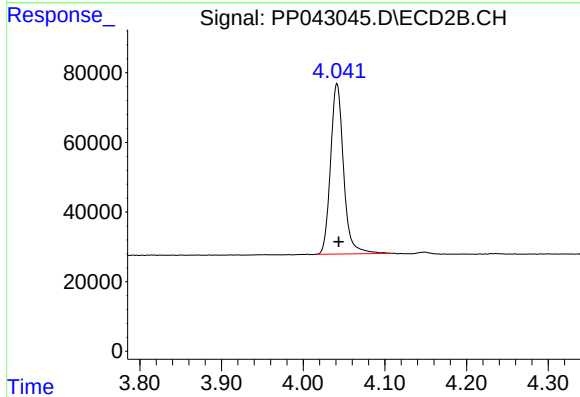


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 542574
Conc: 21.72 ng/ml

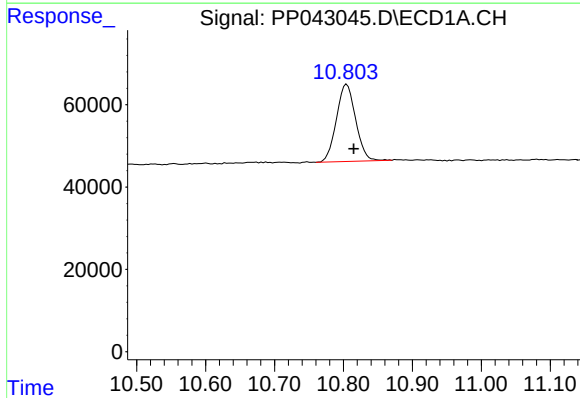


#2 Decachlorobiphenyl

R.T.: 10.805 min
Delta R.T.: -0.010 min
Response: 363800
Conc: 24.89 ng/ml

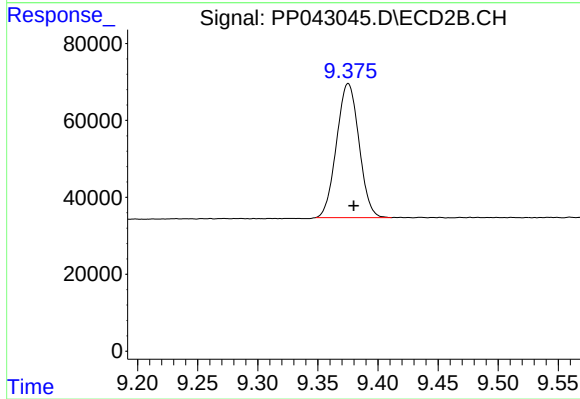

#2 Decachlorobiphenyl


R.T.: 9.375 min
Delta R.T.: -0.005 min
Response: 453240
Conc: 23.24 ng/ml

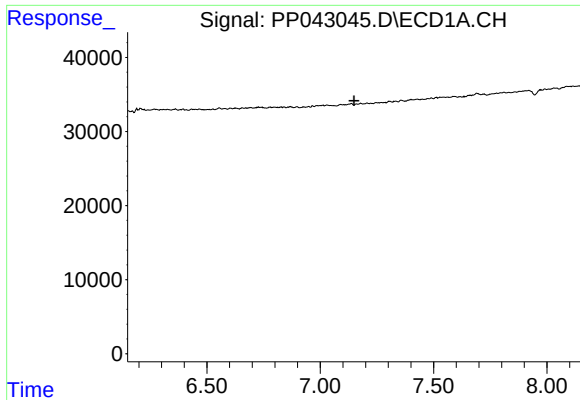

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

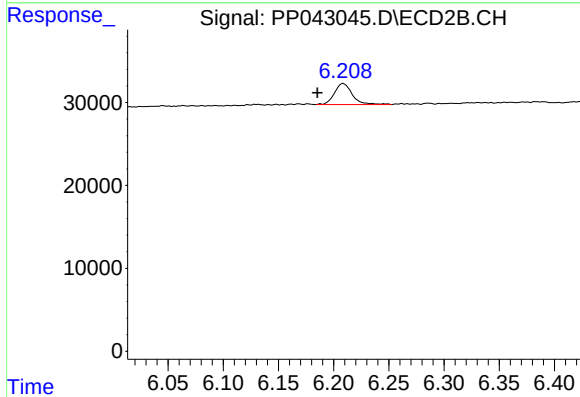


#20 AR-1242-5

R.T.: 6.208 min
Delta R.T.: 0.023 min
Response: 28582
Conc: 39.72 ng/ml

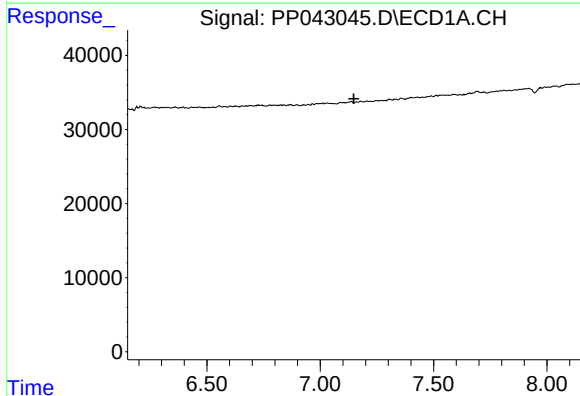


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

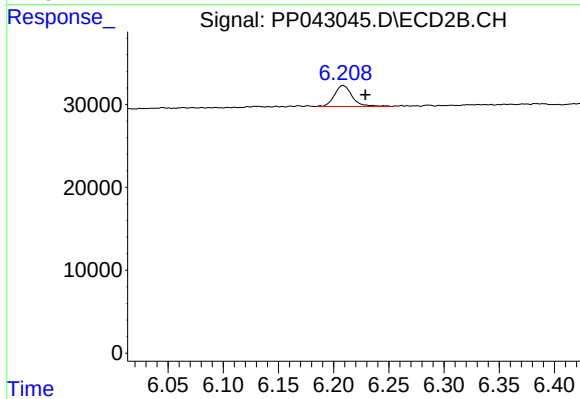

#25 AR-1248-5


R.T.: 6.208 min
Delta R.T.: -0.020 min
Response: 28582
Conc: 29.94 ng/ml

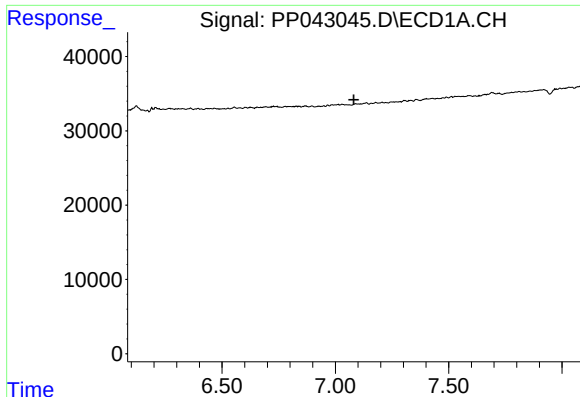

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.082 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

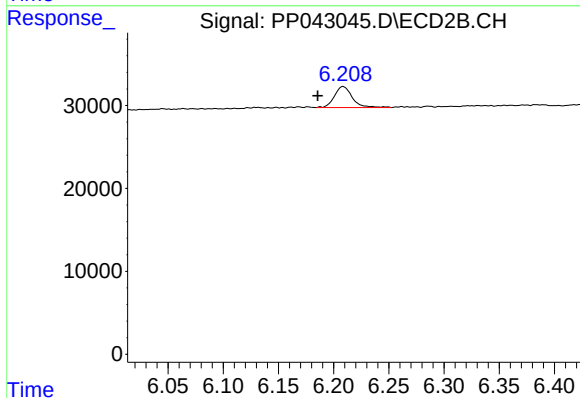


#26 AR-1254-1

R.T.: 6.208 min
Delta R.T.: 0.023 min
Response: 28582
Conc: 18.43 ng/ml

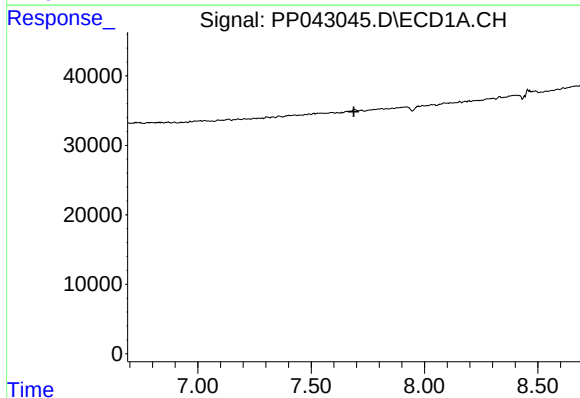


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.688 min
Response: 0
Conc: N.D.

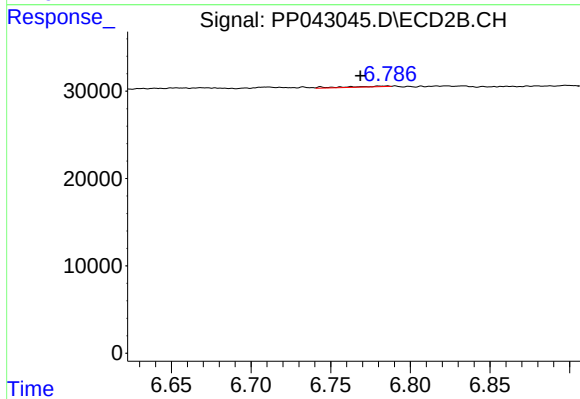

#28 AR-1254-3


R.T.: 6.786 min
Delta R.T.: 0.017 min
Response: 1897
Conc: 0.89 ng/ml

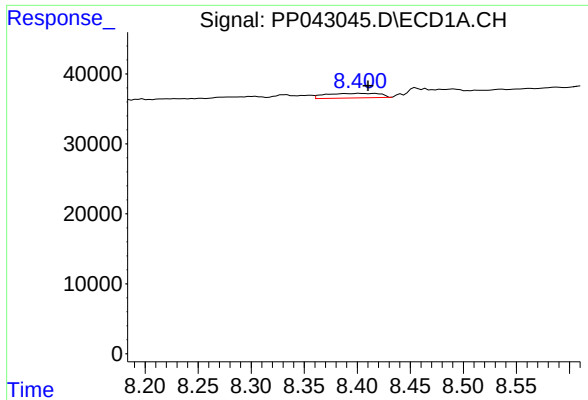

#30 AR-1254-5


R.T.: 8.402 min
Delta R.T.: -0.008 min
Response: 23316
Conc: 24.89 ng/ml

Instrument :
ECD_P
ClientSampleId :

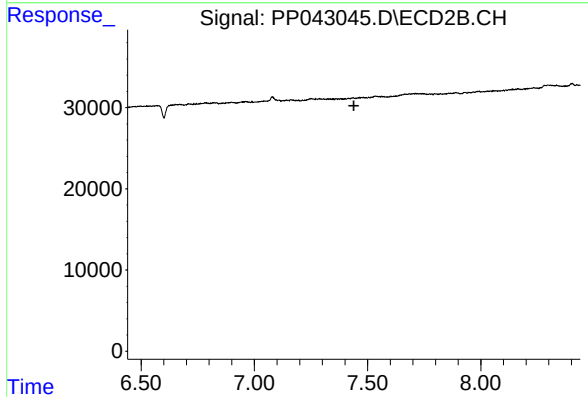


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

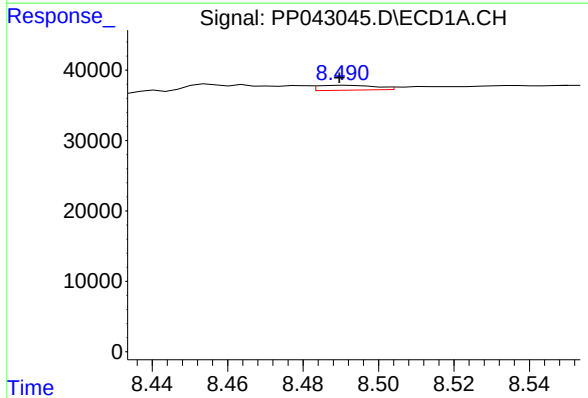


#33 AR-1260-3

R.T.: 8.491 min
Delta R.T.: 0.002 min
Response: 7371
Conc: 9.77 ng/ml

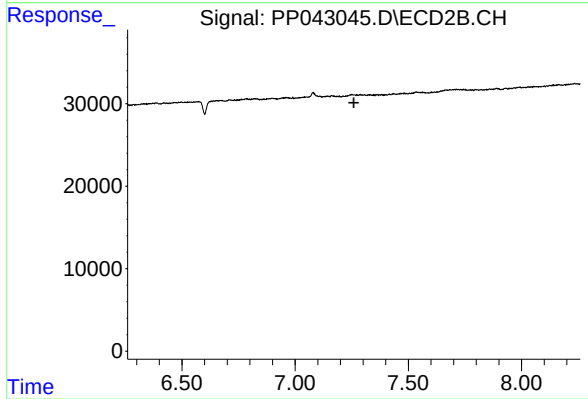

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.260 min
Response: 0
Conc: N.D.

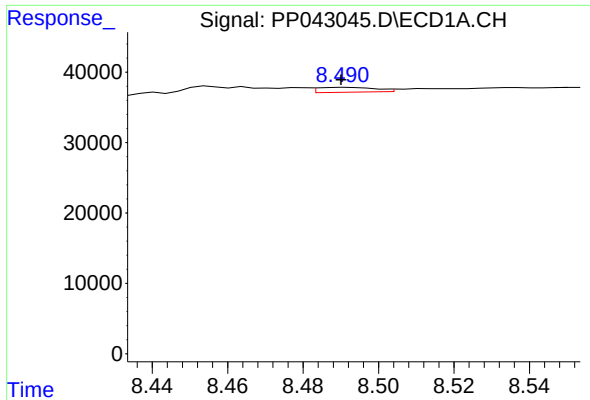

#36 AR-1262-1

R.T.: 8.491 min
Delta R.T.: 0.001 min
Response: 7371
Conc: 6.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

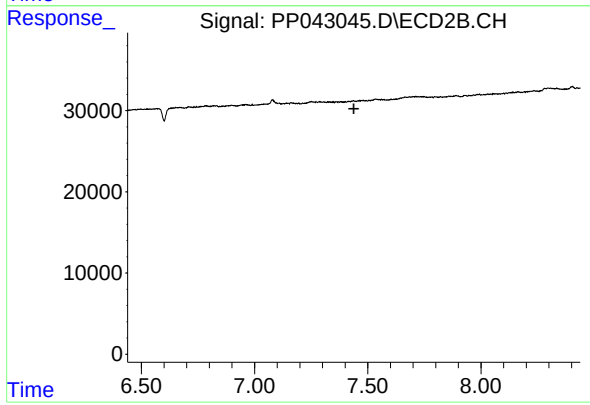

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.439 min
Response: 0
Conc: N.D.