

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
 Data File : PP043054.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 12:45
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:22:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.882	4.042	467959	525424	19.777	21.037
2)	SA Decachlor...	10.815	9.377	361847	459912	24.753	23.577
Target Compounds							
9)	L2 AR-1221-2	0.000	4.398	0	9272	N.D.	38.108 #
20)	L4 AR-1242-5	0.000	6.210f	0	39176	N.D.	54.444 #
25)	L5 AR-1248-5	0.000	6.210f	0	39176	N.D.	41.035 #
26)	L6 AR-1254-1	0.000	6.210f	0	39176	N.D.	25.263 #
29)	L6 AR-1254-4	7.994	0.000	16976	0	19.423	N.D. #
30)	L6 AR-1254-5	8.426f	0.000	22295	0	23.796	N.D. #
32)	L7 AR-1260-2	8.095f	0.000	11914	0	11.536	N.D. #
33)	L7 AR-1260-3	8.474f	0.000	2541	0	3.368	N.D. #
35)	L7 AR-1260-5	9.062f	0.000	2503	0	1.521	N.D. #
36)	L8 AR-1262-1	8.474f	0.000	2541	0	2.407	N.D. #
37)	L8 AR-1262-2	9.062f	0.000	2503	0	1.446	N.D. #
38)	L8 AR-1262-3	9.371f	0.000	5685	0	6.167	N.D. #
39)	L8 AR-1262-4	9.443	0.000	8746	0	16.214	N.D. #
41)	L9 AR-1268-1	9.371f	0.000	5685	0	2.757	N.D. #
42)	L9 AR-1268-2	9.443	0.000	8746	0	4.579	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
Data File : PP043054.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 12:45
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:22:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

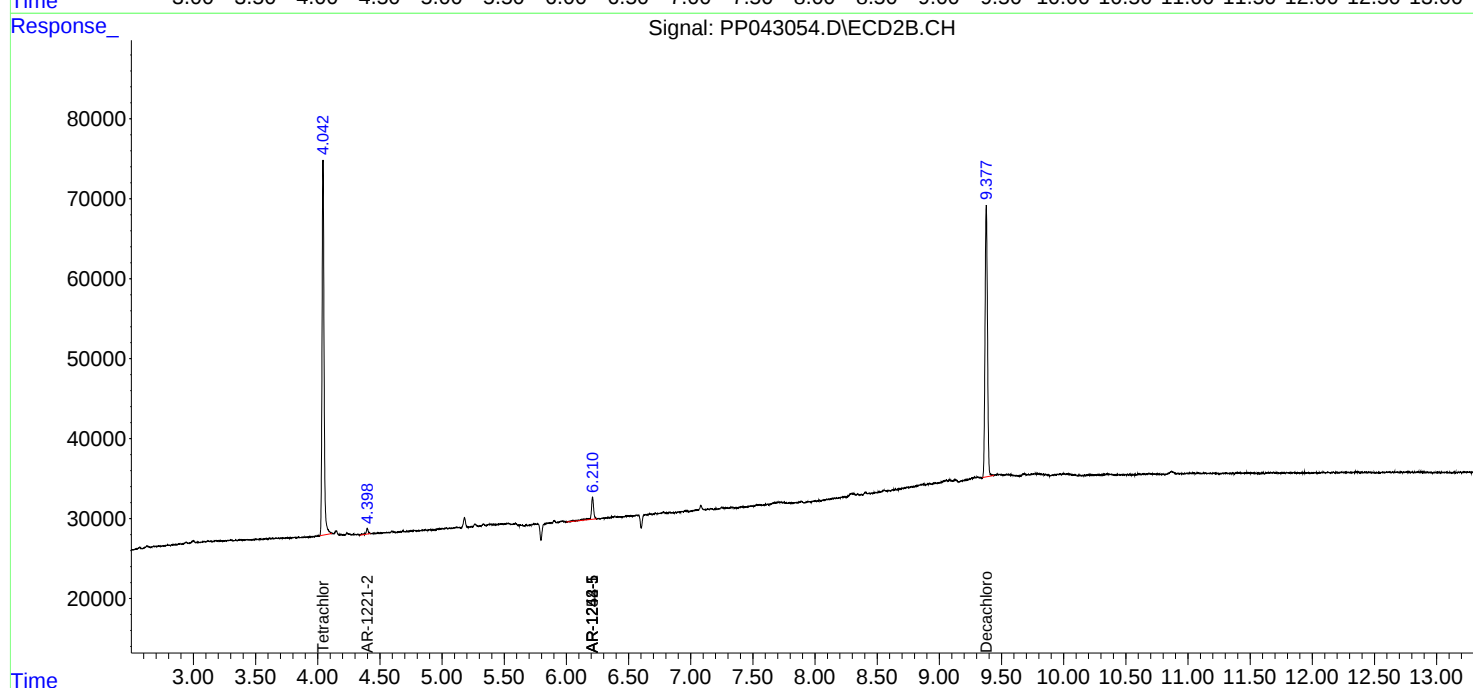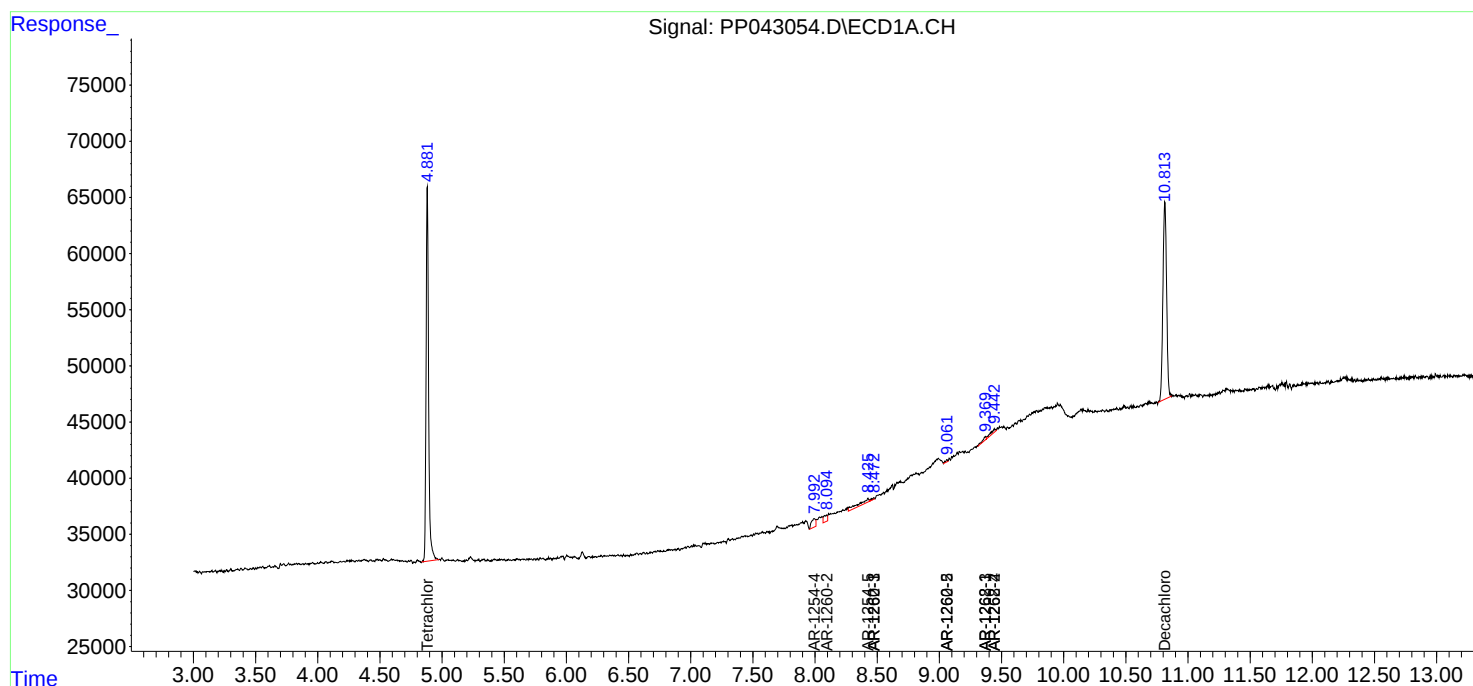


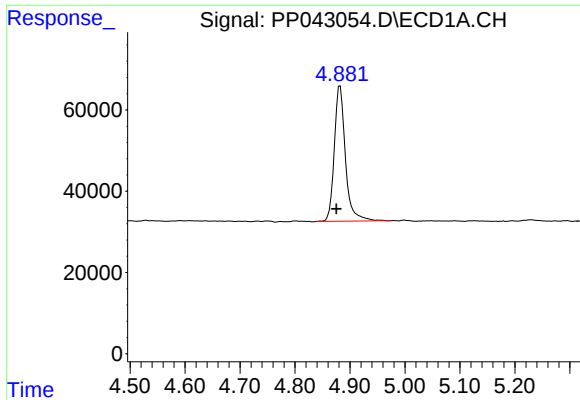

#1 Tetrachloro-m-xylene


R.T.: 4.882 min
Delta R.T.: 0.007 min
Response: 467959
Conc: 19.78 ng/ml

Instrument :
ECD_P
ClientSampleId :

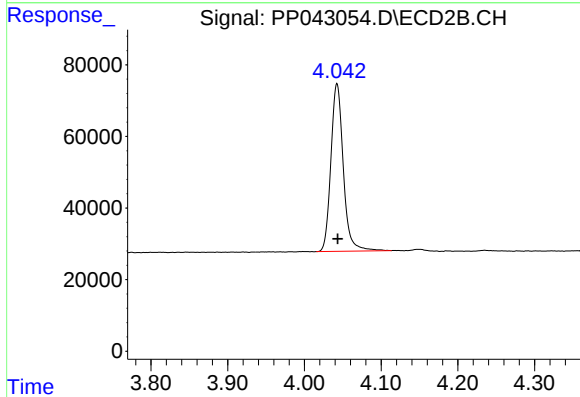


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 525424
Conc: 21.04 ng/ml

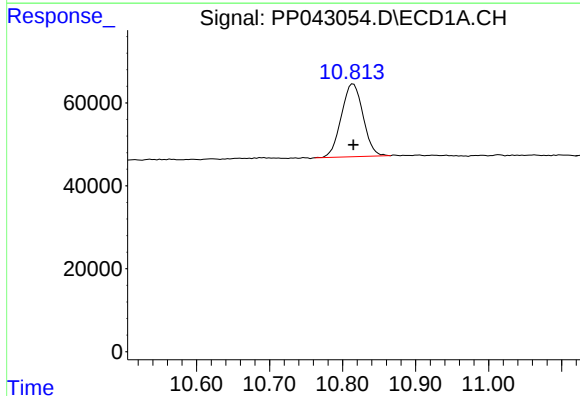


#2 Decachlorobiphenyl

R.T.: 10.815 min
Delta R.T.: 0.000 min
Response: 361847
Conc: 24.75 ng/ml

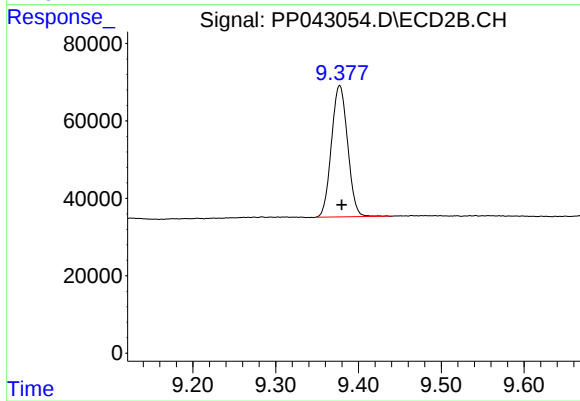

#2 Decachlorobiphenyl


R.T.: 9.377 min
Delta R.T.: -0.003 min
Response: 459912
Conc: 23.58 ng/ml

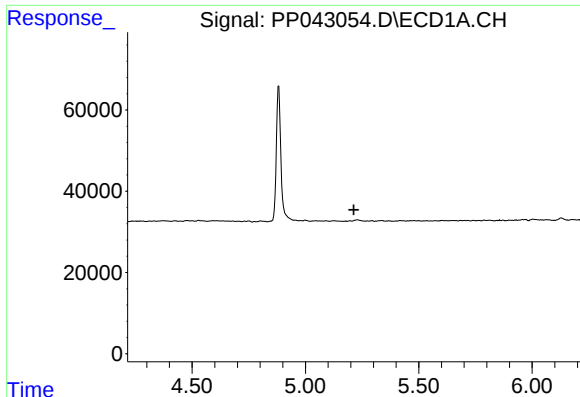

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

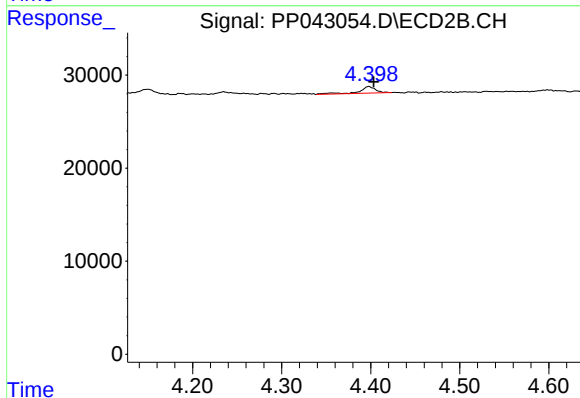


#9 AR-1221-2

R.T.: 4.398 min
Delta R.T.: -0.005 min
Response: 9272
Conc: 38.11 ng/ml

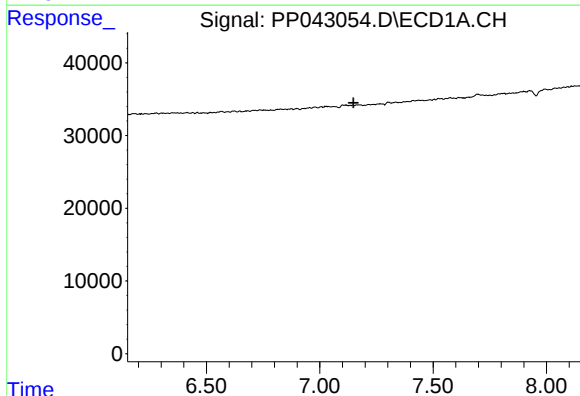


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

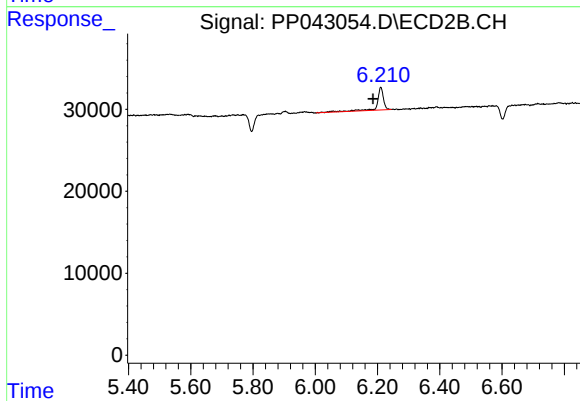

#20 AR-1242-5


R.T.: 6.210 min
Delta R.T.: 0.025 min
Response: 39176
Conc: 54.44 ng/ml

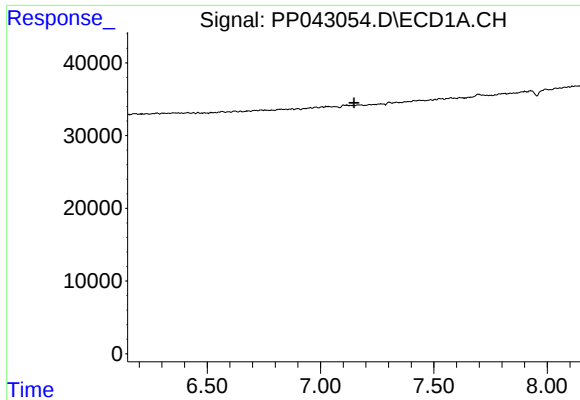

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

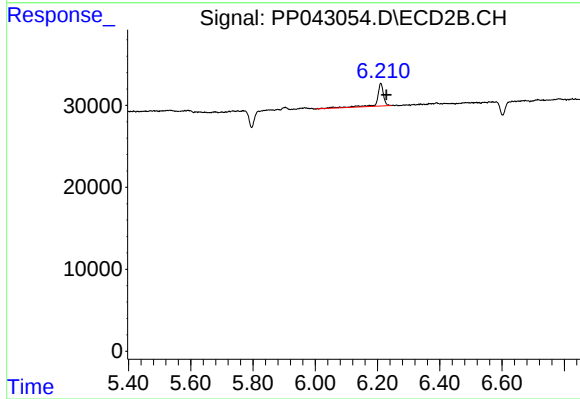


#25 AR-1248-5

R.T.: 6.210 min
Delta R.T.: -0.018 min
Response: 39176
Conc: 41.04 ng/ml

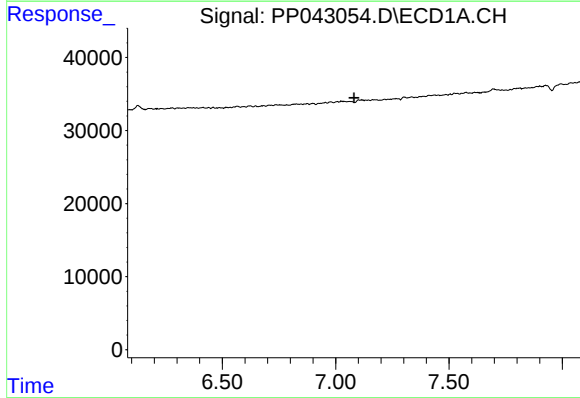


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.082 min
Response: 0
Conc: N.D.

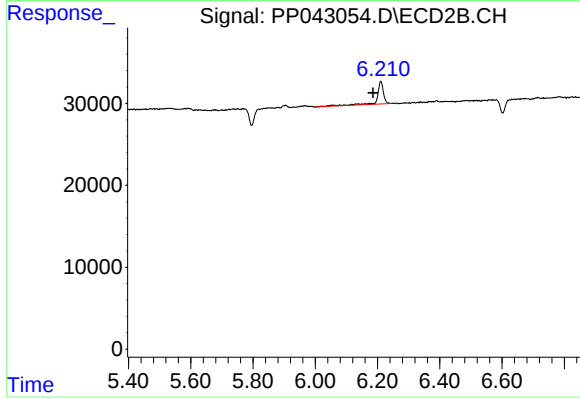

#26 AR-1254-1


R.T.: 6.210 min
Delta R.T.: 0.025 min
Response: 39176
Conc: 25.26 ng/ml

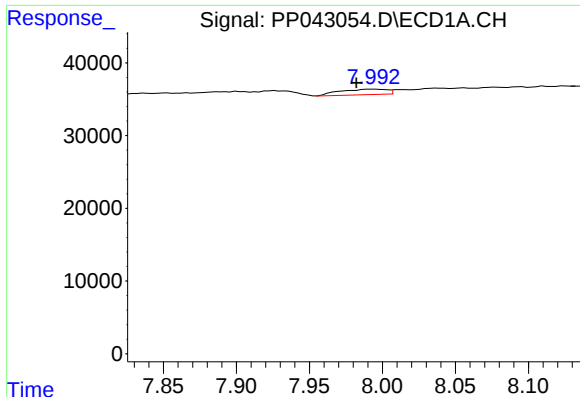

#29 AR-1254-4


R.T.: 7.994 min
Delta R.T.: 0.012 min
Response: 16976
Conc: 19.42 ng/ml

Instrument :
ECD_P
ClientSampleId :

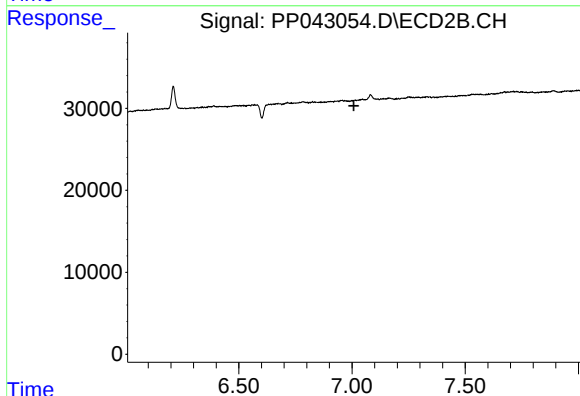


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

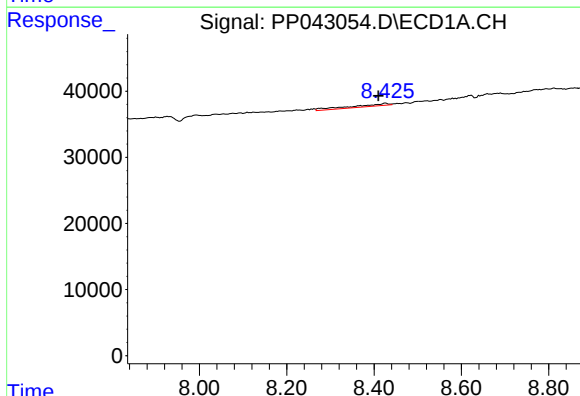


#30 AR-1254-5

R.T.: 8.426 min
Delta R.T.: 0.016 min
Response: 22295
Conc: 23.80 ng/ml

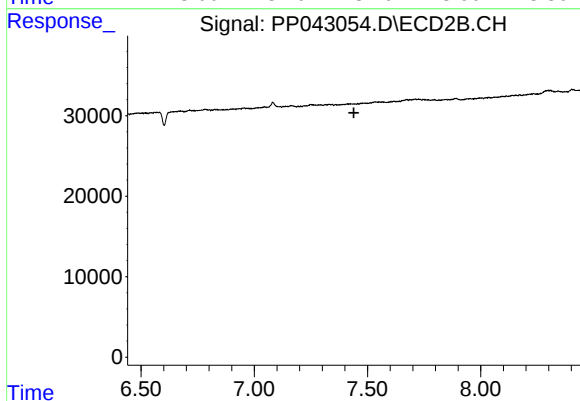

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

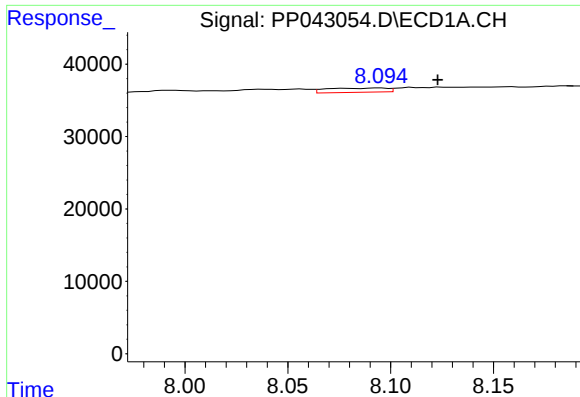

#32 AR-1260-2


R.T.: 8.095 min
Delta R.T.: -0.028 min
Response: 11914
Conc: 11.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

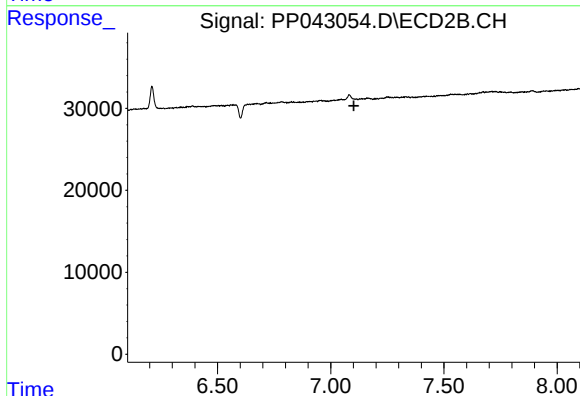


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.102 min
Response: 0
Conc: N.D.

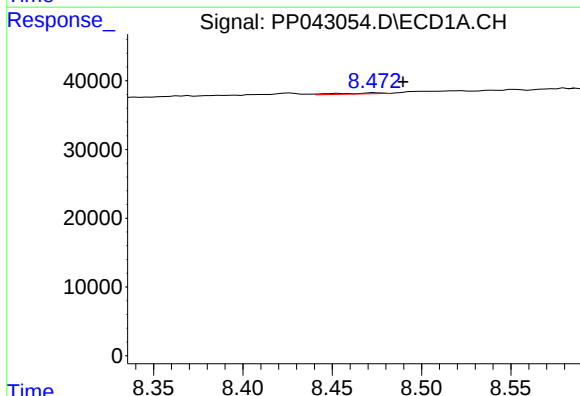


#33 AR-1260-3

R.T.: 8.474 min
Delta R.T.: -0.015 min
Response: 2541
Conc: 3.37 ng/ml

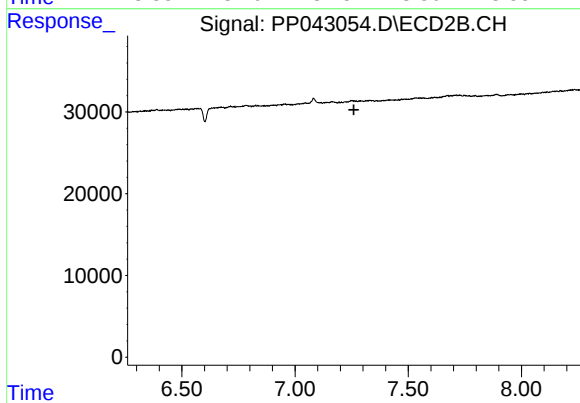

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.260 min
Response: 0
Conc: N.D.

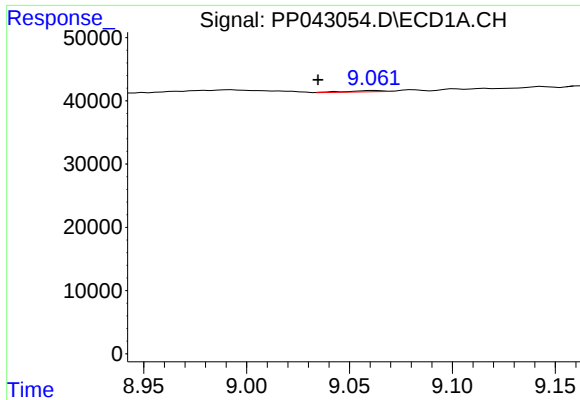

#35 AR-1260-5


R.T.: 9.062 min
Delta R.T.: 0.027 min
Response: 2503
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

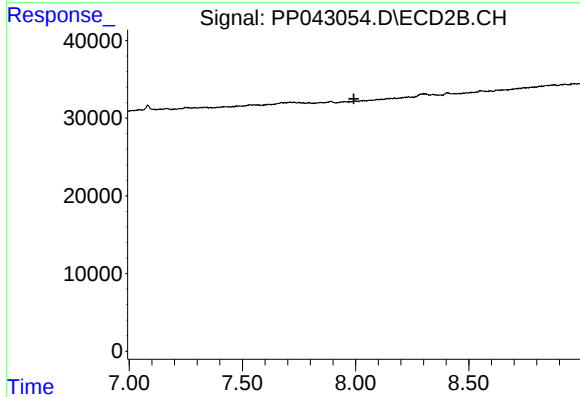


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

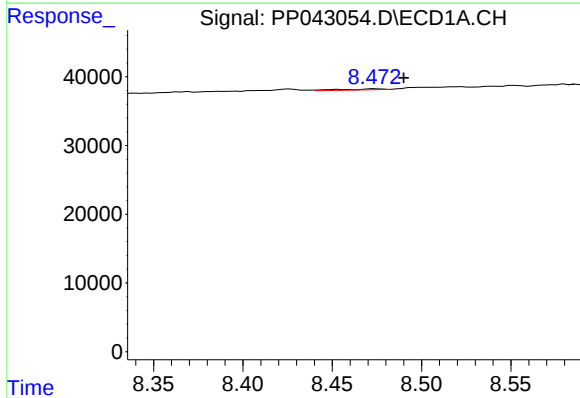


#36 AR-1262-1

R.T.: 8.474 min
Delta R.T.: -0.016 min
Response: 2541
Conc: 2.41 ng/ml

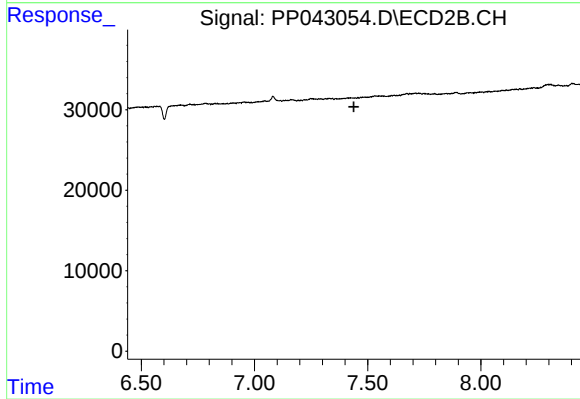

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.439 min
Response: 0
Conc: N.D.

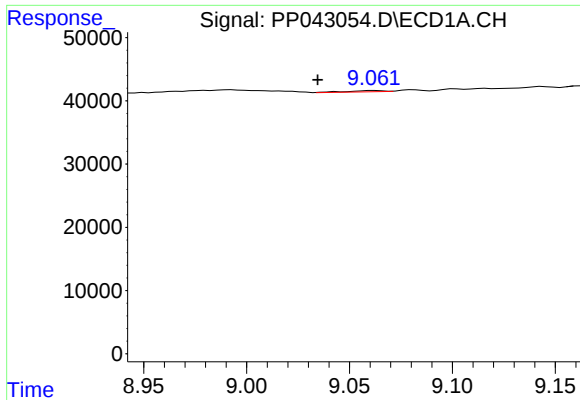

#37 AR-1262-2


R.T.: 9.062 min
Delta R.T.: 0.028 min
Response: 2503
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

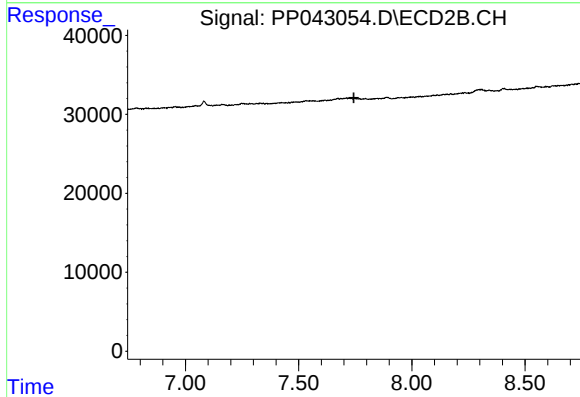


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

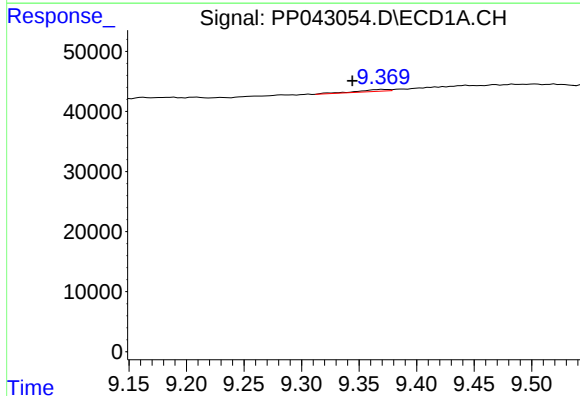


#38 AR-1262-3

R.T.: 9.371 min
Delta R.T.: 0.027 min
Response: 5685
Conc: 6.17 ng/ml

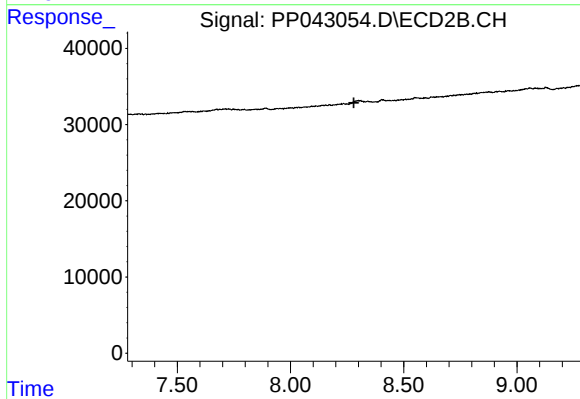

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.280 min
Response: 0
Conc: N.D.

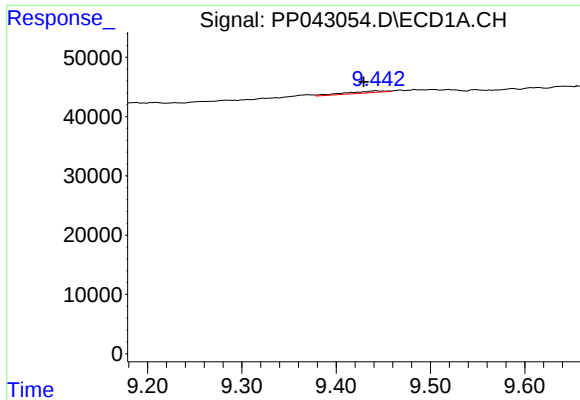

#39 AR-1262-4


R.T.: 9.443 min
Delta R.T.: 0.014 min
Response: 8746
Conc: 16.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

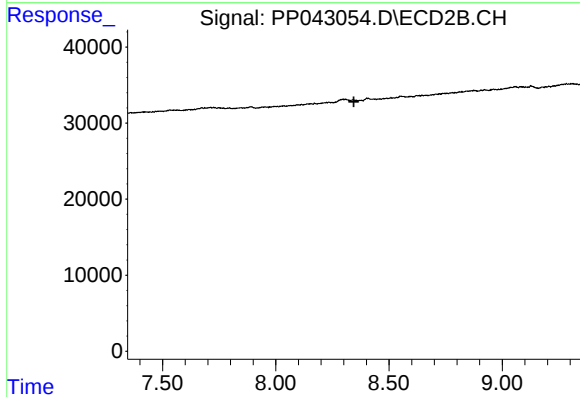


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

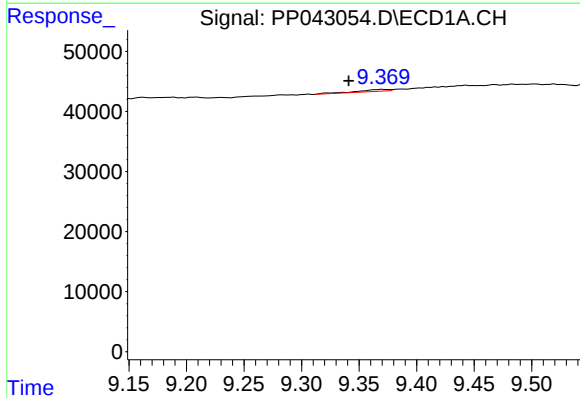


#41 AR-1268-1

R.T.: 9.371 min
Delta R.T.: 0.030 min
Response: 5685
Conc: 2.76 ng/ml

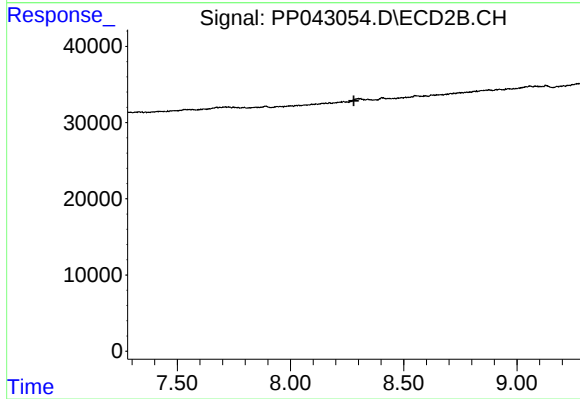

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.280 min
Response: 0
Conc: N.D.

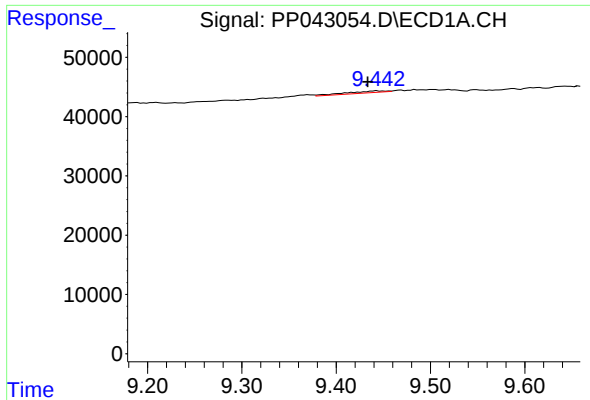

#42 AR-1268-2

R.T.: 9.443 min
Delta R.T.: 0.009 min
Response: 8746
Conc: 4.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

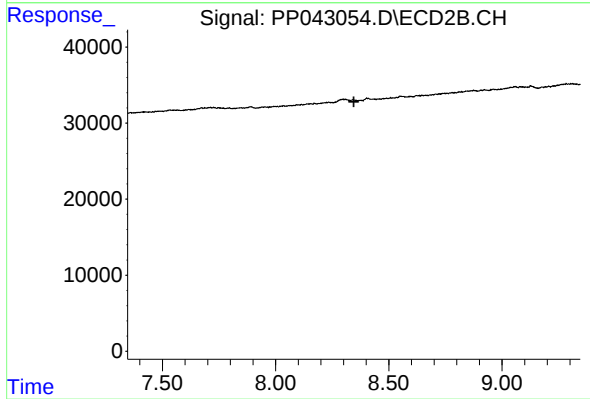

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.