

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
 Data File : PP043058.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 13:51
 Operator : AJ\MA
 Sample : N1162-22 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:23:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.873	4.040	35057	48165	1.482	1.928 #
2)	SA Decachlor...	10.804	9.375	39199	37301	2.681	1.912 #
Target Compounds							
30)	L6 AR-1254-5	8.386f	0.000	2221	0	2.371	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
Data File : PP043058.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 13:51
Operator : AJ\MA
Sample : N1162-22 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:23:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

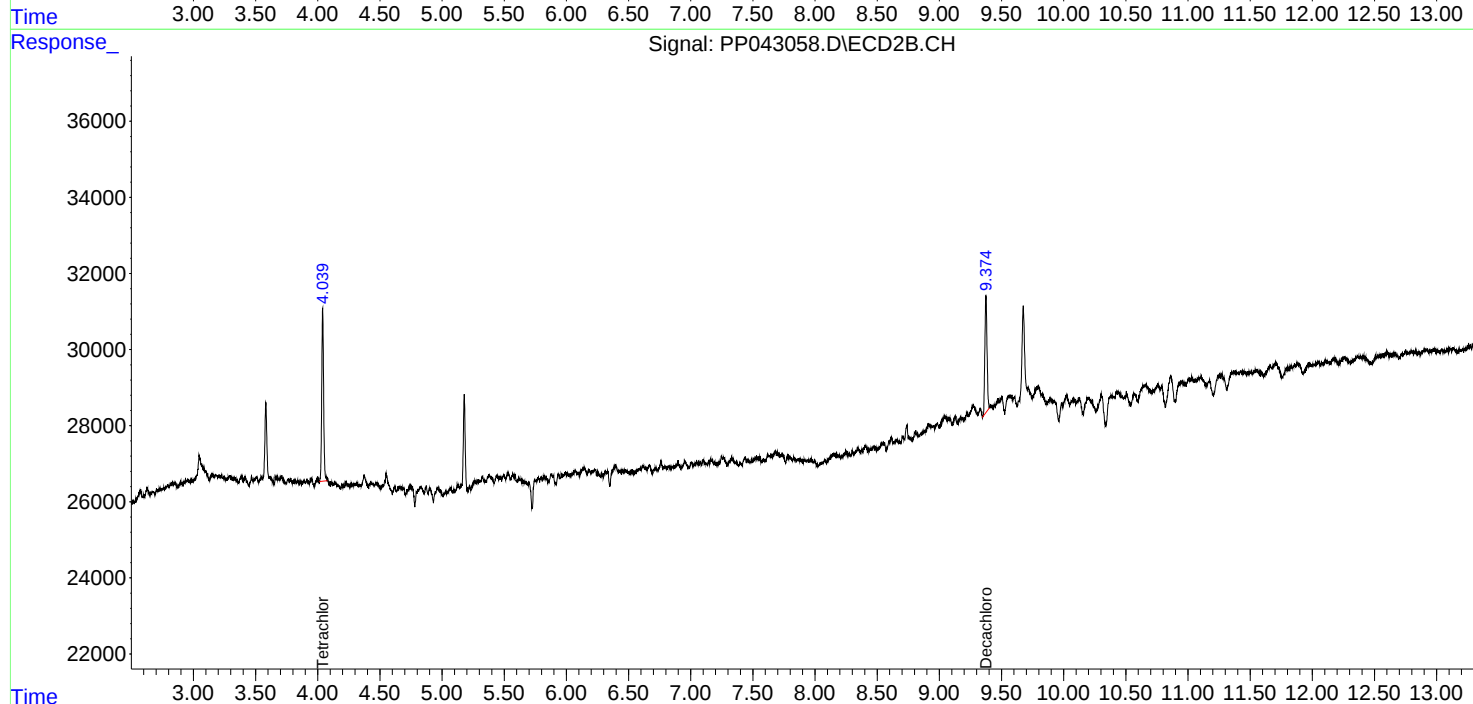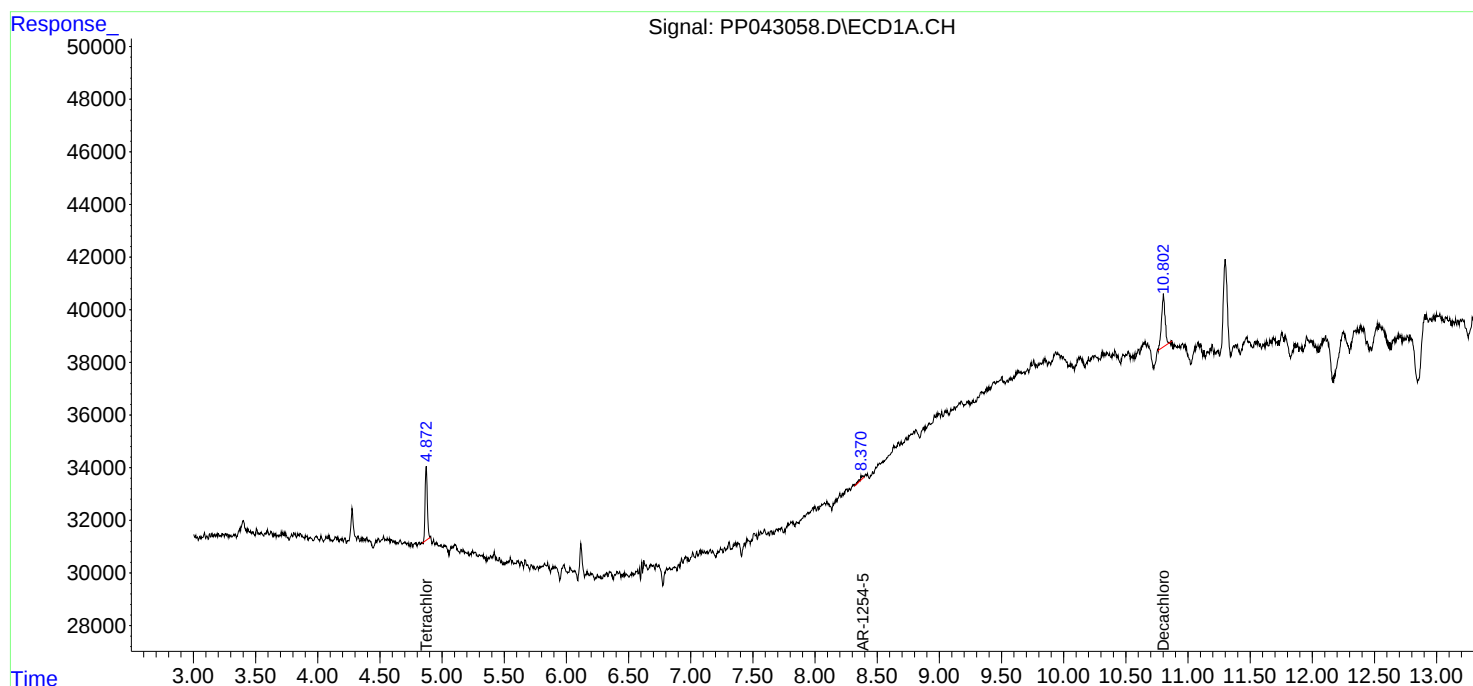


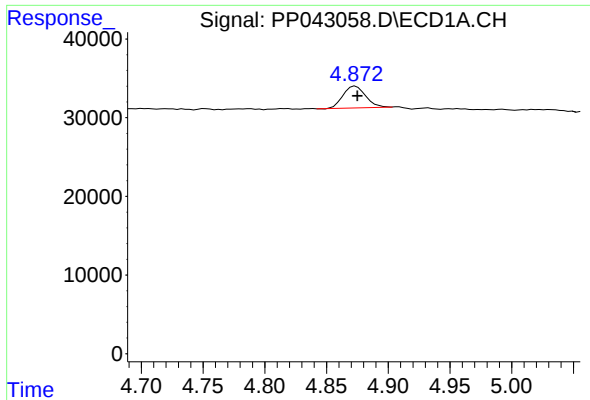

#1 Tetrachloro-m-xylene


R.T.: 4.873 min
Delta R.T.: -0.002 min
Response: 35057
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :

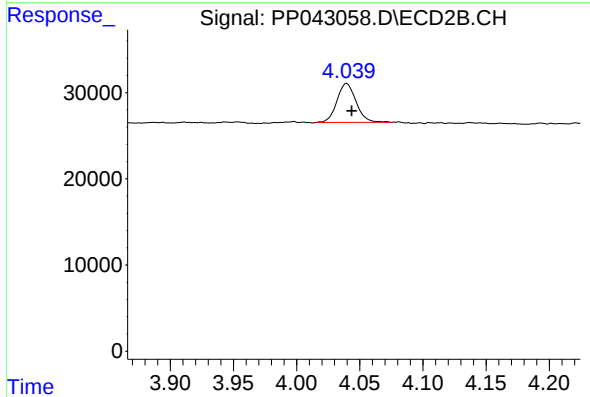


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: -0.004 min
Response: 48165
Conc: 1.93 ng/ml

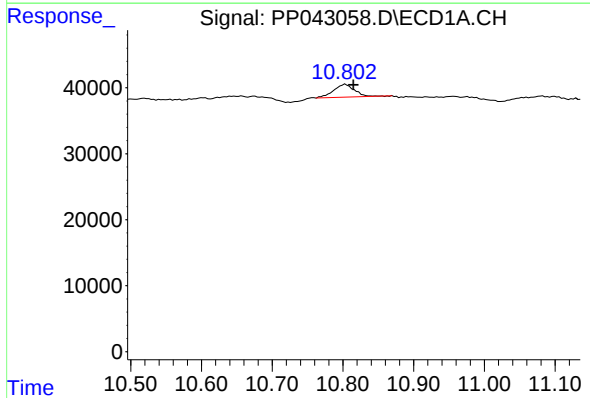


#2 Decachlorobiphenyl

R.T.: 10.804 min
Delta R.T.: -0.011 min
Response: 39199
Conc: 2.68 ng/ml

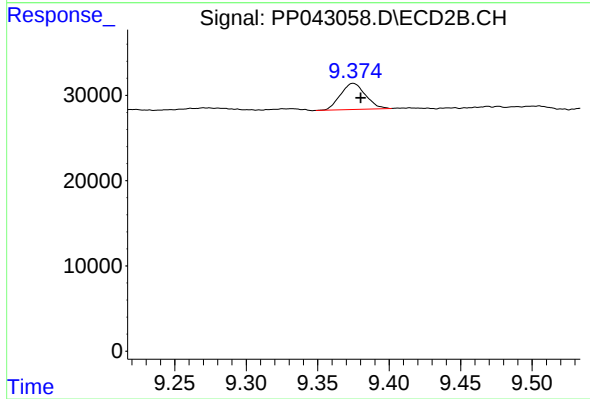

#2 Decachlorobiphenyl


R.T.: 9.375 min
Delta R.T.: -0.005 min
Response: 37301
Conc: 1.91 ng/ml

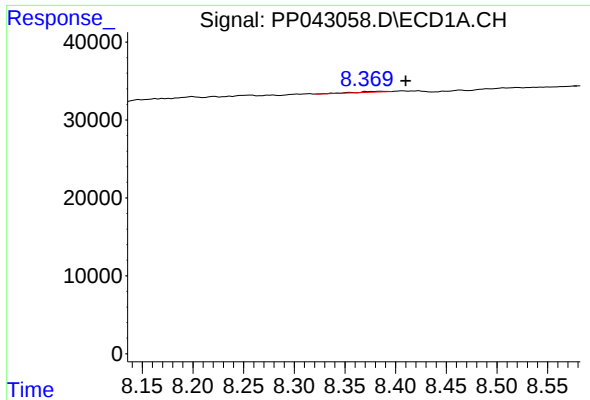

#30 AR-1254-5

R.T.: 8.386 min
Delta R.T.: -0.024 min
Response: 2221
Conc: 2.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

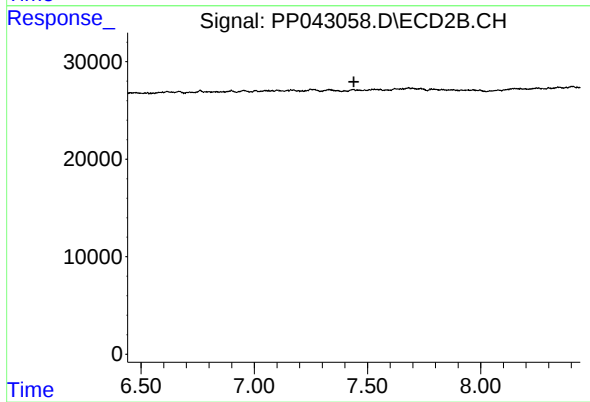

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.