

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
 Data File : PP043064.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 15:30
 Operator : AJ\MA
 Sample : N1162-28 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MMO-16-2022-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2022
 Supervised By :Ankita Jodhani 01/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:25:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.874	4.039	41262	47622	1.744	1.907
2) SA Decachlor...	10.803	9.374	32897	35278	2.250m	1.809

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011822\
Data File : PP043064.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 15:30
Operator : AJ\MA
Sample : N1162-28 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MMO-16-2022-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2022
Supervised By :Ankita Jodhani 01/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:25:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

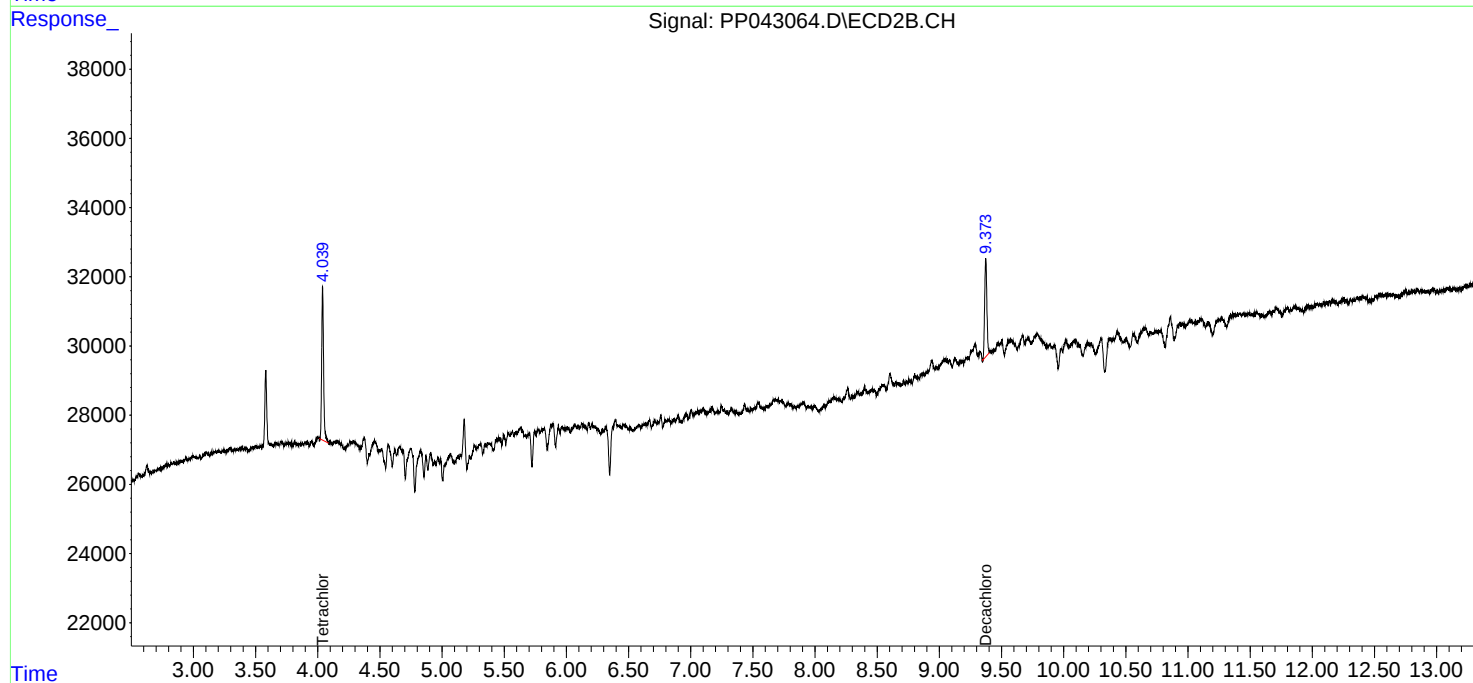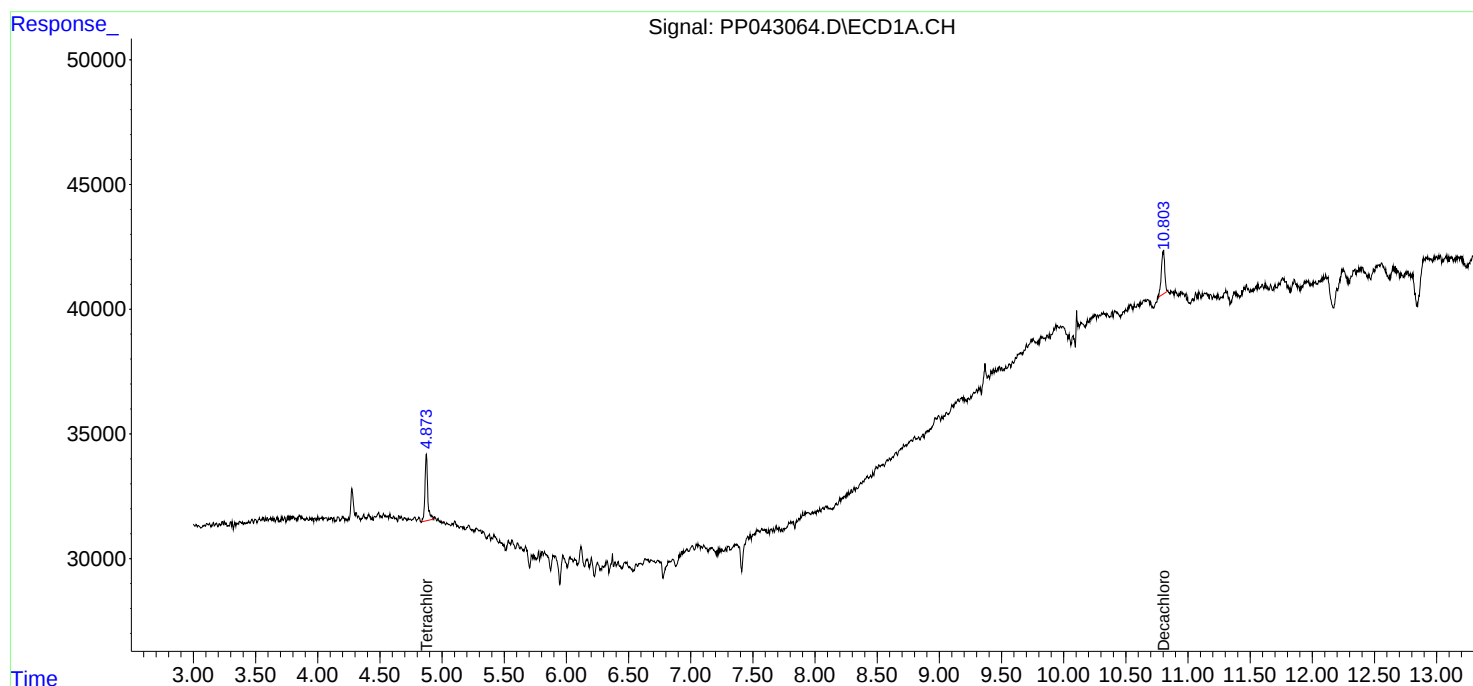

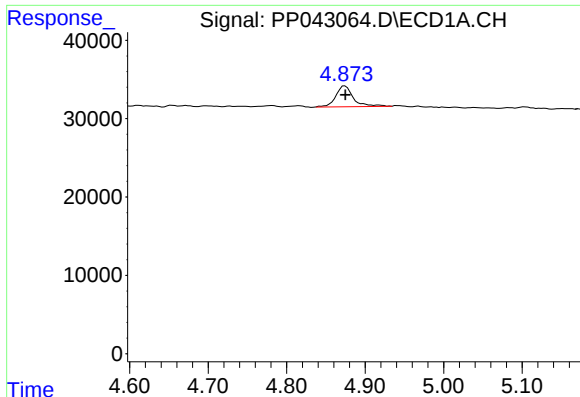


#1 Tetrachloro-m-xylene

R.T.: 4.874 min
Delta R.T.: 0.000 min
Response: 41262
Conc: 1.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MMO-16-2022-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2022
Supervised By :Ankita Jodhani 01/19/2022

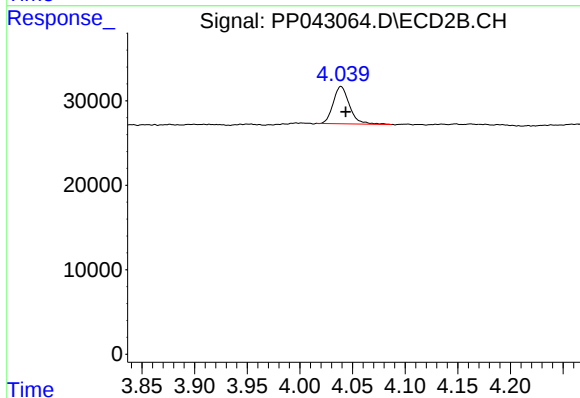


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: -0.005 min
Response: 47622
Conc: 1.91 ng/ml

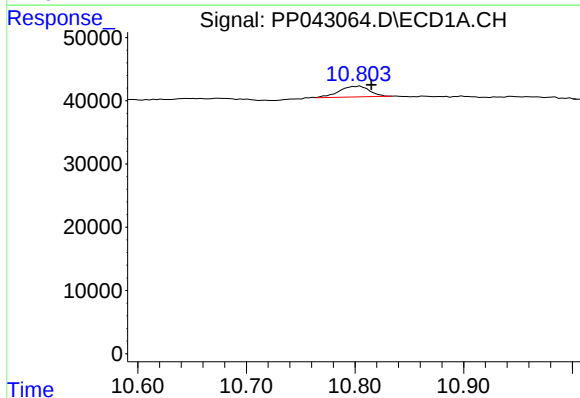

#2 Decachlorobiphenyl

R.T.: 10.803 min
Delta R.T.: -0.012 min
Response: 32897
Conc: 2.25 ng/ml m

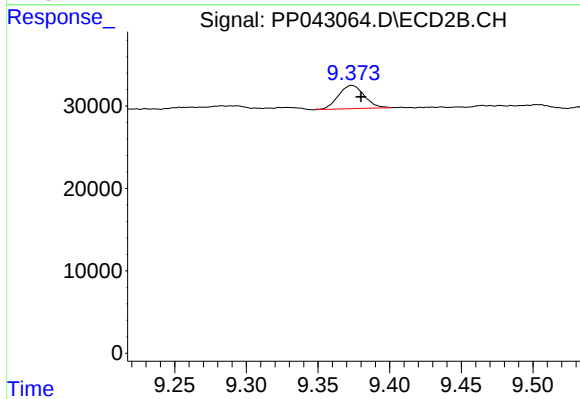

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: -0.006 min
Response: 35278
Conc: 1.81 ng/ml