

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011823\
 Data File : PP054664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 14:06
 Operator : YP\AJ
 Sample : 01175-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 YARD-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2023
 Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 17:30:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 18 04:34:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.578	39361789	33484378	21.437	20.919
2) SA Decachlor...	10.093	8.600	23680499	22802718	17.642m	15.923

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011823\
Data File : PP054664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 14:06
Operator : YP\AJ
Sample : 01175-10
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
YARD-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 17:30:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 18 04:34:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

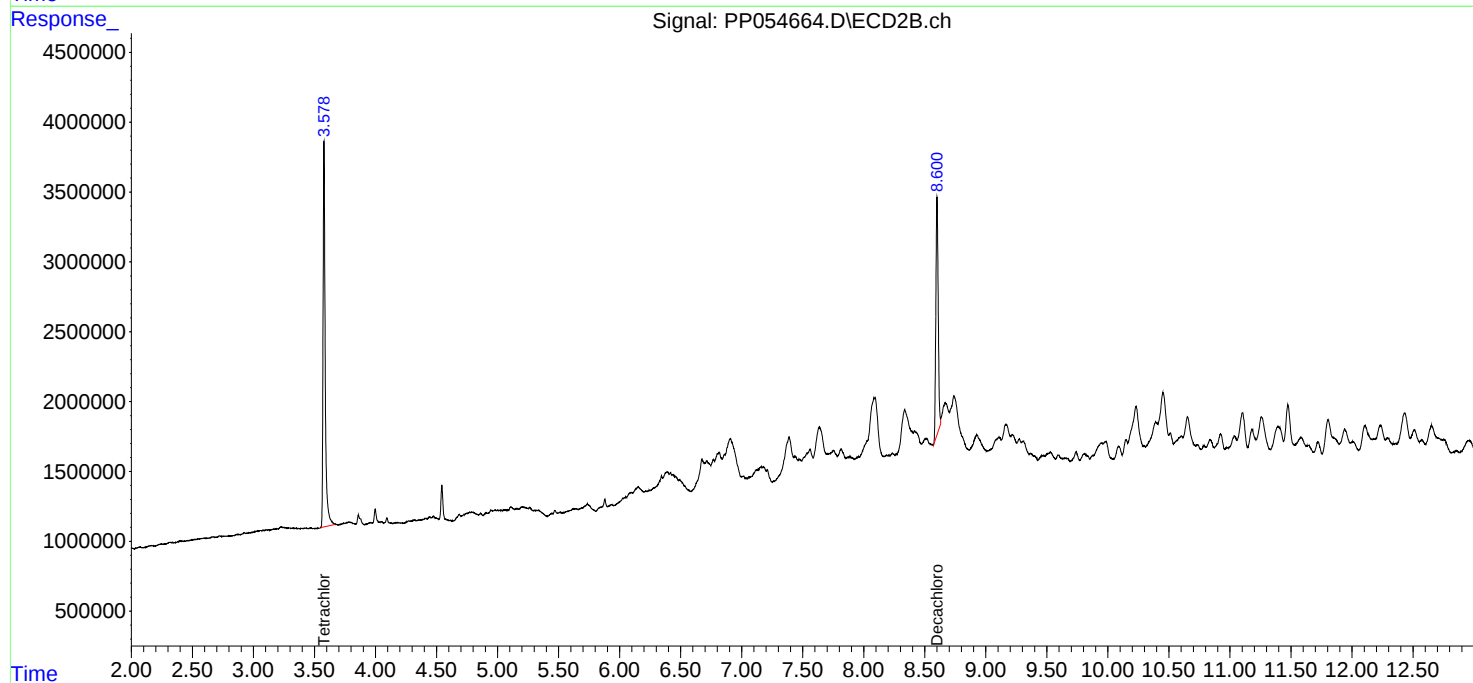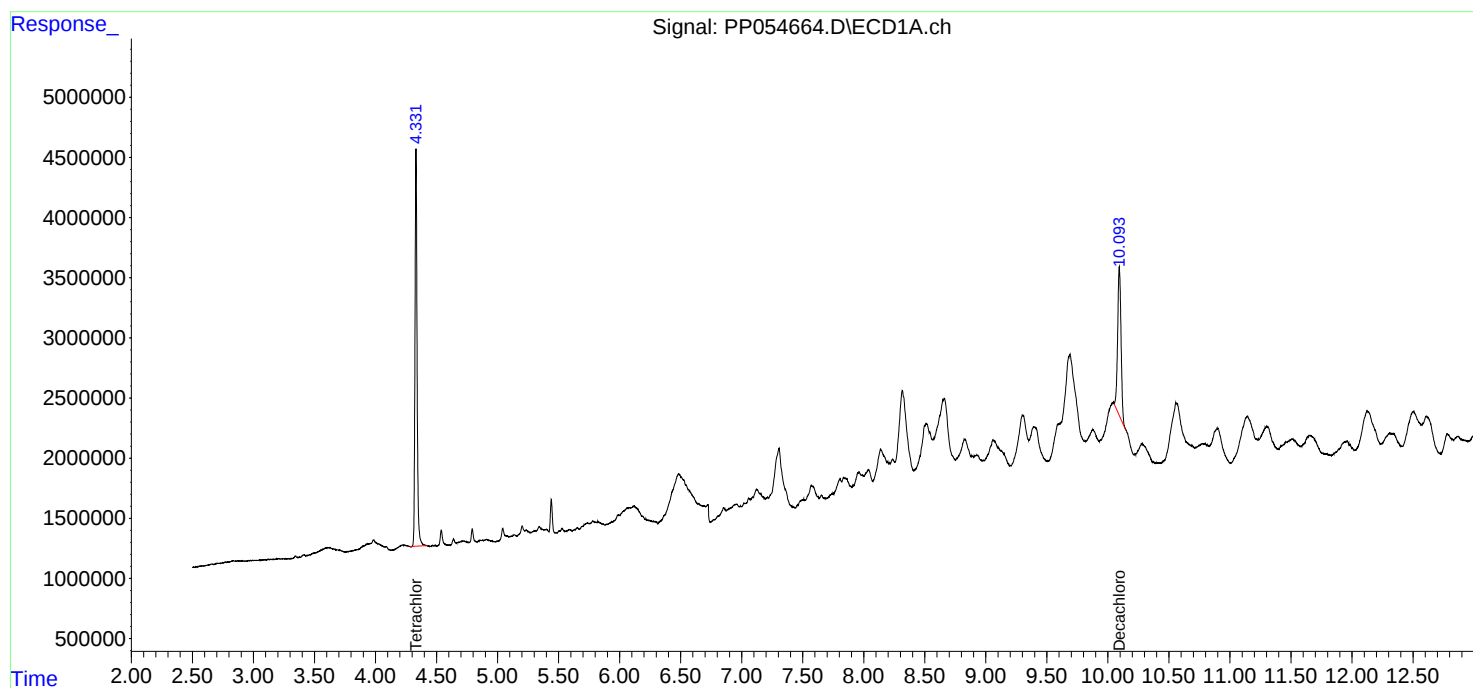

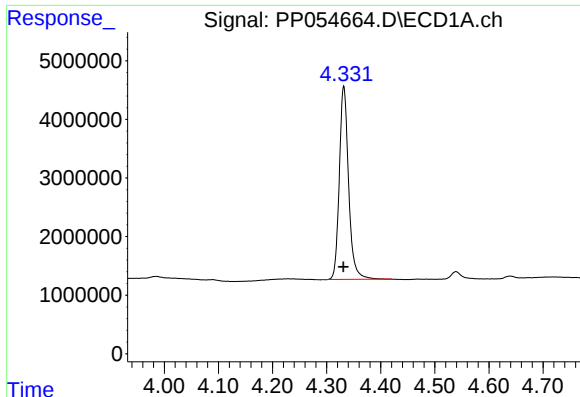


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 39361789
Conc: 21.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
YARD-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

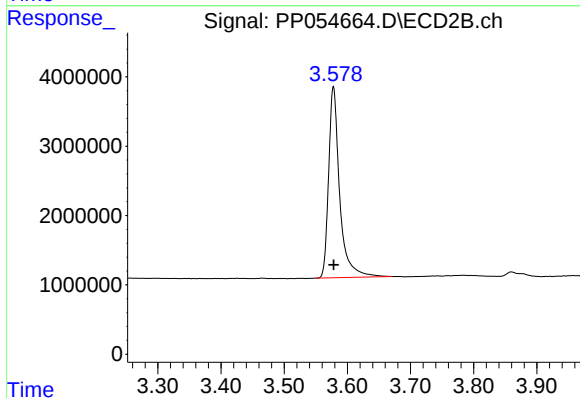


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: 0.000 min
Response: 33484378
Conc: 20.92 ng/ml

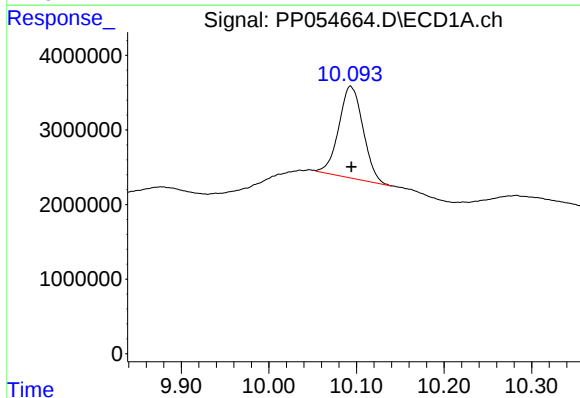

#2 Decachlorobiphenyl

R.T.: 10.093 min
Delta R.T.: -0.001 min
Response: 23680499
Conc: 17.64 ng/ml m

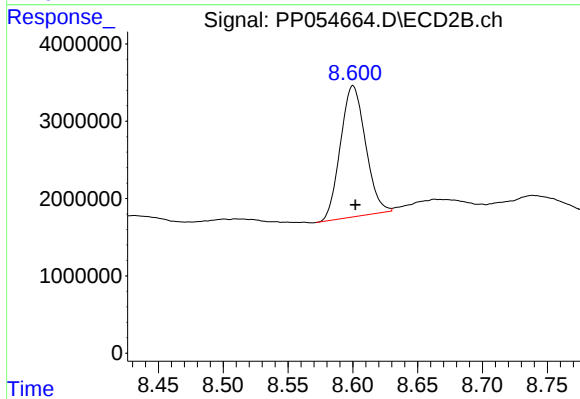

#2 Decachlorobiphenyl

R.T.: 8.600 min
Delta R.T.: -0.002 min
Response: 22802718
Conc: 15.92 ng/ml