

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011823\
 Data File : PP054690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 21:56
 Operator : YP\AJ
 Sample : 01183-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 003

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2023
 Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:34:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 18 04:34:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.592	28343995	30085175	15.436m	18.795m
2) SA Decachlor...	10.091	8.599	25751672	20772756	19.185	14.506

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011823\
Data File : PP054690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 21:56
Operator : YP\AJ
Sample : 01183-03
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:34:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 18 04:34:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

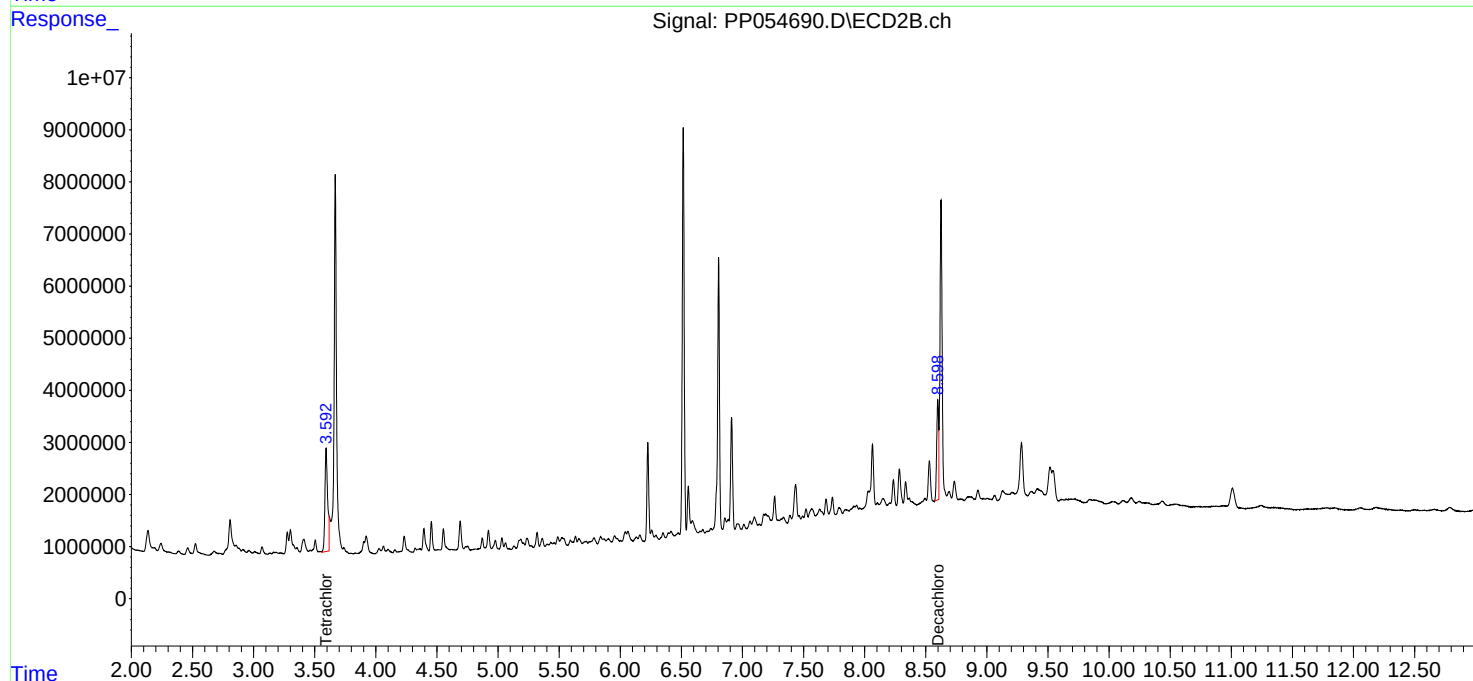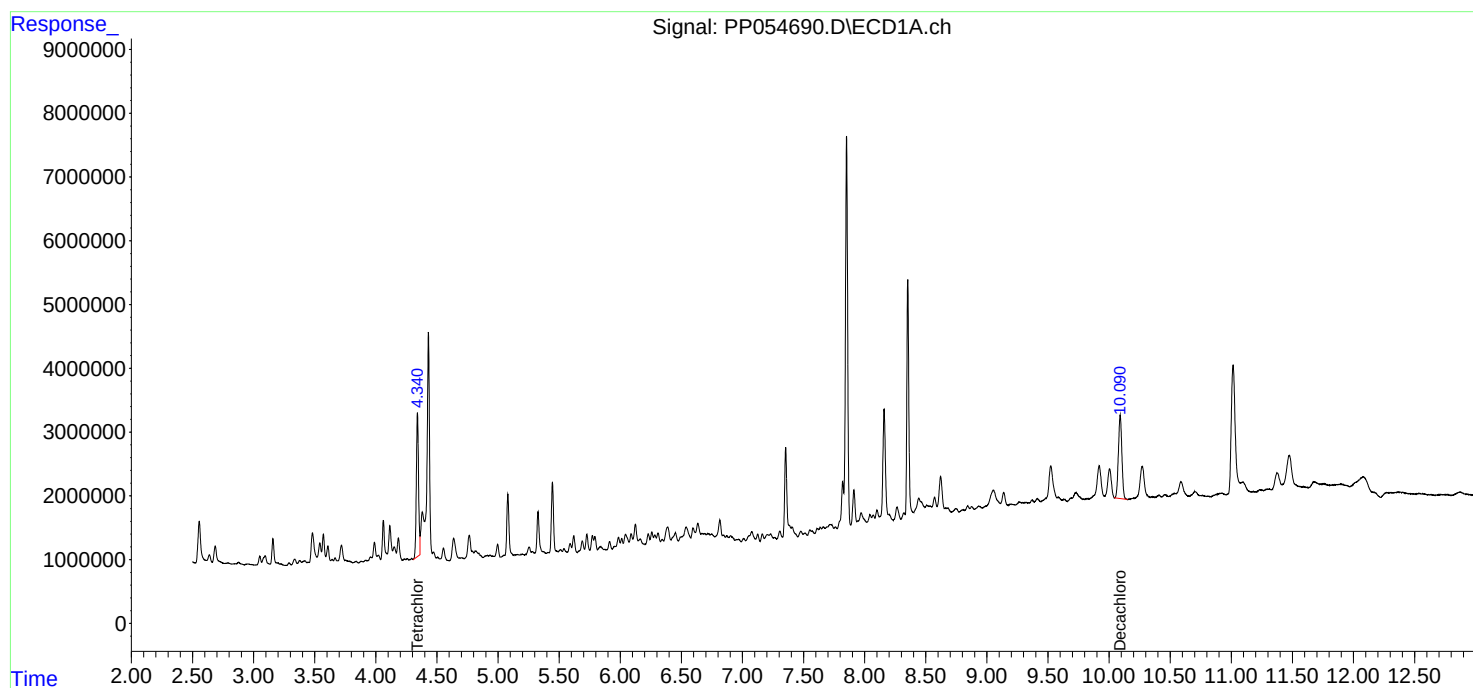

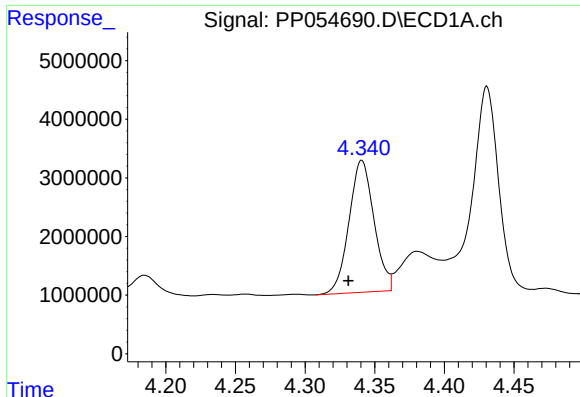


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: 0.009 min
Response: 28343995
Conc: 15.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

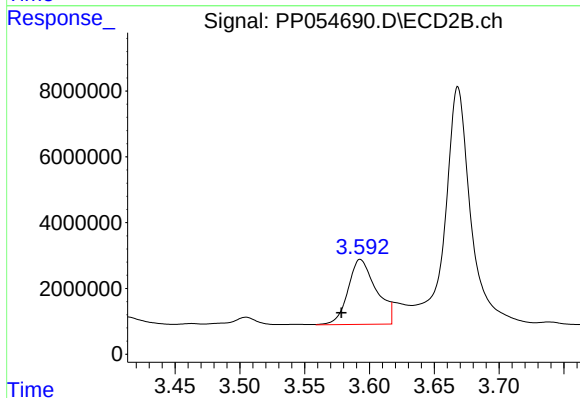


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.014 min
Response: 30085175
Conc: 18.80 ng/ml m

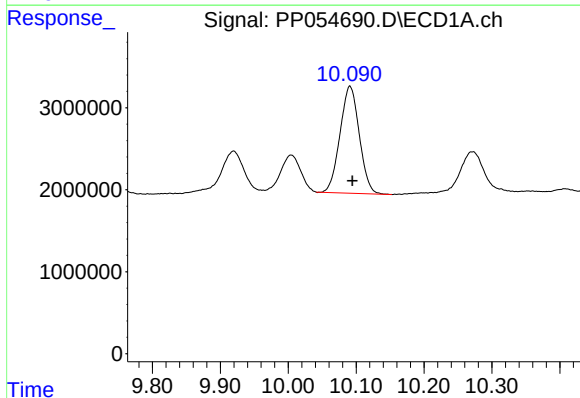

#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: -0.003 min
Response: 25751672
Conc: 19.19 ng/ml

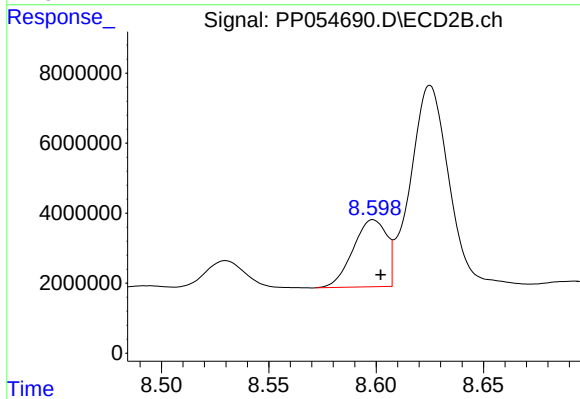

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: -0.003 min
Response: 20772756
Conc: 14.51 ng/ml