

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
 Data File : PP032835.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 12:50
 Operator : DD\AJ
 Sample : M1106-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6-02-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 02:03:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.738	4.009	1253343	954659	21.579	20.295
2)	SA Decachlor...	10.571	9.287	711068	624320	18.023	16.665
Target Compounds							
24)	L5 AR-1248-4	6.967	0.000	65848	0	40.598	N.D. #
26)	L6 AR-1254-1	6.967f	0.000	65848	0	39.647	N.D. #
27)	L6 AR-1254-2	7.175	0.000	38491	0	15.305	N.D. #
30)	L6 AR-1254-5	8.295f	7.371	90879	35784	43.578	14.794 #
32)	L7 AR-1260-2	7.974	7.069f	85302	46656	35.319	20.474 #
38)	L8 AR-1262-3	0.000	8.203	0	51981	N.D.	27.147 #
41)	L9 AR-1268-1	0.000	8.203	0	51981	N.D.	9.219 #
45)	L9 AR-1268-5	10.265	9.046	62624	58971	4.143	4.073



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
Data File : PP032835.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 12:50
Operator : DD\AJ
Sample : M1106-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S6-02-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 02:03:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

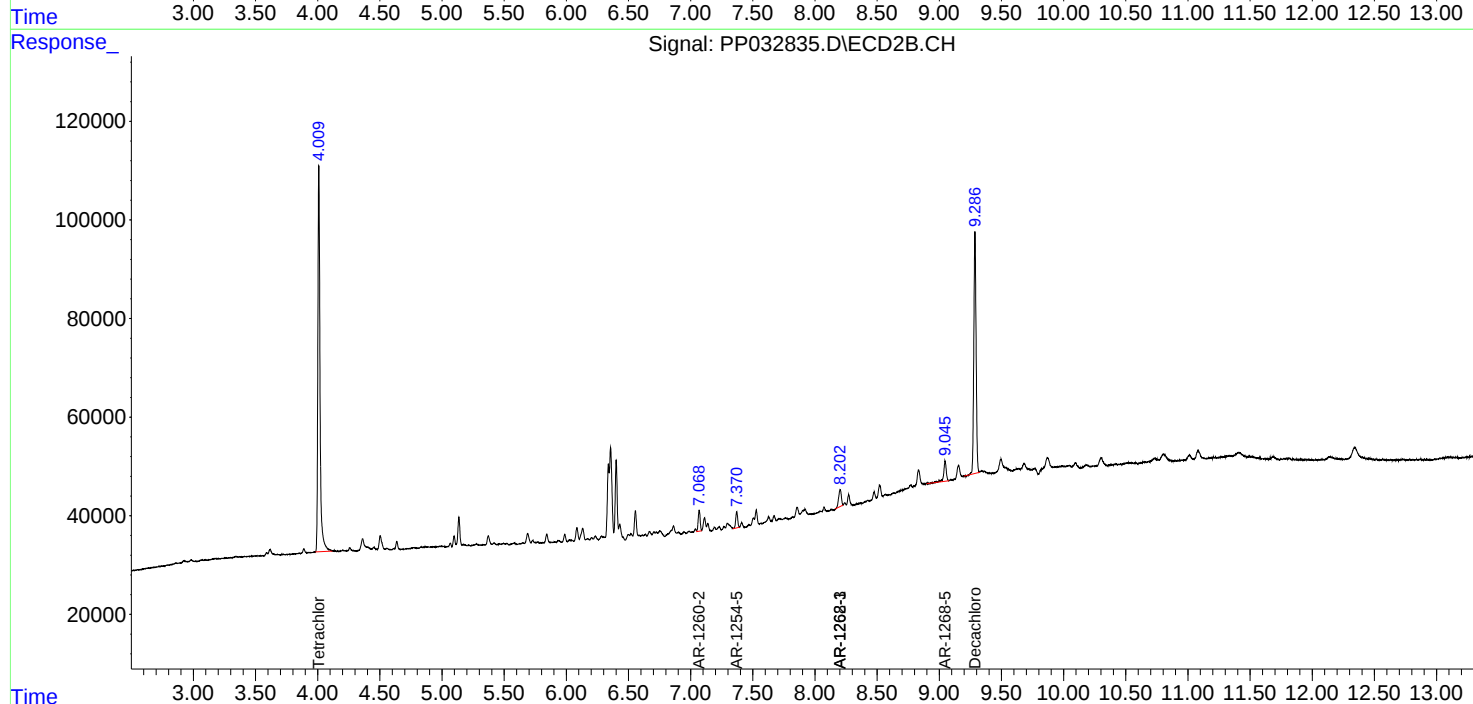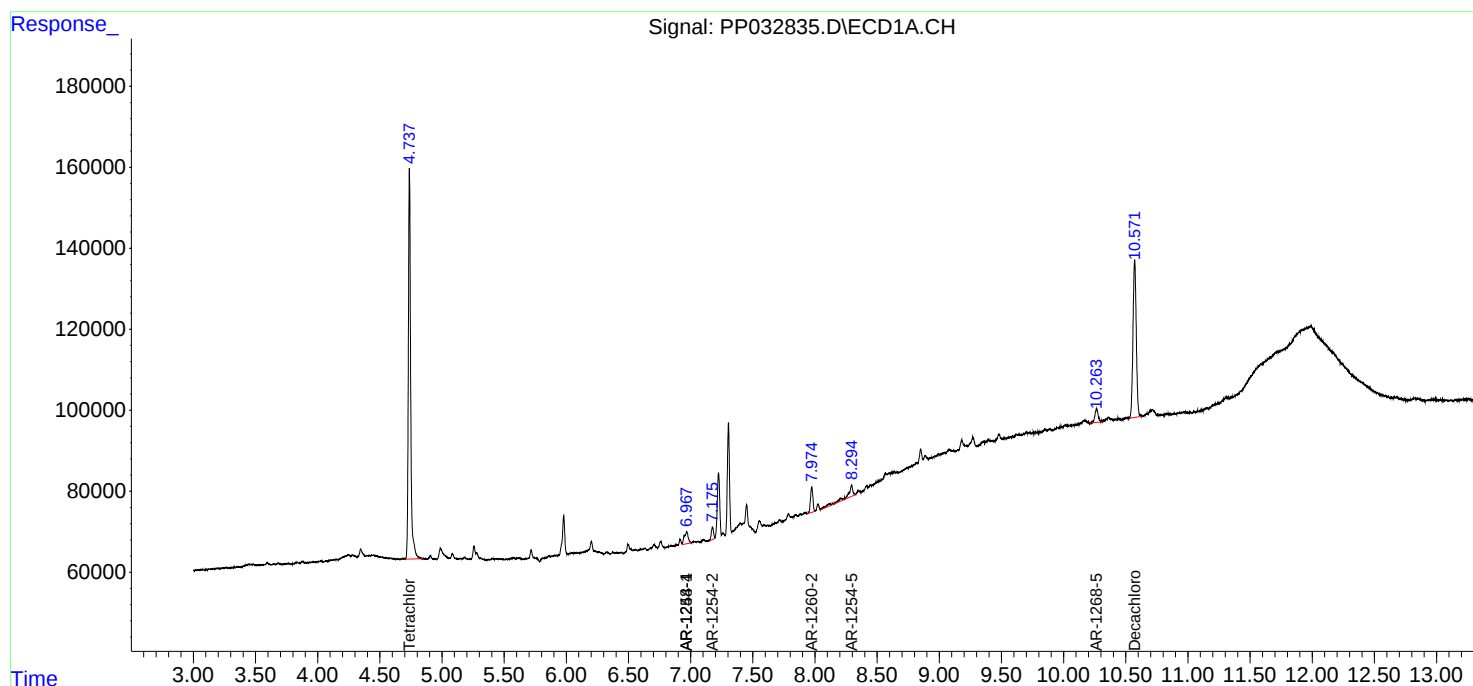


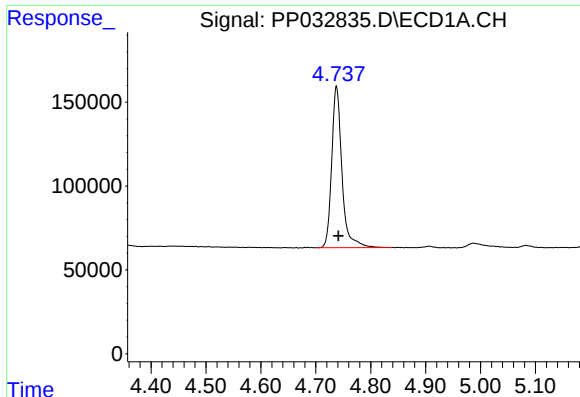

#1 Tetrachloro-m-xylene


R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1253343
Conc: 21.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-02-C

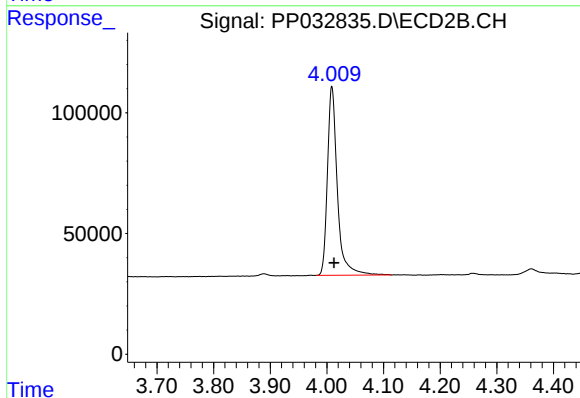


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.004 min
Response: 954659
Conc: 20.29 ng/ml

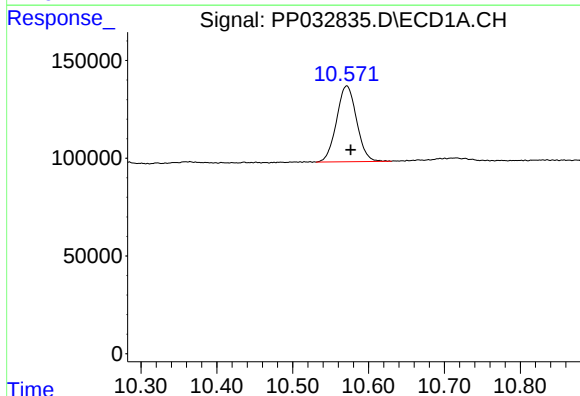


#2 Decachlorobiphenyl

R.T.: 10.571 min
Delta R.T.: -0.005 min
Response: 711068
Conc: 18.02 ng/ml

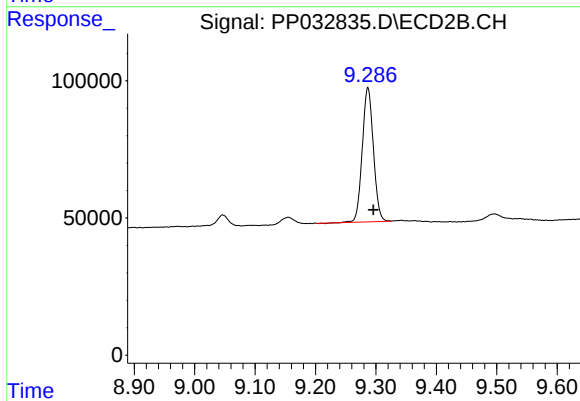

#2 Decachlorobiphenyl


R.T.: 9.287 min
Delta R.T.: -0.009 min
Response: 624320
Conc: 16.67 ng/ml

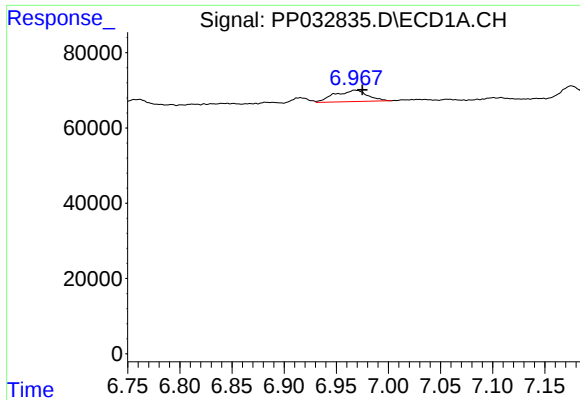

#24 AR-1248-4


R.T.: 6.967 min
Delta R.T.: -0.008 min
Response: 65848
Conc: 40.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-02-C

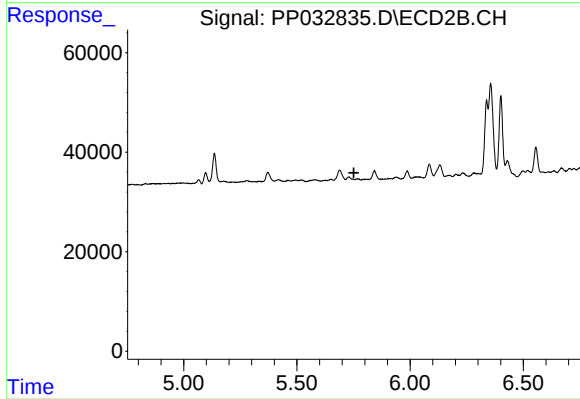


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

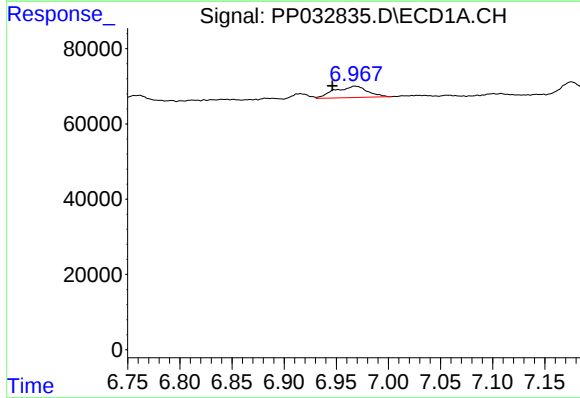


#26 AR-1254-1

R.T.: 6.967 min
Delta R.T.: 0.021 min
Response: 65848
Conc: 39.65 ng/ml

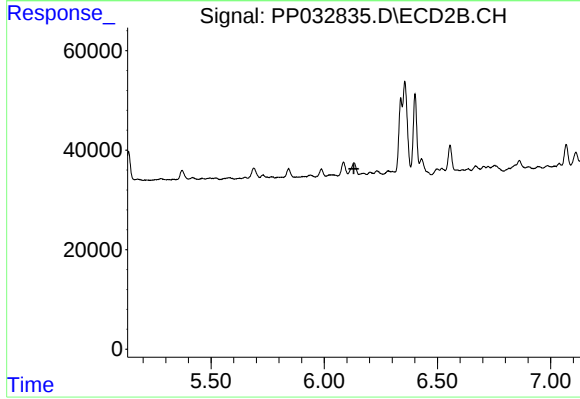

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.131 min
Response: 0
Conc: N.D.

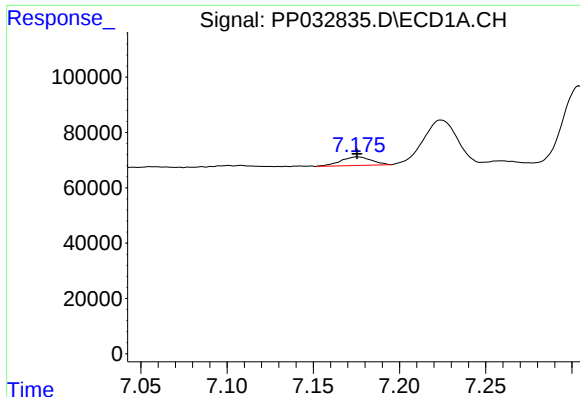

#27 AR-1254-2


R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 38491
Conc: 15.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-02-C

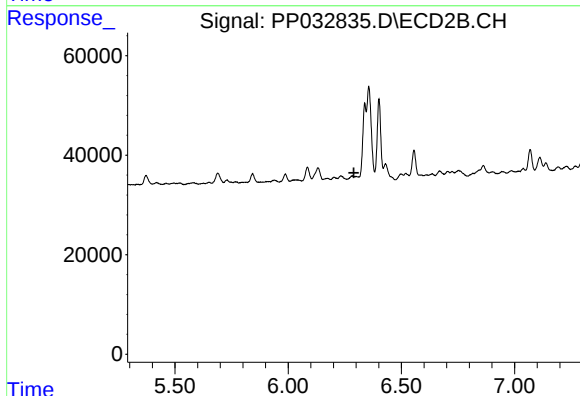


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.290 min
Response: 0
Conc: N.D.

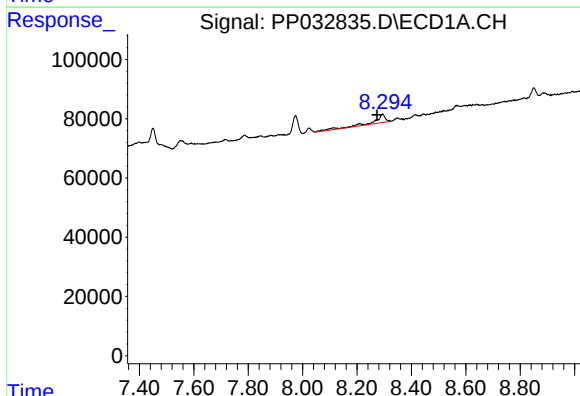


#30 AR-1254-5

R.T.: 8.295 min
Delta R.T.: 0.021 min
Response: 90879
Conc: 43.58 ng/ml

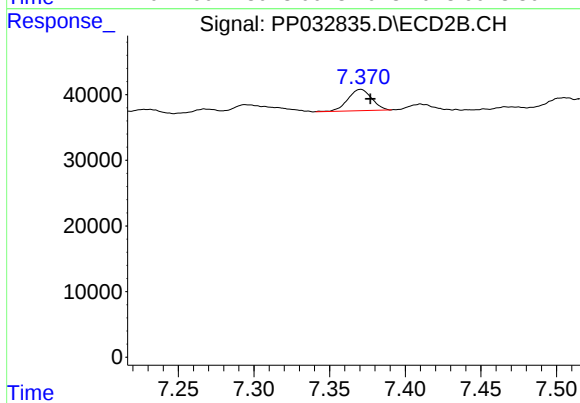

#30 AR-1254-5


R.T.: 7.371 min
Delta R.T.: -0.006 min
Response: 35784
Conc: 14.79 ng/ml

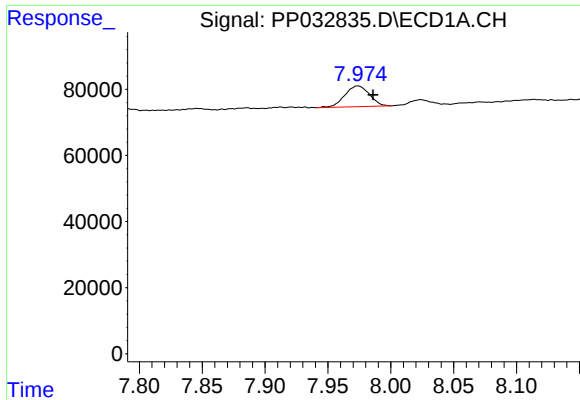

#32 AR-1260-2


R.T.: 7.974 min
Delta R.T.: -0.012 min
Response: 85302
Conc: 35.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-02-C

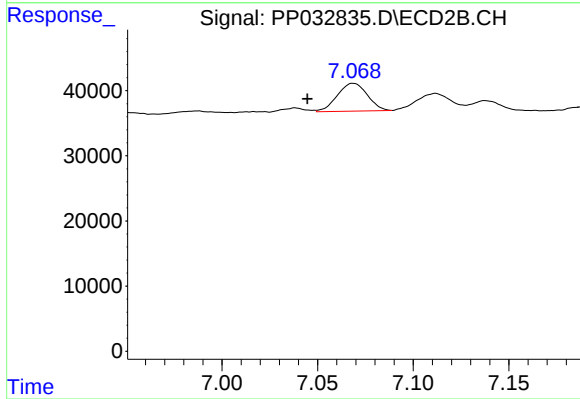


#32 AR-1260-2

R.T.: 7.069 min
Delta R.T.: 0.024 min
Response: 46656
Conc: 20.47 ng/ml

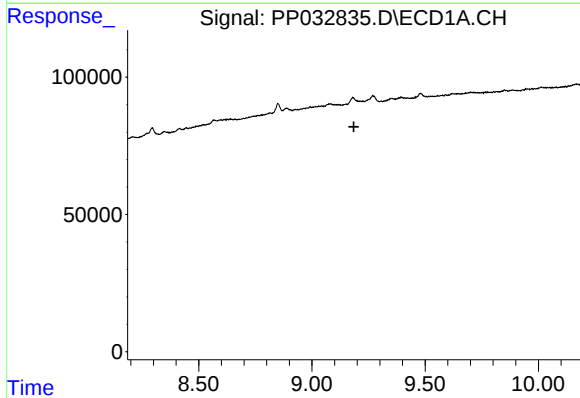


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.185 min
Response: 0
Conc: N.D.

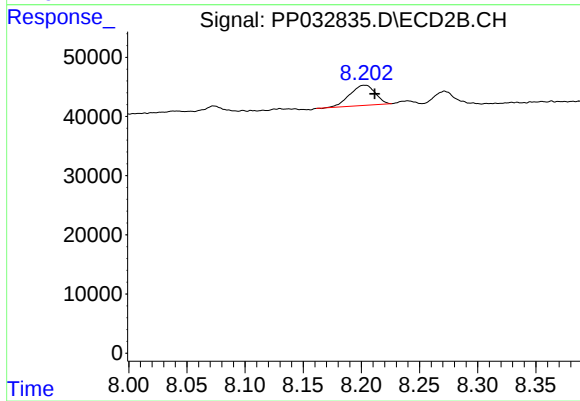

#38 AR-1262-3


R.T.: 8.203 min
Delta R.T.: -0.009 min
Response: 51981
Conc: 27.15 ng/ml

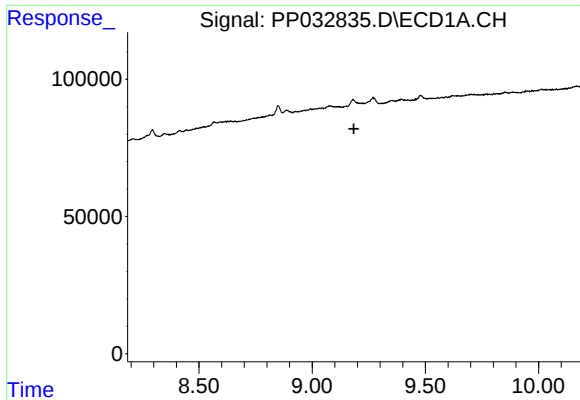

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.185 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6-02-C

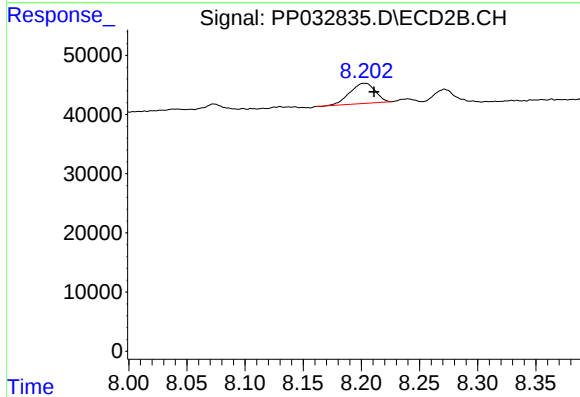


#41 AR-1268-1

R.T.: 8.203 min
Delta R.T.: -0.008 min
Response: 51981
Conc: 9.22 ng/ml

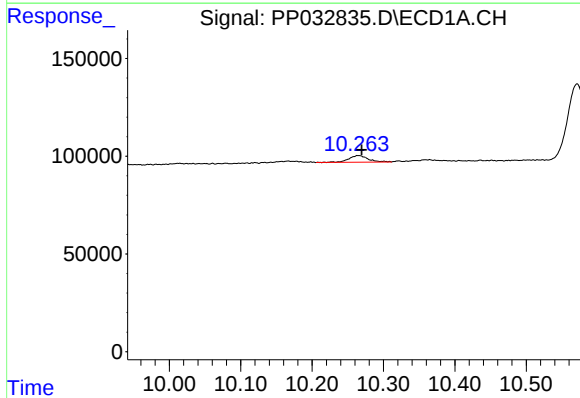

#45 AR-1268-5

R.T.: 10.265 min
Delta R.T.: -0.005 min
Response: 62624
Conc: 4.14 ng/ml

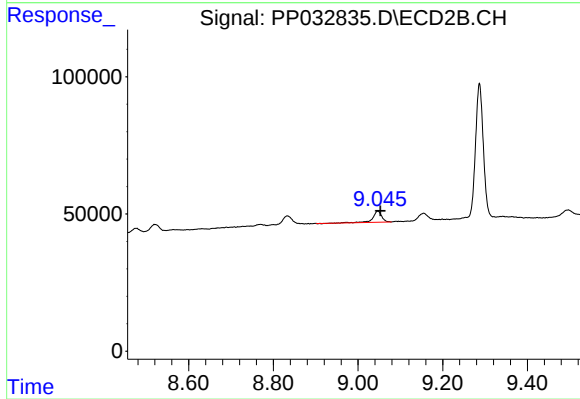

#45 AR-1268-5

R.T.: 9.046 min
Delta R.T.: -0.006 min
Response: 58971
Conc: 4.07 ng/ml