

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
 Data File : PP032852.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 18:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 02:08:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.738	4.008	1143149	871236	19.682	18.521
2) SA Decachlor...	10.572	9.285	837775	750073	21.235	20.022
Target Compounds						
34) L7 AR-1260-4	8.584	0.000	22659	0	10.997	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
Data File : PP032852.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 18:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 02:08:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

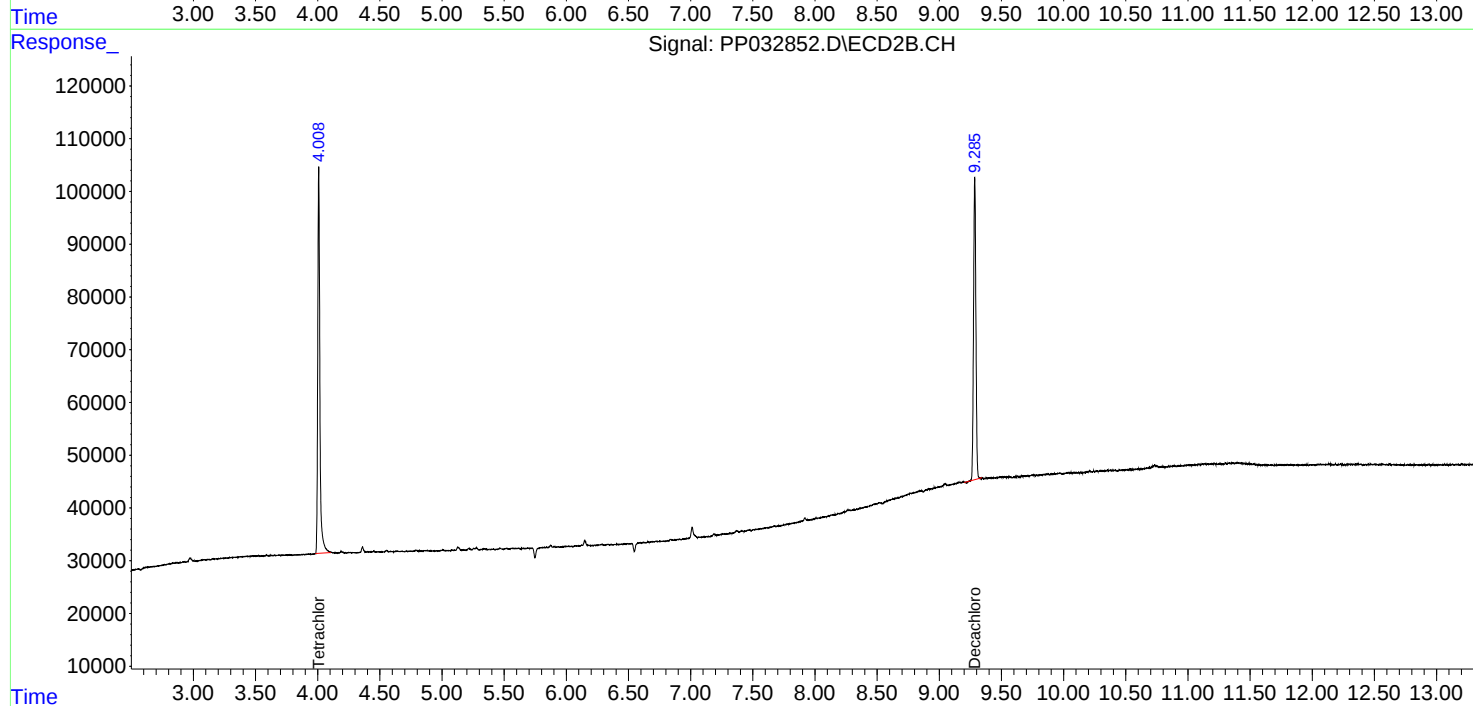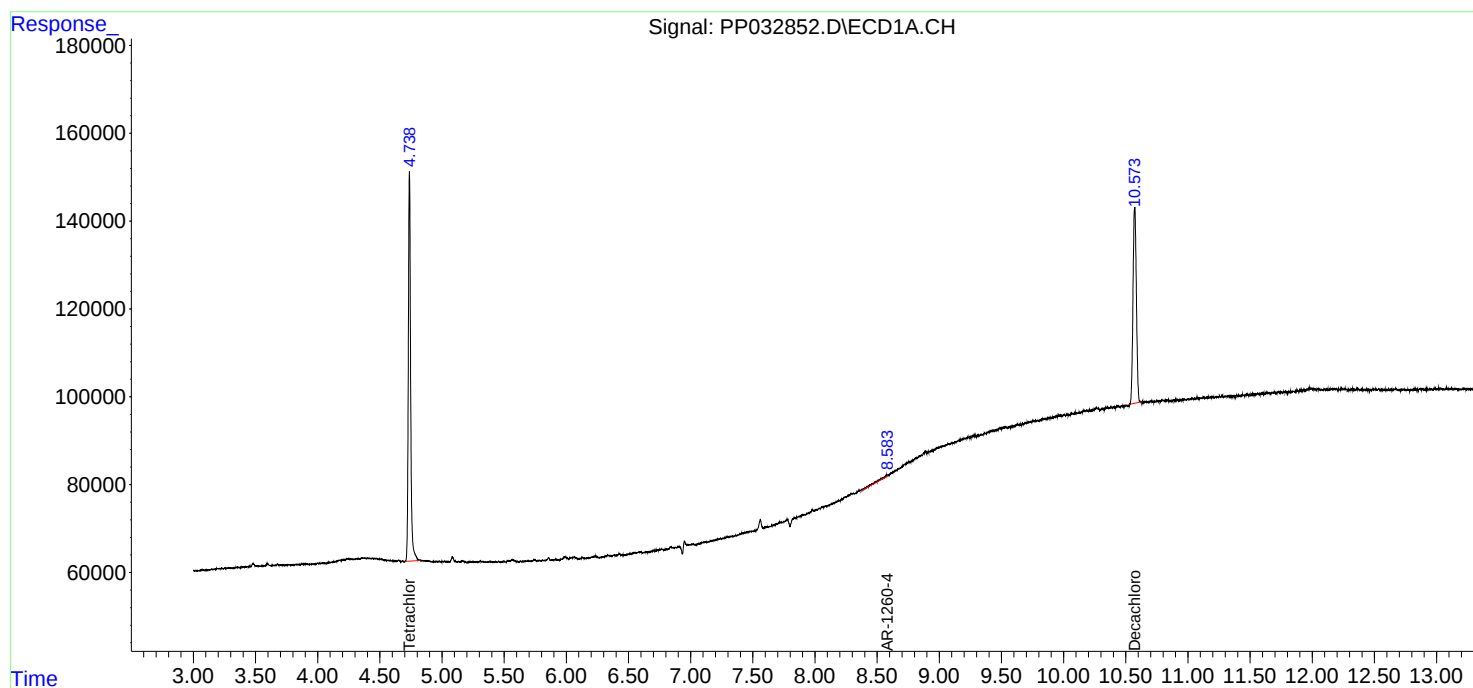


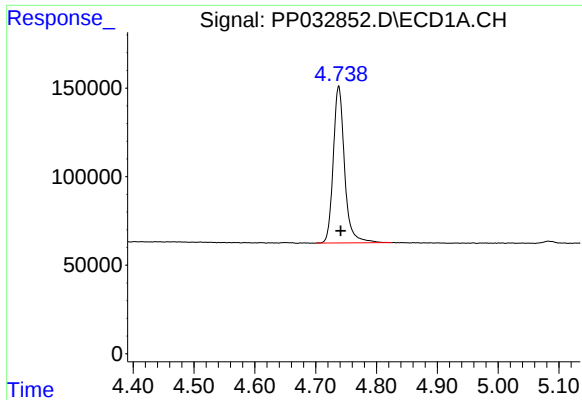

#1 Tetrachloro-m-xylene


R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1143149
Conc: 19.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

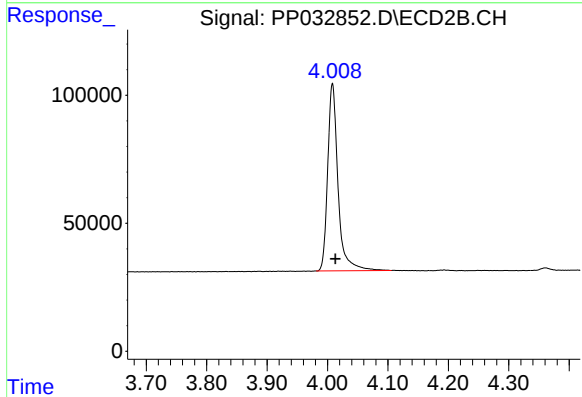


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.005 min
Response: 871236
Conc: 18.52 ng/ml

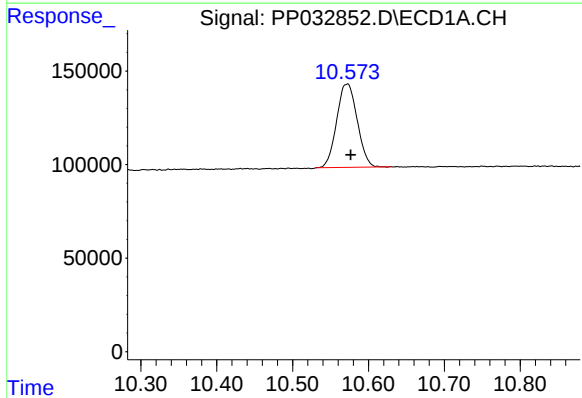


#2 Decachlorobiphenyl

R.T.: 10.572 min
Delta R.T.: -0.005 min
Response: 837775
Conc: 21.23 ng/ml

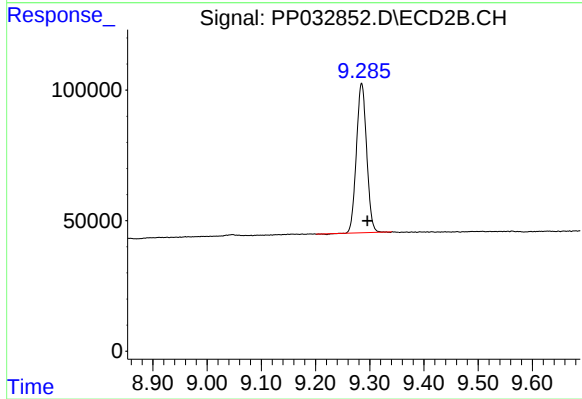

#2 Decachlorobiphenyl


R.T.: 9.285 min
Delta R.T.: -0.011 min
Response: 750073
Conc: 20.02 ng/ml

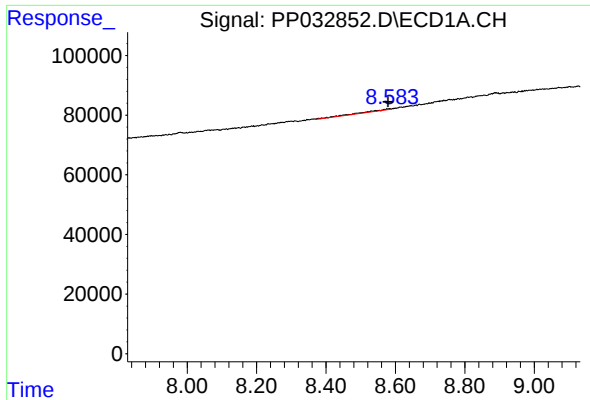

#34 AR-1260-4

R.T.: 8.584 min
Delta R.T.: 0.005 min
Response: 22659
Conc: 11.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

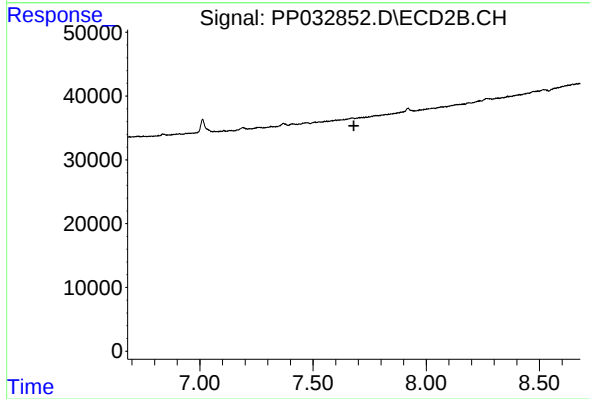

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.680 min
Response: 0
Conc: N.D.