

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
 Data File : PP032835.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 12:50
 Operator : DD\AJ
 Sample : M1106-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6-02-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 02:03:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.738	4.009	1253343	954659	21.579	20.295
2) SA Decachlor...	10.571	9.287	711068	624320	18.023	16.665

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
Data File : PP032835.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 12:50
Operator : DD\AJ
Sample : M1106-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S6-02-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 02:03:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

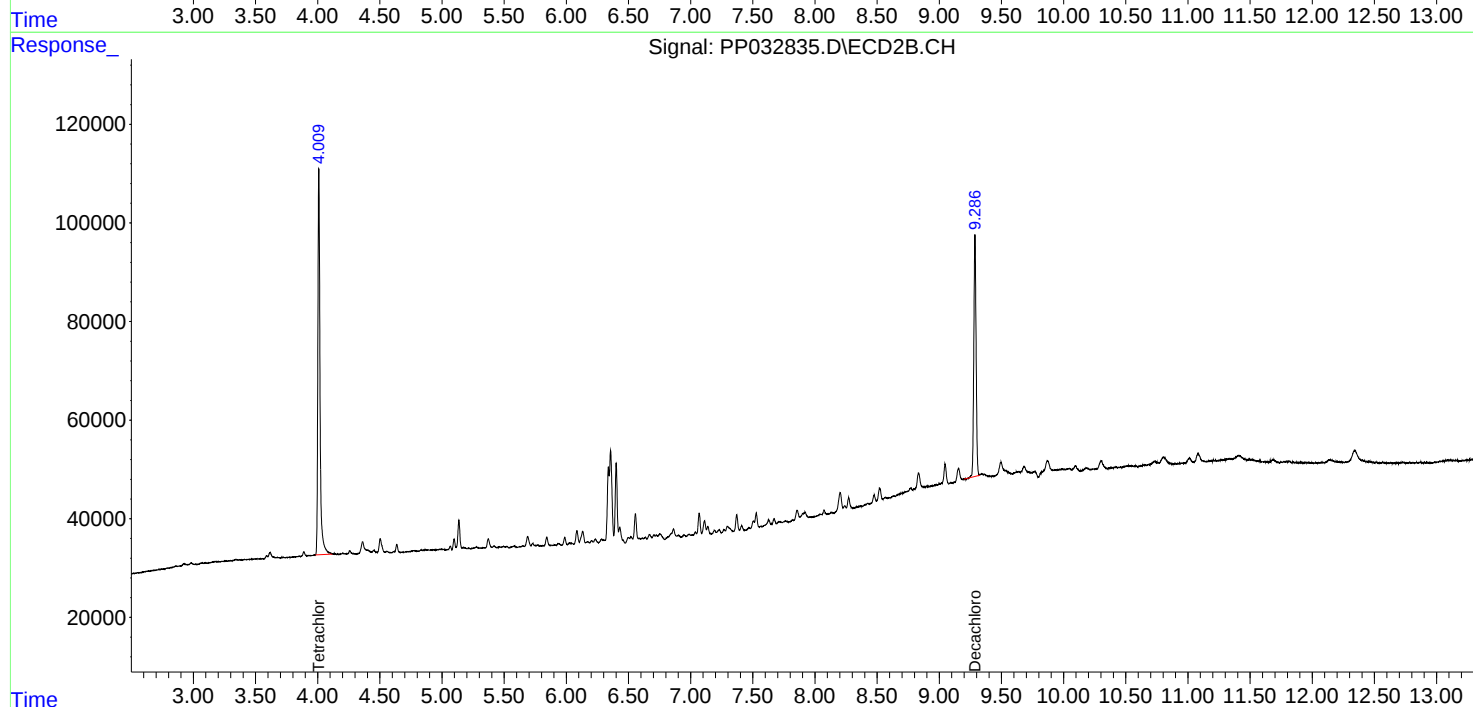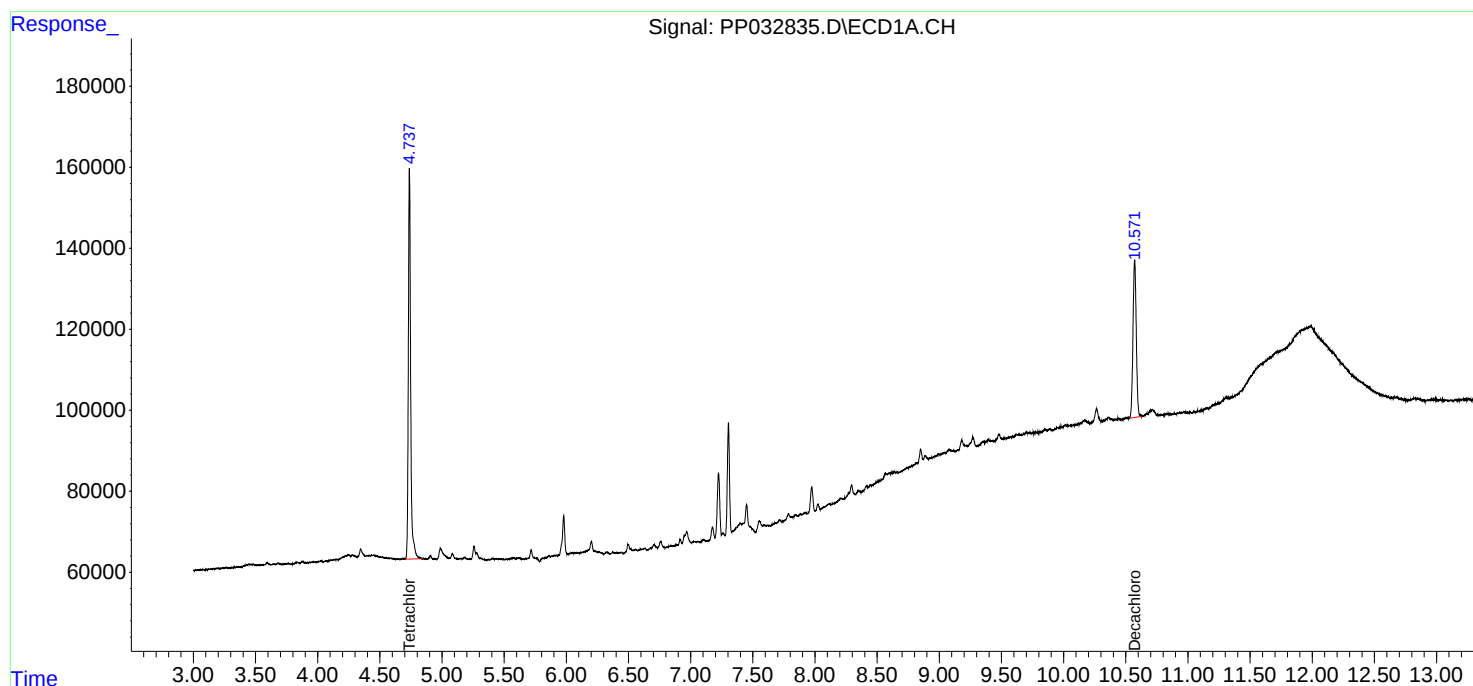


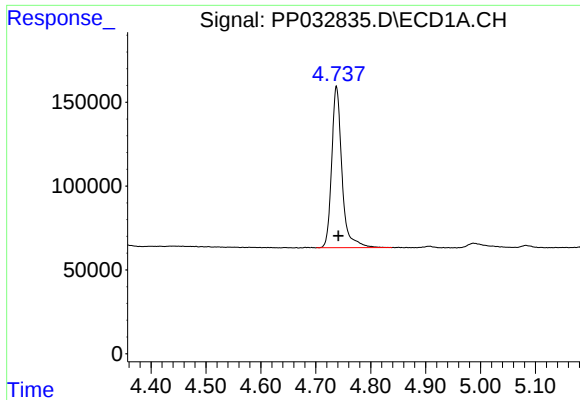

#1 Tetrachloro-m-xylene


R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1253343
Conc: 21.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6-02-C

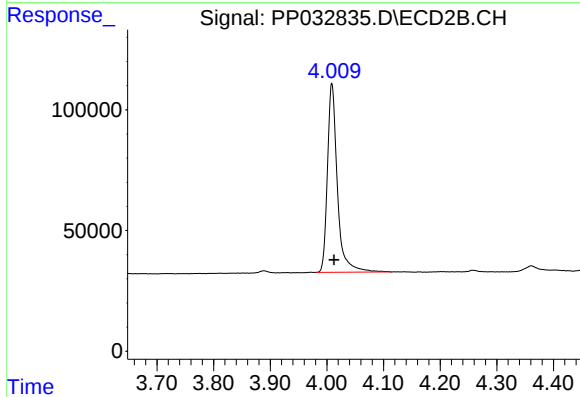


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.004 min
Response: 954659
Conc: 20.29 ng/ml

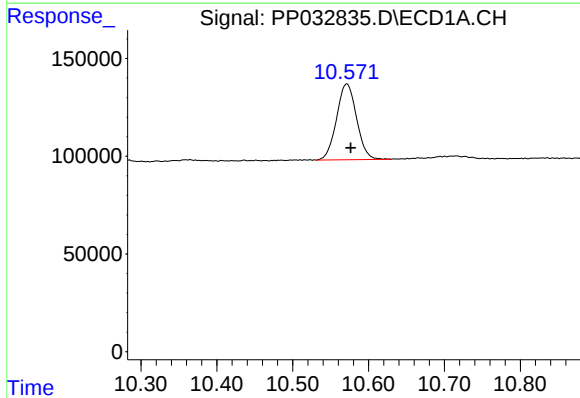

#2 Decachlorobiphenyl

R.T.: 10.571 min
Delta R.T.: -0.005 min
Response: 711068
Conc: 18.02 ng/ml

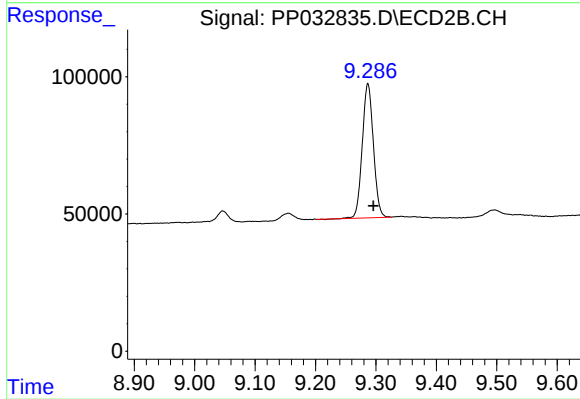

#2 Decachlorobiphenyl

R.T.: 9.287 min
Delta R.T.: -0.009 min
Response: 624320
Conc: 16.67 ng/ml