

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
 Data File : PP032849.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 16:55
 Operator : DD\AJ
 Sample : M1111-07DL2 20X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S20-01-EDL2

Manual Integrations
 APPROVED

Ankita
 1/20/2021 9:59:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 02:07:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.737	4.008	51760	39443	0.891	0.839
2)	SA Decachlor...	10.572	9.285	1423558	1264517	36.082	33.754
Target Compounds							
26)	L6 AR-1254-1	6.942	6.124	65630	73871	39.516m	36.082m
27)	L6 AR-1254-2	7.169	6.283	197833	159004	78.662	90.537
28)	L6 AR-1254-3	7.548	6.703	317204	343905	117.730	119.746
29)	L6 AR-1254-4	7.843	6.943	257068	219054	130.504	132.286
30)	L6 AR-1254-5	8.269	7.370	570422	525915	273.525	217.421
41)	L9 AR-1268-1	9.180	8.204	4820565	3752661	728.143	665.535
42)	L9 AR-1268-2	9.270	8.269	3400084	2914351	564.428	537.592
43)	L9 AR-1268-3	9.480	8.473	4102905	3358308	766.476	707.288
44)	L9 AR-1268-4	9.884	8.766	873395	705155	425.871	389.875
45)	L9 AR-1268-5	10.266	9.045	10931224	9478597	723.138	654.680

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011921\
Data File : PP032849.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 16:55
Operator : DD\AJ
Sample : M1111-07DL2 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 02:07:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

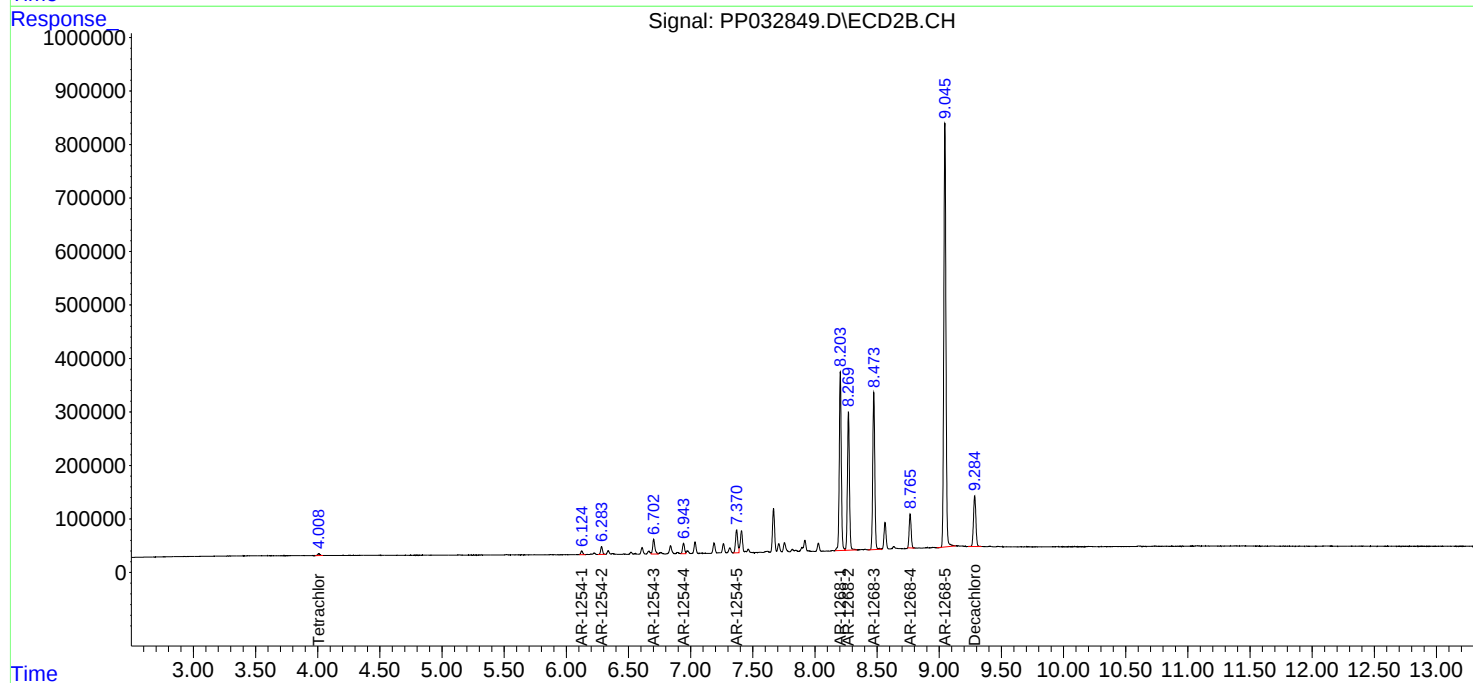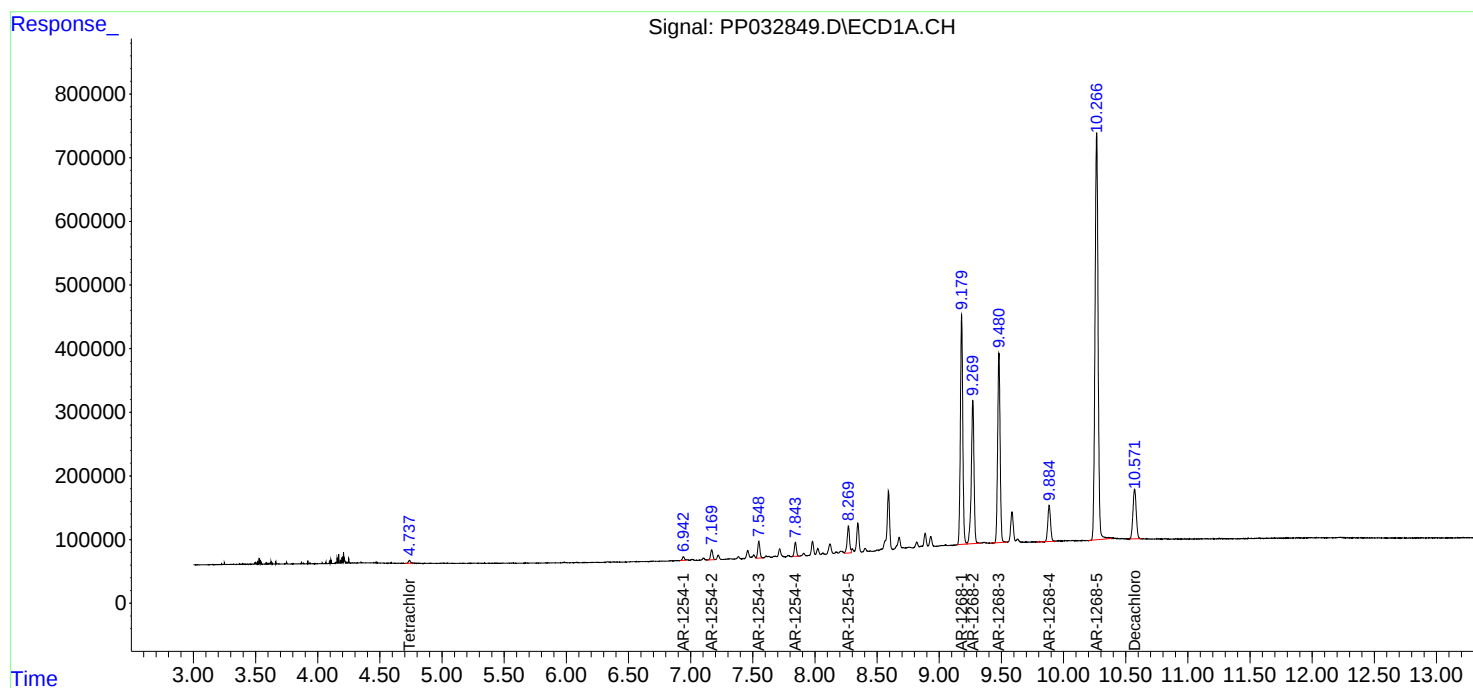

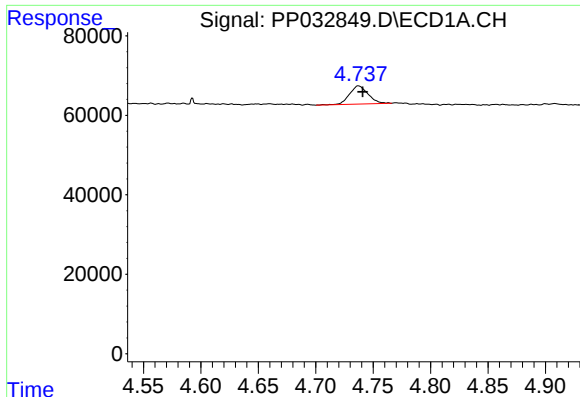


#1 Tetrachloro-m-xylene

R.T.: 4.737 min
Delta R.T.: -0.004 min
Response: 51760
Conc: 0.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

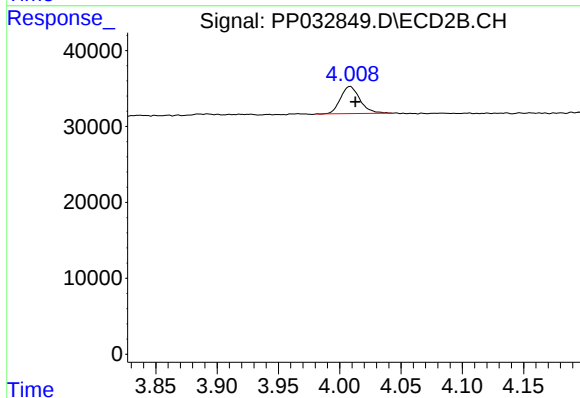


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.004 min
Response: 39443
Conc: 0.84 ng/ml

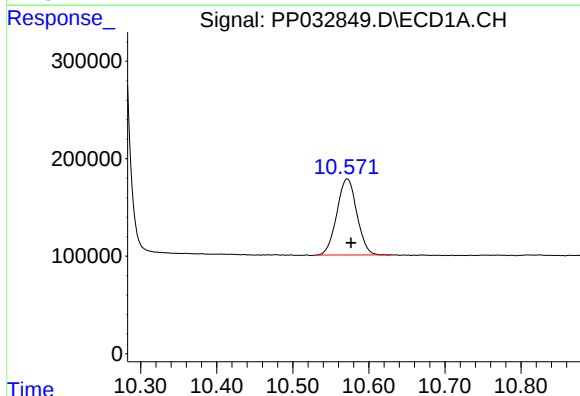


#2 Decachlorobiphenyl

R.T.: 10.572 min
Delta R.T.: -0.005 min
Response: 1423558
Conc: 36.08 ng/ml

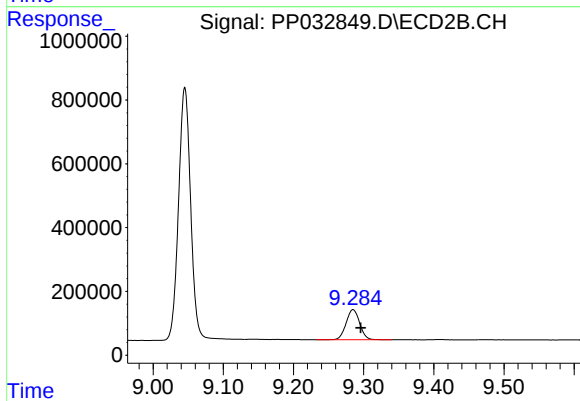

#2 Decachlorobiphenyl

R.T.: 9.285 min
Delta R.T.: -0.011 min
Response: 1264517
Conc: 33.75 ng/ml

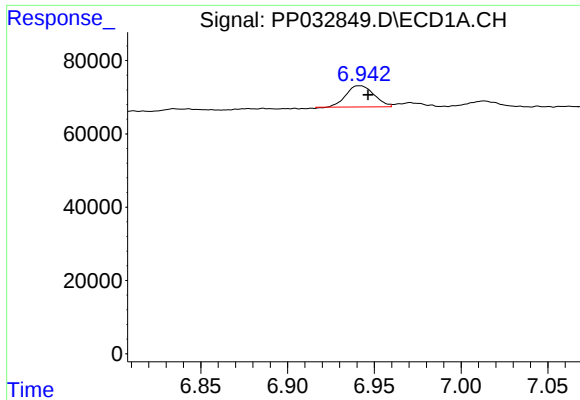


#26 AR-1254-1

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 65630
Conc: 39.52 ng/ml m

Instrument :
ECD_P
ClientSampleId :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

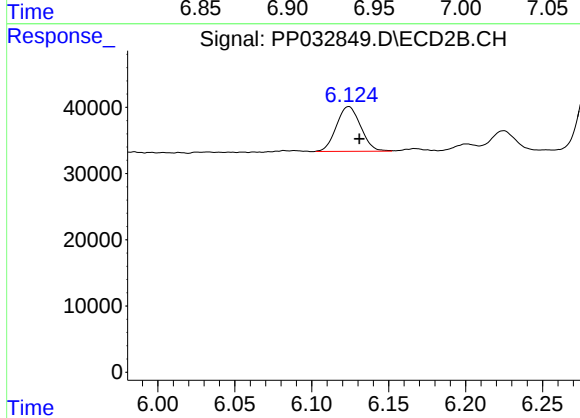


#26 AR-1254-1

R.T.: 6.124 min
Delta R.T.: -0.007 min
Response: 73871
Conc: 36.08 ng/ml m

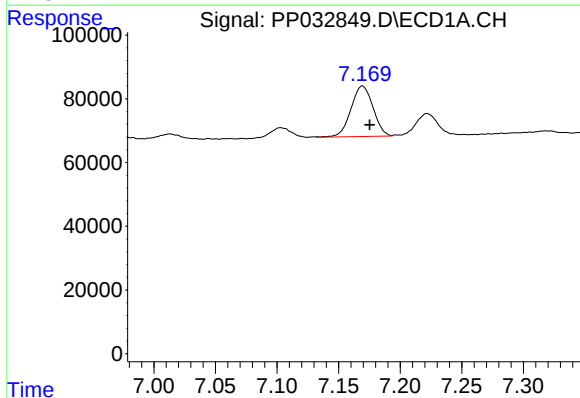


#27 AR-1254-2

R.T.: 7.169 min
Delta R.T.: -0.006 min
Response: 197833
Conc: 78.66 ng/ml

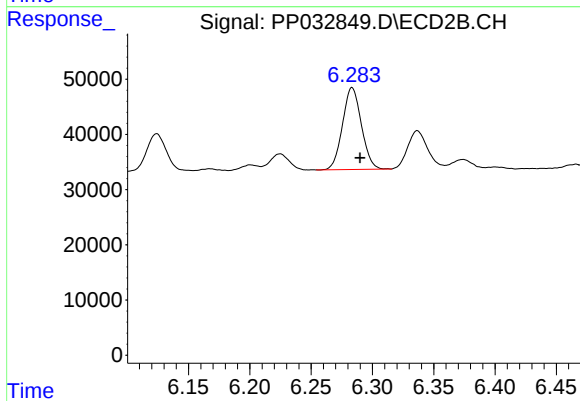

#27 AR-1254-2

R.T.: 6.283 min
Delta R.T.: -0.006 min
Response: 159004
Conc: 90.54 ng/ml

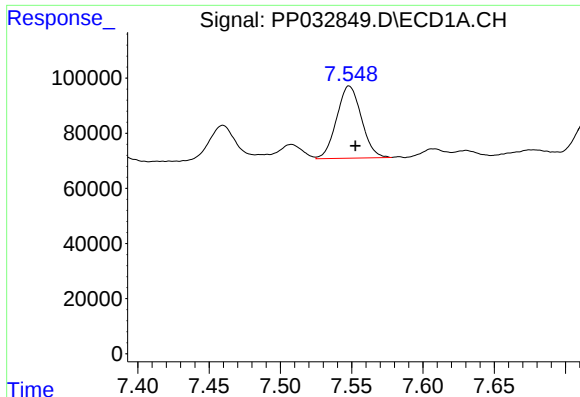


#28 AR-1254-3

R.T.: 7.548 min
Delta R.T.: -0.005 min
Response: 317204
Conc: 117.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

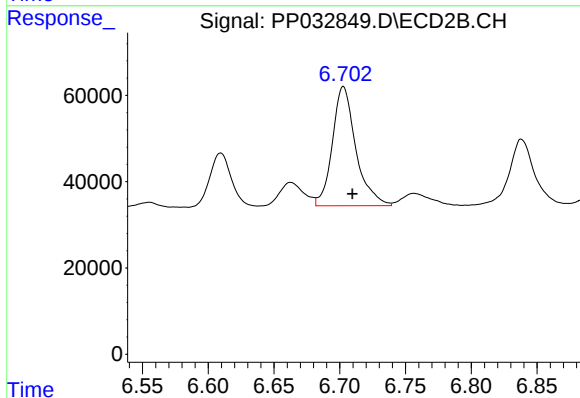


#28 AR-1254-3

R.T.: 6.703 min
Delta R.T.: -0.007 min
Response: 343905
Conc: 119.75 ng/ml

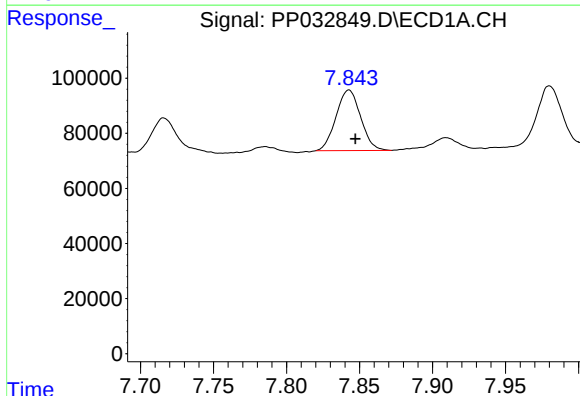


#29 AR-1254-4

R.T.: 7.843 min
Delta R.T.: -0.004 min
Response: 257068
Conc: 130.50 ng/ml

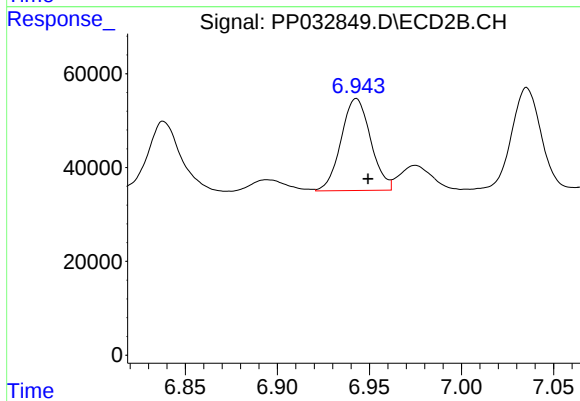

#29 AR-1254-4

R.T.: 6.943 min
Delta R.T.: -0.006 min
Response: 219054
Conc: 132.29 ng/ml

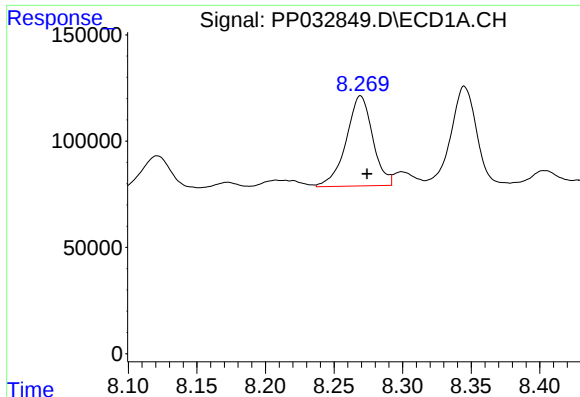


#30 AR-1254-5

R.T.: 8.269 min
Delta R.T.: -0.005 min
Response: 570422
Conc: 273.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

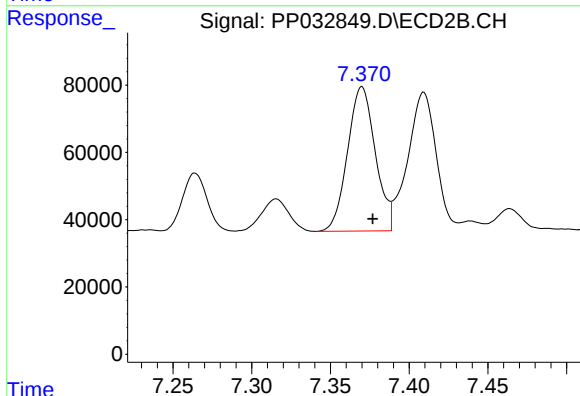


#30 AR-1254-5

R.T.: 7.370 min
Delta R.T.: -0.007 min
Response: 525915
Conc: 217.42 ng/ml

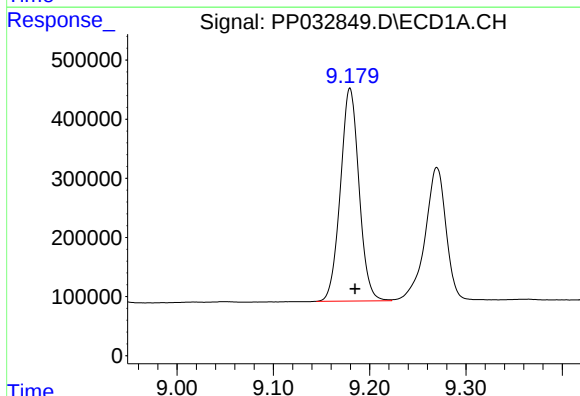


#41 AR-1268-1

R.T.: 9.180 min
Delta R.T.: -0.005 min
Response: 4820565
Conc: 728.14 ng/ml

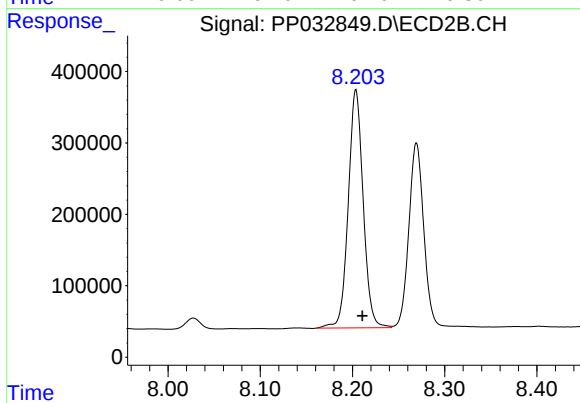

#41 AR-1268-1

R.T.: 8.204 min
Delta R.T.: -0.007 min
Response: 3752661
Conc: 665.54 ng/ml

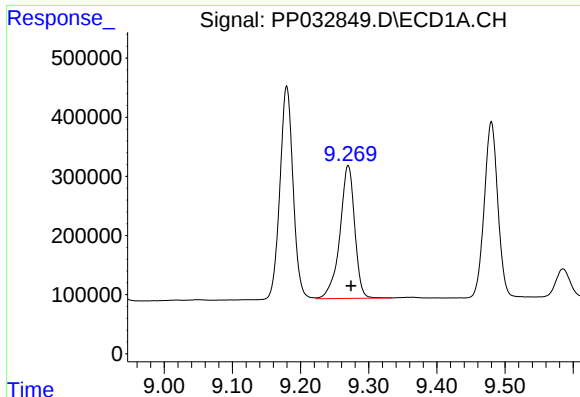


#42 AR-1268-2

R.T.: 9.270 min
Delta R.T.: -0.004 min
Response: 3400084
Conc: 564.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

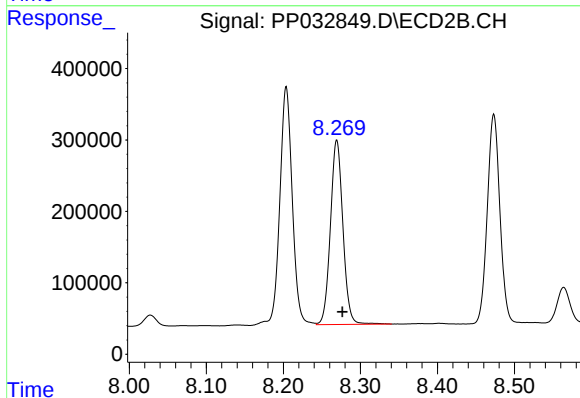


#42 AR-1268-2

R.T.: 8.269 min
Delta R.T.: -0.007 min
Response: 2914351
Conc: 537.59 ng/ml

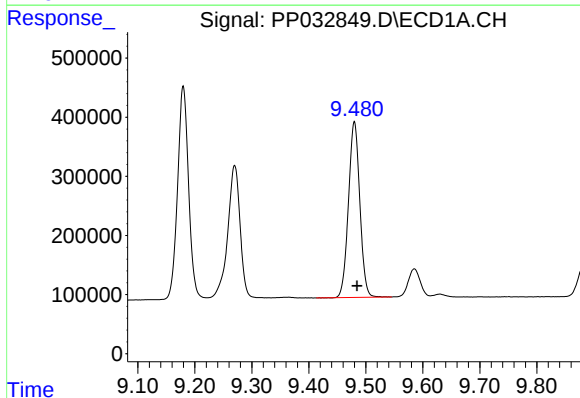


#43 AR-1268-3

R.T.: 9.480 min
Delta R.T.: -0.005 min
Response: 4102905
Conc: 766.48 ng/ml

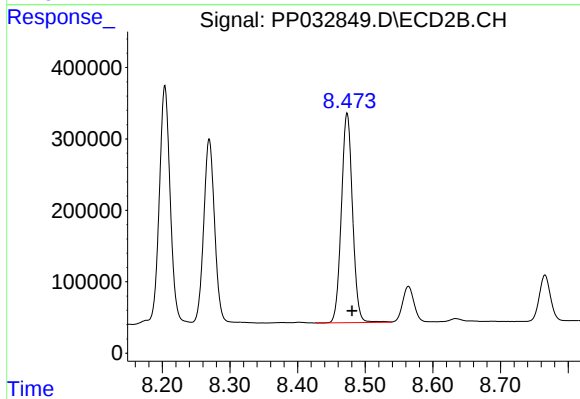

#43 AR-1268-3

R.T.: 8.473 min
Delta R.T.: -0.007 min
Response: 3358308
Conc: 707.29 ng/ml

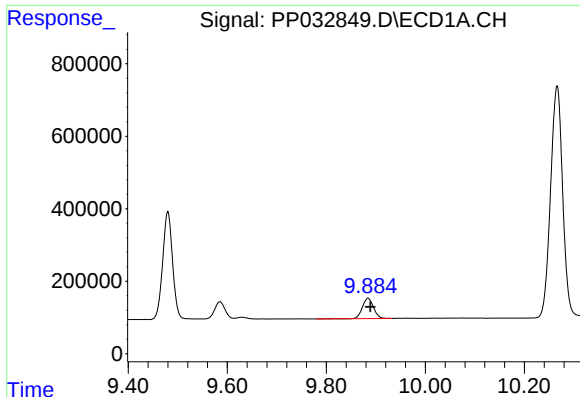


#44 AR-1268-4

R.T.: 9.884 min
Delta R.T.: -0.005 min
Response: 873395
Conc: 425.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
S20-01-EDL2


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:32 AM

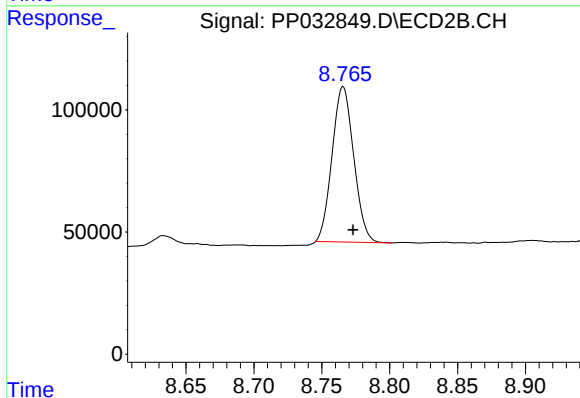


#44 AR-1268-4

R.T.: 8.766 min
Delta R.T.: -0.007 min
Response: 705155
Conc: 389.87 ng/ml

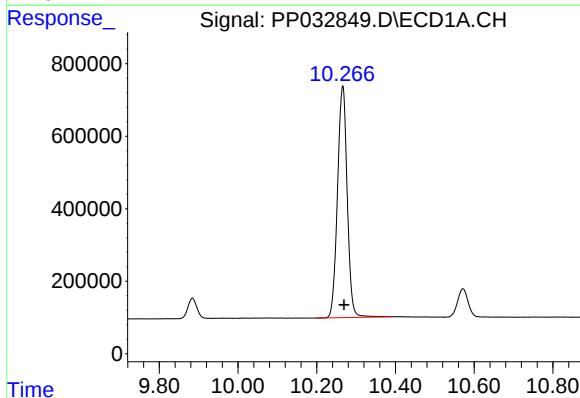

#45 AR-1268-5

R.T.: 10.266 min
Delta R.T.: -0.003 min
Response: 10931224
Conc: 723.14 ng/ml

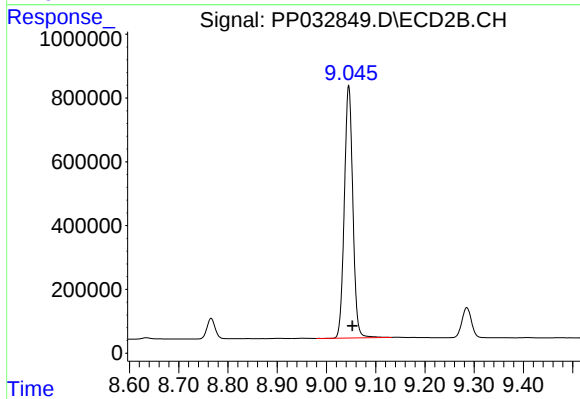

#45 AR-1268-5

R.T.: 9.045 min
Delta R.T.: -0.007 min
Response: 9478597
Conc: 654.68 ng/ml