

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011922\
 Data File : PP043092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2022 11:51
 Operator : AJ\MA
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/20/2022
 Supervised By :Ankita Jodhani 01/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 02:46:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.874	4.040	1104161	1226509	46.665	49.107
2) SA Decachlor...	10.798	9.371	811653	978989	55.522m	50.188
Target Compounds						
21) L5 AR-1248-1	6.176	5.303	194152	286624	473.698	510.246
22) L5 AR-1248-2	6.471	5.568	269536	397805	478.758	490.124
23) L5 AR-1248-3	6.685	5.613	324999	410388	479.351	477.479
24) L5 AR-1248-4	7.109	5.799	339384	475909	470.512	495.879m
25) L5 AR-1248-5	7.149	6.223	338082	485002	463.361	508.021

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011922\
Data File : PP043092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2022 11:51
Operator : AJ\MA
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 02:46:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

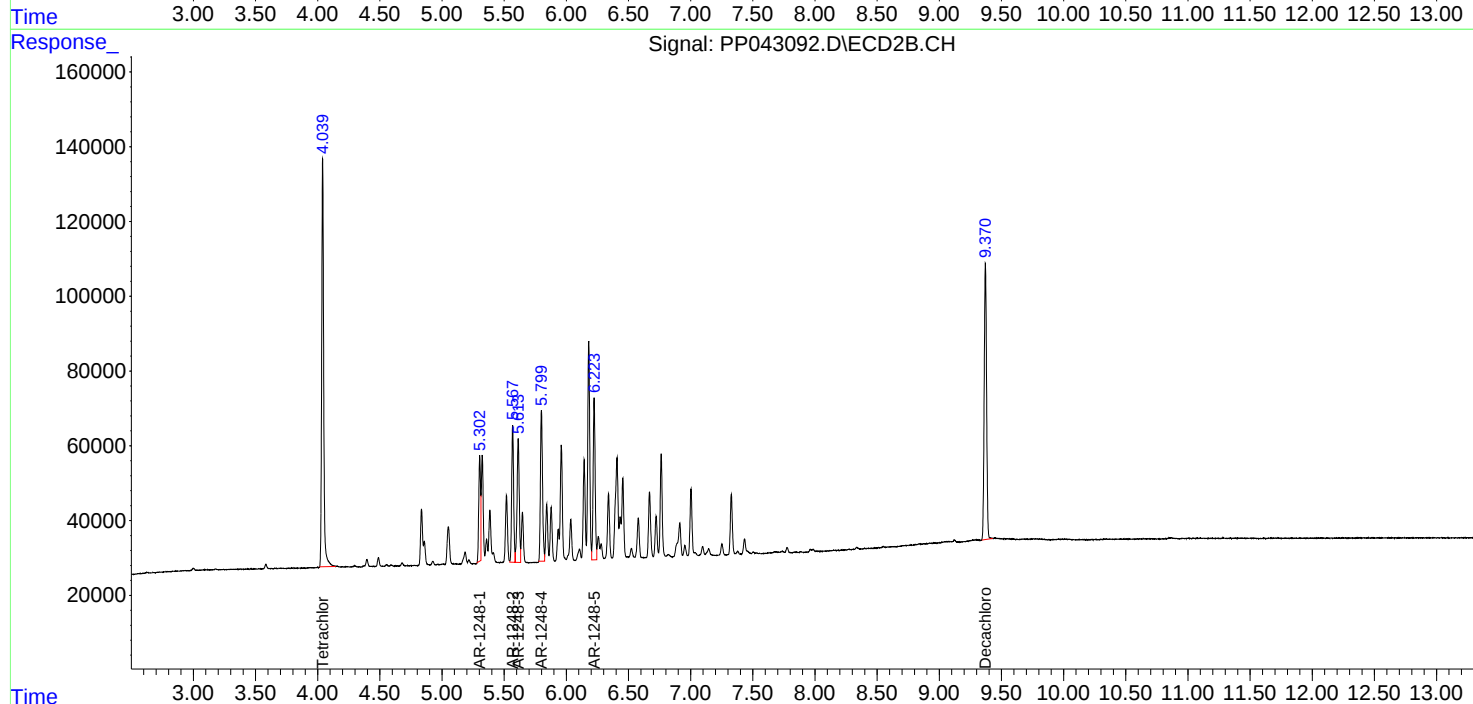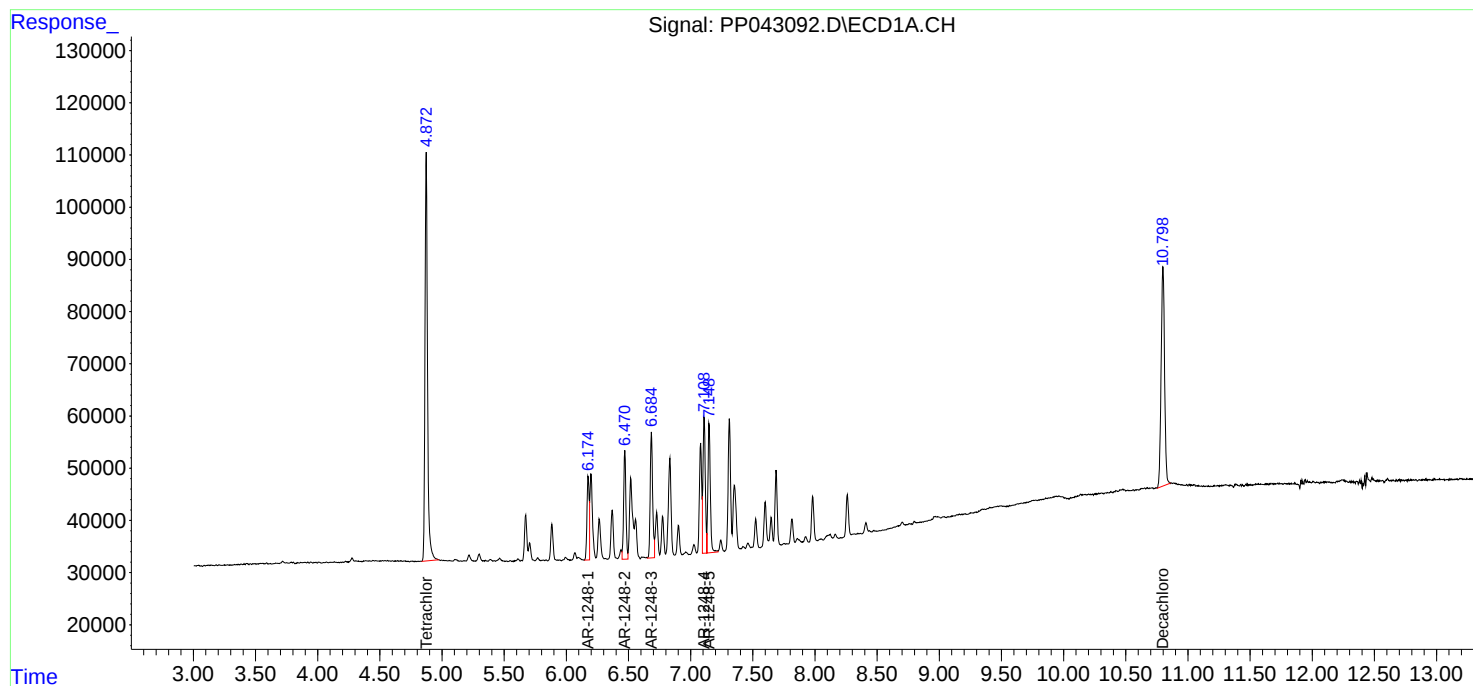

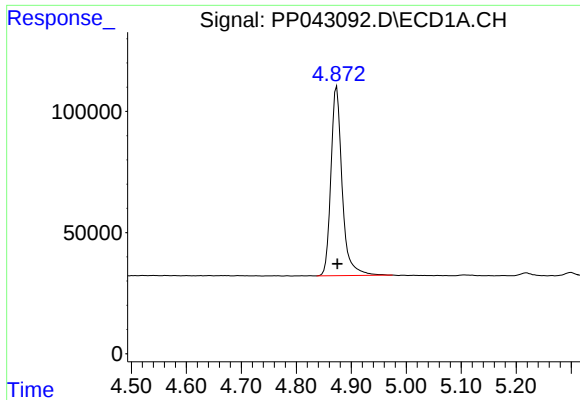


#1 Tetrachloro-m-xylene

R.T.: 4.874 min
Delta R.T.: -0.001 min
Response: 1104161
Conc: 46.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

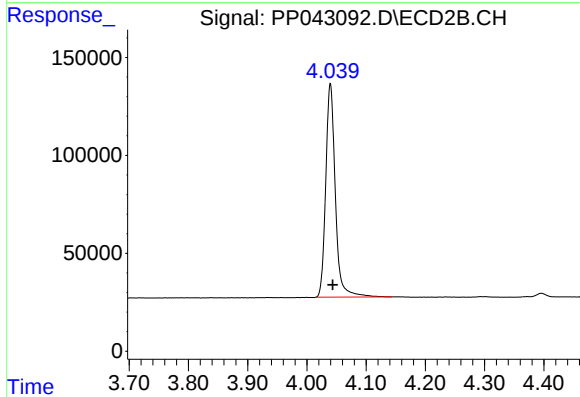


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: -0.004 min
Response: 1226509
Conc: 49.11 ng/ml

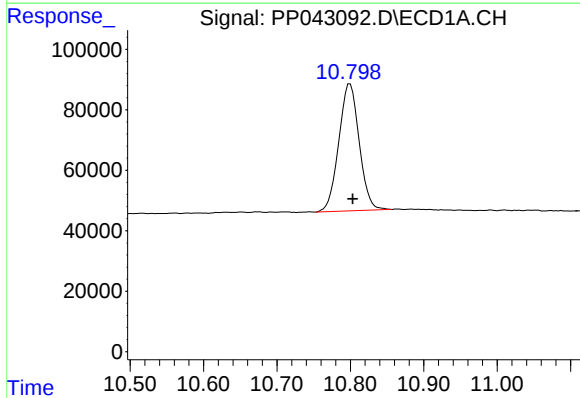


#2 Decachlorobiphenyl

R.T.: 10.798 min
Delta R.T.: -0.005 min
Response: 811653
Conc: 55.52 ng/ml m

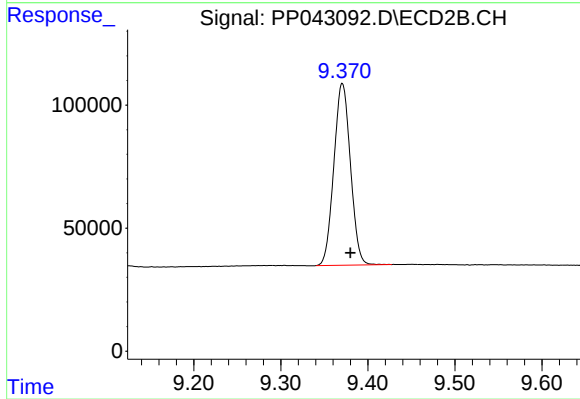

#2 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.009 min
Response: 978989
Conc: 50.19 ng/ml

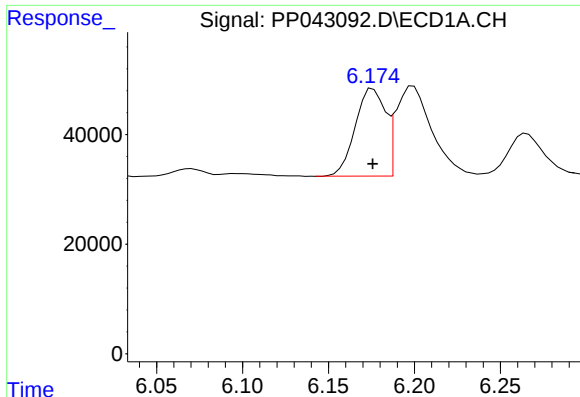


#21 AR-1248-1

R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 194152
Conc: 473.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

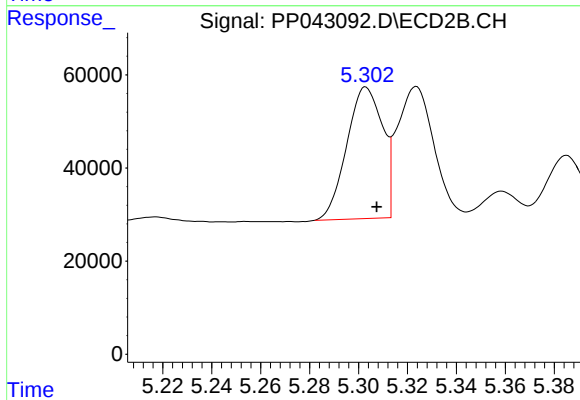


#21 AR-1248-1

R.T.: 5.303 min
Delta R.T.: -0.005 min
Response: 286624
Conc: 510.25 ng/ml

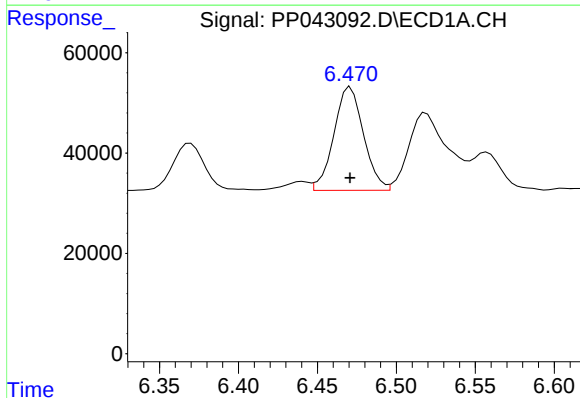


#22 AR-1248-2

R.T.: 6.471 min
Delta R.T.: 0.000 min
Response: 269536
Conc: 478.76 ng/ml

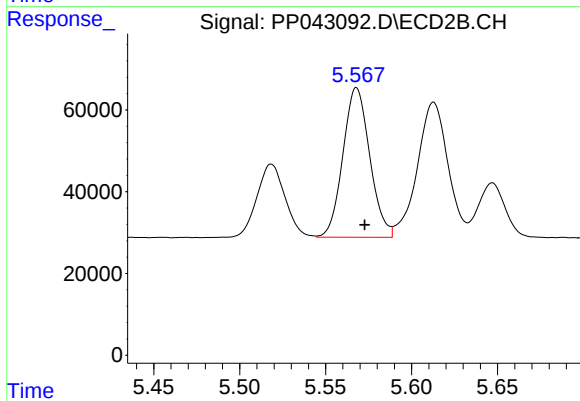

#22 AR-1248-2

R.T.: 5.568 min
Delta R.T.: -0.005 min
Response: 397805
Conc: 490.12 ng/ml

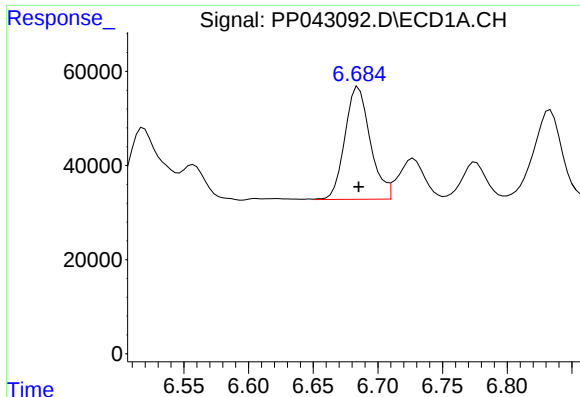


#23 AR-1248-3

R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 324999
Conc: 479.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

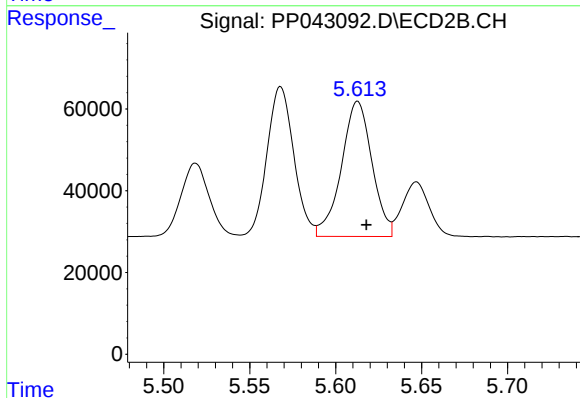


#23 AR-1248-3

R.T.: 5.613 min
Delta R.T.: -0.005 min
Response: 410388
Conc: 477.48 ng/ml

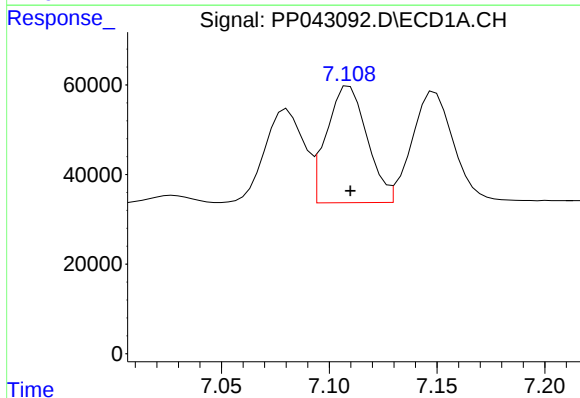


#24 AR-1248-4

R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 339384
Conc: 470.51 ng/ml

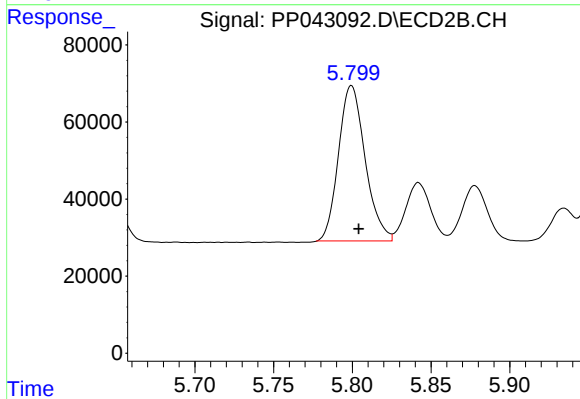

#24 AR-1248-4

R.T.: 5.799 min
Delta R.T.: -0.005 min
Response: 475909
Conc: 495.88 ng/ml m

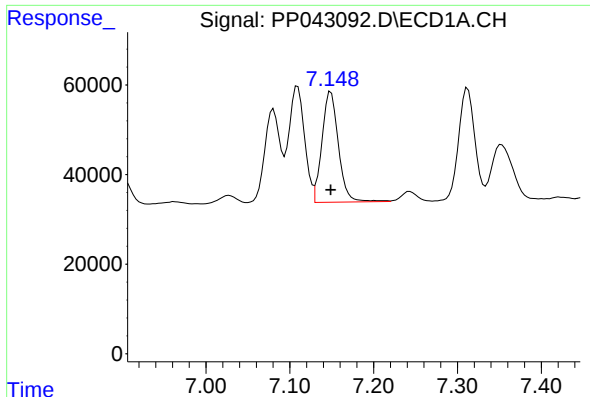


#25 AR-1248-5

R.T.: 7.149 min
Delta R.T.: 0.000 min
Response: 338082
Conc: 463.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

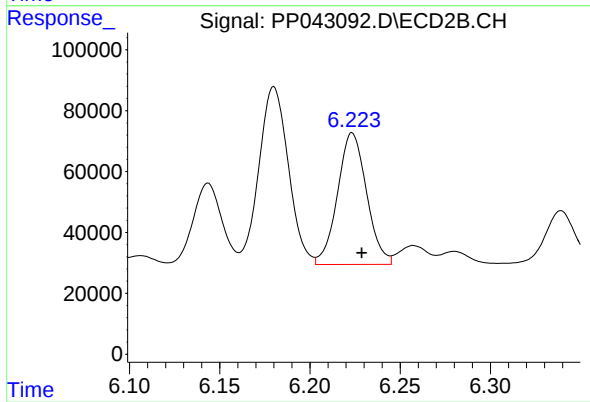

#25 AR-1248-5

R.T.: 6.223 min
Delta R.T.: -0.005 min
Response: 485002
Conc: 508.02 ng/ml