

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011922\
 Data File : PP043097.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2022 13:14
 Operator : AJ\MA
 Sample : N1176-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/20/2022
 Supervised By :Ankita Jodhani 01/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 02:48:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.039	472295	542886	19.961	21.736
2) SA Decachlor...	10.798	9.370	354680	454673	24.262	23.309
Target Compounds						
31) L7 AR-1260-1	7.857	6.896	18453	52380	19.352	40.524 #
32) L7 AR-1260-2	8.112	7.111	21746	55135	21.056m	35.299 #
33) L7 AR-1260-3	8.488	7.252	15766	26050	20.896	18.024
34) L7 AR-1260-4	8.714	7.736	11064	32889	12.989m	29.030 #
35) L7 AR-1260-5	9.032	7.982	35748	97324	21.727	38.805 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011922\
Data File : PP043097.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2022 13:14
Operator : AJ\MA
Sample : N1176-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 02:48:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

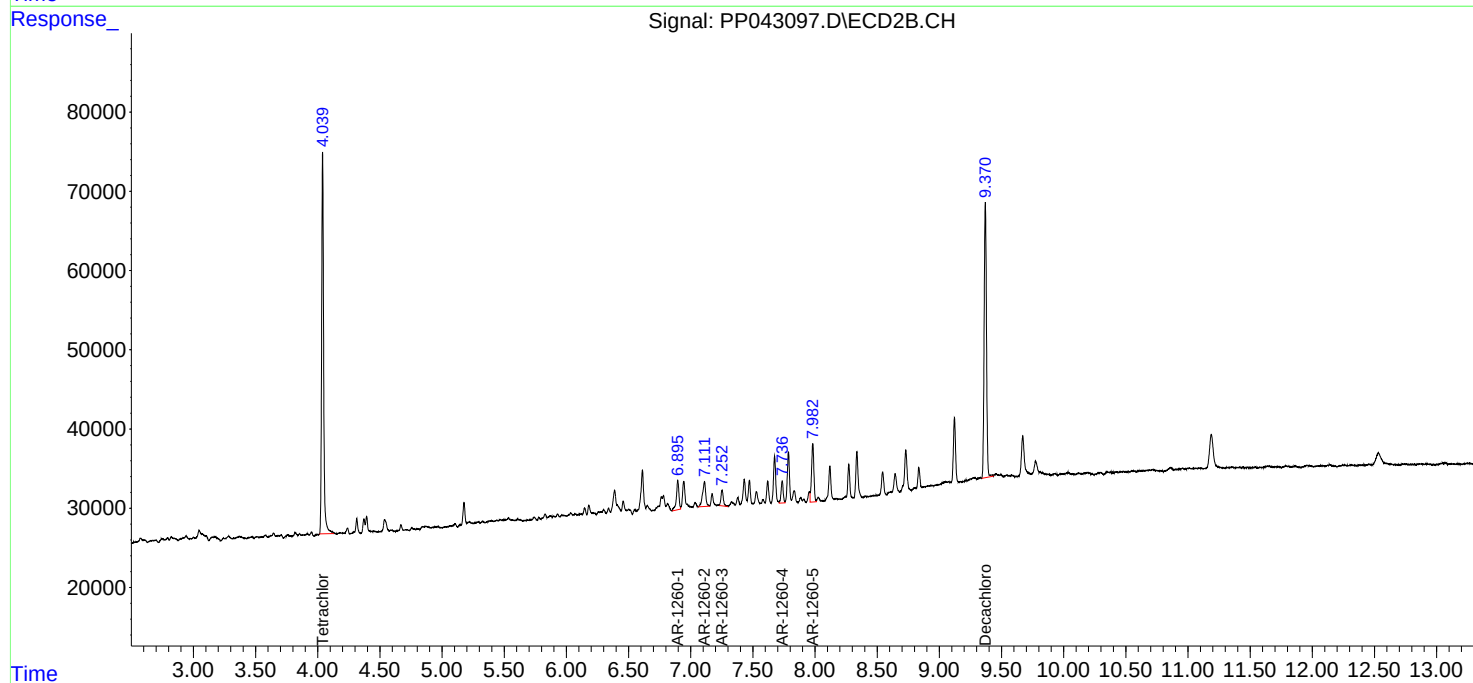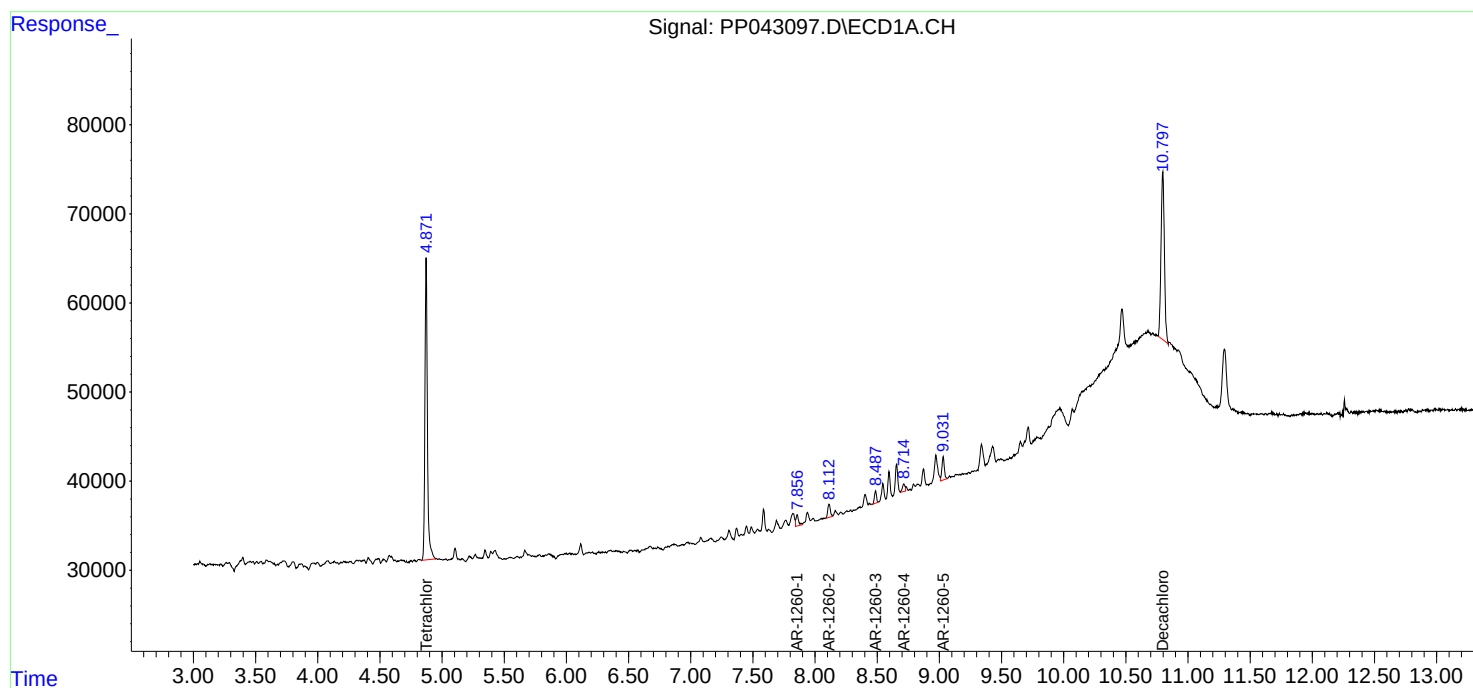

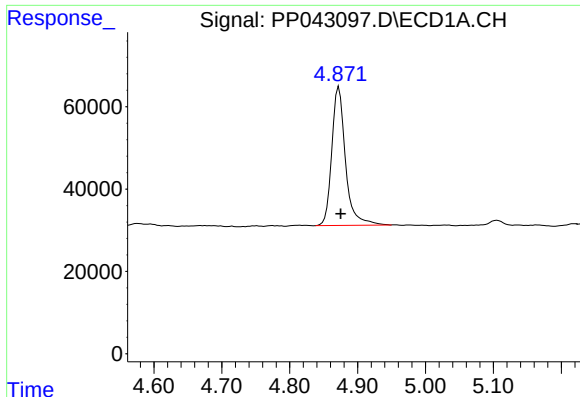


#1 Tetrachloro-m-xylene

R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 472295
Conc: 19.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

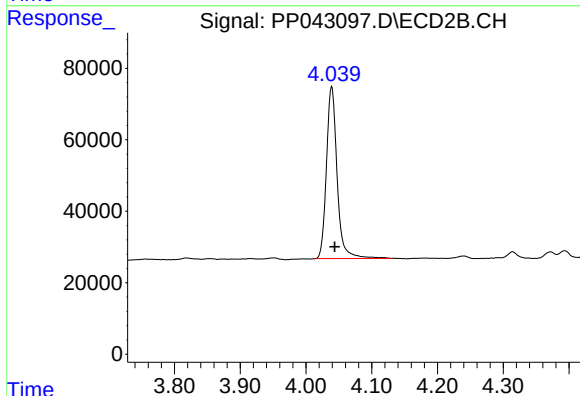


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: -0.005 min
Response: 542886
Conc: 21.74 ng/ml

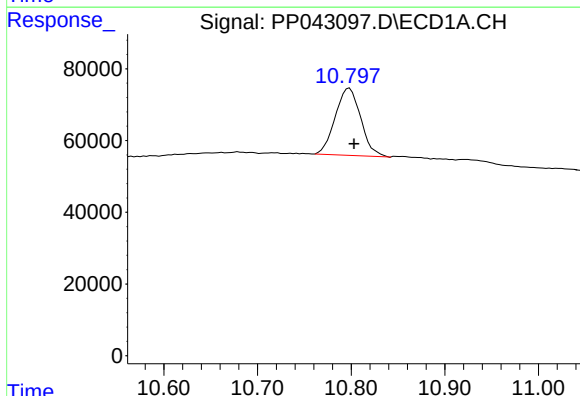


#2 Decachlorobiphenyl

R.T.: 10.798 min
Delta R.T.: -0.005 min
Response: 354680
Conc: 24.26 ng/ml

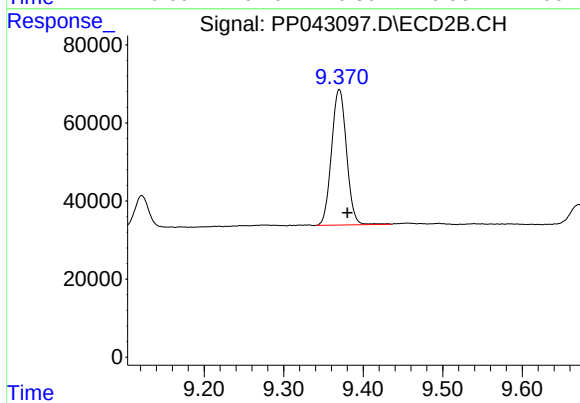

#2 Decachlorobiphenyl

R.T.: 9.370 min
Delta R.T.: -0.010 min
Response: 454673
Conc: 23.31 ng/ml

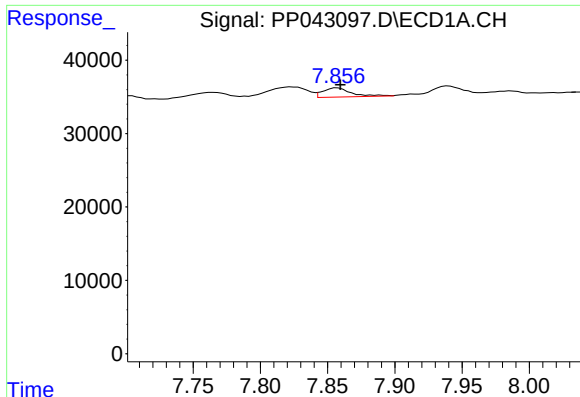


#31 AR-1260-1

R.T.: 7.857 min
Delta R.T.: -0.002 min
Response: 18453
Conc: 19.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

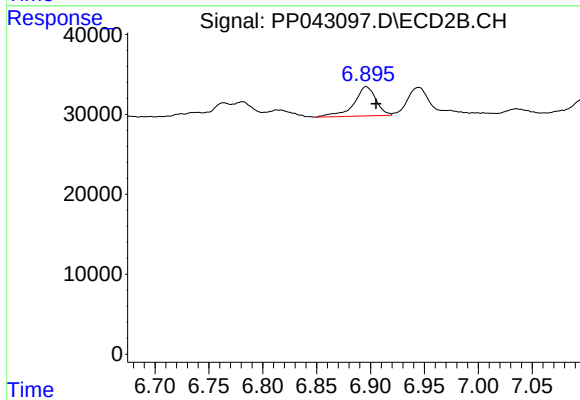


#31 AR-1260-1

R.T.: 6.896 min
Delta R.T.: -0.009 min
Response: 52380
Conc: 40.52 ng/ml

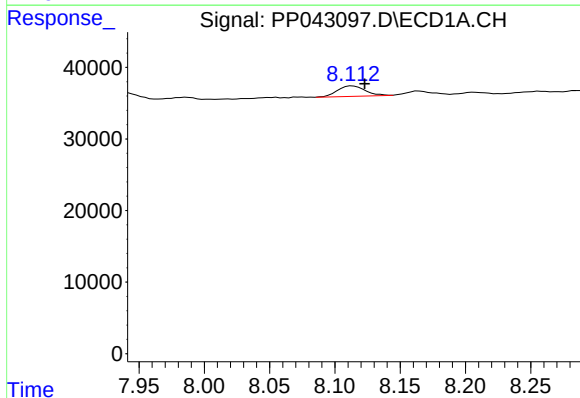


#32 AR-1260-2

R.T.: 8.112 min
Delta R.T.: -0.011 min
Response: 21746
Conc: 21.06 ng/ml m

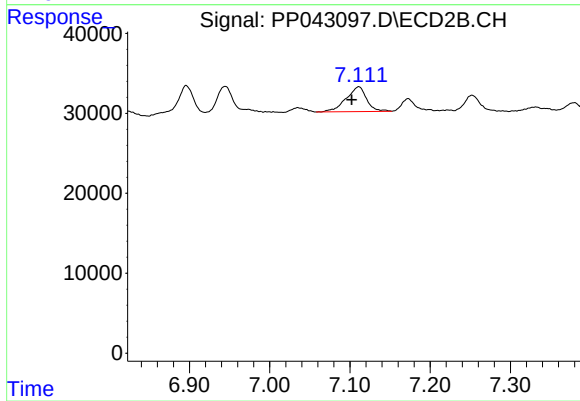

#32 AR-1260-2

R.T.: 7.111 min
Delta R.T.: 0.009 min
Response: 55135
Conc: 35.30 ng/ml

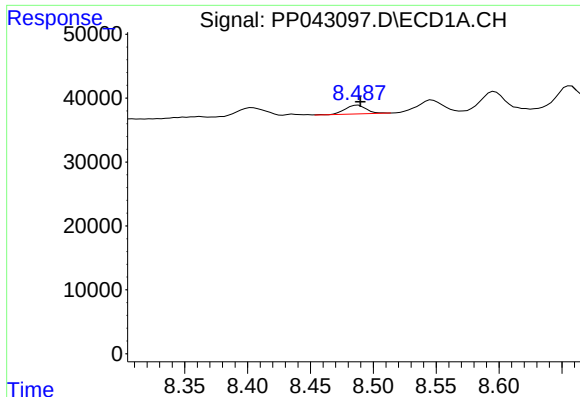


#33 AR-1260-3

R.T.: 8.488 min
Delta R.T.: -0.002 min
Response: 15766
Conc: 20.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

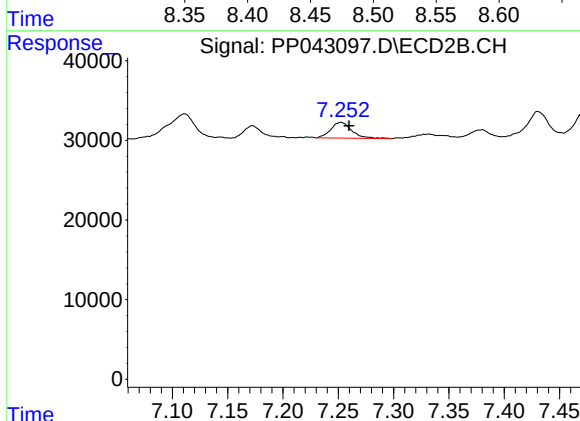


#33 AR-1260-3

R.T.: 7.252 min
Delta R.T.: -0.007 min
Response: 26050
Conc: 18.02 ng/ml

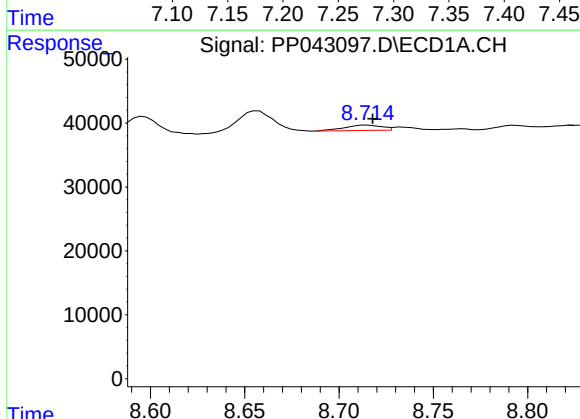


#34 AR-1260-4

R.T.: 8.714 min
Delta R.T.: -0.004 min
Response: 11064
Conc: 12.99 ng/ml m

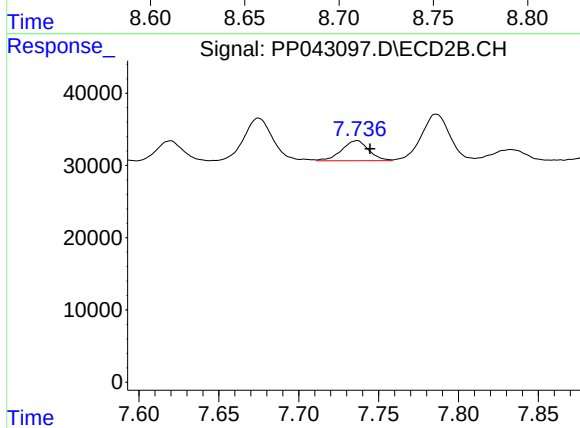

#34 AR-1260-4

R.T.: 7.736 min
Delta R.T.: -0.008 min
Response: 32889
Conc: 29.03 ng/ml

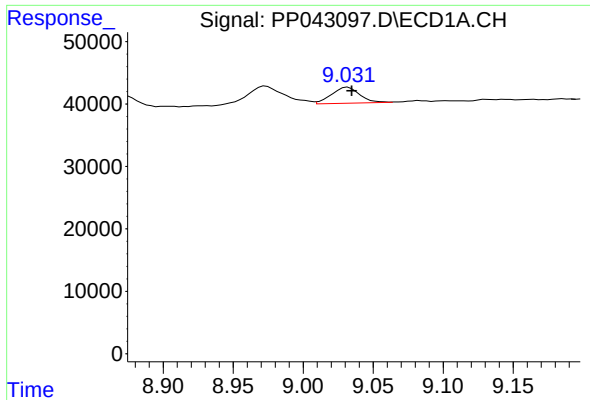


#35 AR-1260-5

R.T.: 9.032 min
Delta R.T.: -0.003 min
Response: 35748
Conc: 21.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2022
Supervised By :Ankita Jodhani 01/20/2022

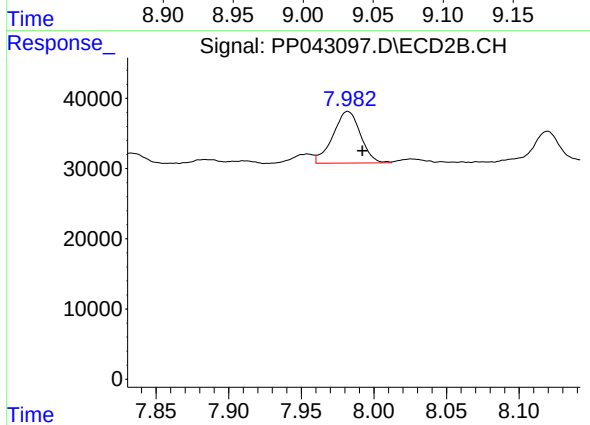

#35 AR-1260-5

R.T.: 7.982 min
Delta R.T.: -0.010 min
Response: 97324
Conc: 38.80 ng/ml