

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011923\
 Data File : PP054721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 15:16
 Operator : YP\AJ
 Sample : 01217-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BORING-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/20/2023
 Supervised By :Ankita Jodhani 01/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 20:53:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 18 04:34:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.578	39991025	34237637	21.780	21.389
2) SA Decachlor...	10.094	8.600	25166819	25051030	18.749	17.493
Target Compounds						
26) L6 AR-1254-1	6.362	5.469	2009449	2670292	28.430	31.407
27) L6 AR-1254-2	6.585	5.618	4104997	1268409	42.888	17.431 #
28) L6 AR-1254-3	6.951	6.023	3339944	2743916	38.496	24.245 #
29) L6 AR-1254-4	7.237	6.252	956909	1382519	15.274m	22.212 #
30) L6 AR-1254-5	7.659	6.672	1540830	1756993	22.018m	18.540

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011923\
Data File : PP054721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 15:16
Operator : YP\AJ
Sample : 01217-14
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BORING-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2023
Supervised By :Ankita Jodhani 01/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 20:53:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 18 04:34:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

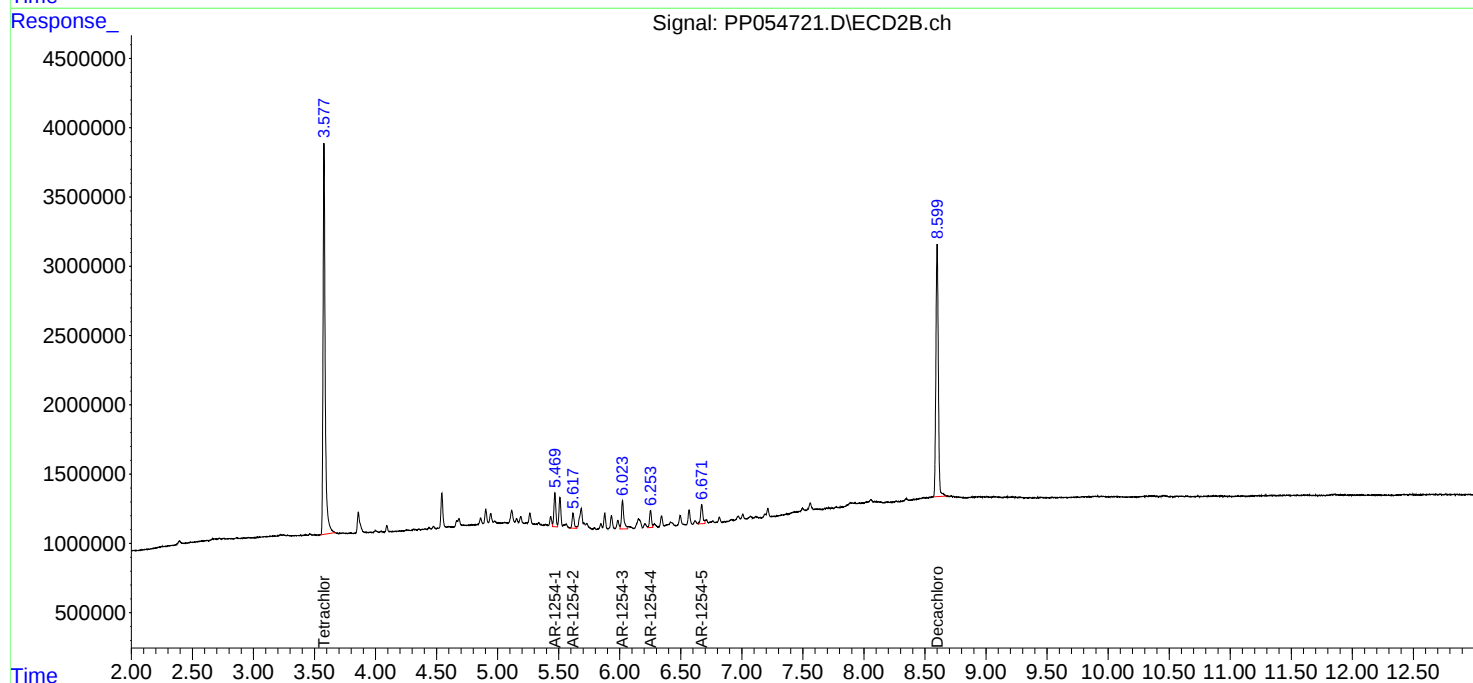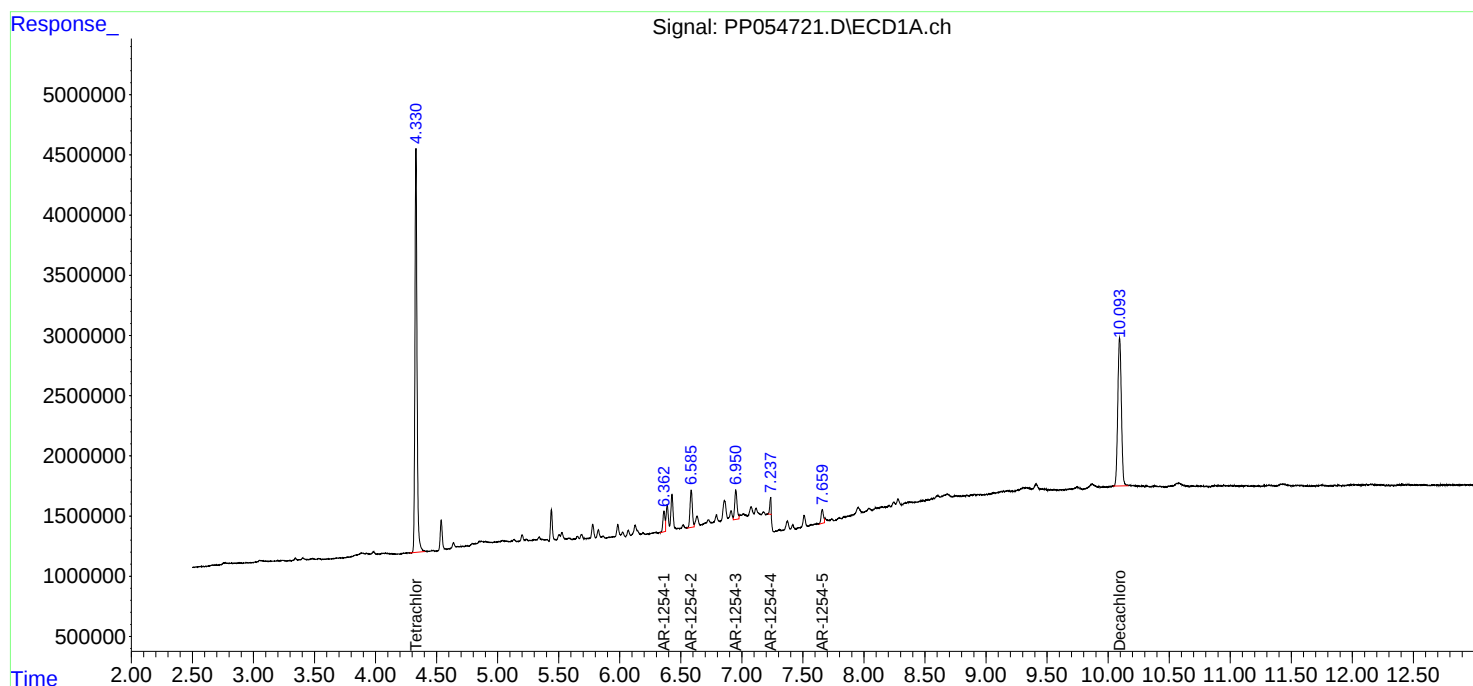

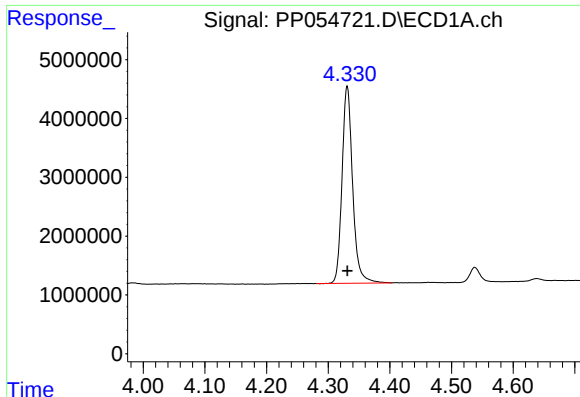


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: 0.000 min
Response: 39991025
Conc: 21.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
BORING-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2023
Supervised By :Ankita Jodhani 01/20/2023

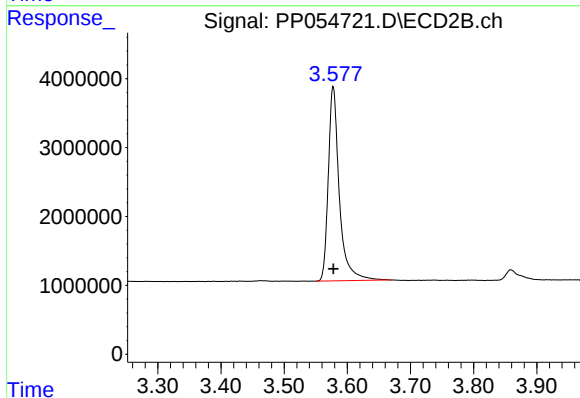


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: 0.000 min
Response: 34237637
Conc: 21.39 ng/ml

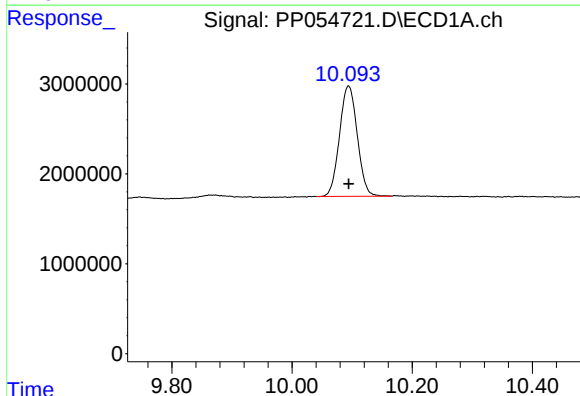


#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: 0.000 min
Response: 25166819
Conc: 18.75 ng/ml

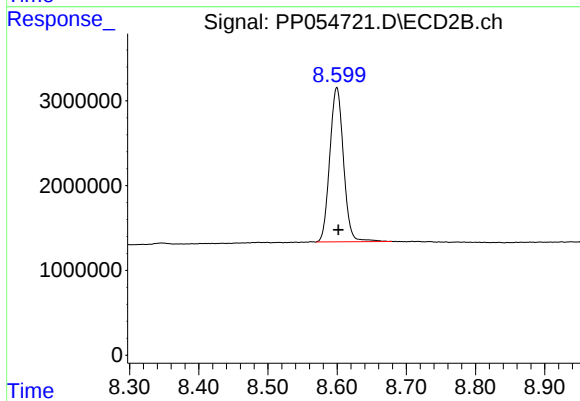

#2 Decachlorobiphenyl

R.T.: 8.600 min
Delta R.T.: -0.002 min
Response: 25051030
Conc: 17.49 ng/ml

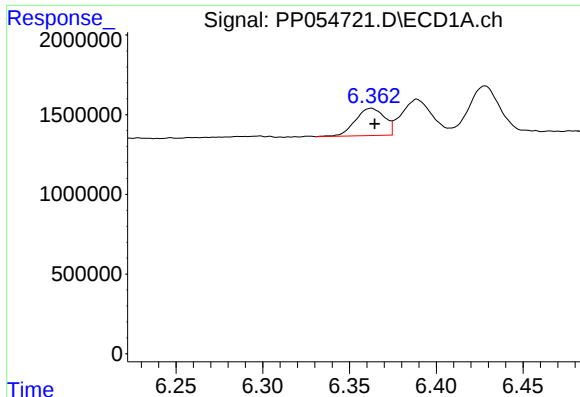


#26 AR-1254-1

R.T.: 6.362 min
Delta R.T.: -0.002 min
Response: 2009449
Conc: 28.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
BORING-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2023
Supervised By :Ankita Jodhani 01/20/2023

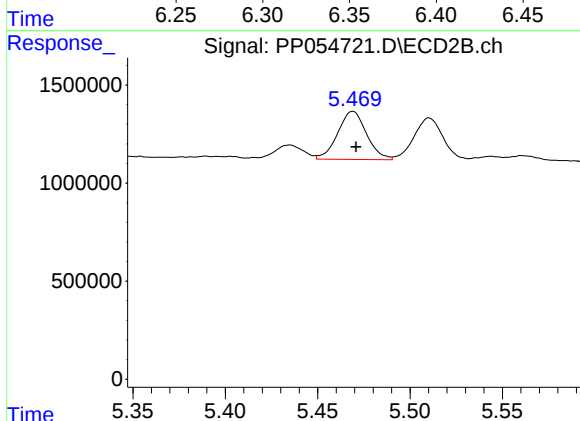


#26 AR-1254-1

R.T.: 5.469 min
Delta R.T.: -0.002 min
Response: 2670292
Conc: 31.41 ng/ml

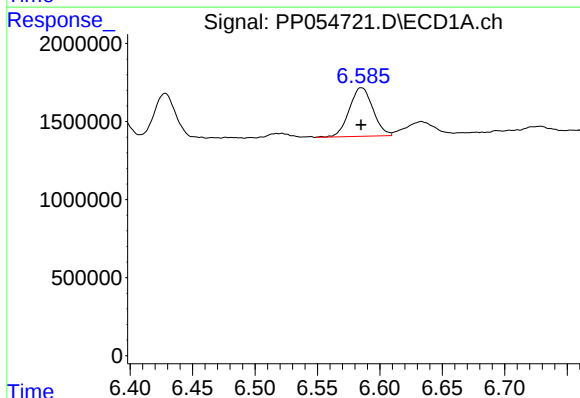


#27 AR-1254-2

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 4104997
Conc: 42.89 ng/ml

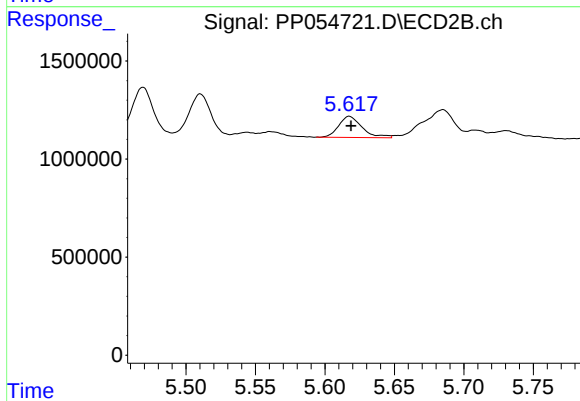

#27 AR-1254-2

R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 1268409
Conc: 17.43 ng/ml

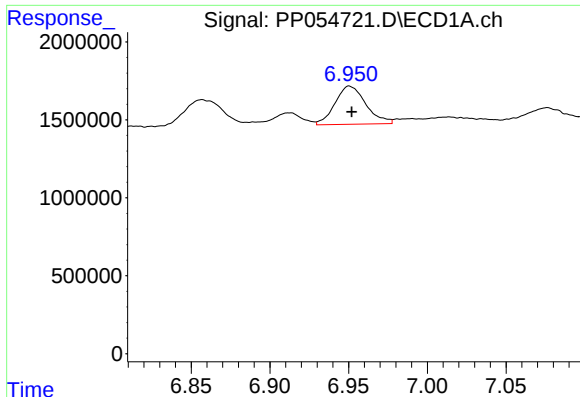


#28 AR-1254-3

R.T.: 6.951 min
Delta R.T.: -0.001 min
Response: 3339944
Conc: 38.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
BORING-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2023
Supervised By :Ankita Jodhani 01/20/2023

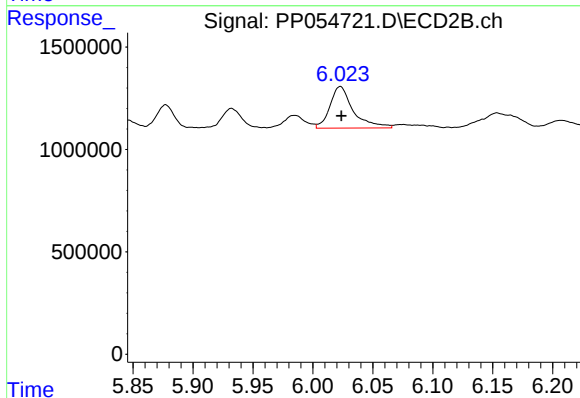


#28 AR-1254-3

R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 2743916
Conc: 24.24 ng/ml

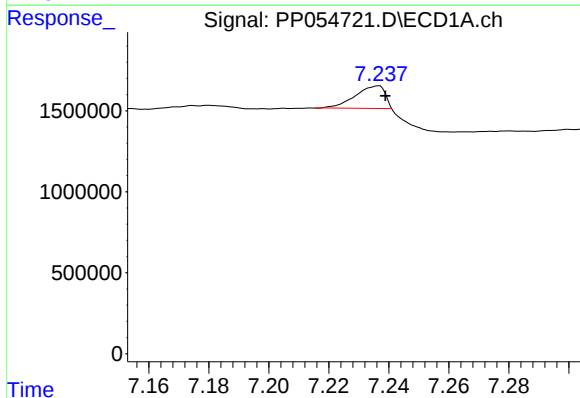


#29 AR-1254-4

R.T.: 7.237 min
Delta R.T.: -0.002 min
Response: 956909
Conc: 15.27 ng/ml m

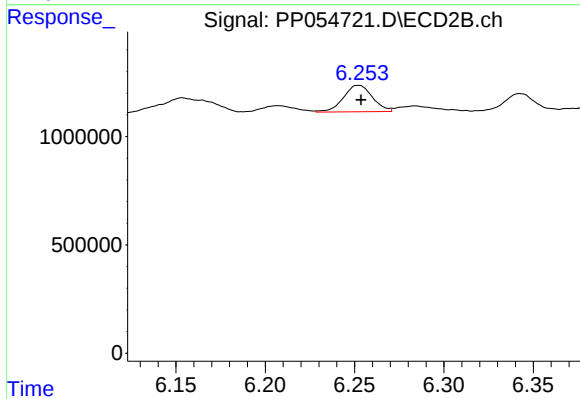

#29 AR-1254-4

R.T.: 6.252 min
Delta R.T.: -0.001 min
Response: 1382519
Conc: 22.21 ng/ml

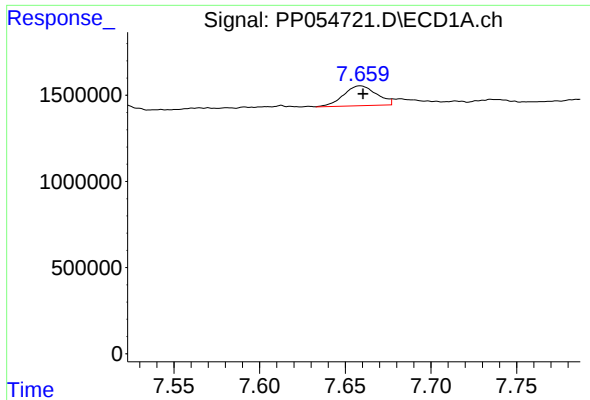


#30 AR-1254-5

R.T.: 7.659 min
Delta R.T.: -0.002 min
Response: 1540830
Conc: 22.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
BORING-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2023
Supervised By :Ankita Jodhani 01/20/2023

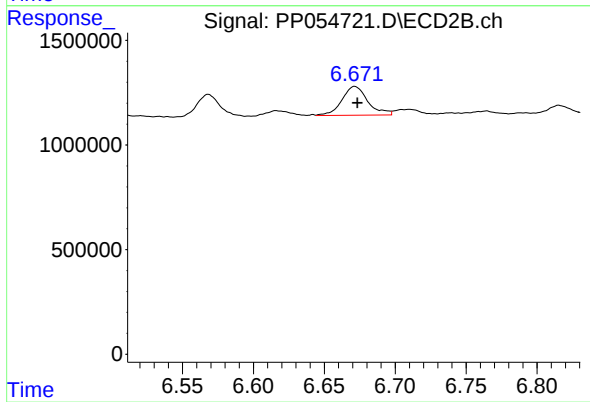

#30 AR-1254-5

R.T.: 6.672 min
Delta R.T.: -0.002 min
Response: 1756993
Conc: 18.54 ng/ml