

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP012020\  
Data File : PP030601.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 20 Jan 2020 8:40  
Operator : DD\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 20 14:31:05 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP011720.M  
Quant Title : 8080.M  
QLast Update : Sat Jan 18 00:30:15 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP012020\  
Data File : PP030601.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 20 Jan 2020 8:40  
Operator : DD\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 20 14:31:05 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP011720.M  
Quant Title : 8080.M  
QLast Update : Sat Jan 18 00:30:15 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

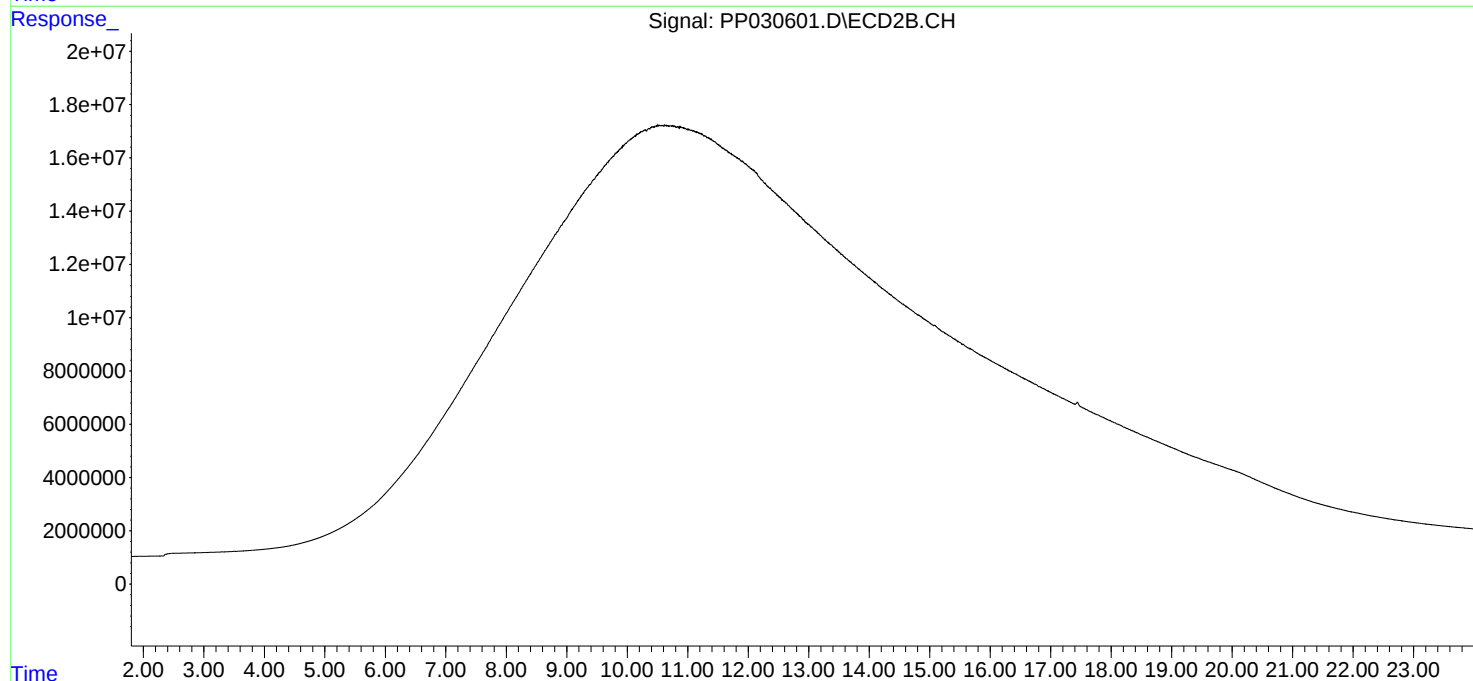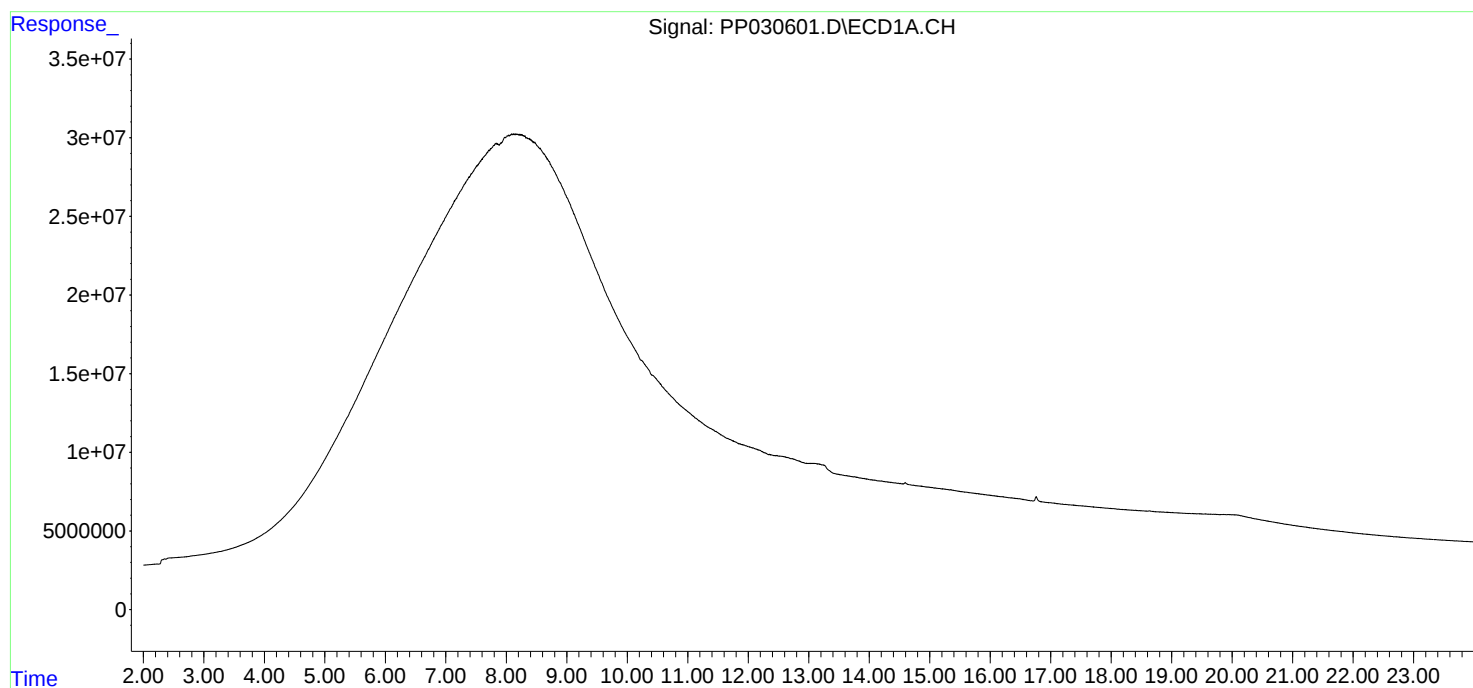


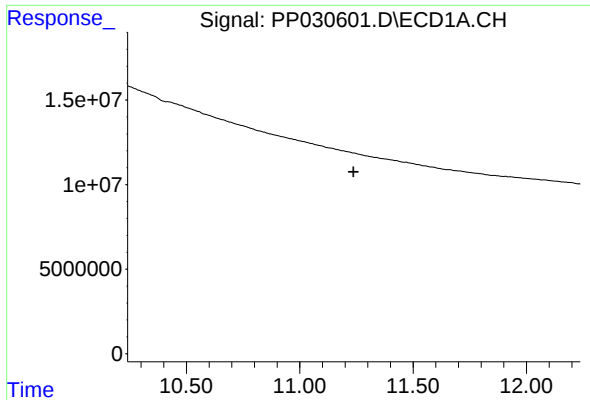

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 11.237 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
HEXANE

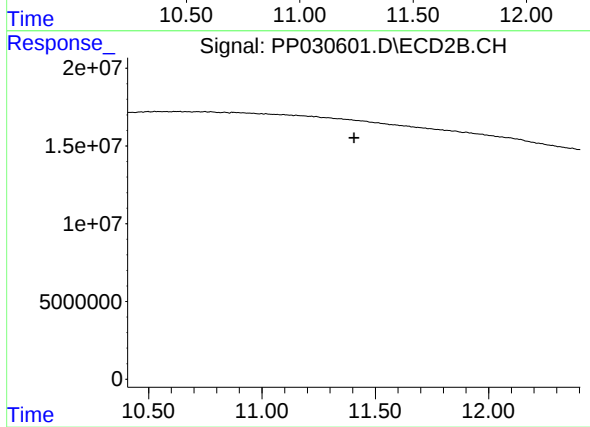

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 11.406 min  
Response: 0  
Conc: N.D.