

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
 Data File : PP043132.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 10:09
 Operator : AJ\MA
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2022
 Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:17:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.039	1192608	1307573	50.403	52.353
2) SA Decachlor...	10.795	9.368	875536	1064156	59.892	54.554
Target Compounds						
26) L6 AR-1254-1	7.080	6.178	356356	781286	454.148	503.825m
27) L6 AR-1254-2	7.308	6.336	591356	715619	469.856	527.138m
28) L6 AR-1254-3	7.686	6.761	653881	1111536	503.993	519.667
29) L6 AR-1254-4	7.980	7.001	472387	666922	540.470	534.566
30) L6 AR-1254-5	8.408	7.431	490568	878601	523.599	515.257

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
Data File : PP043132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 10:09
Operator : AJ\MA
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:17:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

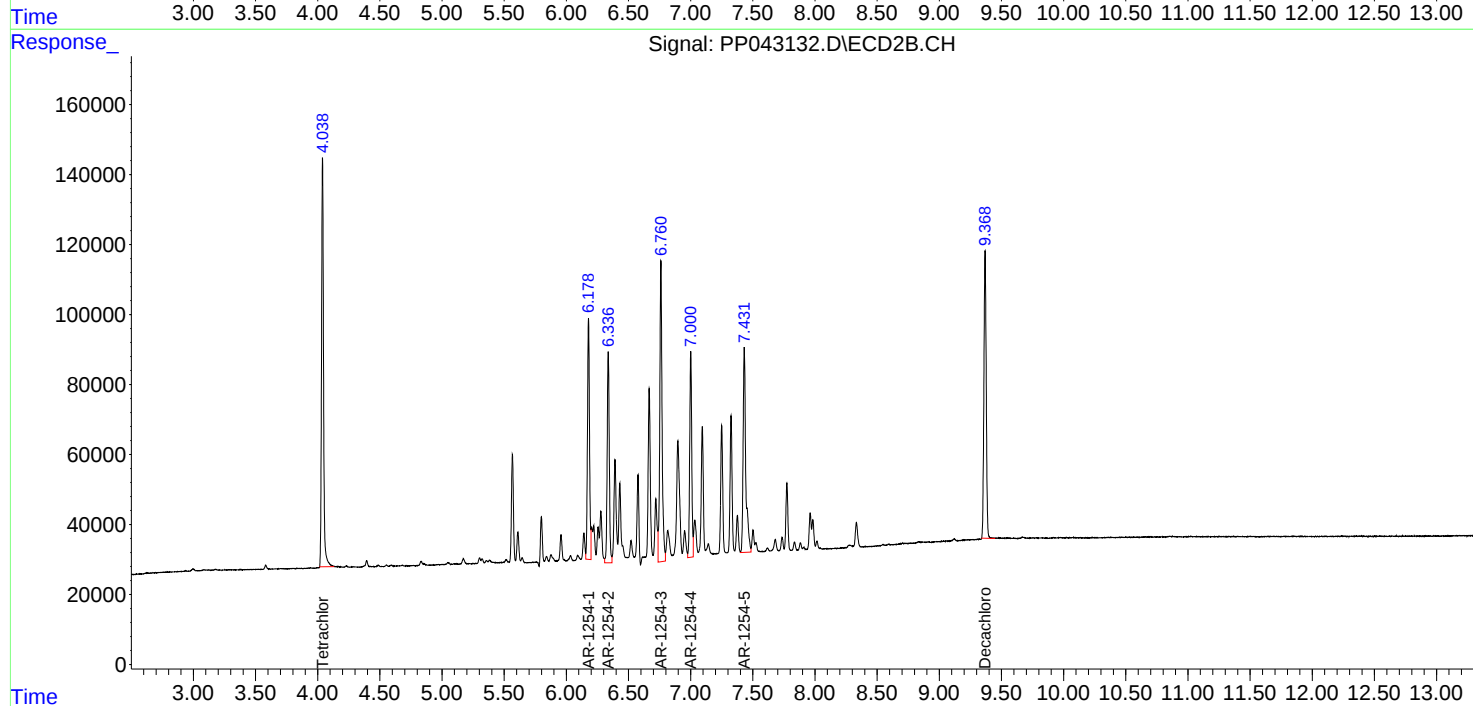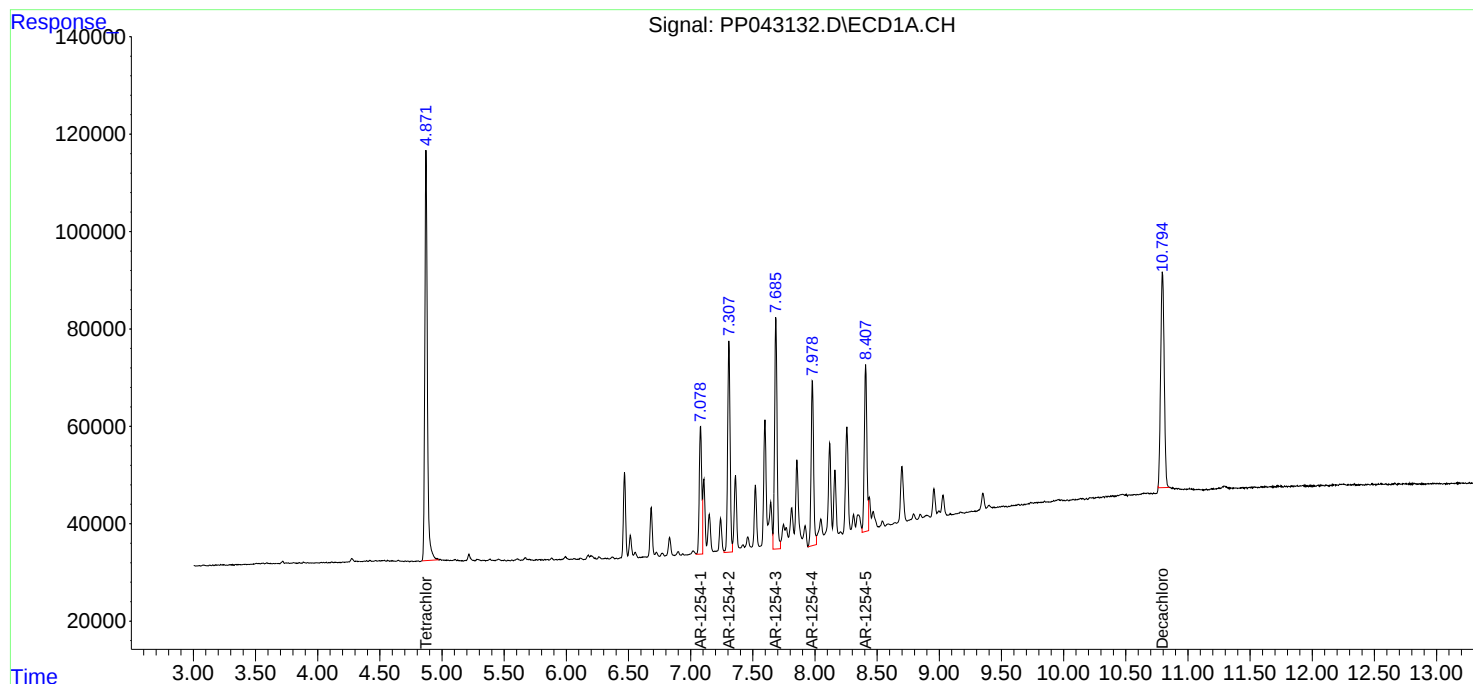

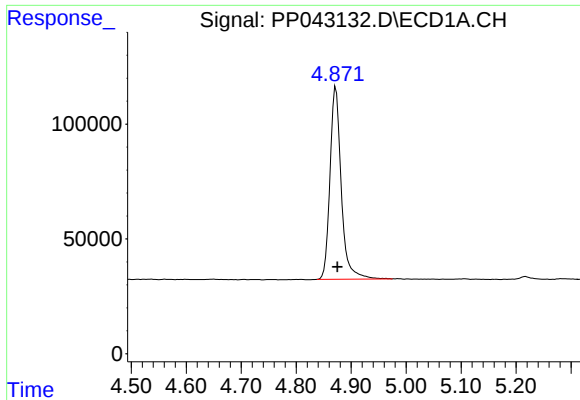


#1 Tetrachloro-m-xylene

R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 1192608
Conc: 50.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

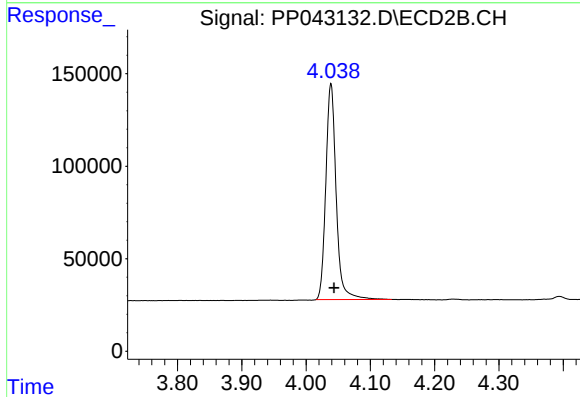


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: -0.005 min
Response: 1307573
Conc: 52.35 ng/ml

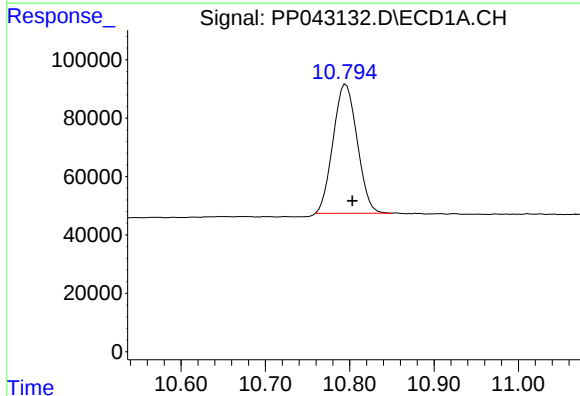


#2 Decachlorobiphenyl

R.T.: 10.795 min
Delta R.T.: -0.008 min
Response: 875536
Conc: 59.89 ng/ml

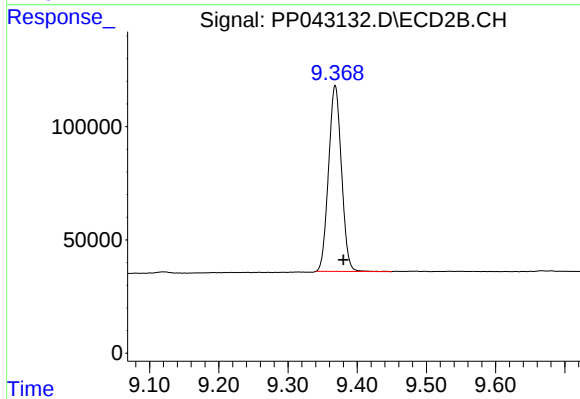

#2 Decachlorobiphenyl

R.T.: 9.368 min
Delta R.T.: -0.012 min
Response: 1064156
Conc: 54.55 ng/ml

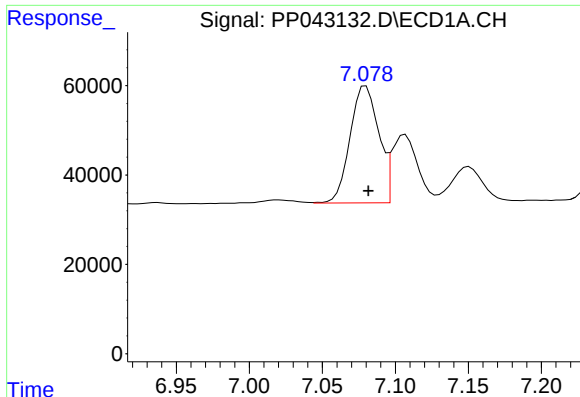


#26 AR-1254-1

R.T.: 7.080 min
Delta R.T.: -0.002 min
Response: 356356
Conc: 454.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

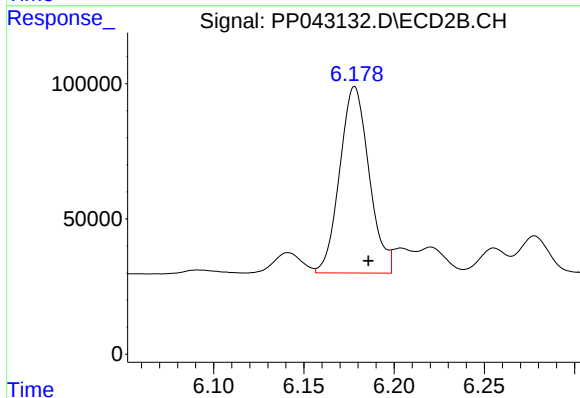


#26 AR-1254-1

R.T.: 6.178 min
Delta R.T.: -0.008 min
Response: 781286
Conc: 503.83 ng/ml m

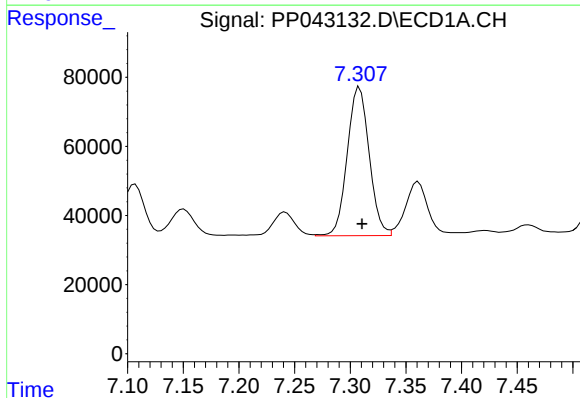


#27 AR-1254-2

R.T.: 7.308 min
Delta R.T.: -0.002 min
Response: 591356
Conc: 469.86 ng/ml

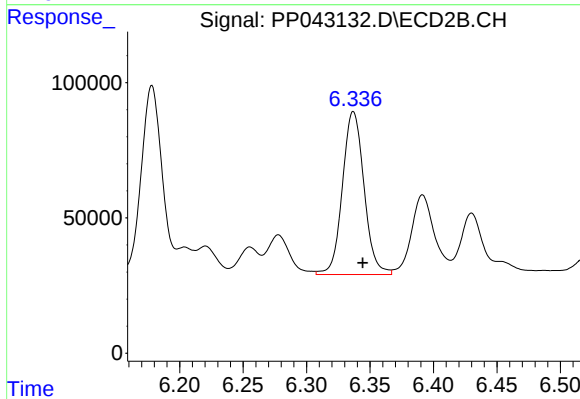

#27 AR-1254-2

R.T.: 6.336 min
Delta R.T.: -0.008 min
Response: 715619
Conc: 527.14 ng/ml m

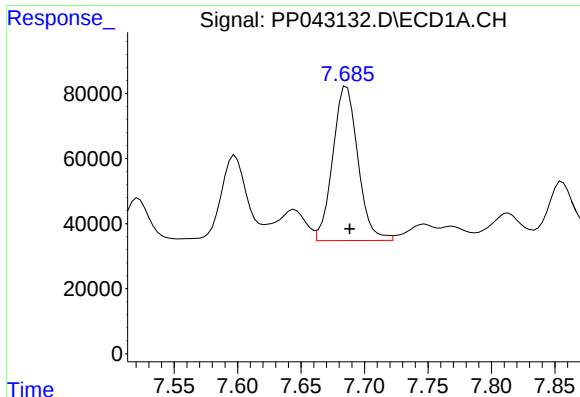


#28 AR-1254-3

R.T.: 7.686 min
Delta R.T.: -0.002 min
Response: 653881
Conc: 503.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

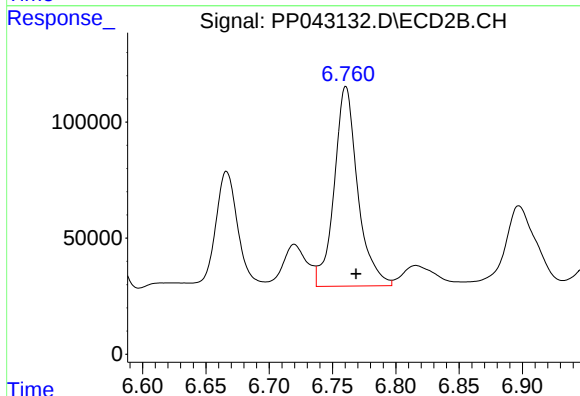


#28 AR-1254-3

R.T.: 6.761 min
Delta R.T.: -0.008 min
Response: 1111536
Conc: 519.67 ng/ml

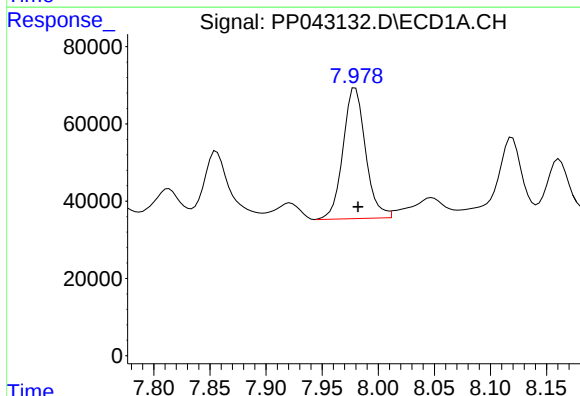


#29 AR-1254-4

R.T.: 7.980 min
Delta R.T.: -0.002 min
Response: 472387
Conc: 540.47 ng/ml

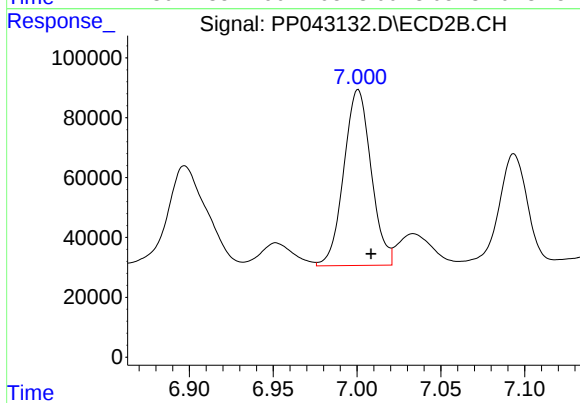

#29 AR-1254-4

R.T.: 7.001 min
Delta R.T.: -0.008 min
Response: 666922
Conc: 534.57 ng/ml

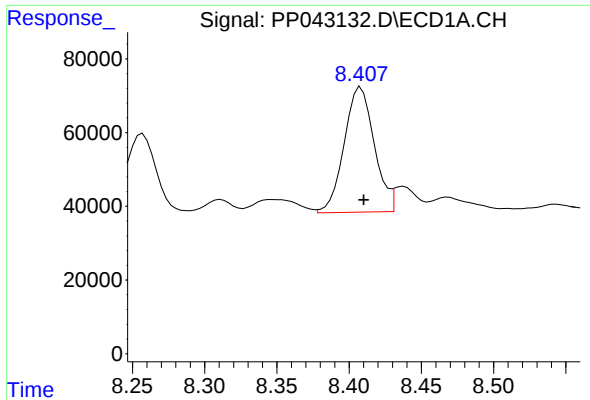


#30 AR-1254-5

R.T.: 8.408 min
Delta R.T.: -0.002 min
Response: 490568
Conc: 523.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

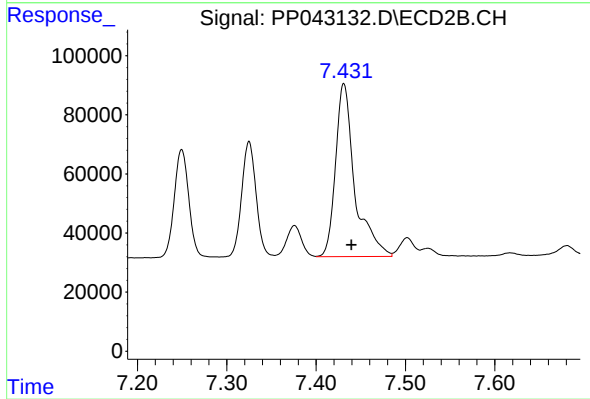

#30 AR-1254-5

R.T.: 7.431 min
Delta R.T.: -0.009 min
Response: 878601
Conc: 515.26 ng/ml