

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
 Data File : PP043135.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 11:21
 Operator : AJ\MA
 Sample : N1186-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:18:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.039	344664	405506	14.567	16.236
2) SA Decachlor...	10.800	9.374	396015	390420	27.090	20.015 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
Data File : PP043135.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 11:21
Operator : AJ\MA
Sample : N1186-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:18:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

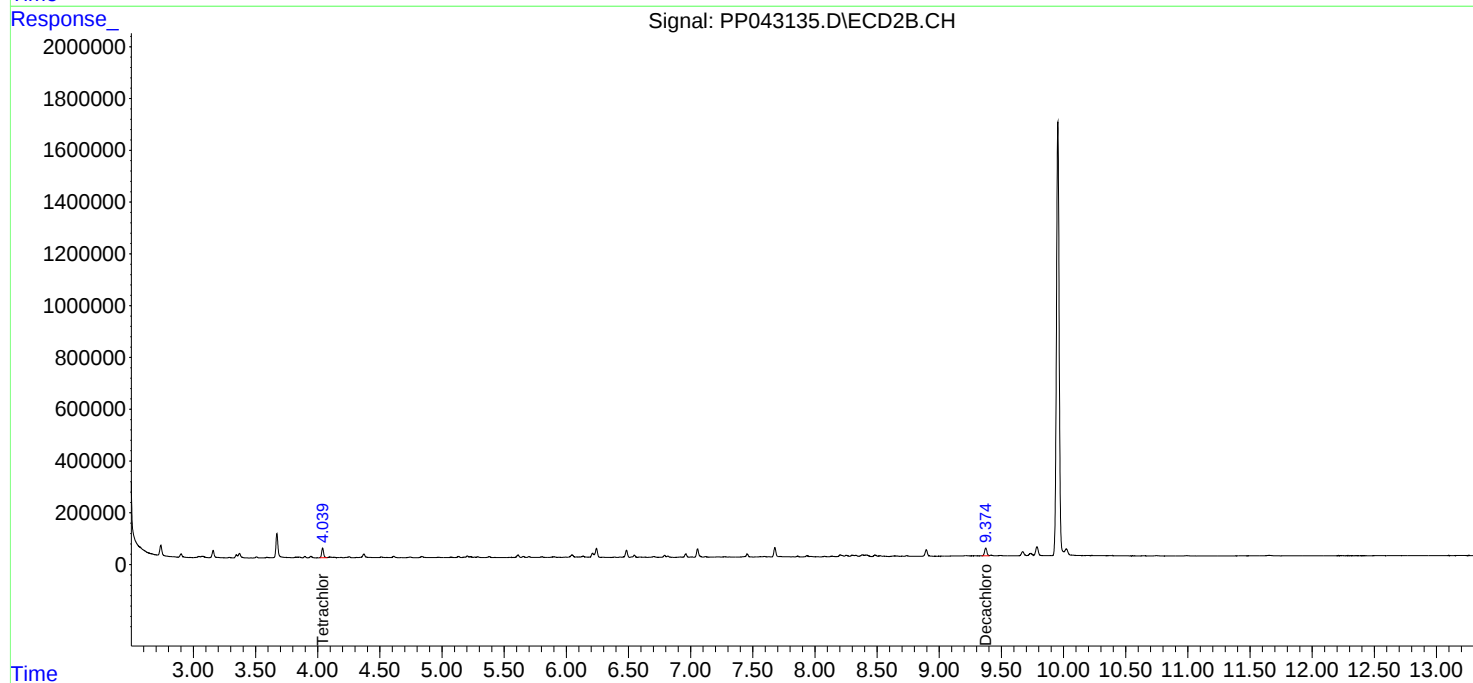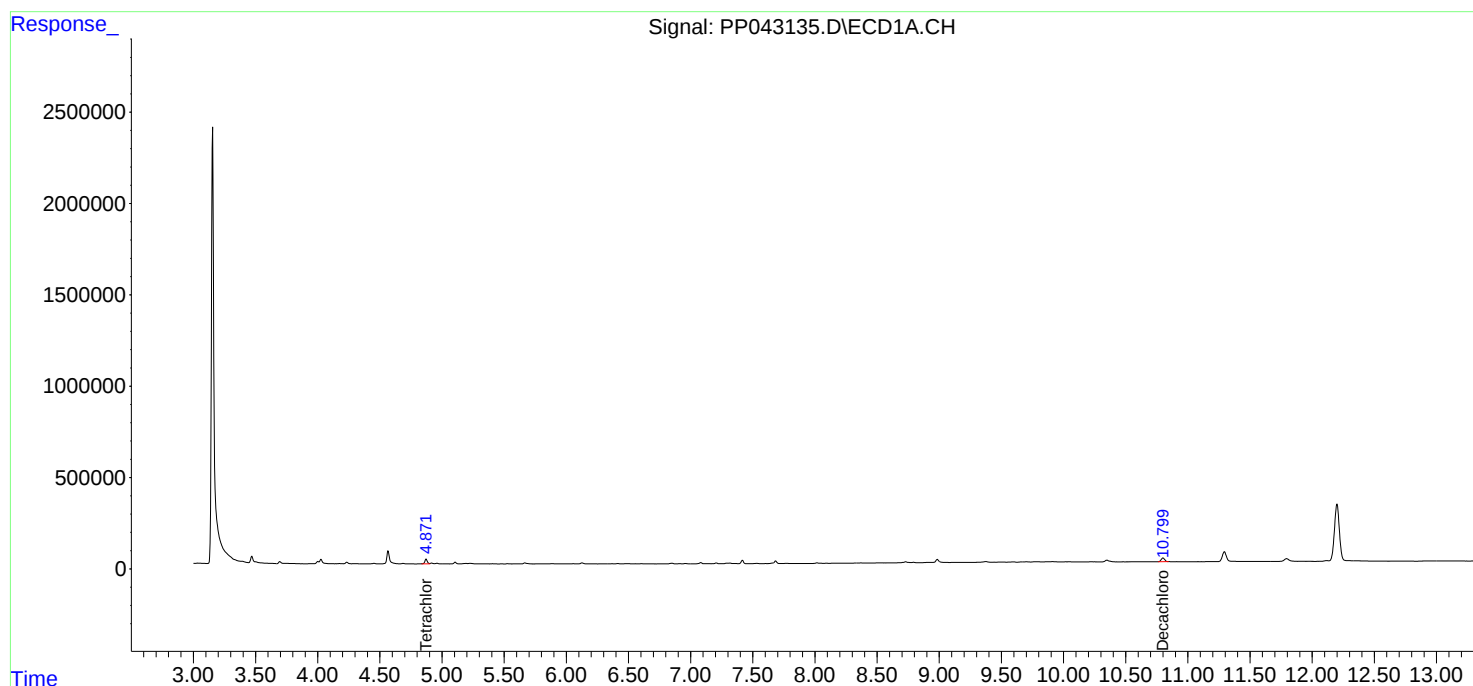


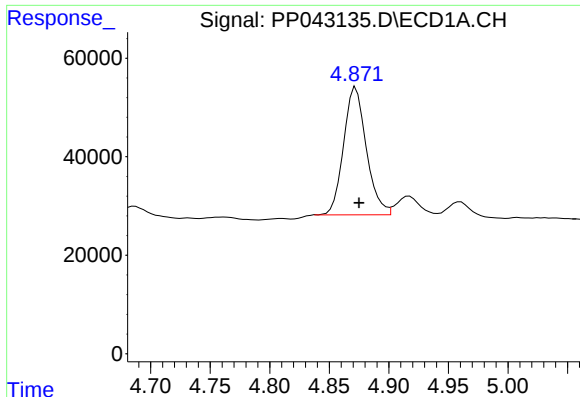

#1 Tetrachloro-m-xylene


R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 344664
Conc: 14.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-1

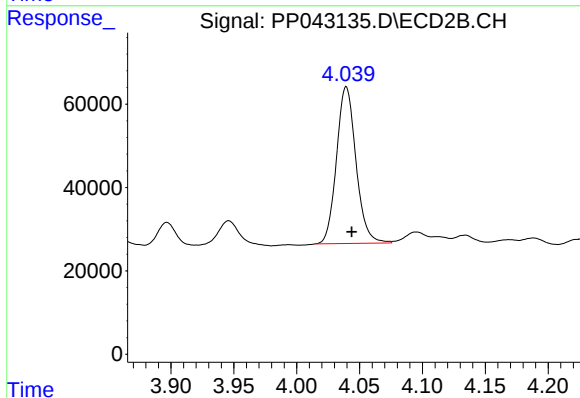


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: -0.004 min
Response: 405506
Conc: 16.24 ng/ml

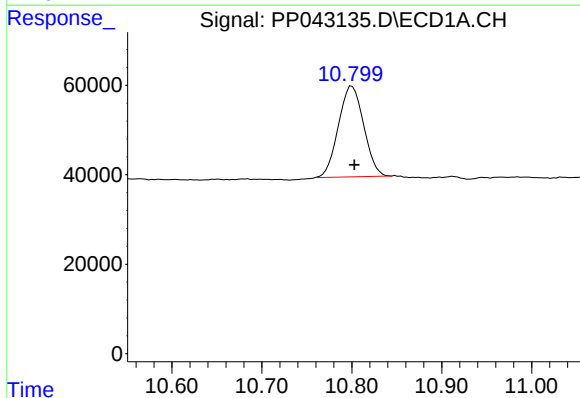

#2 Decachlorobiphenyl

R.T.: 10.800 min
Delta R.T.: -0.003 min
Response: 396015
Conc: 27.09 ng/ml

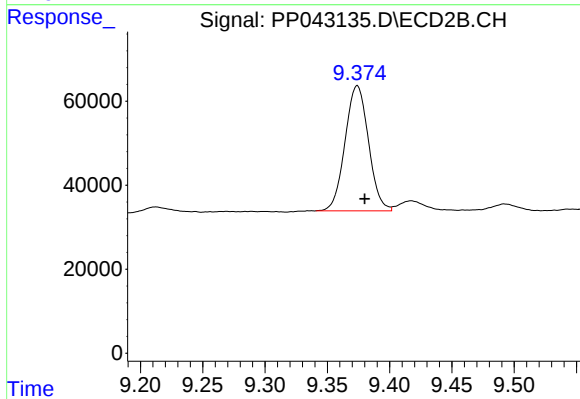

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: -0.006 min
Response: 390420
Conc: 20.01 ng/ml