

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
 Data File : PP043143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 13:33
 Operator : AJ\MA
 Sample : N1195-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CL-02-011922

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2022
 Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:22:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.871	4.038	448911	510037	18.972	20.421
2) SA Decachlor...	10.792	9.366	340773	383955	23.311	19.683
Target Compounds						
26) L6 AR-1254-1	7.087	6.179	46791	62195	59.632	40.108m#
27) L6 AR-1254-2	7.310	6.335	43608	36601	34.648	26.961
28) L6 AR-1254-3	7.686	6.759	36680	69275	28.272	32.388
29) L6 AR-1254-4	7.977	6.999	18592	36013	21.272m	28.866 #
30) L6 AR-1254-5	8.407	7.429	31330	62362	33.439	36.572m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
Data File : PP043143.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 13:33
Operator : AJ\MA
Sample : N1195-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CL-02-011922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:22:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

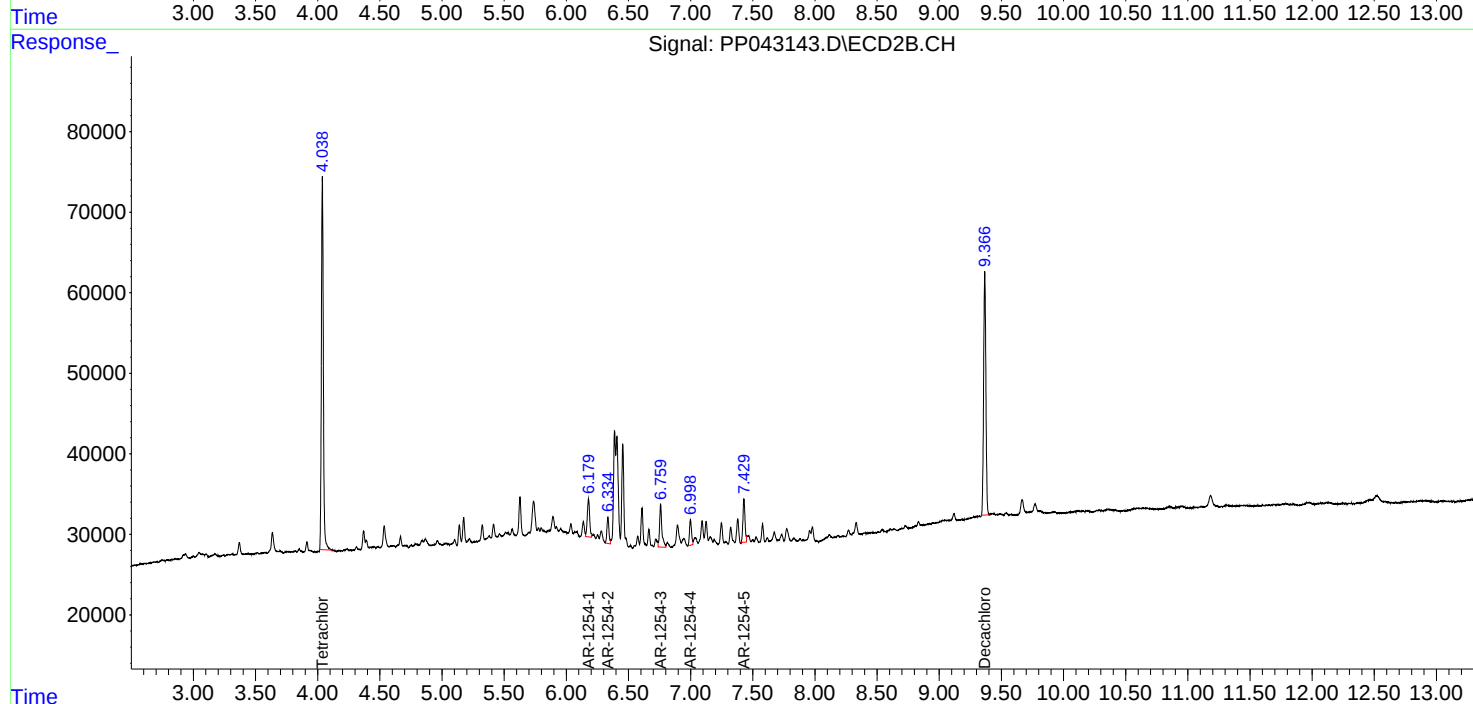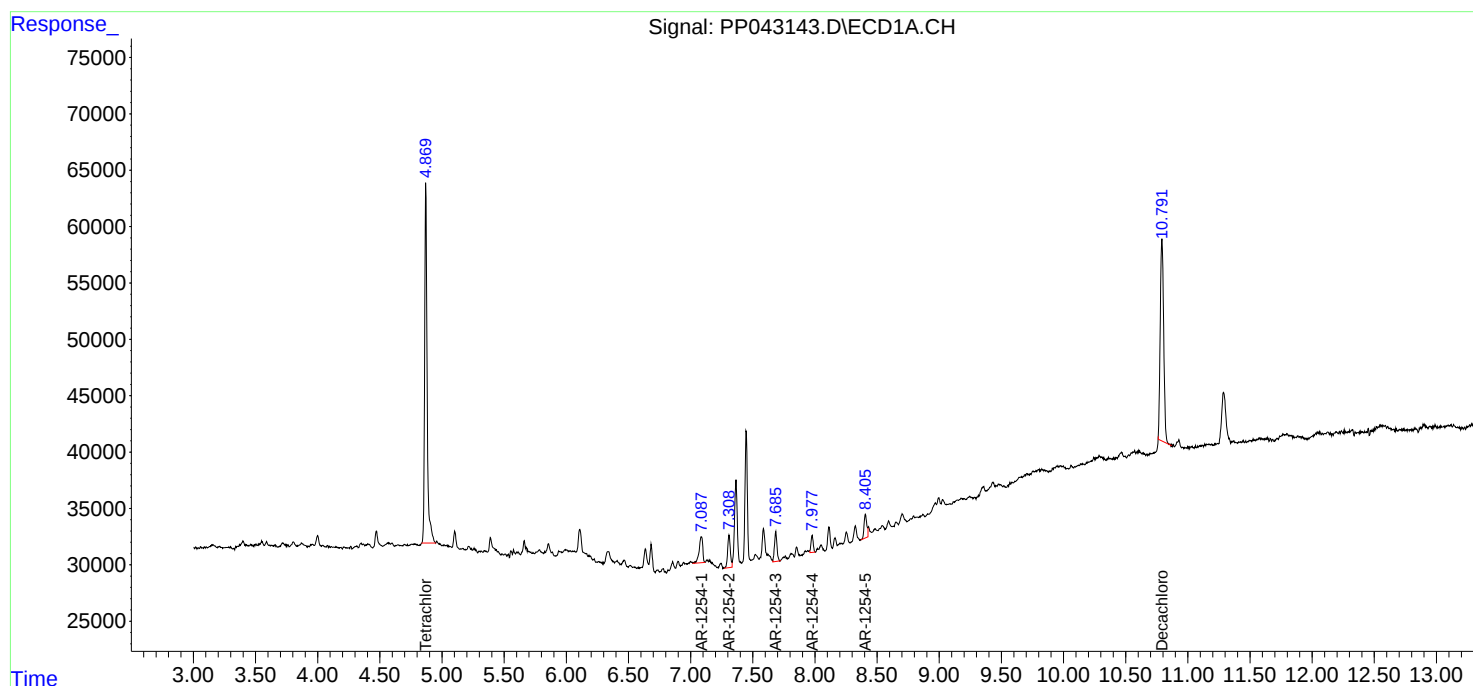

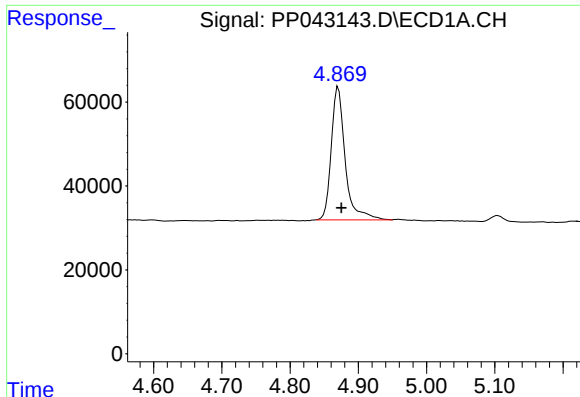


#1 Tetrachloro-m-xylene

R.T.: 4.871 min
Delta R.T.: -0.004 min
Response: 448911
Conc: 18.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-02-011922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

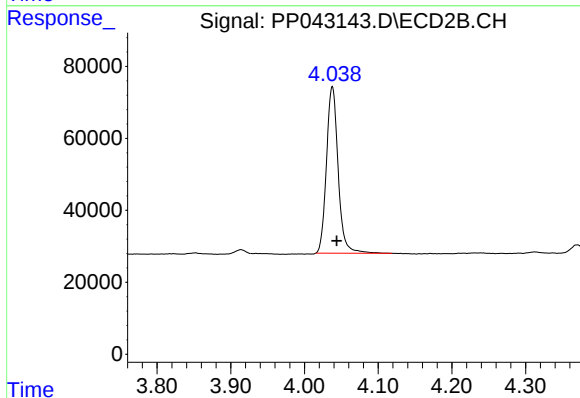


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.006 min
Response: 510037
Conc: 20.42 ng/ml

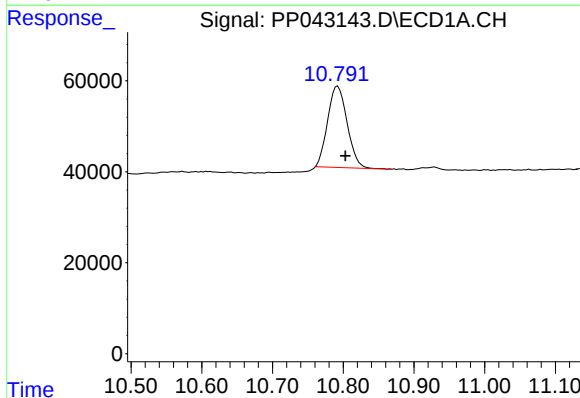


#2 Decachlorobiphenyl

R.T.: 10.792 min
Delta R.T.: -0.011 min
Response: 340773
Conc: 23.31 ng/ml

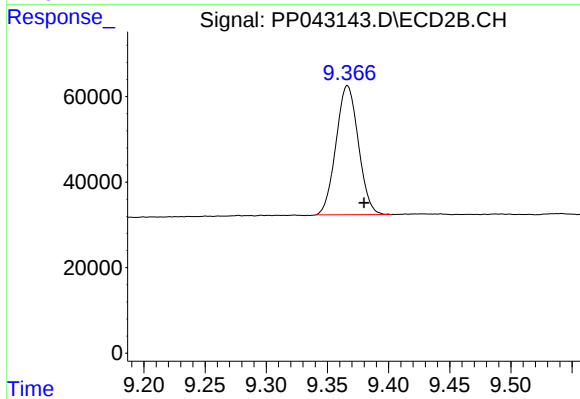

#2 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.014 min
Response: 383955
Conc: 19.68 ng/ml

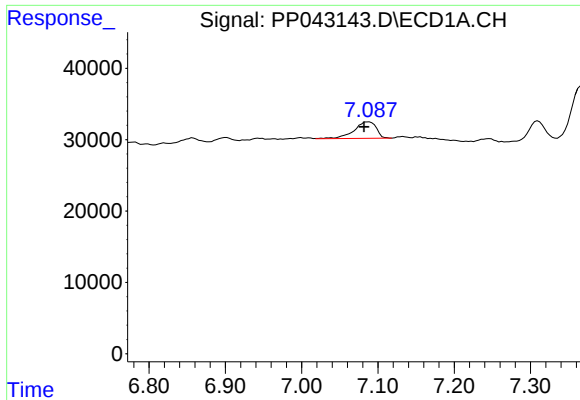


#26 AR-1254-1

R.T.: 7.087 min
Delta R.T.: 0.006 min
Response: 46791
Conc: 59.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-02-011922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

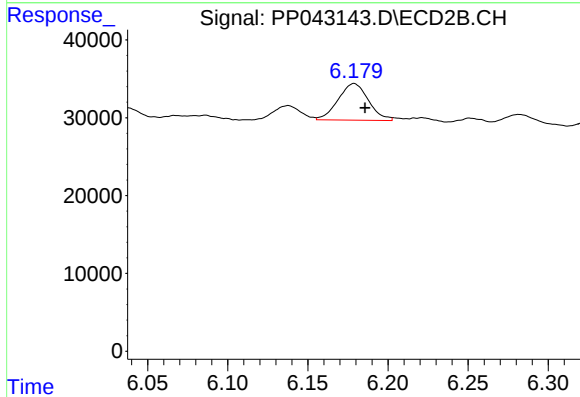


#26 AR-1254-1

R.T.: 6.179 min
Delta R.T.: -0.007 min
Response: 62195
Conc: 40.11 ng/ml m

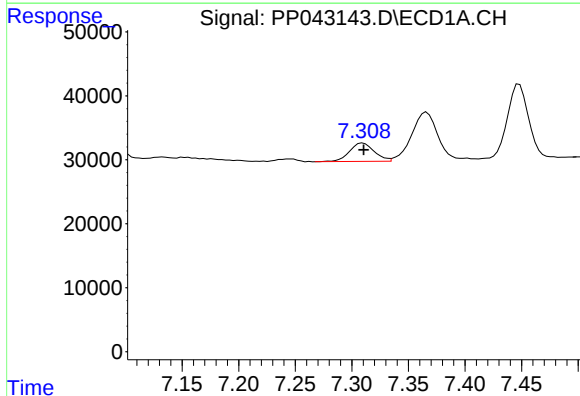


#27 AR-1254-2

R.T.: 7.310 min
Delta R.T.: 0.000 min
Response: 43608
Conc: 34.65 ng/ml

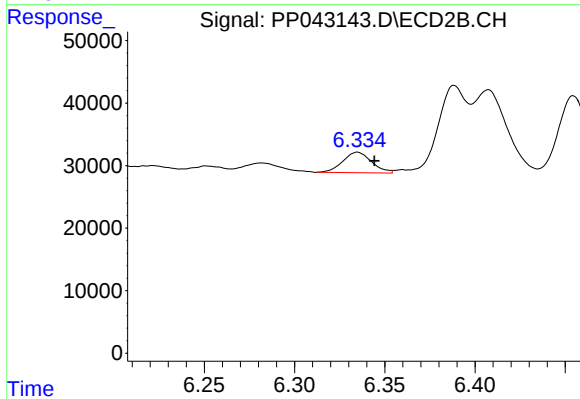

#27 AR-1254-2

R.T.: 6.335 min
Delta R.T.: -0.009 min
Response: 36601
Conc: 26.96 ng/ml

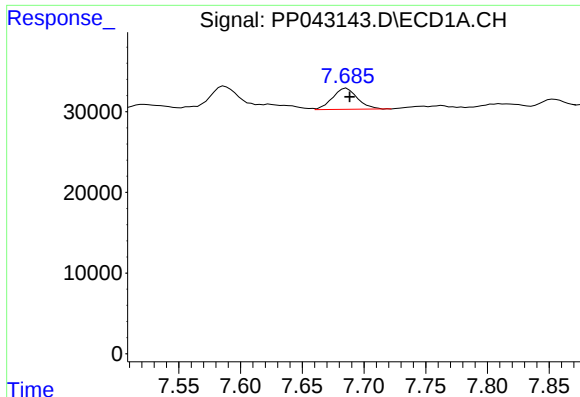


#28 AR-1254-3

R.T.: 7.686 min
Delta R.T.: -0.003 min
Response: 36680
Conc: 28.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-02-011922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

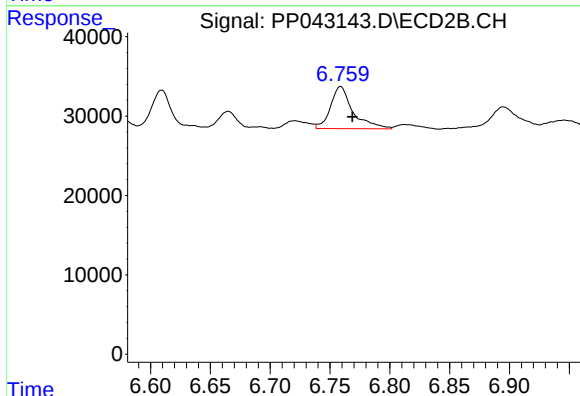


#28 AR-1254-3

R.T.: 6.759 min
Delta R.T.: -0.010 min
Response: 69275
Conc: 32.39 ng/ml

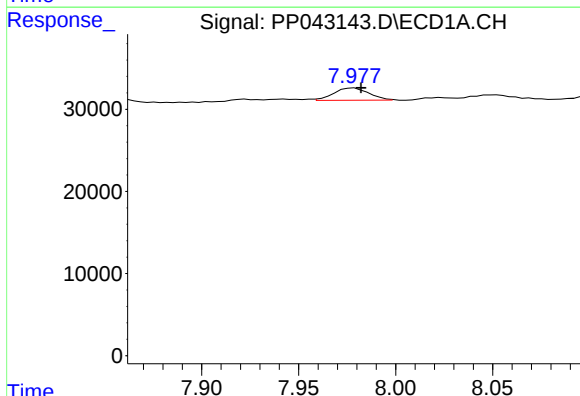


#29 AR-1254-4

R.T.: 7.977 min
Delta R.T.: -0.005 min
Response: 18592
Conc: 21.27 ng/ml m

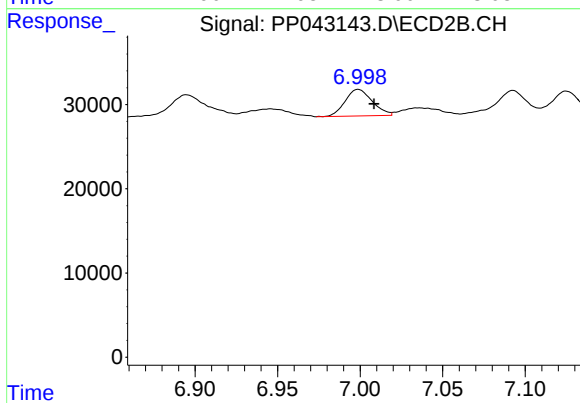

#29 AR-1254-4

R.T.: 6.999 min
Delta R.T.: -0.010 min
Response: 36013
Conc: 28.87 ng/ml

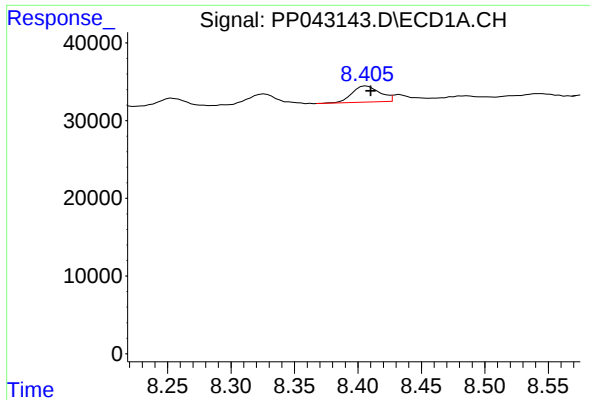


#30 AR-1254-5

R.T.: 8.407 min
Delta R.T.: -0.003 min
Response: 31330
Conc: 33.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-02-011922

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

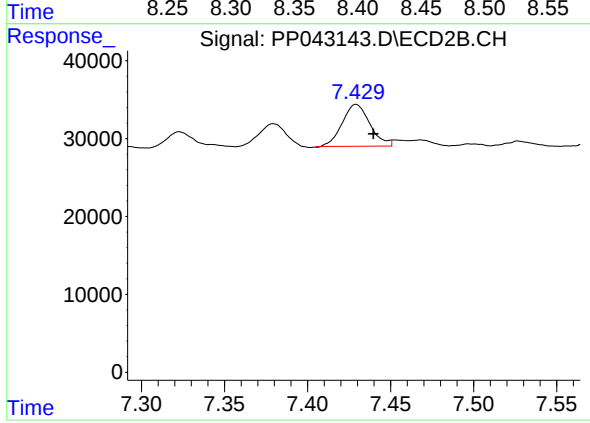

#30 AR-1254-5

R.T.: 7.429 min
Delta R.T.: -0.011 min
Response: 62362
Conc: 36.57 ng/ml m