

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
 Data File : PP043151.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 16:31
 Operator : AJ\MA
 Sample : N1076-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2022
 Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 08:45:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.871	4.038	495519	548384	20.942	21.956
2) SA Decachlor...	10.793	9.366	464609	482607	31.782	24.741
Target Compounds						
26) L6 AR-1254-1	7.080	6.178	25344	49629	32.299	32.004
27) L6 AR-1254-2	7.307	6.336	30280	33069	24.059	24.359
28) L6 AR-1254-3	7.686	6.759	60593	94954	46.703	44.393m
29) L6 AR-1254-4	7.978	6.999	20142	26924	23.045	21.581
30) L6 AR-1254-5	8.404	7.430	76508	127244	81.660m	74.623

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
Data File : PP043151.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 16:31
Operator : AJ\MA
Sample : N1076-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 08:45:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

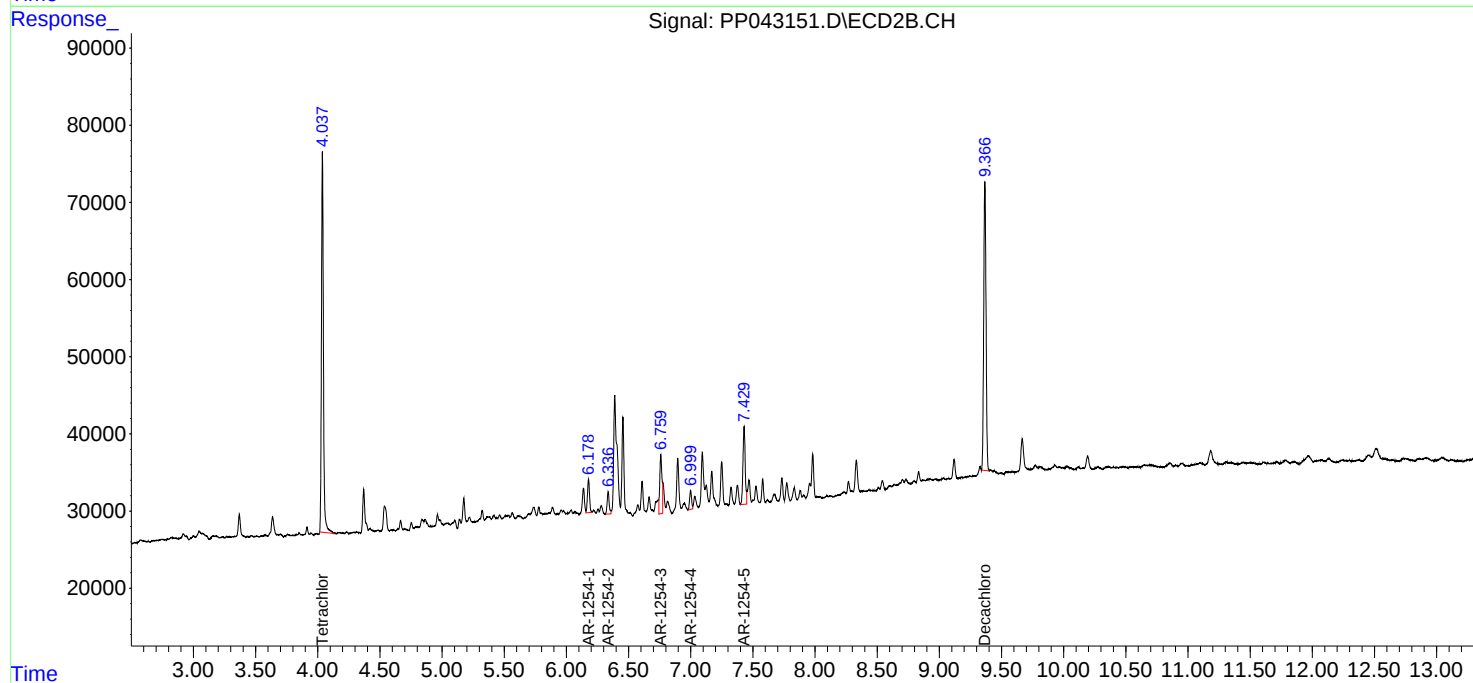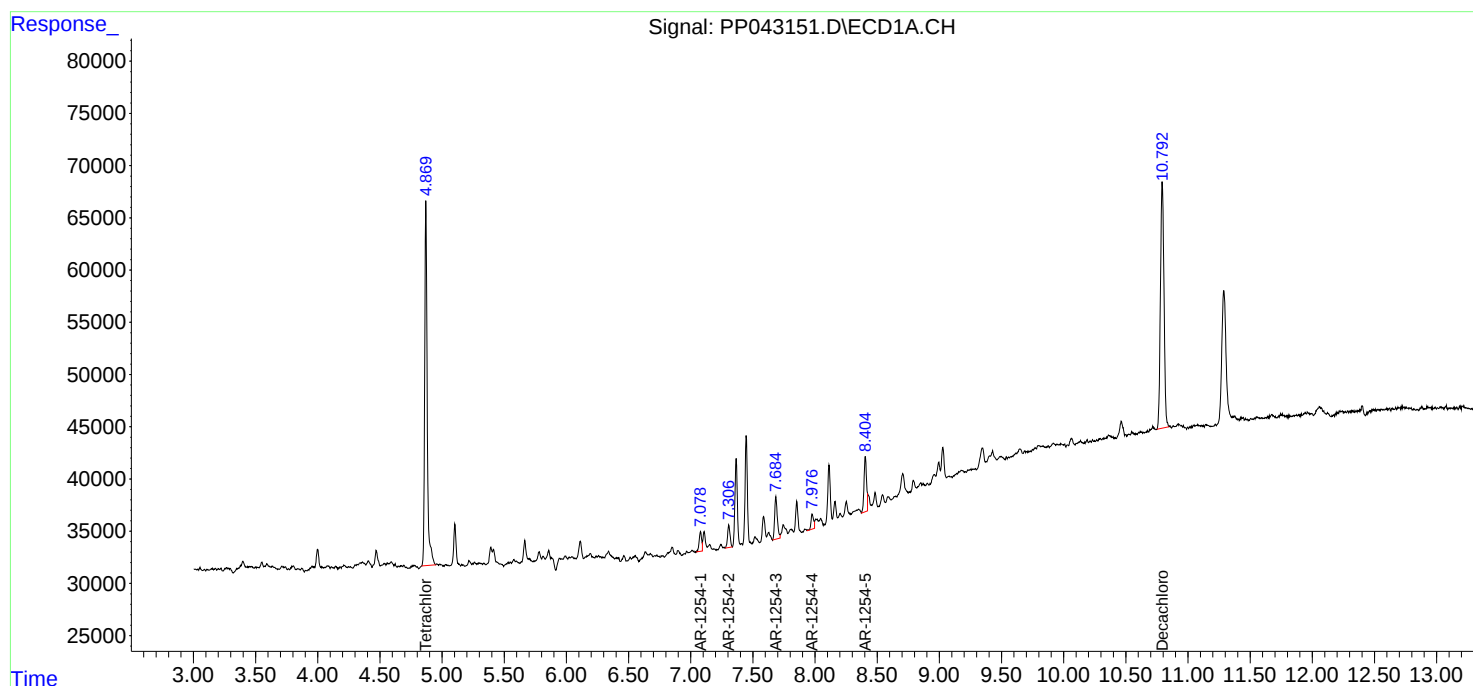

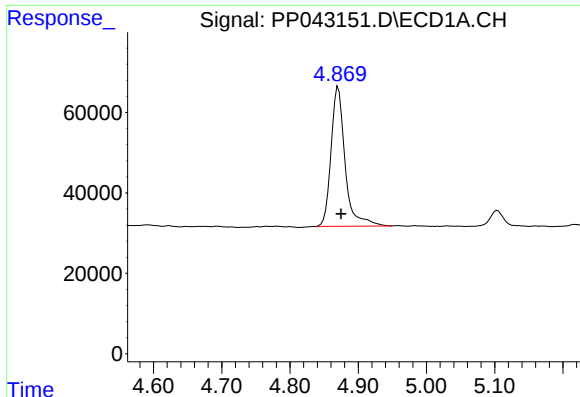


#1 Tetrachloro-m-xylene

R.T.: 4.871 min
Delta R.T.: -0.004 min
Response: 495519
Conc: 20.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

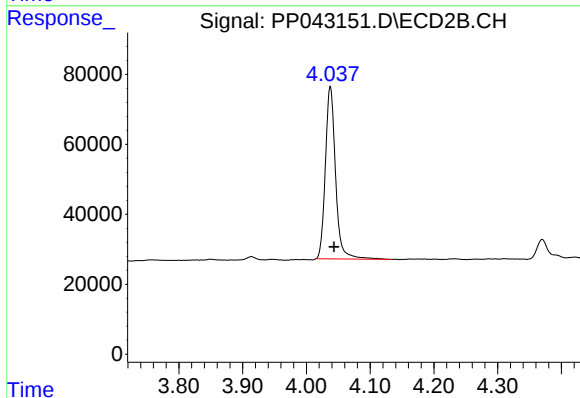


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.006 min
Response: 548384
Conc: 21.96 ng/ml

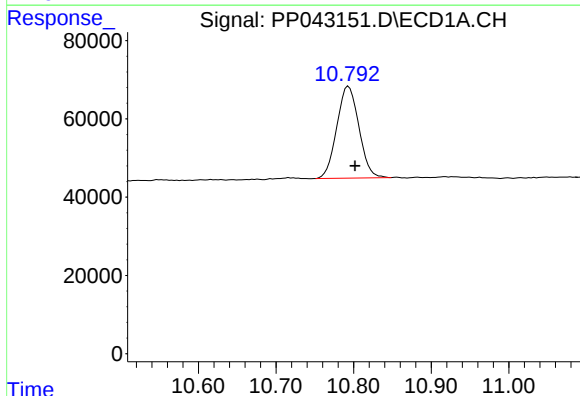


#2 Decachlorobiphenyl

R.T.: 10.793 min
Delta R.T.: -0.009 min
Response: 464609
Conc: 31.78 ng/ml

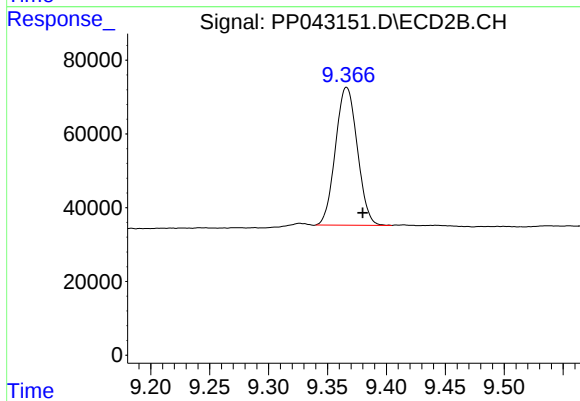

#2 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.014 min
Response: 482607
Conc: 24.74 ng/ml

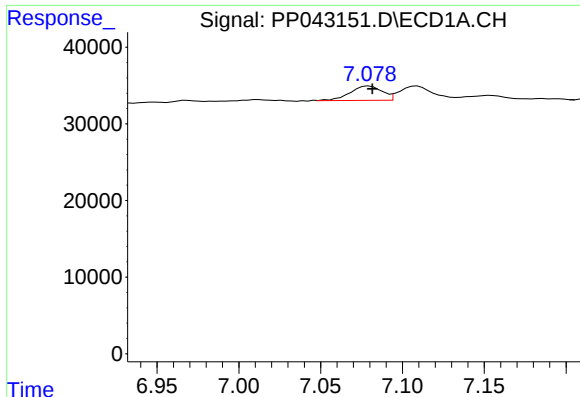


#26 AR-1254-1

R.T.: 7.080 min
Delta R.T.: -0.002 min
Response: 25344
Conc: 32.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

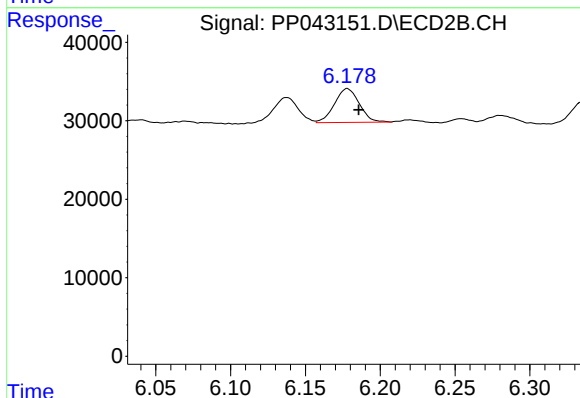


#26 AR-1254-1

R.T.: 6.178 min
Delta R.T.: -0.008 min
Response: 49629
Conc: 32.00 ng/ml

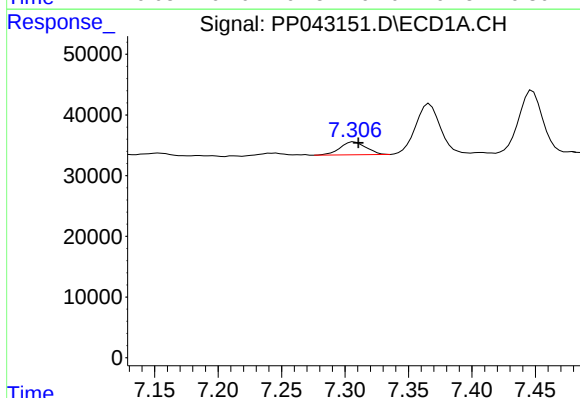


#27 AR-1254-2

R.T.: 7.307 min
Delta R.T.: -0.003 min
Response: 30280
Conc: 24.06 ng/ml

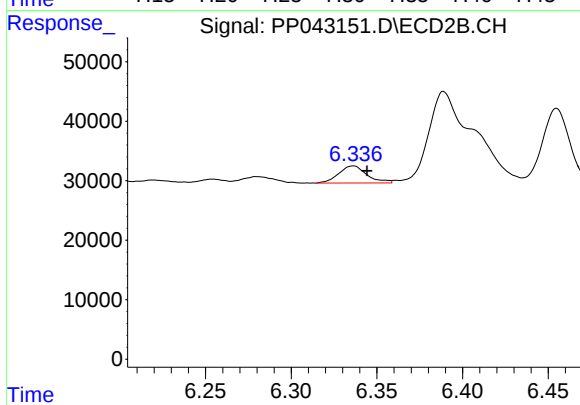

#27 AR-1254-2

R.T.: 6.336 min
Delta R.T.: -0.008 min
Response: 33069
Conc: 24.36 ng/ml

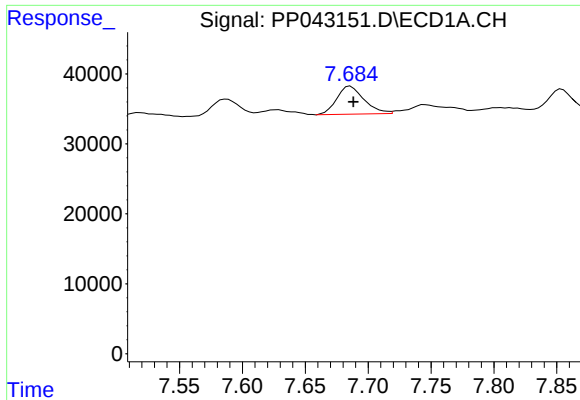


#28 AR-1254-3

R.T.: 7.686 min
Delta R.T.: -0.003 min
Response: 60593
Conc: 46.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

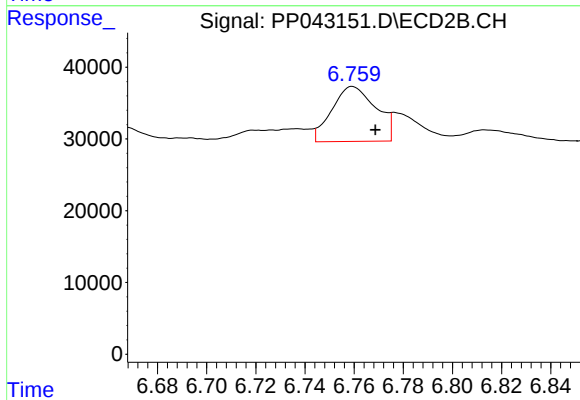


#28 AR-1254-3

R.T.: 6.759 min
Delta R.T.: -0.010 min
Response: 94954
Conc: 44.39 ng/ml m

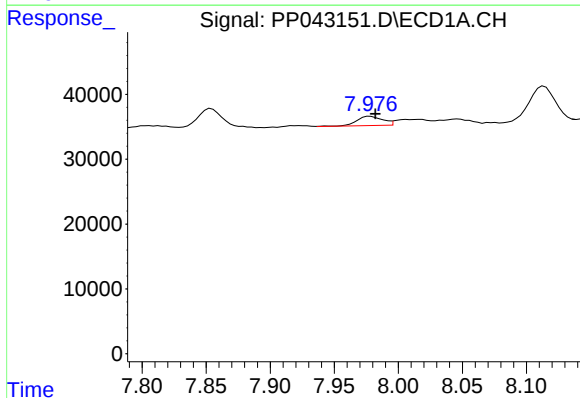


#29 AR-1254-4

R.T.: 7.978 min
Delta R.T.: -0.004 min
Response: 20142
Conc: 23.05 ng/ml

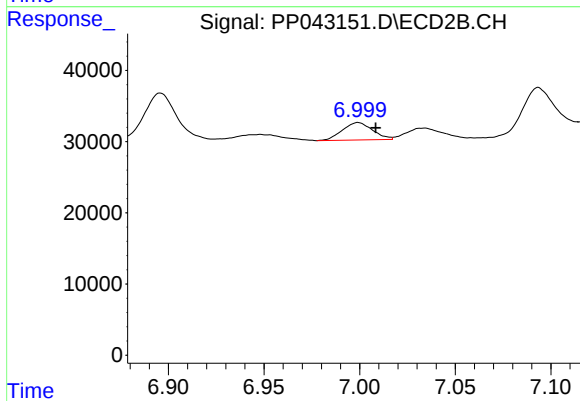

#29 AR-1254-4

R.T.: 6.999 min
Delta R.T.: -0.009 min
Response: 26924
Conc: 21.58 ng/ml

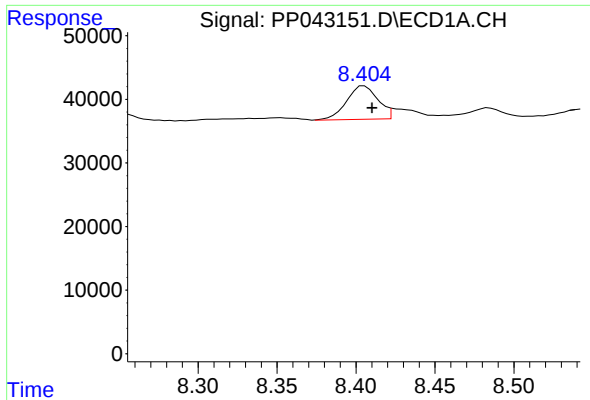


#30 AR-1254-5

R.T.: 8.404 min
Delta R.T.: -0.006 min
Response: 76508
Conc: 81.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

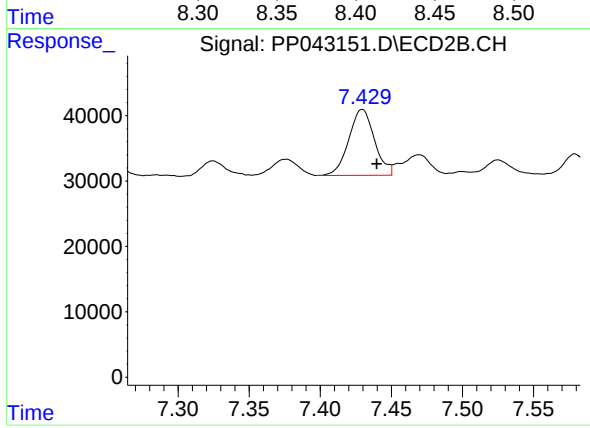

#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: -0.010 min
Response: 127244
Conc: 74.62 ng/ml