

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
 Data File : PP043158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 19:08
 Operator : AJ\MA
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2022
 Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 02:23:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.871	4.038	1167296	1242167	49.333	49.734
2) SA Decachlor...	10.792	9.365	846909	924365	57.934	47.387m
Target Compounds						
26) L6 AR-1254-1	7.078	6.177	363140	741012	462.793	477.854
27) L6 AR-1254-2	7.307	6.336	542442	639342	430.992	470.951
28) L6 AR-1254-3	7.684	6.760	574712	984035	442.972	460.058
29) L6 AR-1254-4	7.978	7.000	401060	599823	458.864	480.783
30) L6 AR-1254-5	8.406	7.430	437552	787680	467.014	461.937

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012022\
Data File : PP043158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 19:08
Operator : AJ\MA
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 02:23:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

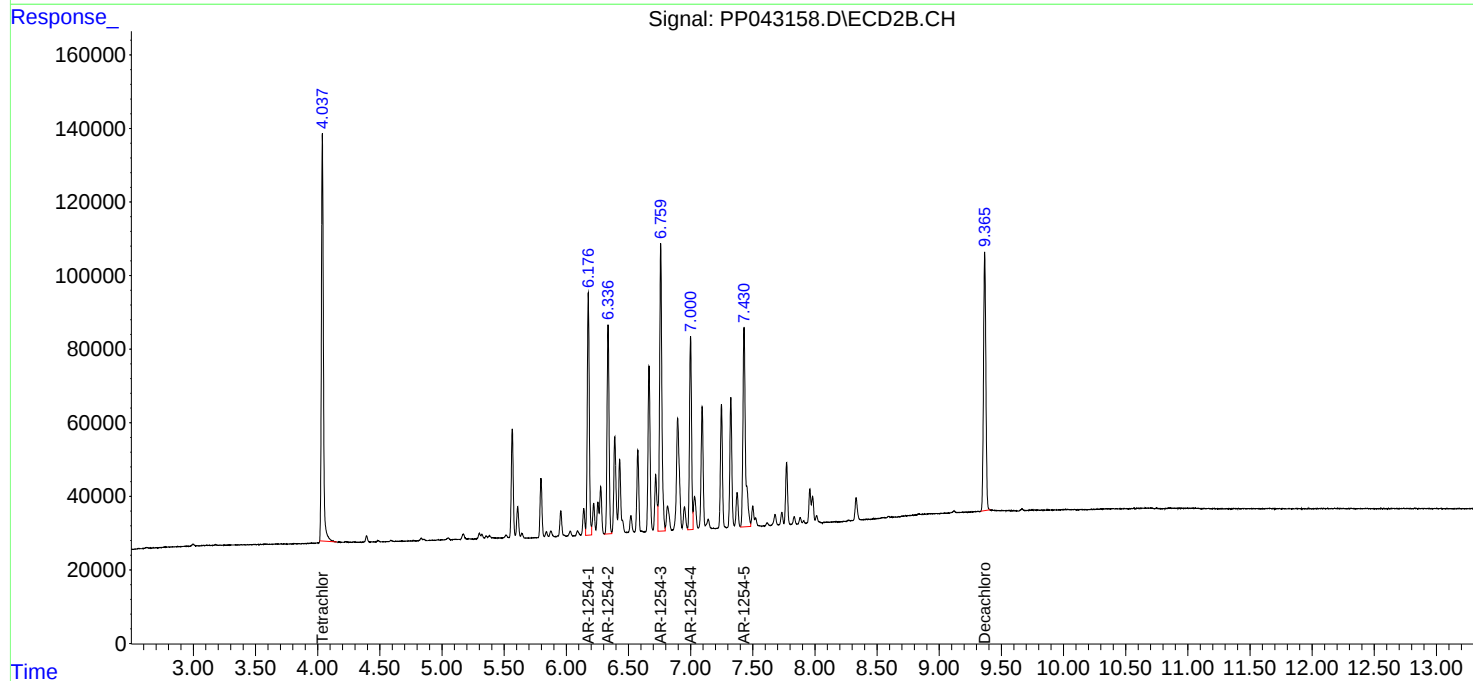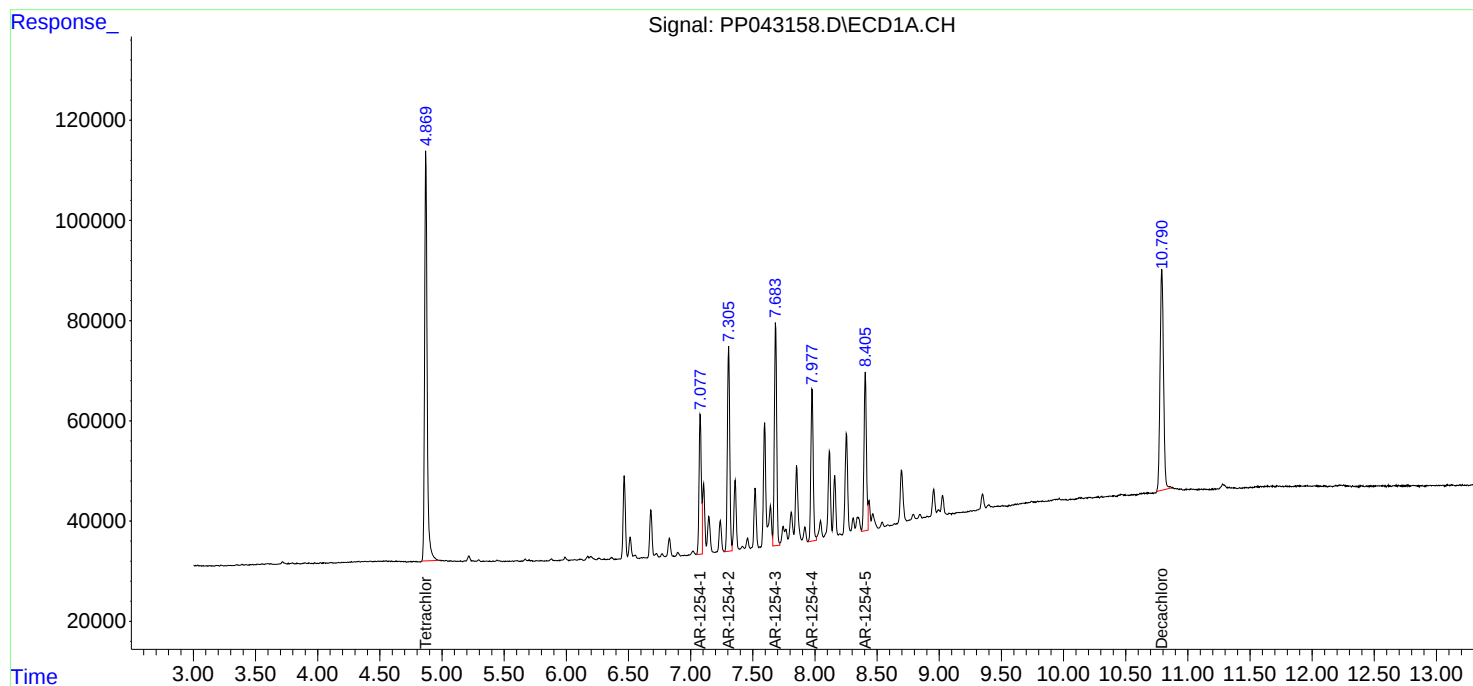

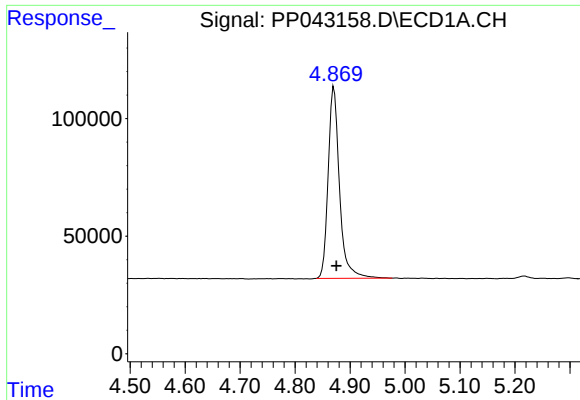


#1 Tetrachloro-m-xylene

R.T.: 4.871 min
Delta R.T.: -0.004 min
Response: 1167296
Conc: 49.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

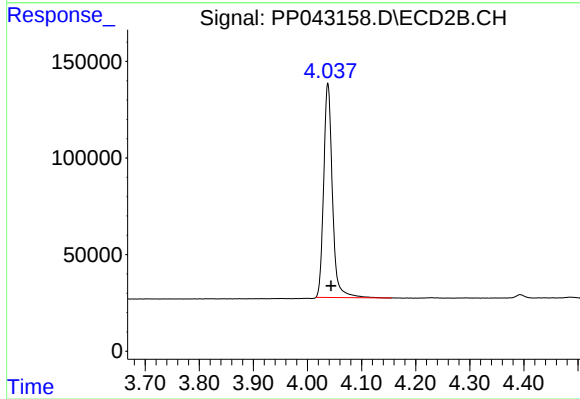


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.006 min
Response: 1242167
Conc: 49.73 ng/ml

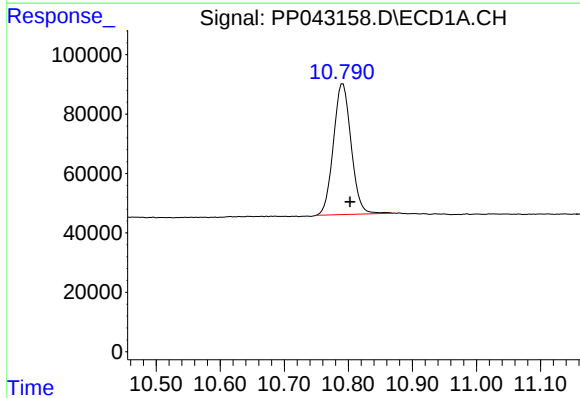


#2 Decachlorobiphenyl

R.T.: 10.792 min
Delta R.T.: -0.011 min
Response: 846909
Conc: 57.93 ng/ml

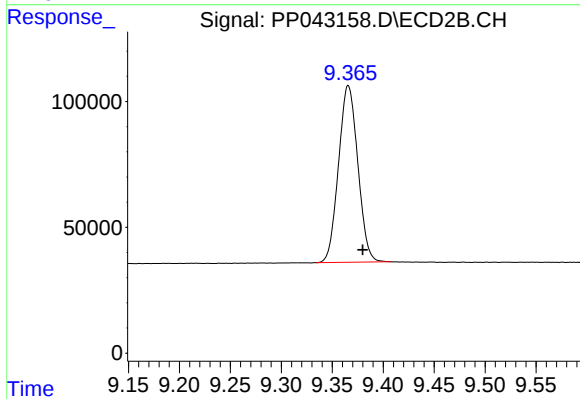

#2 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.015 min
Response: 924365
Conc: 47.39 ng/ml m

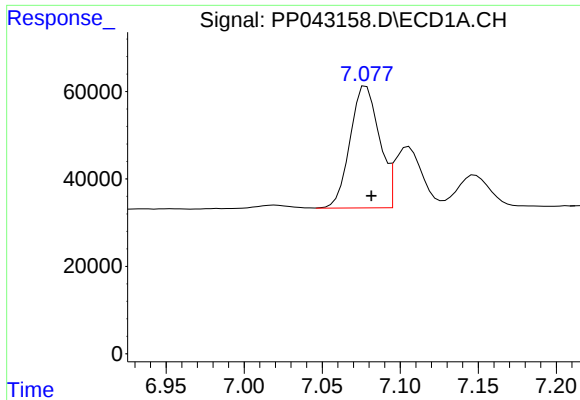


#26 AR-1254-1

R.T.: 7.078 min
Delta R.T.: -0.003 min
Response: 363140
Conc: 462.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

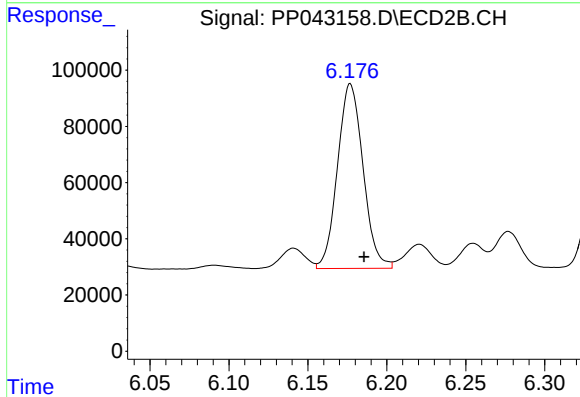


#26 AR-1254-1

R.T.: 6.177 min
Delta R.T.: -0.009 min
Response: 741012
Conc: 477.85 ng/ml

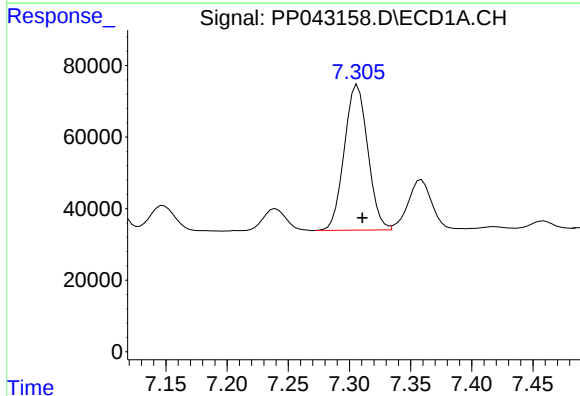


#27 AR-1254-2

R.T.: 7.307 min
Delta R.T.: -0.004 min
Response: 542442
Conc: 430.99 ng/ml

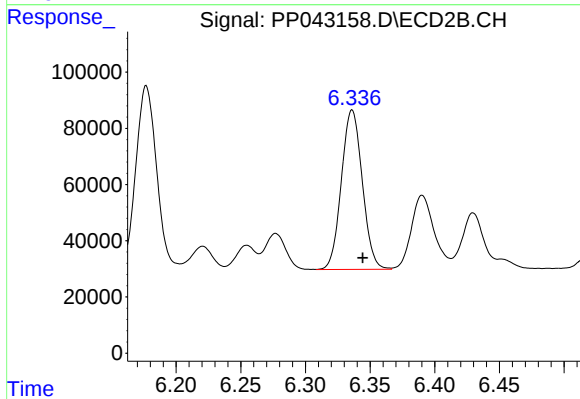

#27 AR-1254-2

R.T.: 6.336 min
Delta R.T.: -0.008 min
Response: 639342
Conc: 470.95 ng/ml

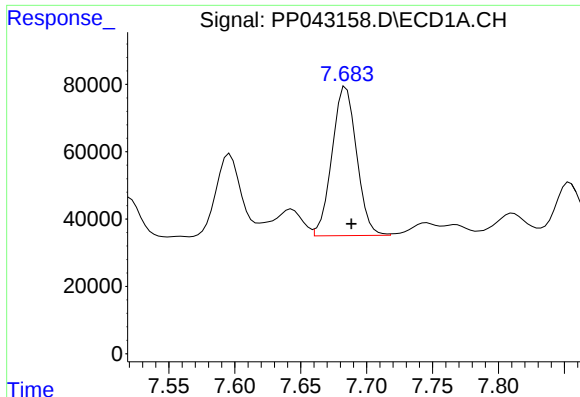


#28 AR-1254-3

R.T.: 7.684 min
Delta R.T.: -0.004 min
Response: 574712
Conc: 442.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

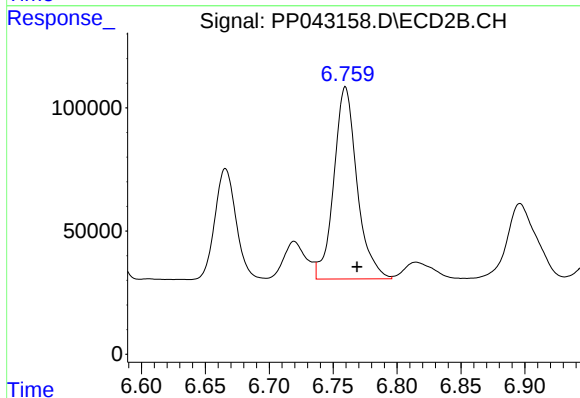


#28 AR-1254-3

R.T.: 6.760 min
Delta R.T.: -0.009 min
Response: 984035
Conc: 460.06 ng/ml

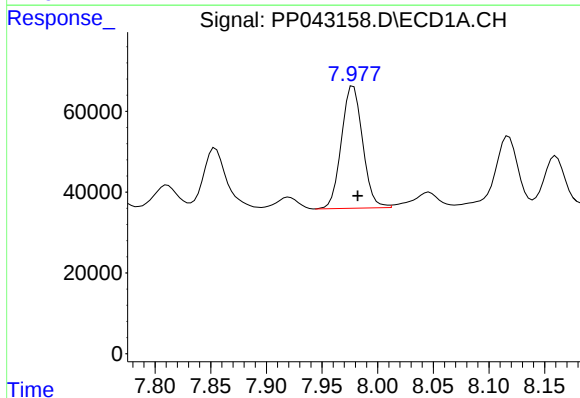


#29 AR-1254-4

R.T.: 7.978 min
Delta R.T.: -0.004 min
Response: 401060
Conc: 458.86 ng/ml

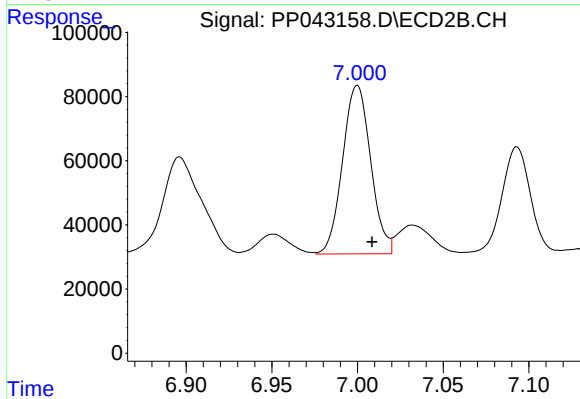

#29 AR-1254-4

R.T.: 7.000 min
Delta R.T.: -0.009 min
Response: 599823
Conc: 480.78 ng/ml

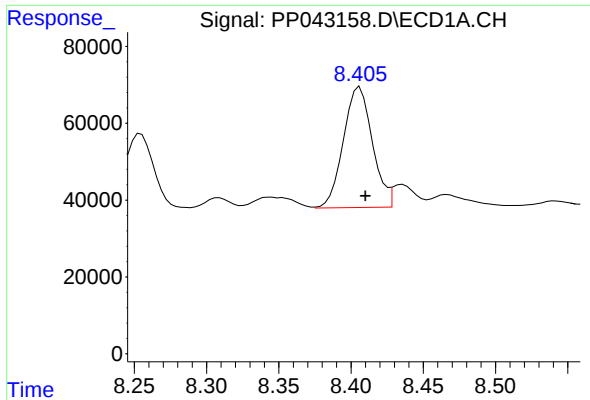


#30 AR-1254-5

R.T.: 8.406 min
Delta R.T.: -0.004 min
Response: 437552
Conc: 467.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

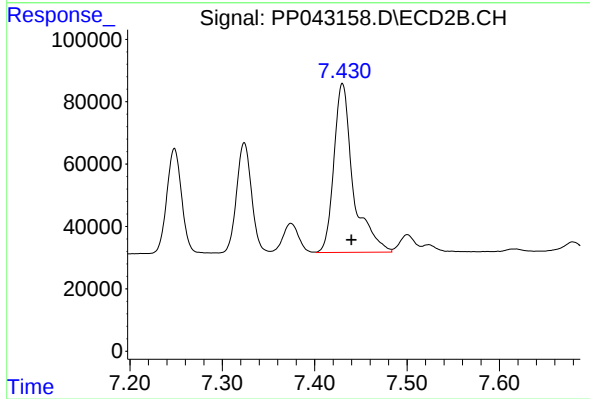

#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: -0.010 min
Response: 787680
Conc: 461.94 ng/ml