

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012121\
 Data File : PP032876.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2021 17:54
 Operator : DD\AJ
 Sample : M1200-01 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 012021TB01

Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:11:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.738	4.010	184199	182690	3.171	3.884
2) SA Decachlor...	10.547f	9.289	8608959	214443	218.206m	5.724 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012121\
Data File : PP032876.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2021 17:54
Operator : DD\AJ
Sample : M1200-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
012021TB01


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:11:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

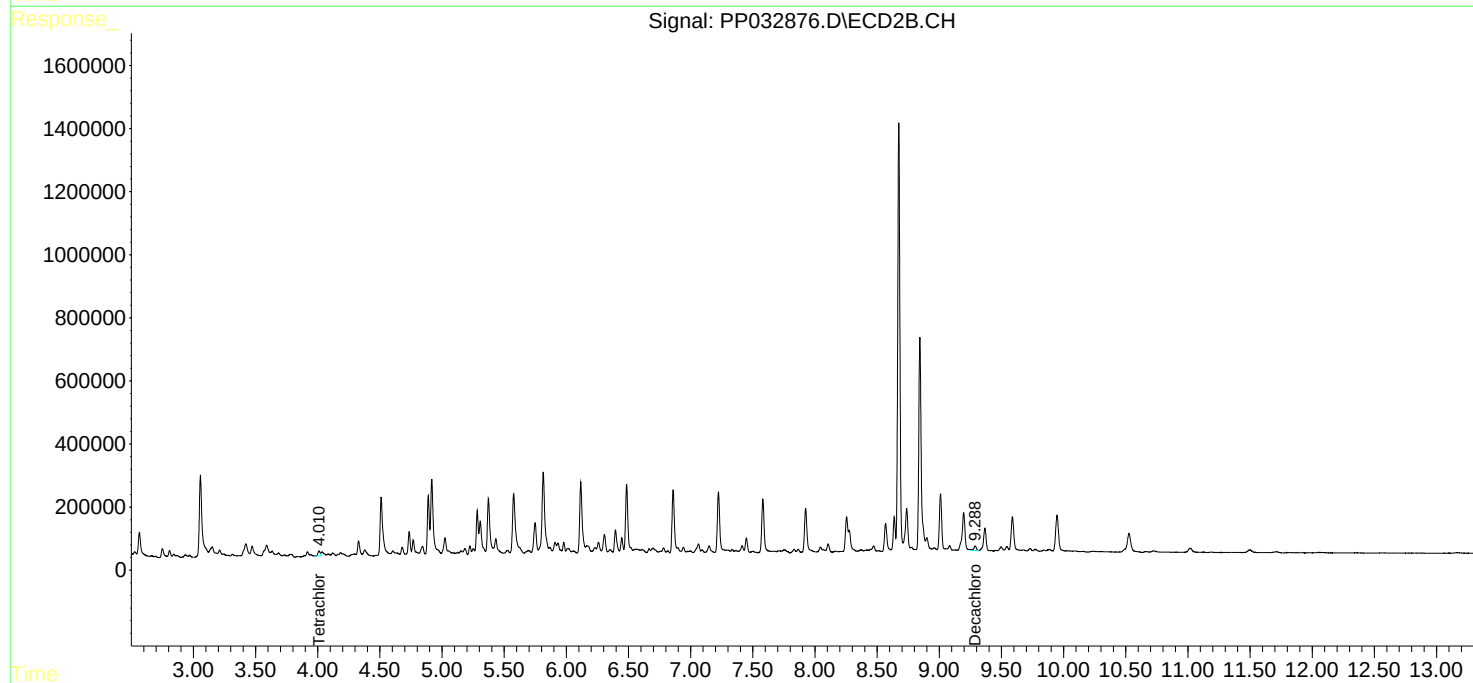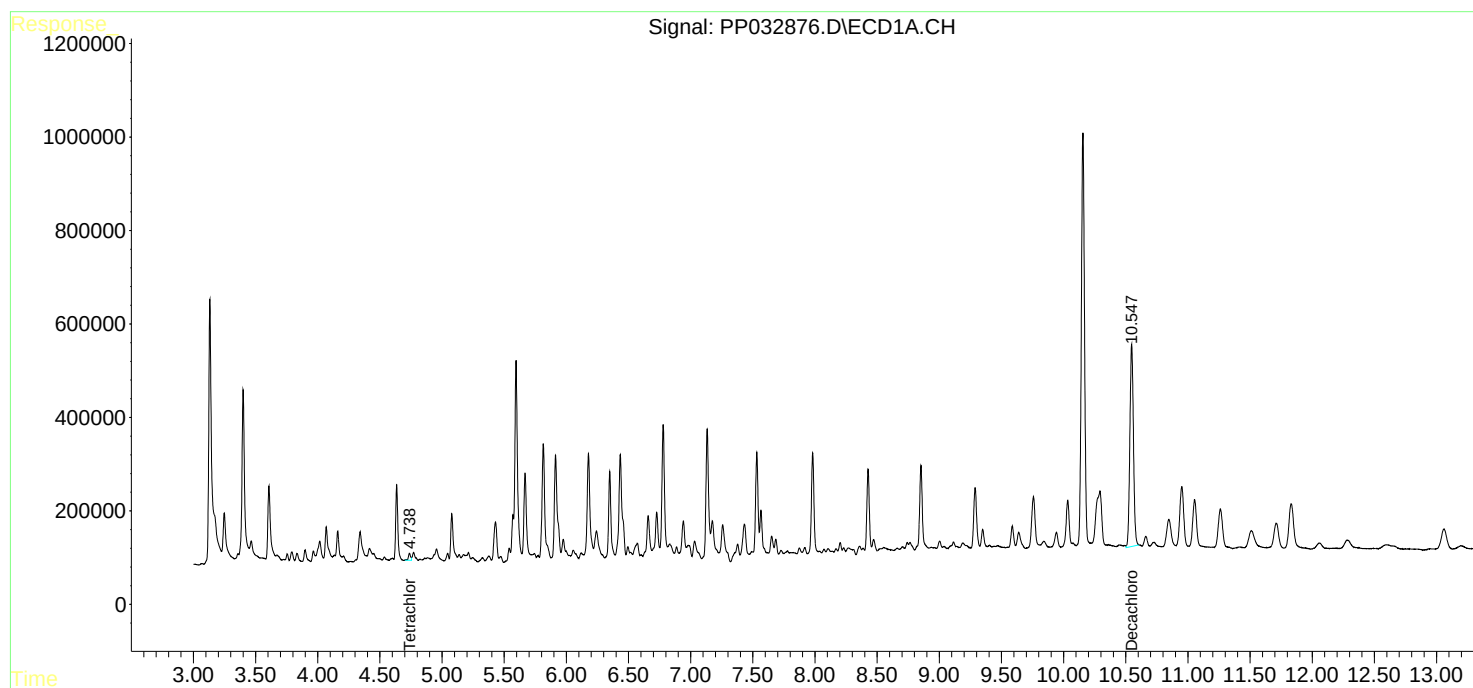

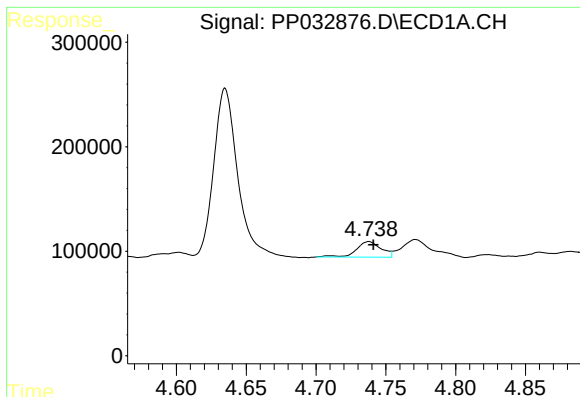


#1 Tetrachloro-m-xylene

R.T.: 4.738 min
 Delta R.T.: -0.003 min
 Response: 184199
 Conc: 3.17 ng/ml

Instrument :
 ECD_P
 ClientSampleId :
 012021TB01


Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:03 PM

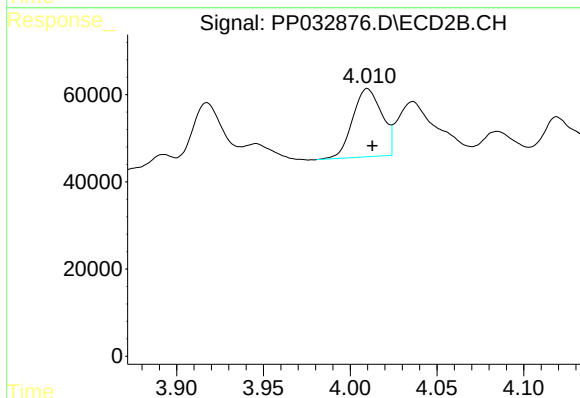


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
 Delta R.T.: -0.003 min
 Response: 182690
 Conc: 3.88 ng/ml

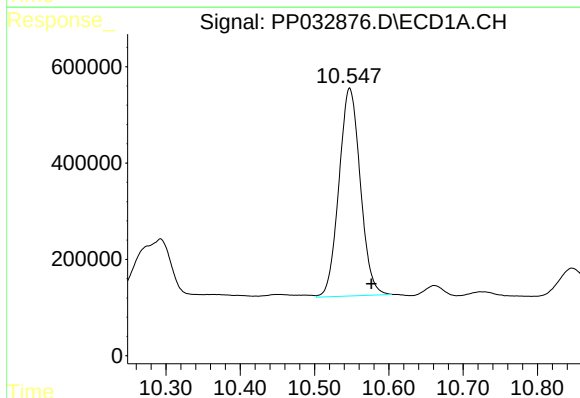

#2 Decachlorobiphenyl

R.T.: 10.547 min
 Delta R.T.: -0.030 min
 Response: 8608959
 Conc: 218.21 ng/ml m

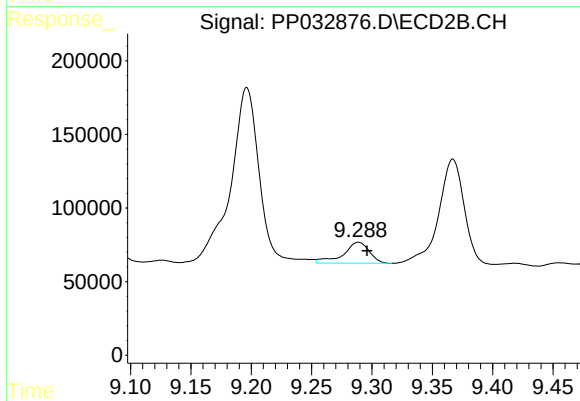

#2 Decachlorobiphenyl

R.T.: 9.289 min
 Delta R.T.: -0.007 min
 Response: 214443
 Conc: 5.72 ng/ml