

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
 Data File : PL072150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 08:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:54:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.492	9567868	29105529	17.234	17.921
28)	SA Decachlor...	10.318	11.383	15117645	27372965	17.016	16.965
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	264796	N.D.	0.108 #
9)	A Endosulfan I	0.000	8.377	0	36451	N.D.	0.020 #
10)	B gamma-Chl...	0.000	8.237	0	47648	N.D.	0.024 #
11)	B alpha-Chl...	0.000	8.320	0	536796	N.D.	0.271 #
15)	B Endosulfa...	0.000	9.112f	0	93770	N.D.	0.055 #
17)	MA 4,4'-DDT	0.000	9.332f	0	52208	N.D.	0.033 #
20)	A Methoxychlor	0.000	9.874f	0	49321	N.D.	0.060 #
25)	Chlordane-3	0.000	8.237	0	47648	N.D.	0.171 #
26)	Chlordane-4	0.000	8.320	0	536796	N.D.	1.617 #
27)	Chlordane-5	0.000	9.191	0	45178	N.D.	0.740 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012122\
Data File : PL072150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 08:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:54:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

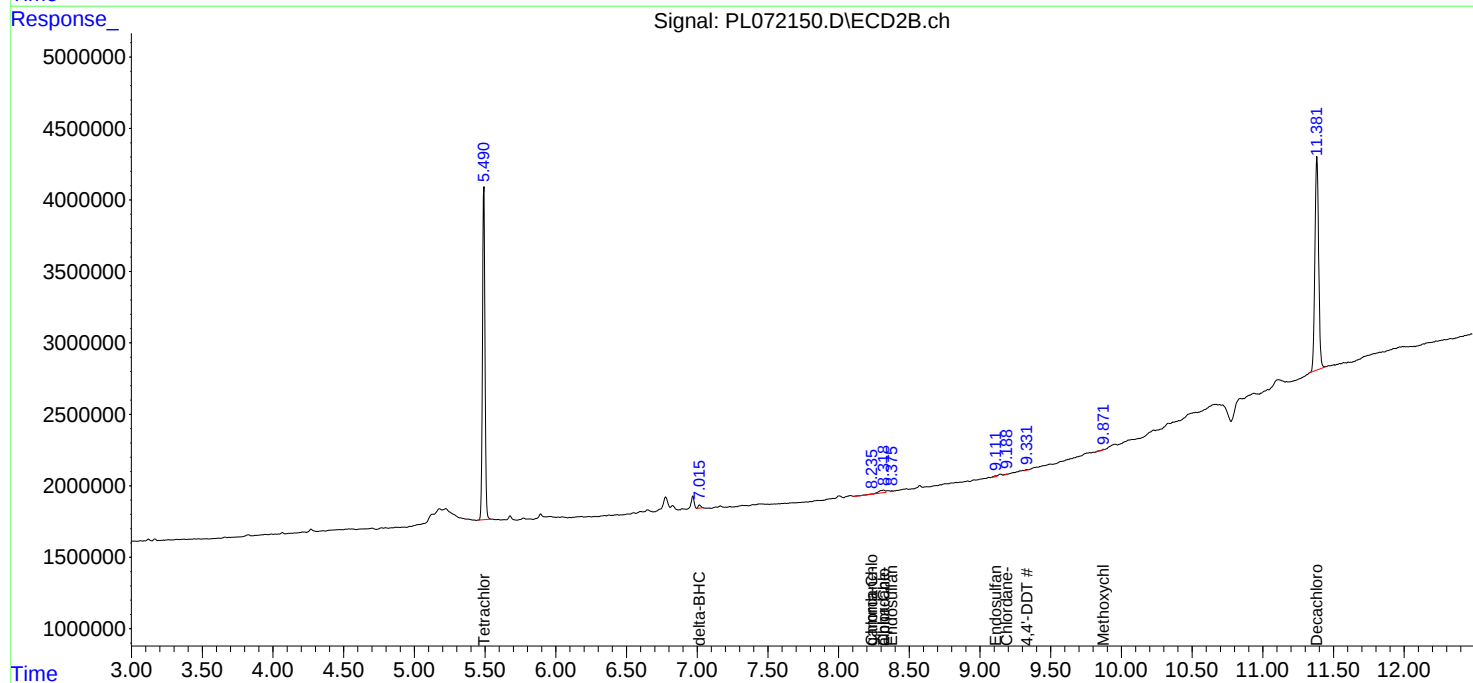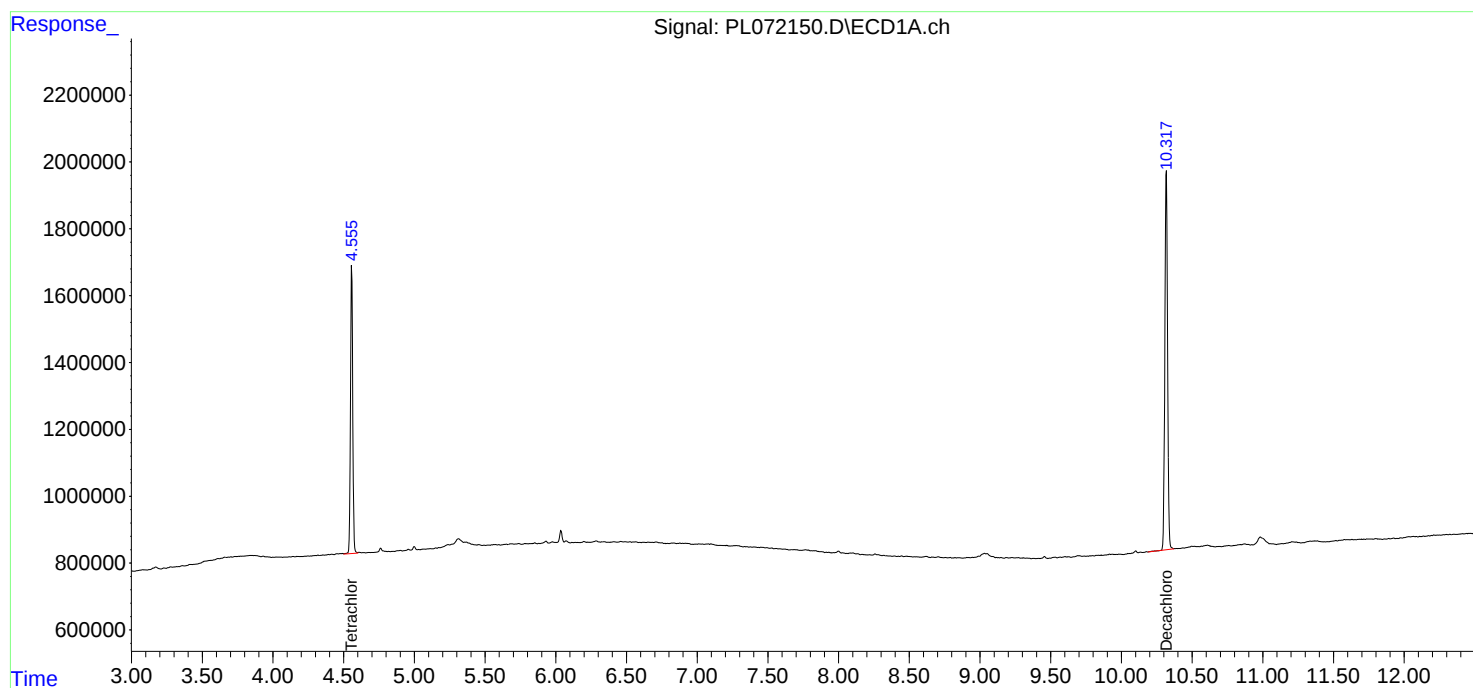


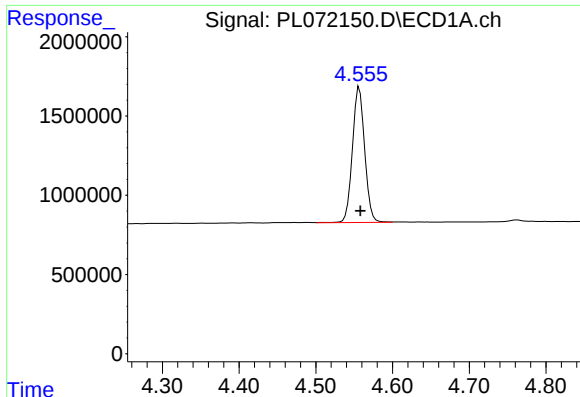

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: -0.001 min
Response: 9567868
Conc: 17.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

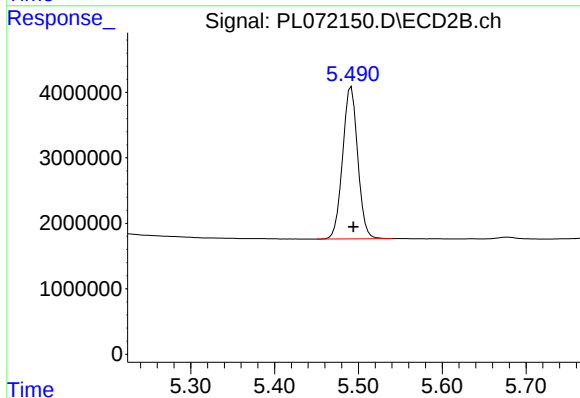


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 29105529
Conc: 17.92 ng/ml

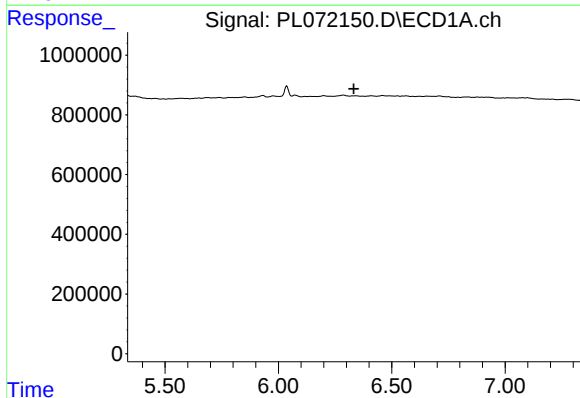


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

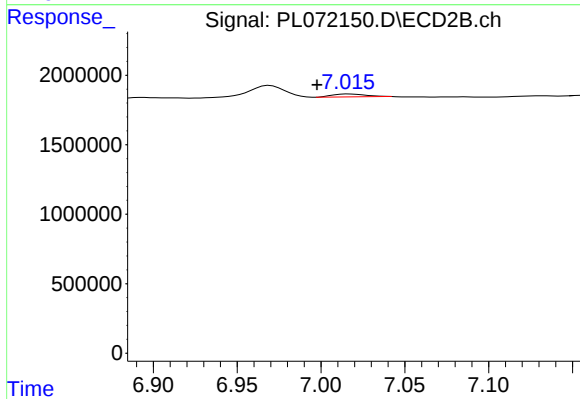

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 264796
Conc: 0.11 ng/ml

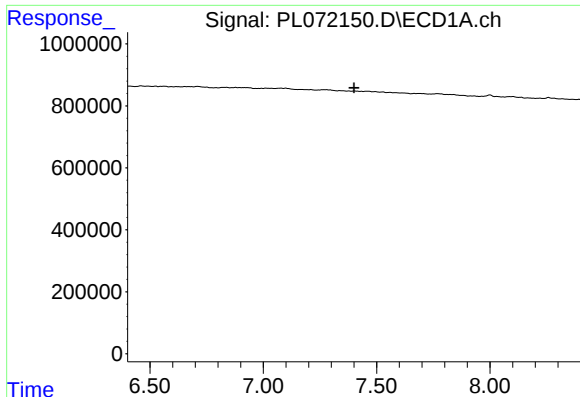

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

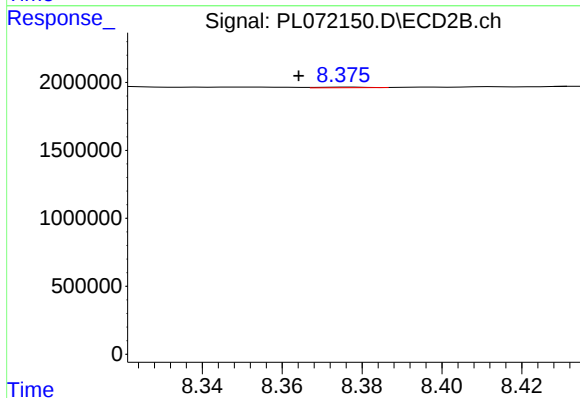


#9 Endosulfan I

R.T.: 8.377 min
Delta R.T.: 0.013 min
Response: 36451
Conc: 0.02 ng/ml

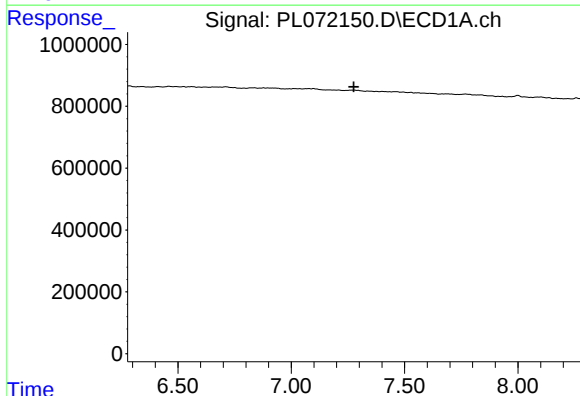


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

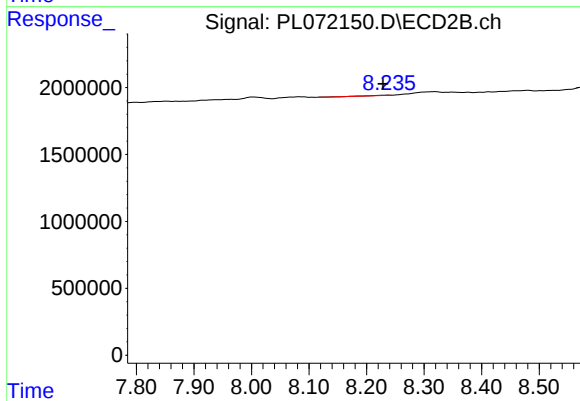

#10 gamma-Chlordane


R.T.: 8.237 min
Delta R.T.: 0.008 min
Response: 47648
Conc: 0.02 ng/ml

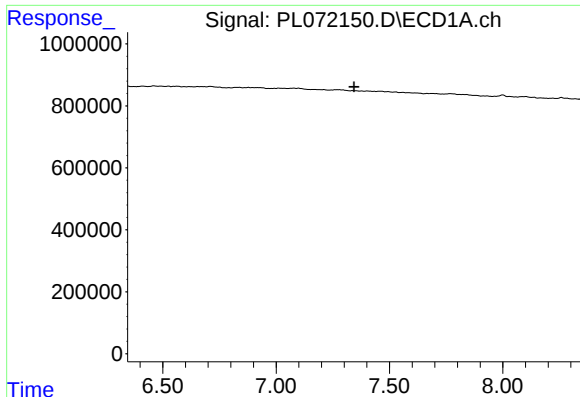

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

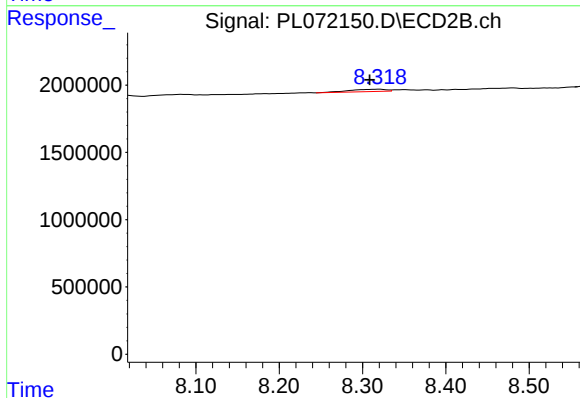


#11 alpha-Chlordane

R.T.: 8.320 min
Delta R.T.: 0.011 min
Response: 536796
Conc: 0.27 ng/ml

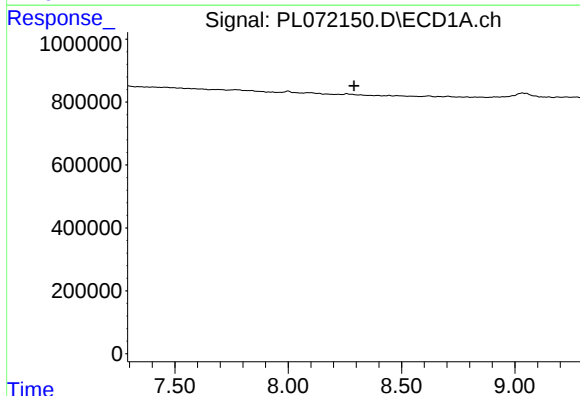


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

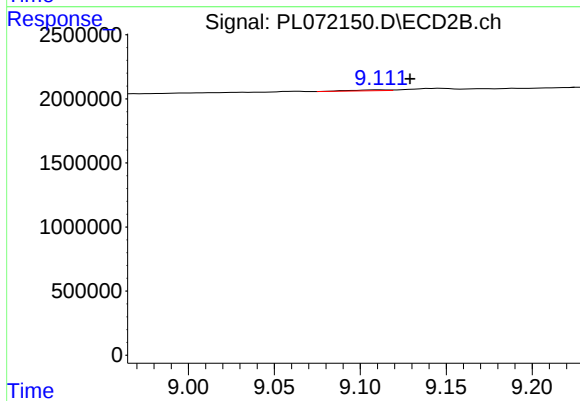

#15 Endosulfan II


R.T.: 9.112 min
Delta R.T.: -0.017 min
Response: 93770
Conc: 0.05 ng/ml

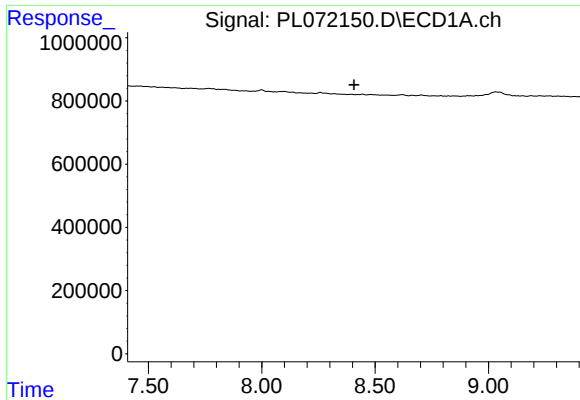

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

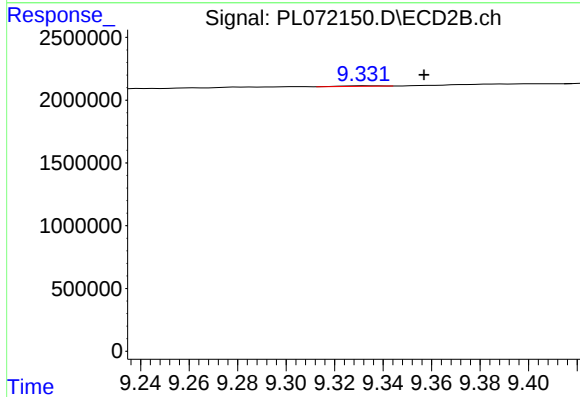


#17 4,4'-DDT

R.T.: 9.332 min
Delta R.T.: -0.025 min
Response: 52208
Conc: 0.03 ng/ml

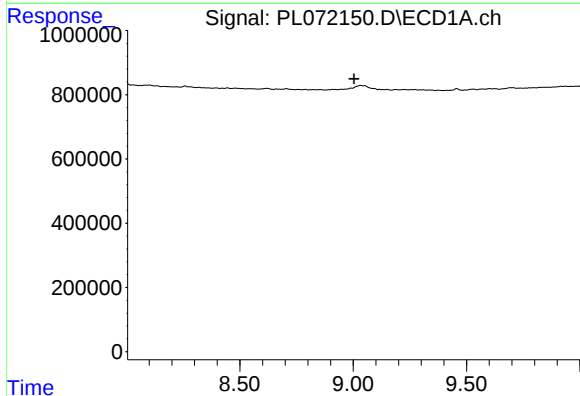


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

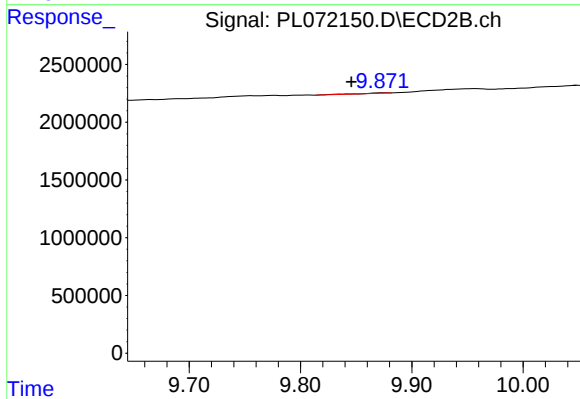

#20 Methoxychlor


R.T.: 9.874 min
Delta R.T.: 0.028 min
Response: 49321
Conc: 0.06 ng/ml

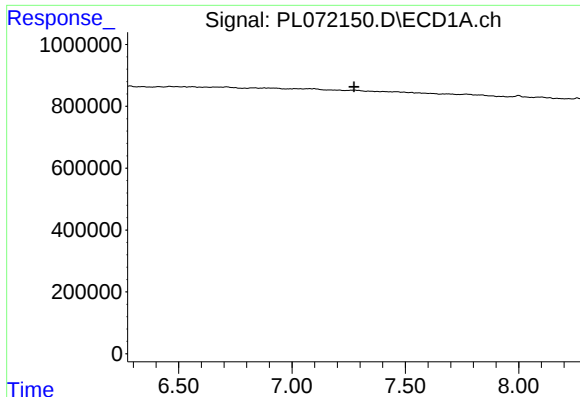

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

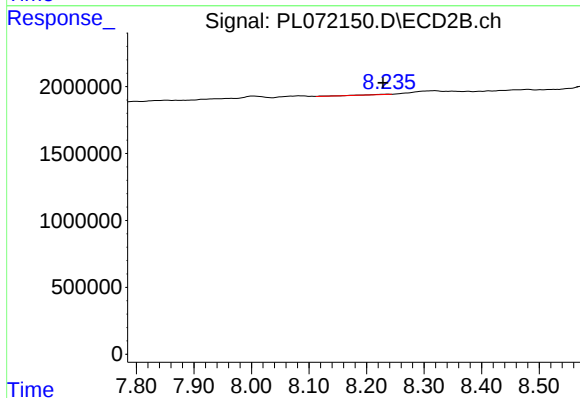


#25 Chlordane-3

R.T.: 8.237 min
Delta R.T.: 0.008 min
Response: 47648
Conc: 0.17 ng/ml

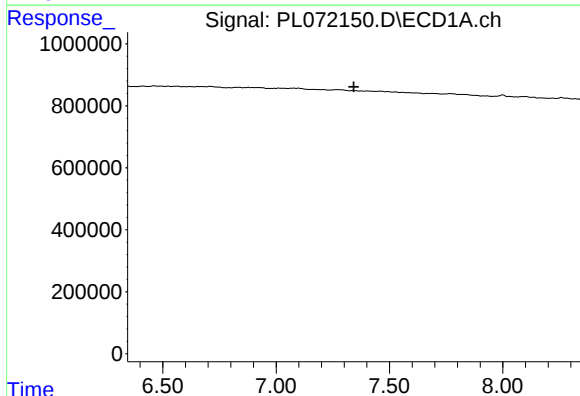


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

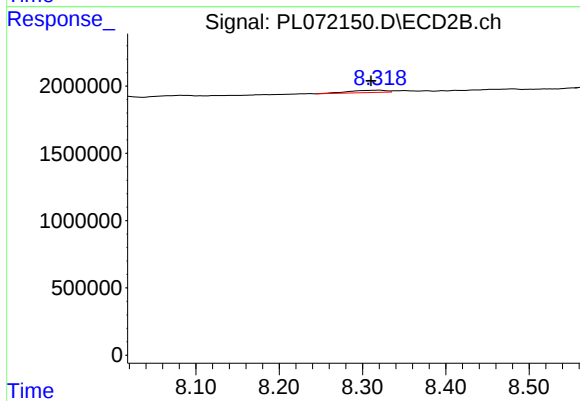

#26 Chlordane-4


R.T.: 8.320 min
Delta R.T.: 0.010 min
Response: 536796
Conc: 1.62 ng/ml

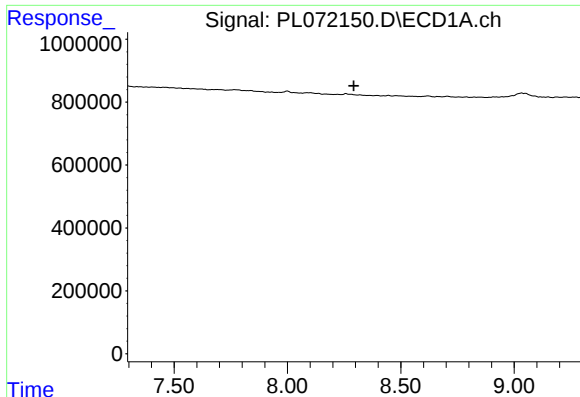

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

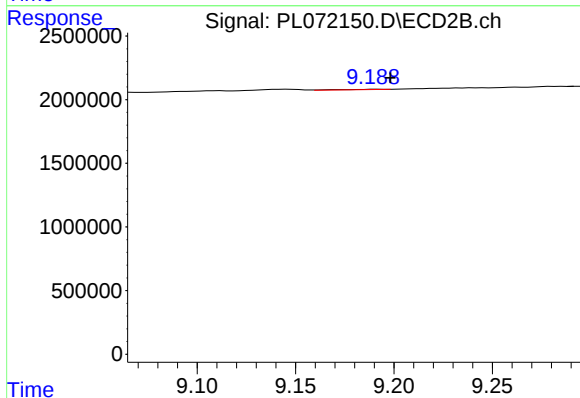


#27 Chlordane-5

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 45178
Conc: 0.74 ng/ml

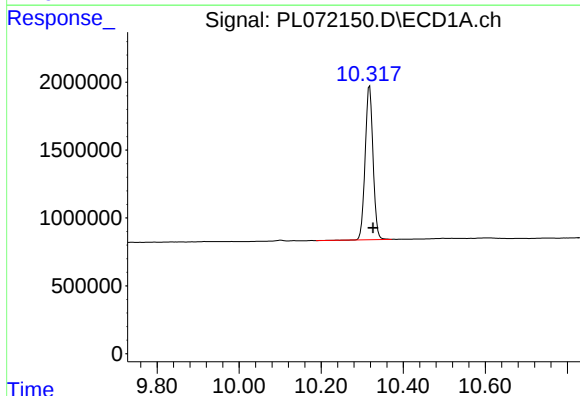

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 15117645
Conc: 17.02 ng/ml

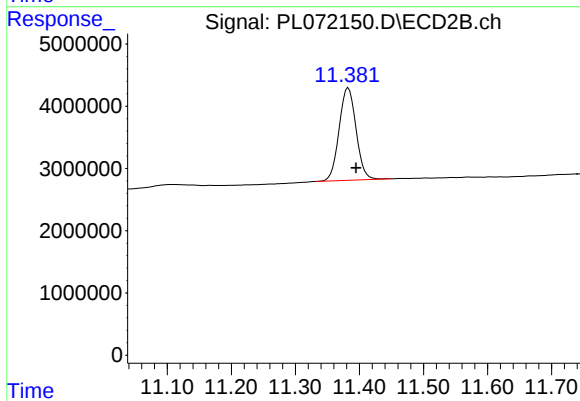

#28 Decachlorobiphenyl

R.T.: 11.383 min
Delta R.T.: -0.012 min
Response: 27372965
Conc: 16.96 ng/ml