

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032880.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 9:22
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:28:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
20)	L4	AR-1242-5	7.013	0.000	98102	0	102.593	N.D.	#
24)	L5	AR-1248-4	6.966	0.000	148993	0	91.859	N.D.	#
25)	L5	AR-1248-5	7.013	0.000	98102	0	61.352	N.D.	#
26)	L6	AR-1254-1	6.966f	0.000	148993	0	89.708	N.D.	#
28)	L6	AR-1254-3	7.574f	0.000	598210	0	222.026	N.D.	#
30)	L6	AR-1254-5	8.256f	0.000	972101	0	466.136	N.D.	#
35)	L7	AR-1260-5	8.876f	0.000	434016	0	95.811	N.D.	#
37)	L8	AR-1262-2	8.876f	0.000	434016	0	85.676	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032880.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 9:22
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:28:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

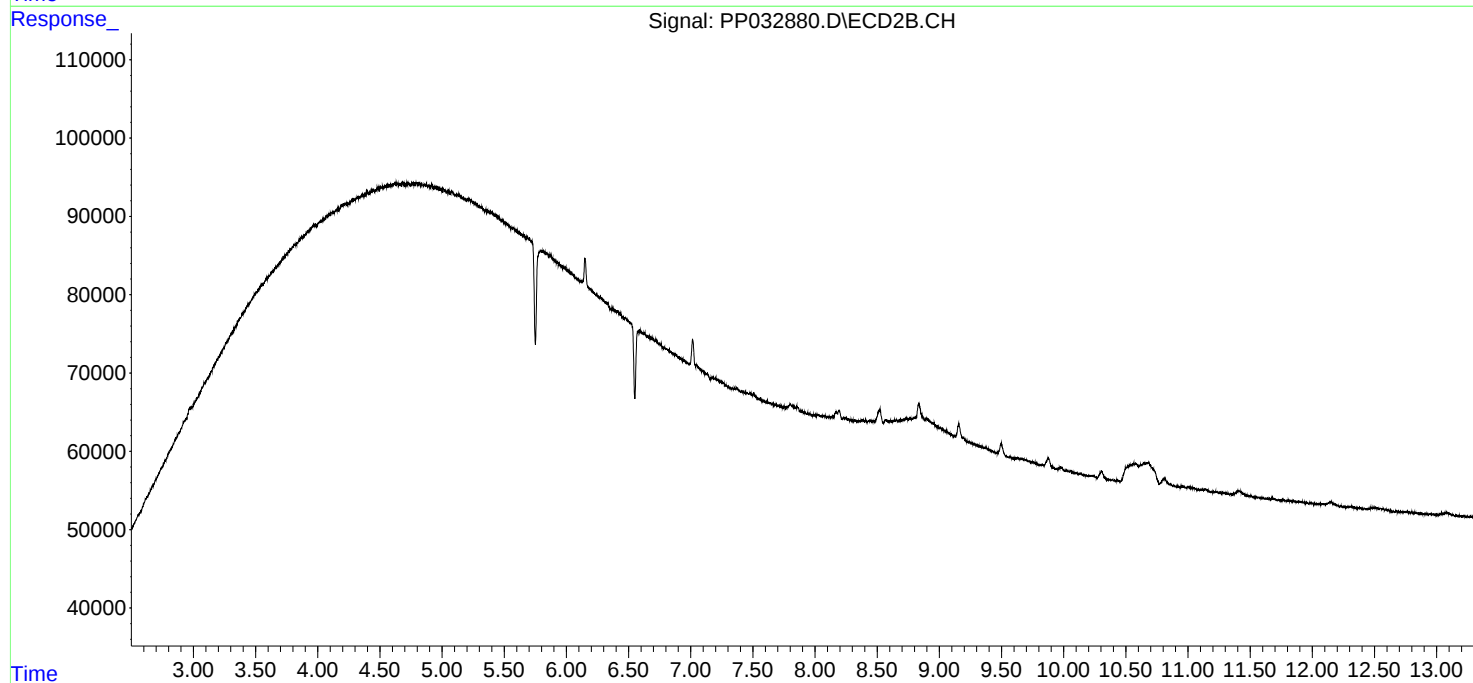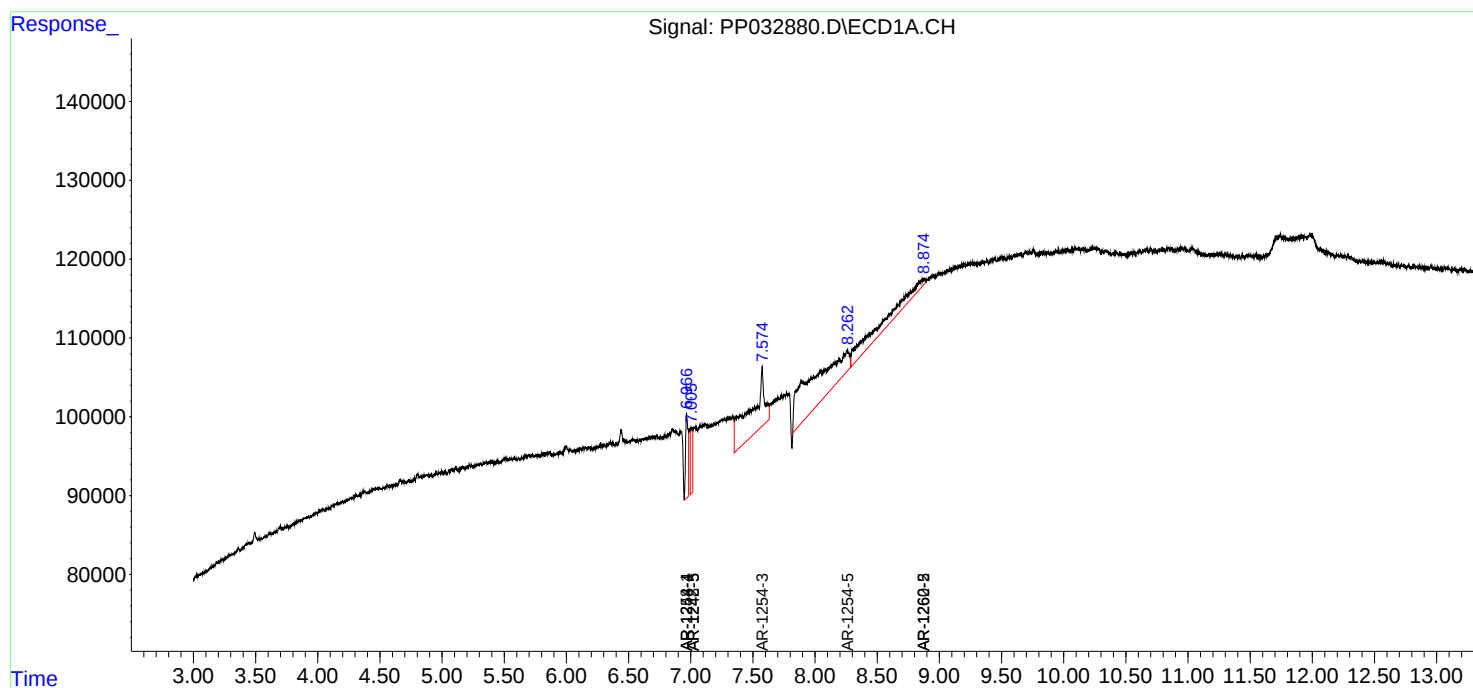


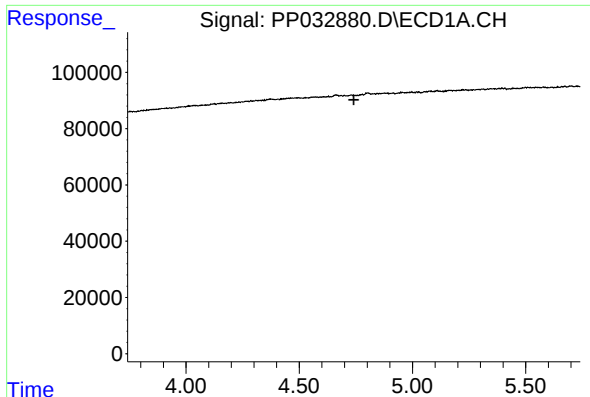

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.741 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

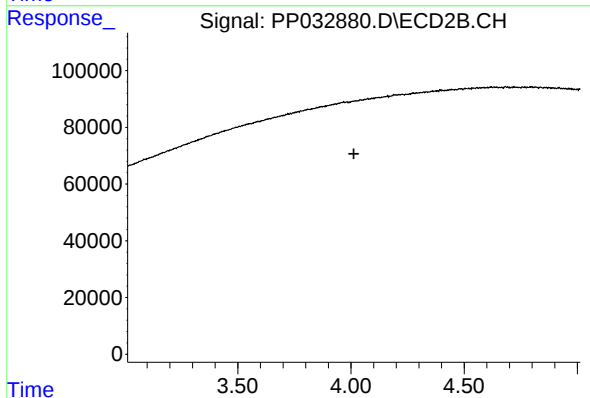


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.013 min
Response: 0
Conc: N.D.

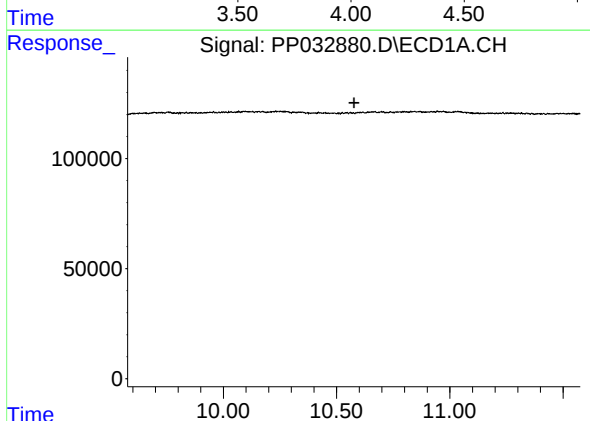


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.577 min
Response: 0
Conc: N.D.

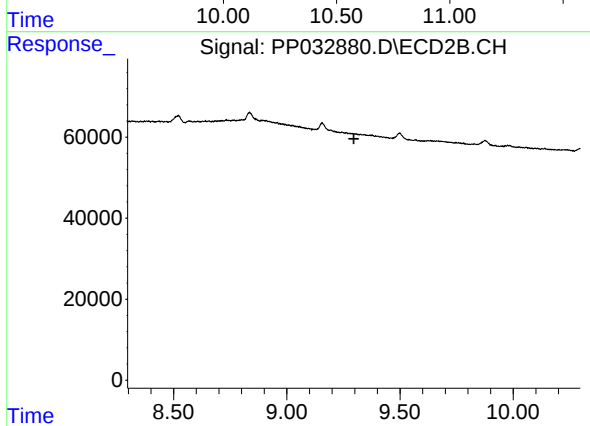

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.296 min
Response: 0
Conc: N.D.

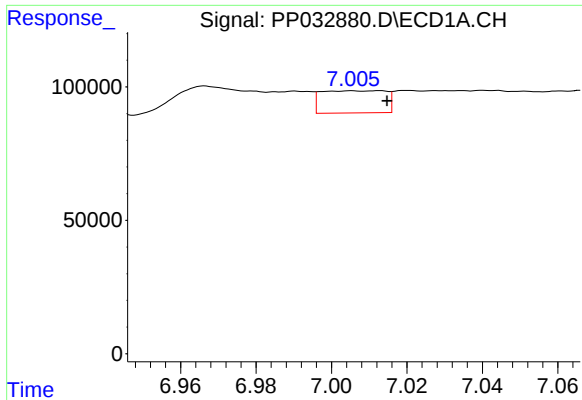

#20 AR-1242-5


R.T.: 7.013 min
Delta R.T.: -0.002 min
Response: 98102
Conc: 102.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

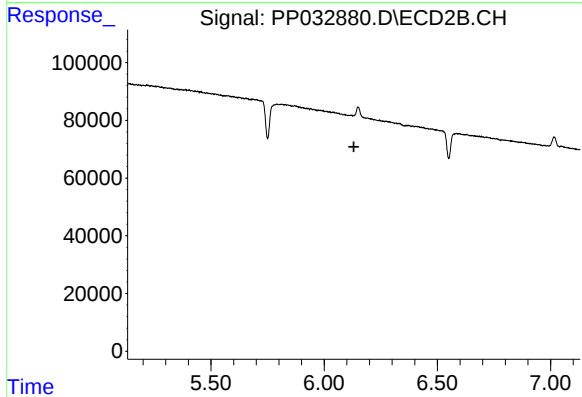


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.131 min
Response: 0
Conc: N.D.

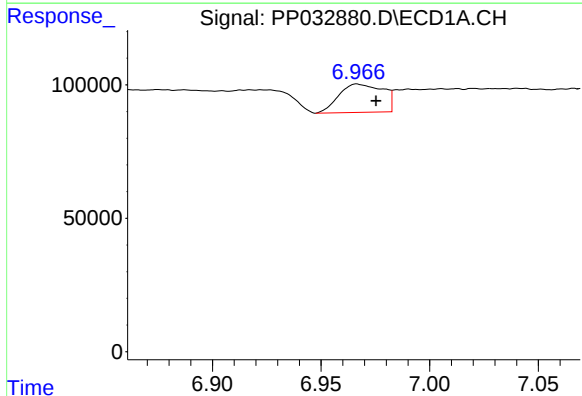


#24 AR-1248-4

R.T.: 6.966 min
Delta R.T.: -0.009 min
Response: 148993
Conc: 91.86 ng/ml

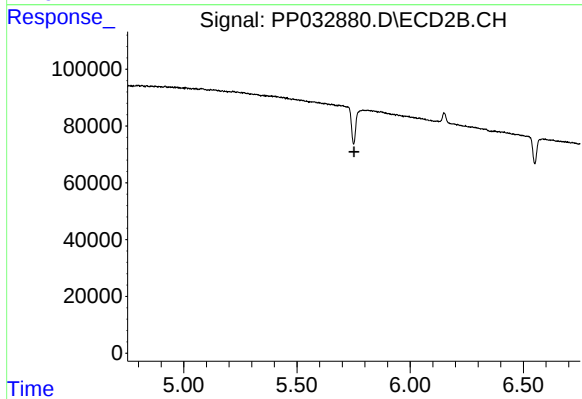

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

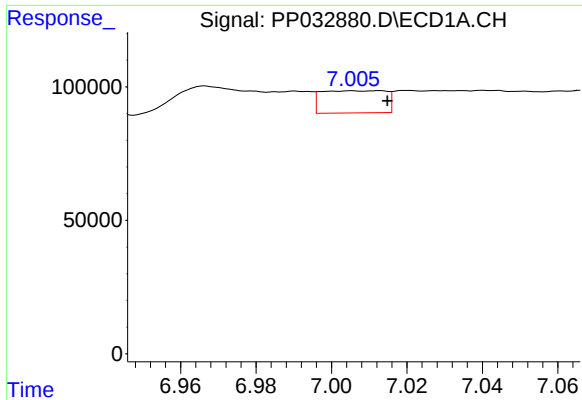

#25 AR-1248-5


R.T.: 7.013 min
Delta R.T.: -0.002 min
Response: 98102
Conc: 61.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

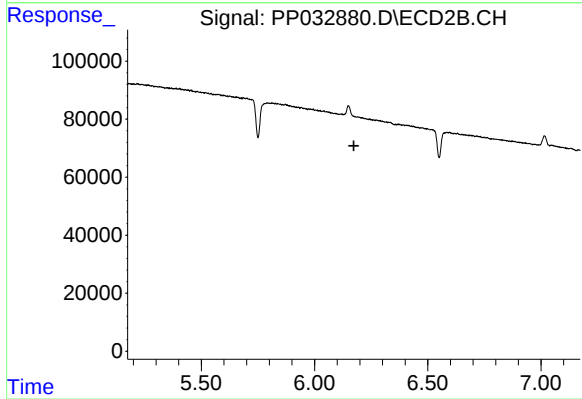


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.174 min
Response: 0
Conc: N.D.

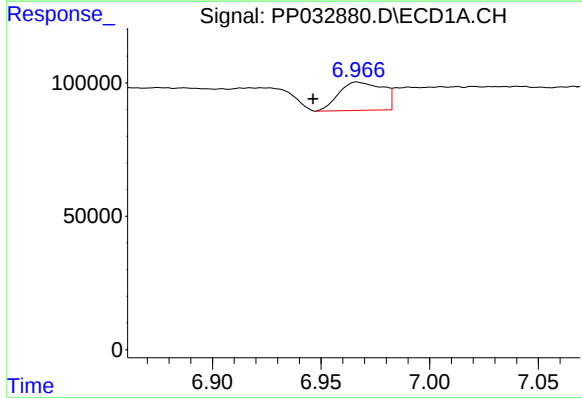


#26 AR-1254-1

R.T.: 6.966 min
Delta R.T.: 0.020 min
Response: 148993
Conc: 89.71 ng/ml

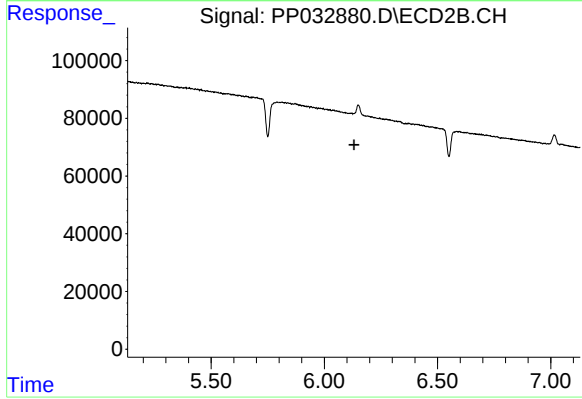

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.131 min
Response: 0
Conc: N.D.

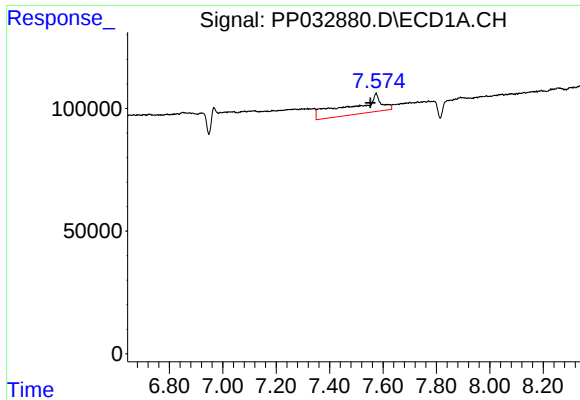

#28 AR-1254-3


R.T.: 7.574 min
Delta R.T.: 0.021 min
Response: 598210
Conc: 222.03 ng/ml

Instrument :
ECD_P
ClientSampleId :

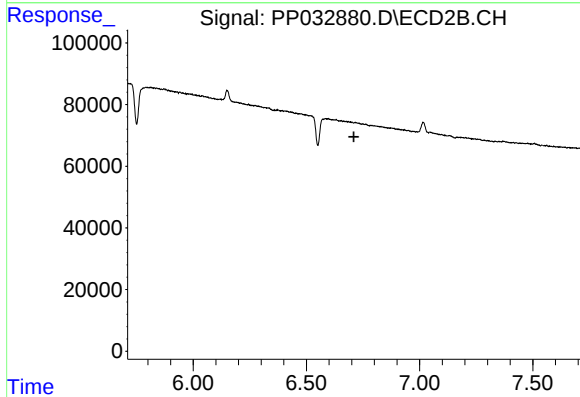


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

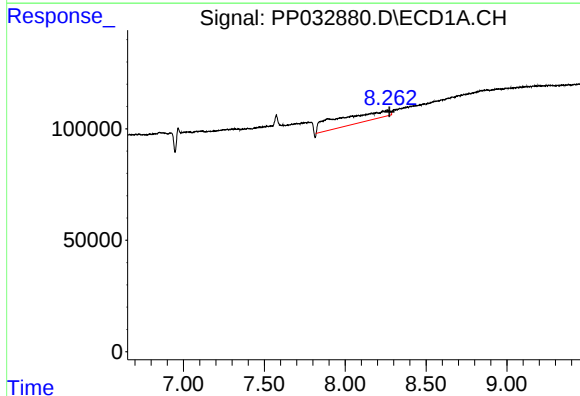


#30 AR-1254-5

R.T.: 8.256 min
Delta R.T.: -0.018 min
Response: 972101
Conc: 466.14 ng/ml

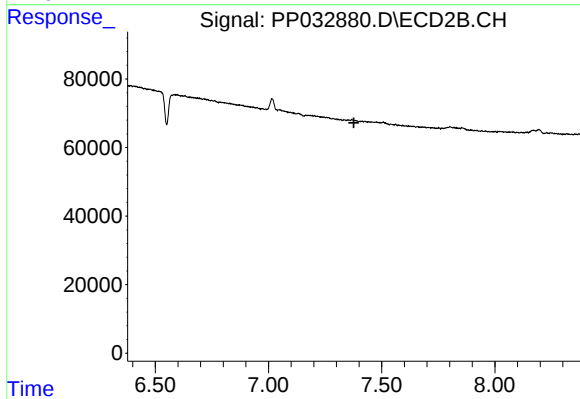

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

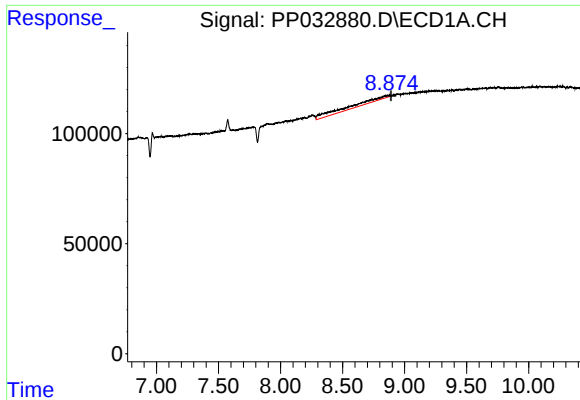

#35 AR-1260-5


R.T.: 8.876 min
Delta R.T.: -0.015 min
Response: 434016
Conc: 95.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

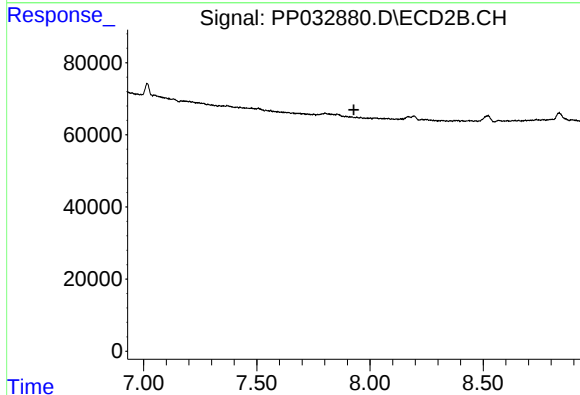


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.928 min
Response: 0
Conc: N.D.

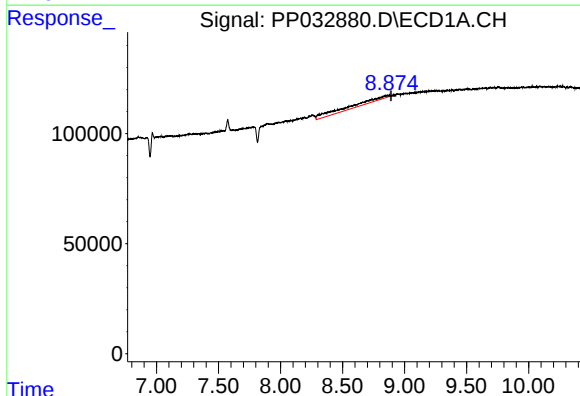

#37 AR-1262-2

R.T.: 8.876 min
Delta R.T.: -0.015 min
Response: 434016
Conc: 85.68 ng/ml

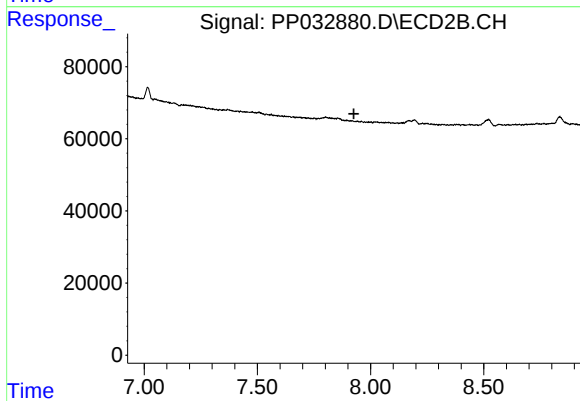

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.927 min
Response: 0
Conc: N.D.