

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032882.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 9:55
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:29:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.738	4.007	1435243	974359	24.711	20.713
2)	SA Decachlor...	10.576	9.287	1024895	837578	25.977	22.358
Target Compounds							
24)	L5 AR-1248-4	6.950f	0.000	25675	0	15.830	N.D. #
26)	L6 AR-1254-1	6.950	0.000	25675	0	15.459	N.D. #
28)	L6 AR-1254-3	7.561	0.000	20973	0	7.784	N.D. #
35)	L7 AR-1260-5	8.892	0.000	81839	0	18.066	N.D. #
37)	L8 AR-1262-2	8.892	0.000	81839	0	16.155	N.D. #
40)	L8 AR-1262-5	9.895	0.000	100203	0	55.228	N.D. #
44)	L9 AR-1268-4	9.895	0.000	100203	0	48.859	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032882.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 9:55
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:29:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

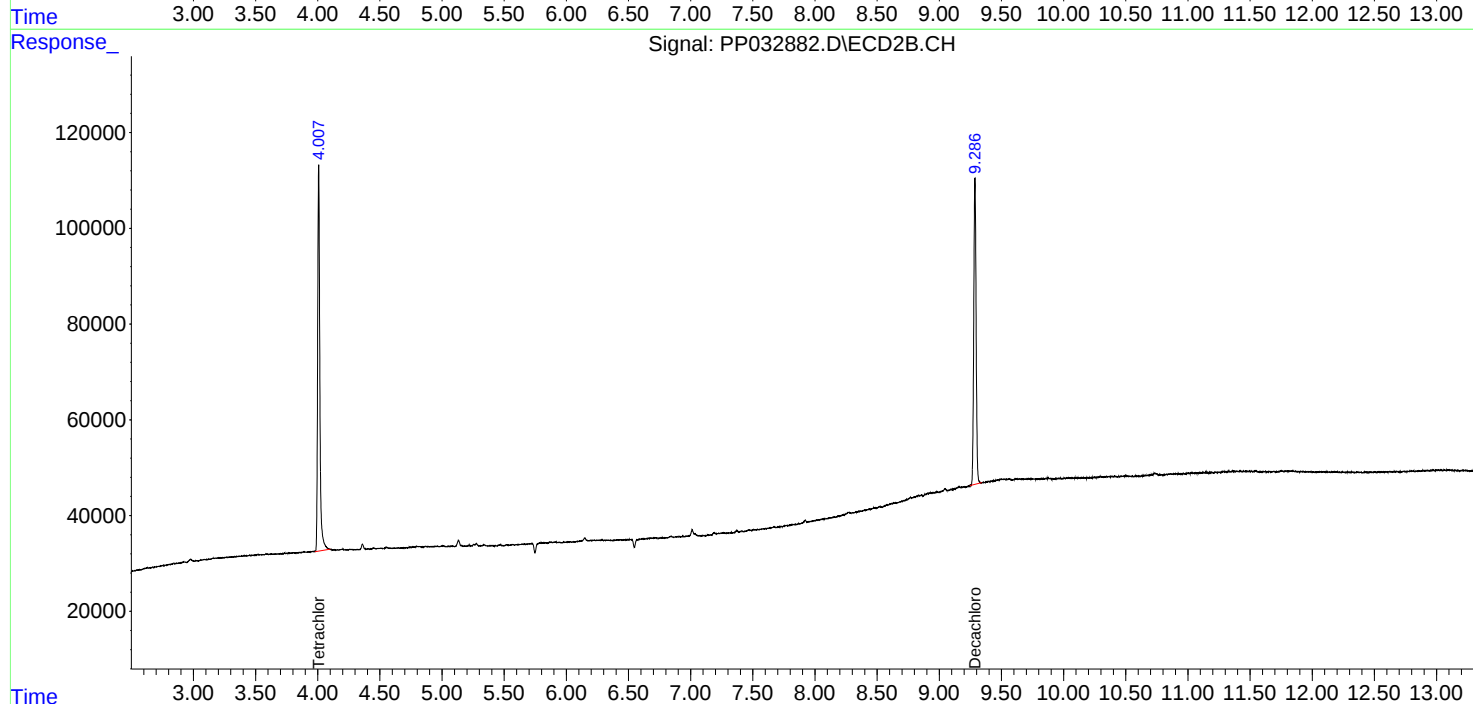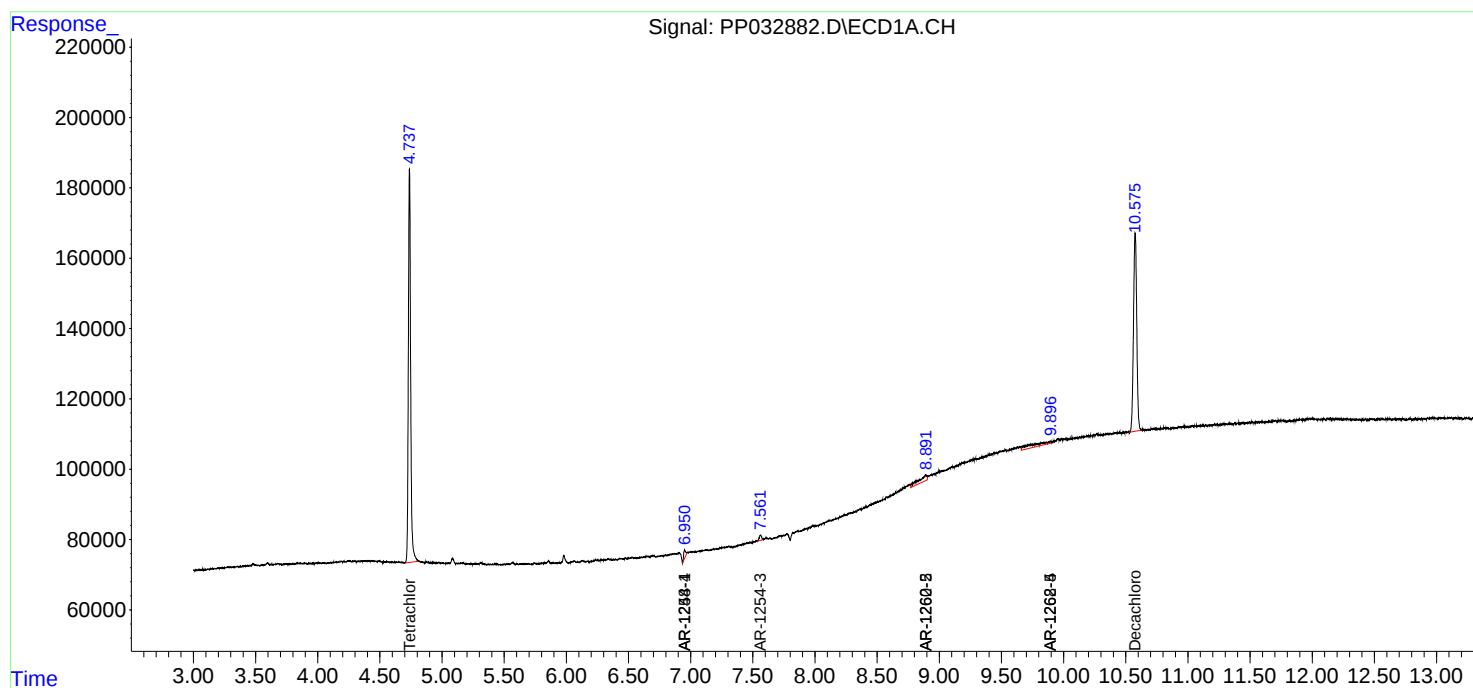


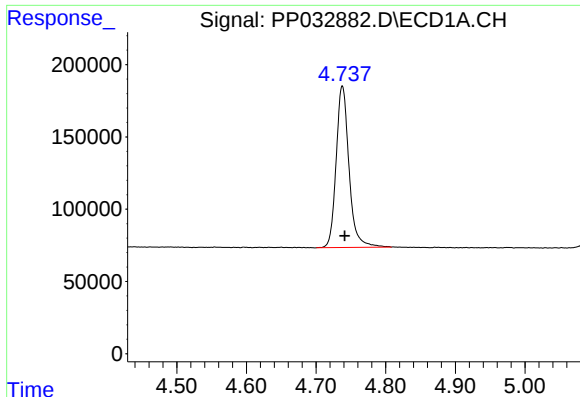

#1 Tetrachloro-m-xylene


R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1435243
Conc: 24.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

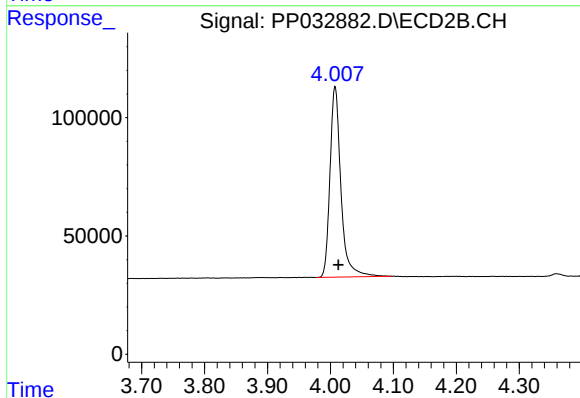


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.005 min
Response: 974359
Conc: 20.71 ng/ml

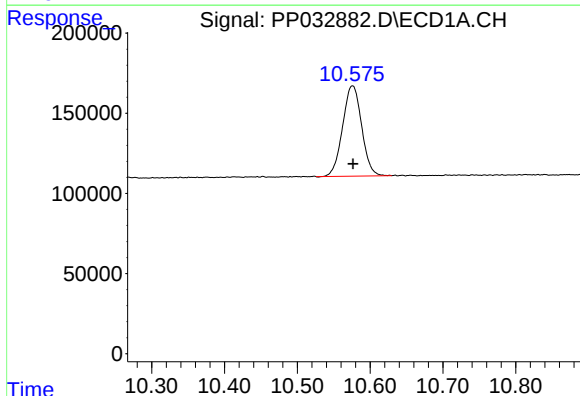


#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: 0.000 min
Response: 1024895
Conc: 25.98 ng/ml

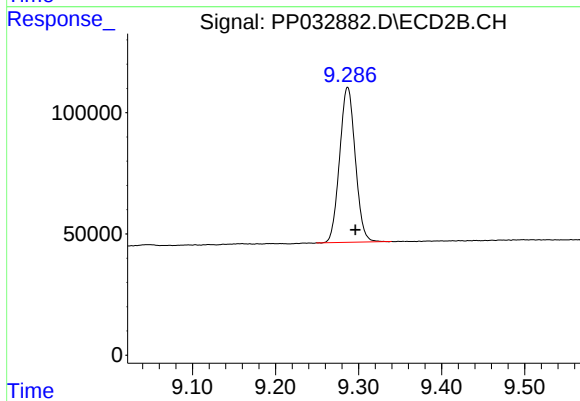

#2 Decachlorobiphenyl


R.T.: 9.287 min
Delta R.T.: -0.009 min
Response: 837578
Conc: 22.36 ng/ml

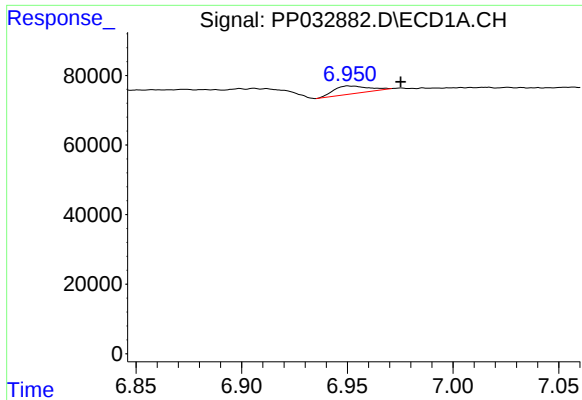

#24 AR-1248-4


R.T.: 6.950 min
Delta R.T.: -0.025 min
Response: 25675
Conc: 15.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

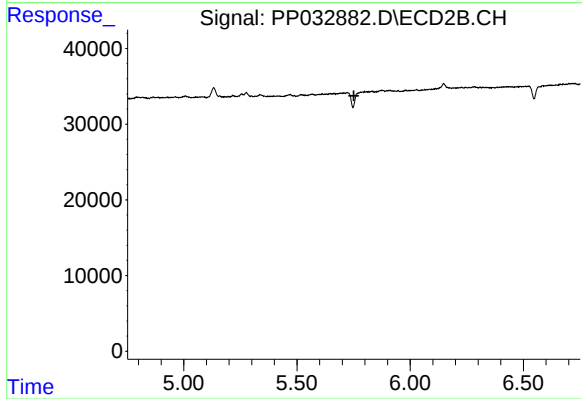


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

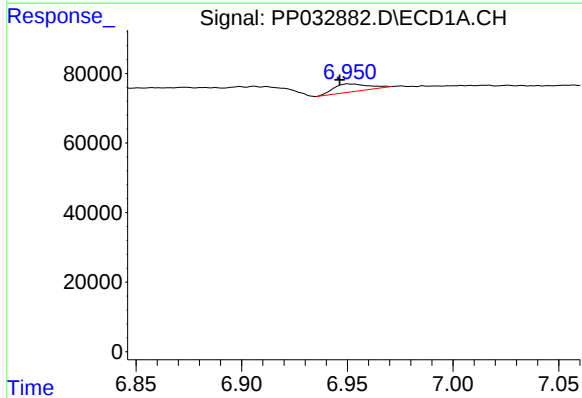


#26 AR-1254-1

R.T.: 6.950 min
Delta R.T.: 0.004 min
Response: 25675
Conc: 15.46 ng/ml

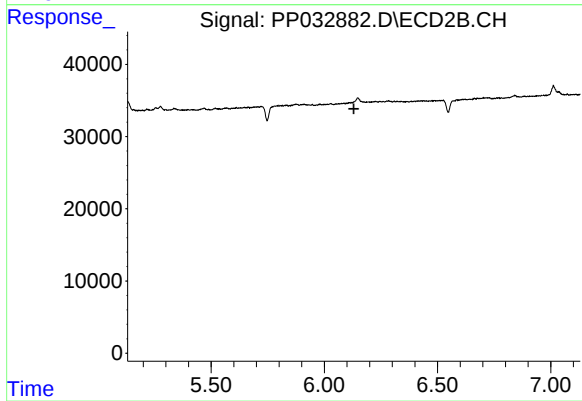

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.131 min
Response: 0
Conc: N.D.

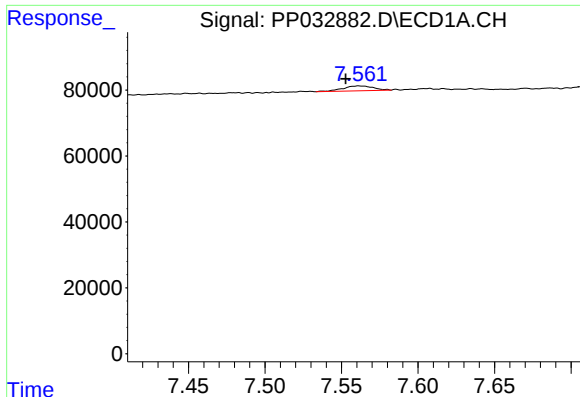

#28 AR-1254-3


R.T.: 7.561 min
Delta R.T.: 0.009 min
Response: 20973
Conc: 7.78 ng/ml

Instrument :
ECD_P
ClientSampleId :

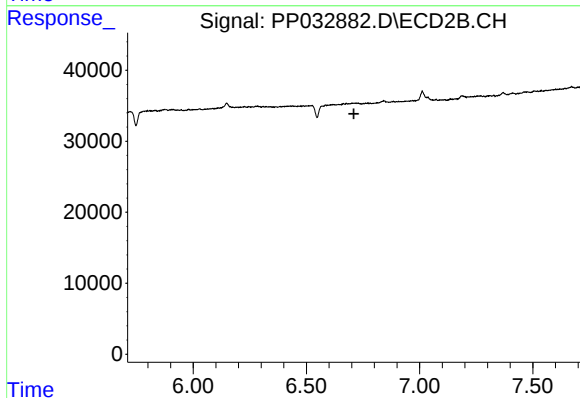


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

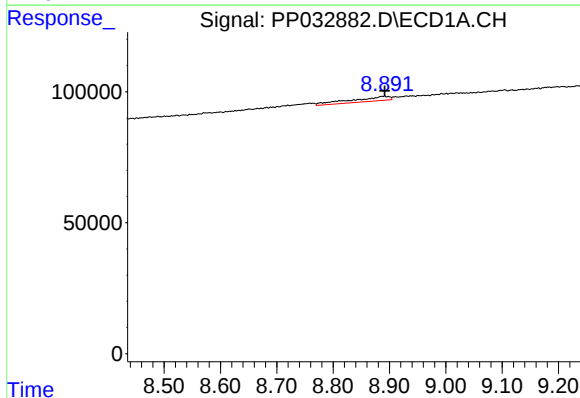


#35 AR-1260-5

R.T.: 8.892 min
Delta R.T.: 0.000 min
Response: 81839
Conc: 18.07 ng/ml

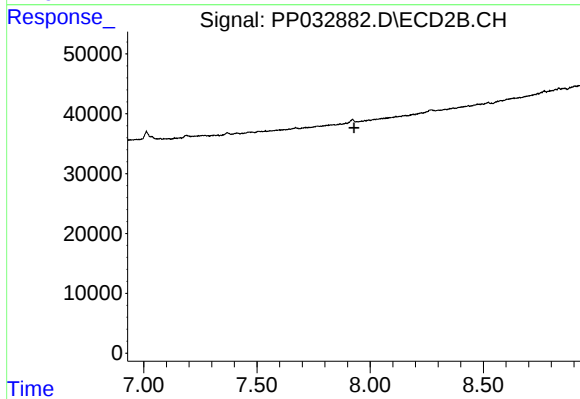

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.928 min
Response: 0
Conc: N.D.

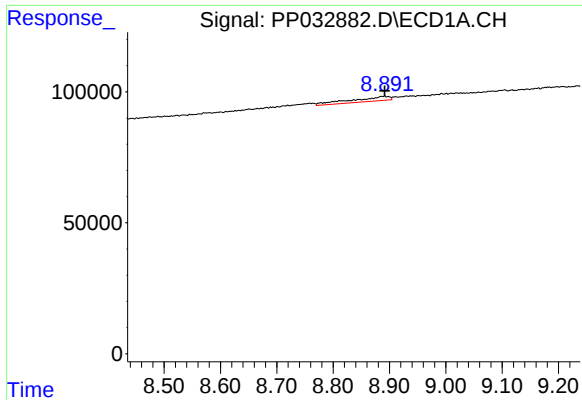

#37 AR-1262-2


R.T.: 8.892 min
Delta R.T.: 0.000 min
Response: 81839
Conc: 16.16 ng/ml

Instrument :
ECD_P
ClientSampleId :

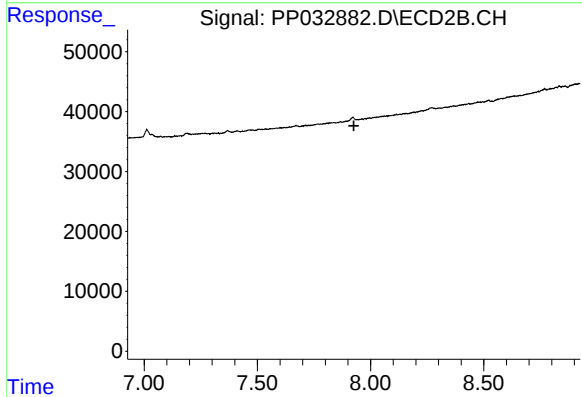


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.927 min
Response: 0
Conc: N.D.

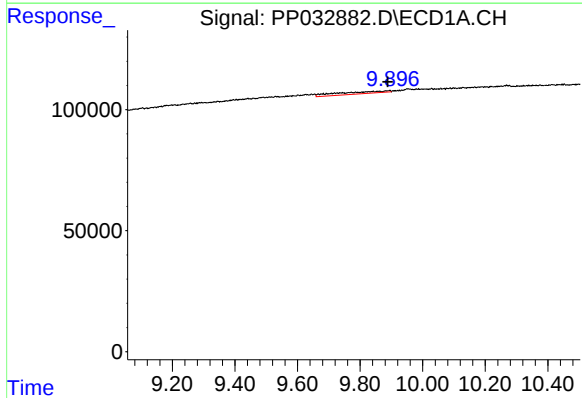


#40 AR-1262-5

R.T.: 9.895 min
Delta R.T.: 0.006 min
Response: 100203
Conc: 55.23 ng/ml

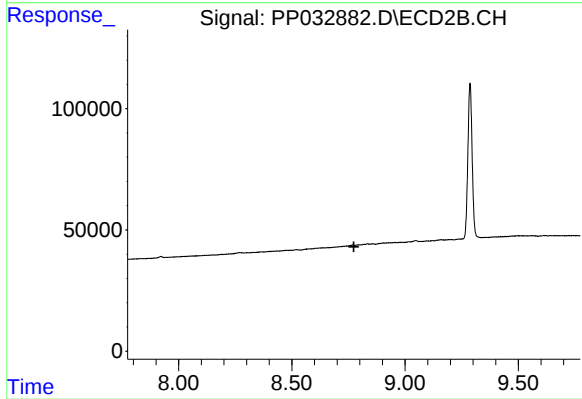

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.774 min
Response: 0
Conc: N.D.

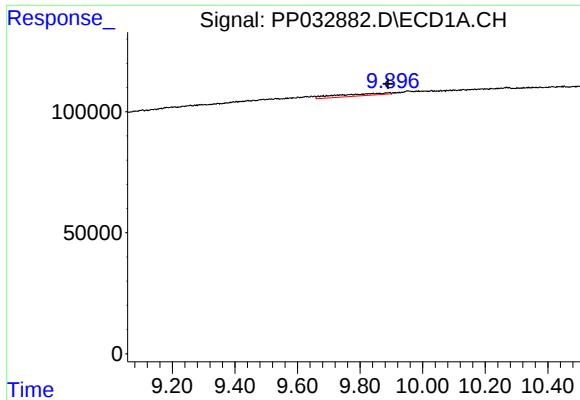

#44 AR-1268-4

R.T.: 9.895 min
Delta R.T.: 0.006 min
Response: 100203
Conc: 48.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

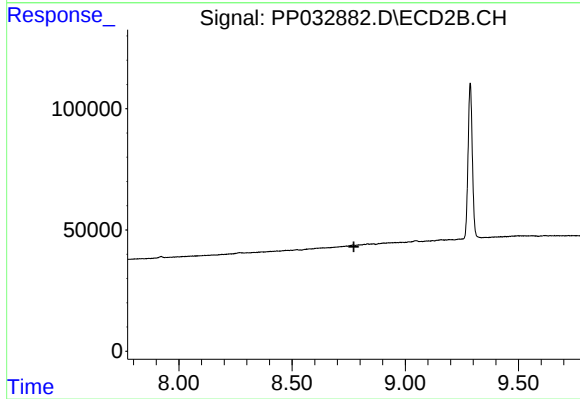

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.773 min
Response: 0
Conc: N.D.