

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032895.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 16:42
 Operator : DD\AJ
 Sample : M1188-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-230

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:49:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:35:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.738	4.007	1201418	1037187	20.685	22.049
2) SA Decachlor...	10.574	9.285	681924	634822	17.284	16.946
Target Compounds						
31) L7 AR-1260-1	7.715	6.837	67756	75980	35.542m	39.830m
32) L7 AR-1260-2	7.980	7.035	167484	165548	69.346	72.645
33) L7 AR-1260-3	8.346	7.191	89081	69830	44.196	31.934m#
34) L7 AR-1260-4	8.572	7.671	83437	71490	40.494m	39.123
35) L7 AR-1260-5	8.888	7.920	188557	204310	41.625	47.496

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032895.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 16:42
Operator : DD\AJ
Sample : M1188-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-230


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:35:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

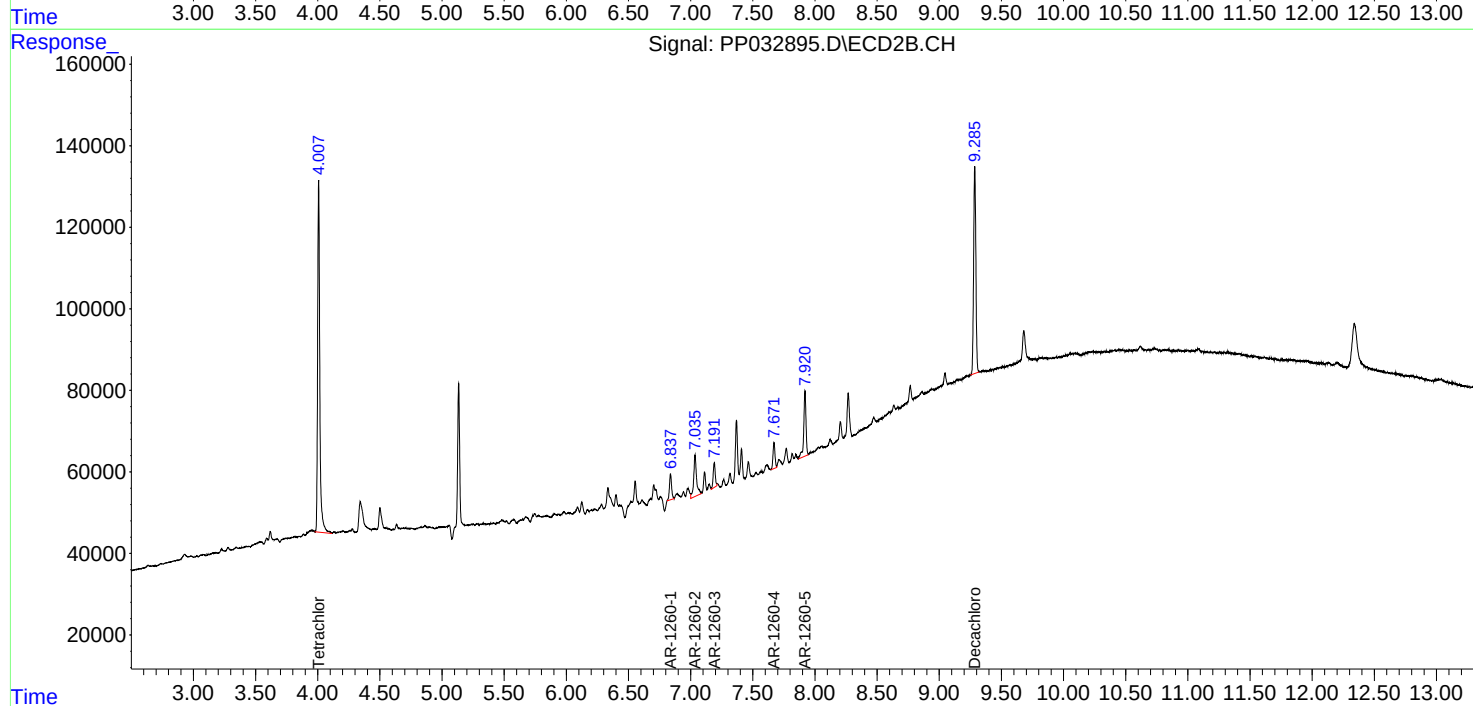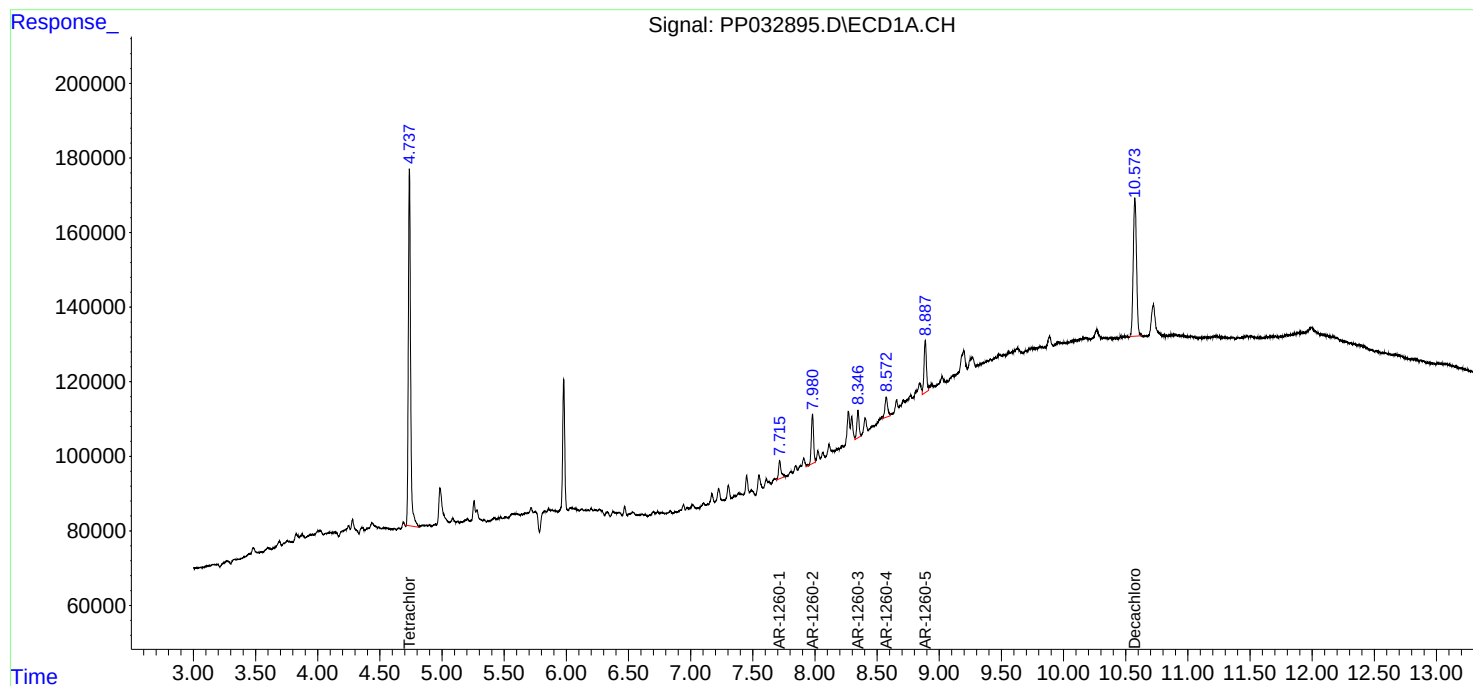

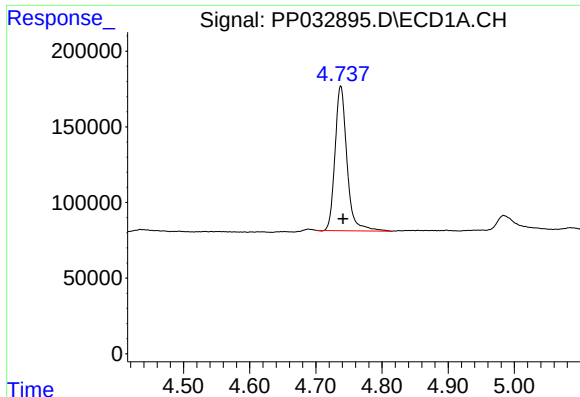


#1 Tetrachloro-m-xylene

R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1201418
Conc: 20.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:28 AM

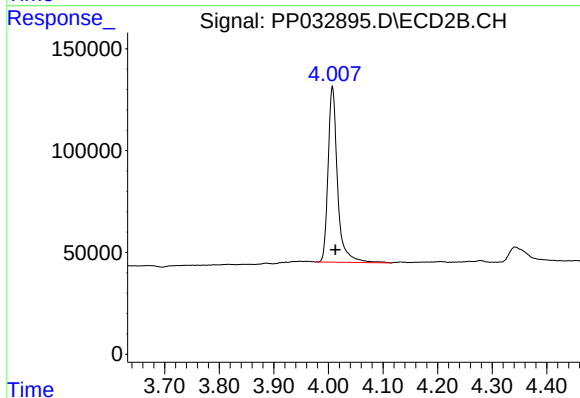


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.005 min
Response: 1037187
Conc: 22.05 ng/ml

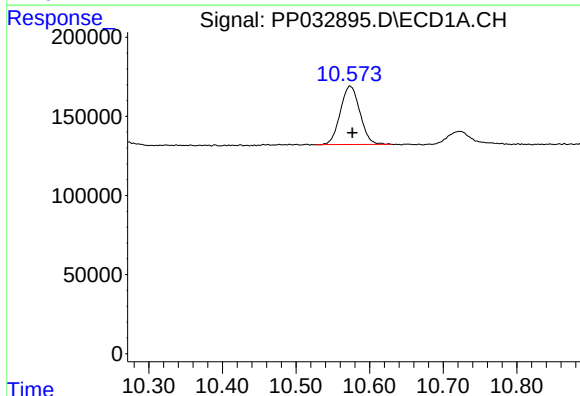


#2 Decachlorobiphenyl

R.T.: 10.574 min
Delta R.T.: -0.003 min
Response: 681924
Conc: 17.28 ng/ml

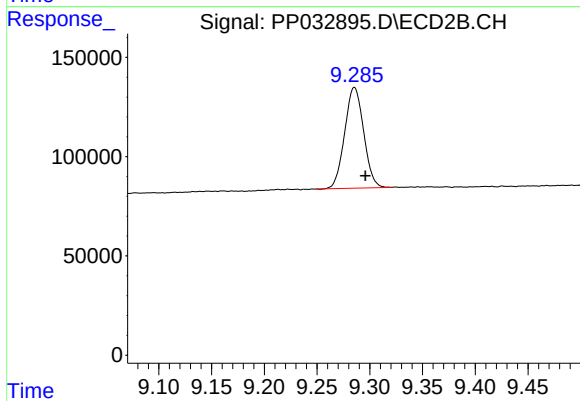

#2 Decachlorobiphenyl

R.T.: 9.285 min
Delta R.T.: -0.011 min
Response: 634822
Conc: 16.95 ng/ml

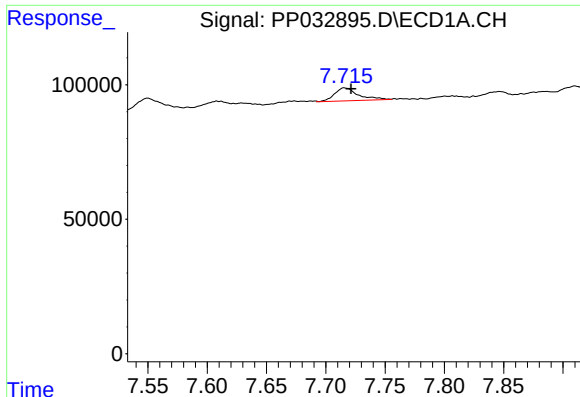


#31 AR-1260-1

R.T.: 7.715 min
Delta R.T.: -0.007 min
Response: 67756
Conc: 35.54 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TP-230


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:28 AM

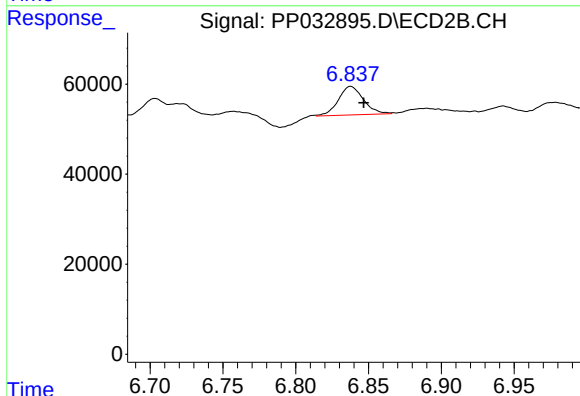


#31 AR-1260-1

R.T.: 6.837 min
Delta R.T.: -0.009 min
Response: 75980
Conc: 39.83 ng/ml m

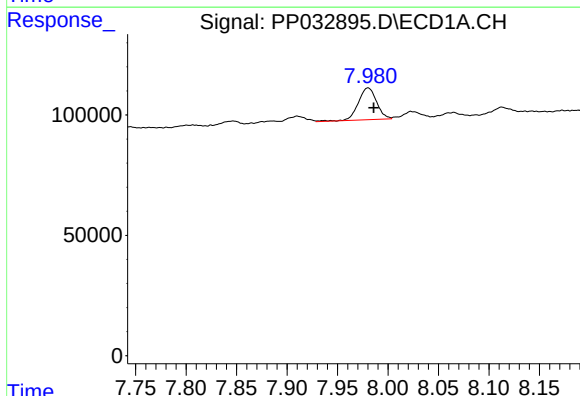


#32 AR-1260-2

R.T.: 7.980 min
Delta R.T.: -0.006 min
Response: 167484
Conc: 69.35 ng/ml

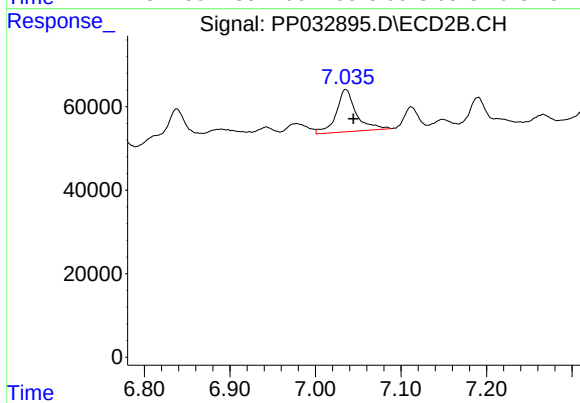

#32 AR-1260-2

R.T.: 7.035 min
Delta R.T.: -0.009 min
Response: 165548
Conc: 72.65 ng/ml

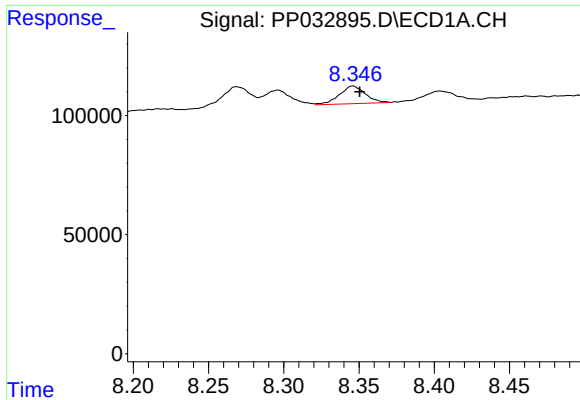


#33 AR-1260-3

R.T.: 8.346 min
Delta R.T.: -0.004 min
Response: 89081
Conc: 44.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:28 AM

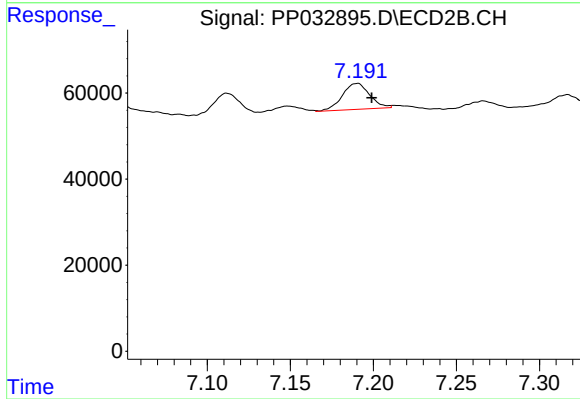


#33 AR-1260-3

R.T.: 7.191 min
Delta R.T.: -0.008 min
Response: 69830
Conc: 31.93 ng/ml m

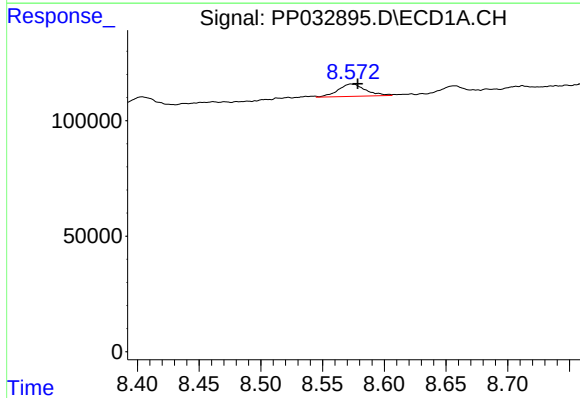


#34 AR-1260-4

R.T.: 8.572 min
Delta R.T.: -0.006 min
Response: 83437
Conc: 40.49 ng/ml m

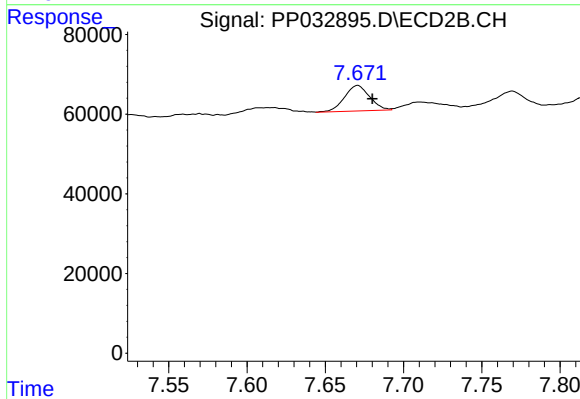

#34 AR-1260-4

R.T.: 7.671 min
Delta R.T.: -0.009 min
Response: 71490
Conc: 39.12 ng/ml

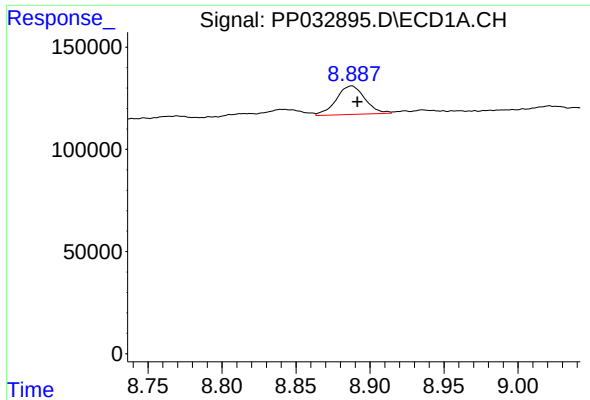


#35 AR-1260-5

R.T.: 8.888 min
Delta R.T.: -0.004 min
Response: 188557
Conc: 41.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230

Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:28 AM

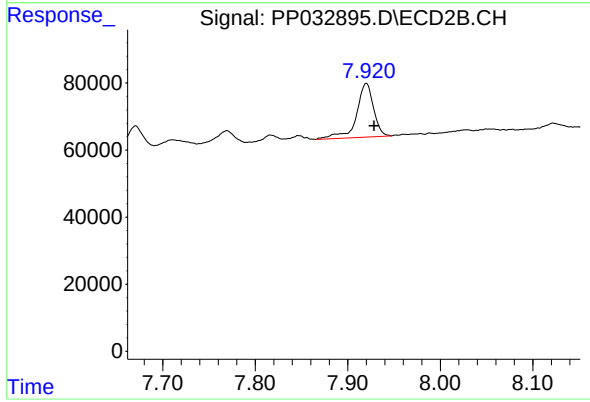

#35 AR-1260-5

R.T.: 7.920 min
Delta R.T.: -0.008 min
Response: 204310
Conc: 47.50 ng/ml