

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032896.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 16:59
 Operator : DD\AJ
 Sample : M1188-02MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-230MS

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:49:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:36:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.738	4.007	1151504	907979	19.826	19.302m
2)	SA Decachlor...	10.574	9.286	757532	675514	19.201	18.032
Target Compounds							
3)	L1 AR-1016-1	6.039	5.255	712790	590058	438.752	434.405
4)	L1 AR-1016-2	6.062	5.275	1020886	824913	413.148	406.701
5)	L1 AR-1016-3	6.127	5.466	624418	475748	420.328	435.418
6)	L1 AR-1016-4	6.233	5.517	491098	338717	394.570	418.415
7)	L1 AR-1016-5	6.546	5.746	456561	460921	402.305	427.790
31)	L7 AR-1260-1	7.716	6.838	852514	917393	447.194	480.912
32)	L7 AR-1260-2	7.981	7.035	1179700	1040751	488.452	456.698
33)	L7 AR-1260-3	8.347	7.189	799392	963514	396.602	440.620
34)	L7 AR-1260-4	8.575	7.671	871424	709782	422.929	388.430
35)	L7 AR-1260-5	8.888	7.920	1856721	1779020	409.879	413.565

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032896.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 16:59
Operator : DD\AJ
Sample : M1188-02MS
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:36:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

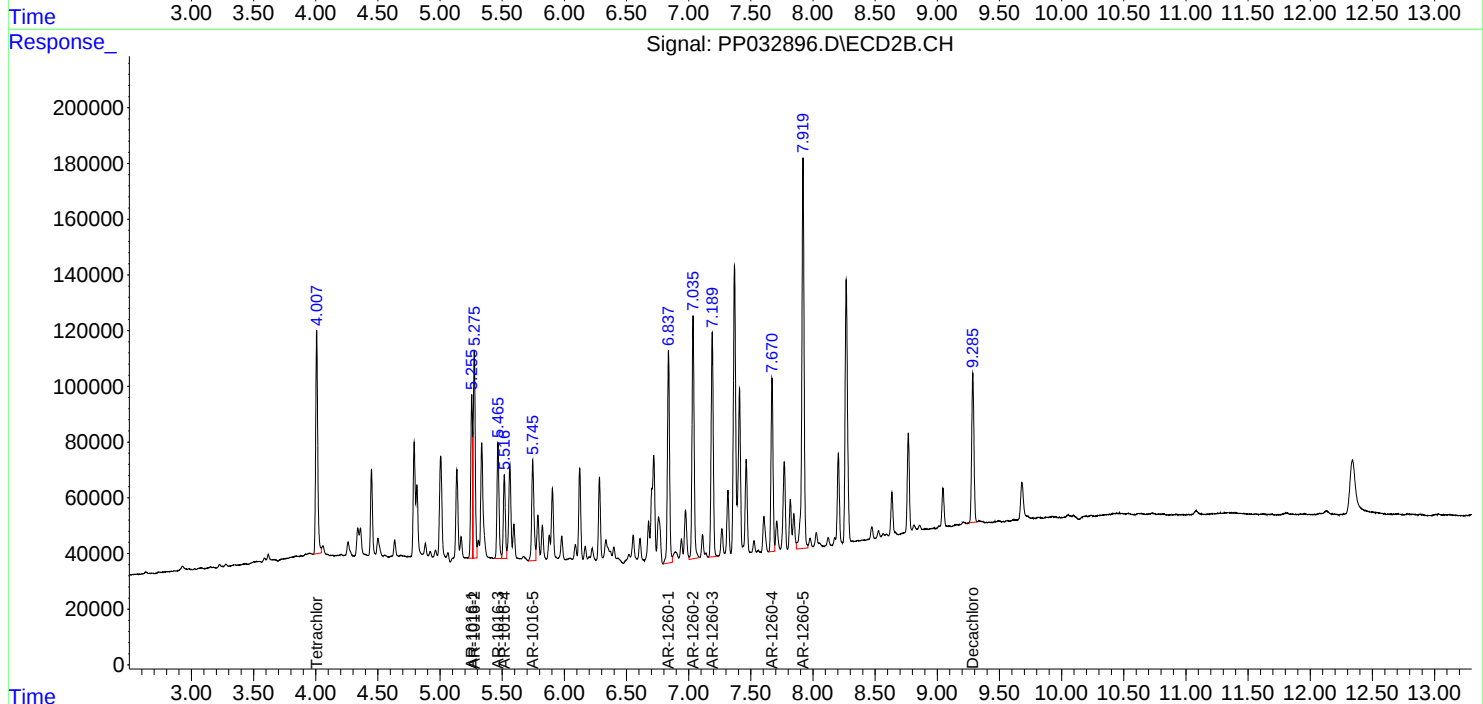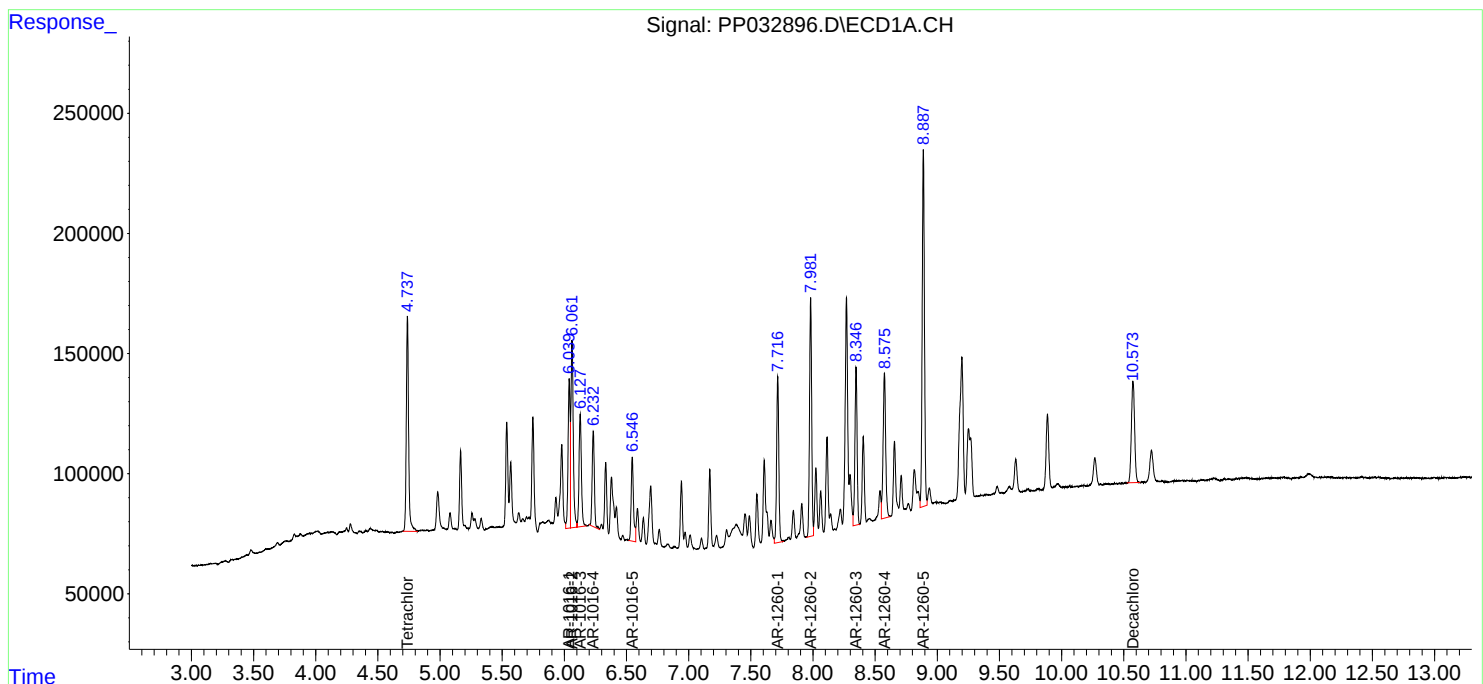

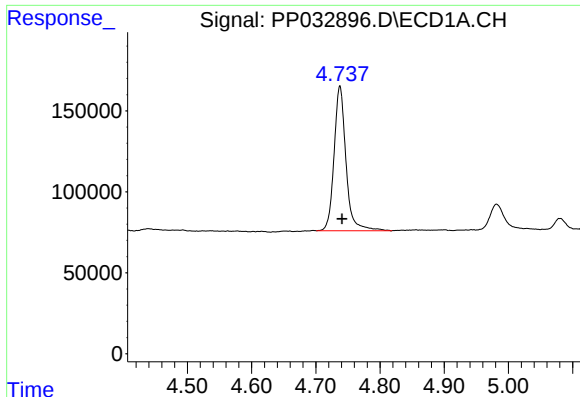


#1 Tetrachloro-m-xylene

R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1151504
Conc: 19.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

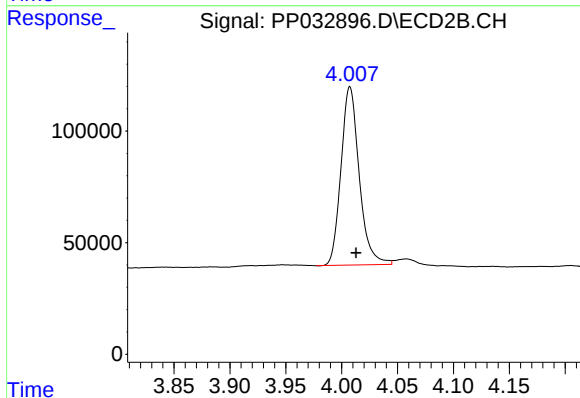


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.006 min
Response: 907979
Conc: 19.30 ng/ml m

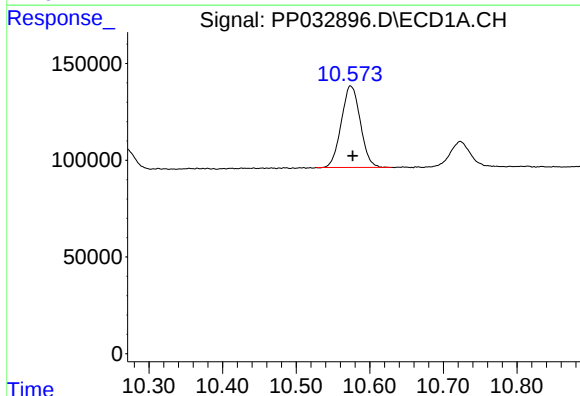


#2 Decachlorobiphenyl

R.T.: 10.574 min
Delta R.T.: -0.003 min
Response: 757532
Conc: 19.20 ng/ml

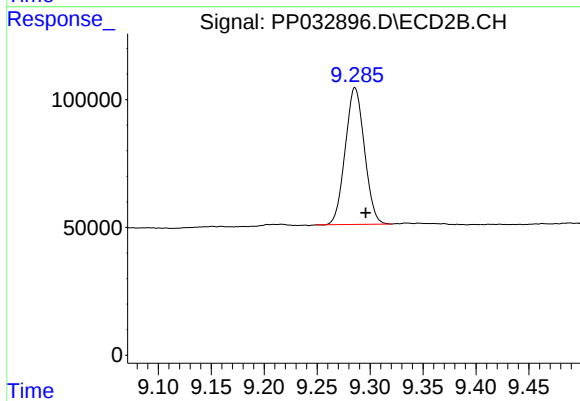

#2 Decachlorobiphenyl

R.T.: 9.286 min
Delta R.T.: -0.010 min
Response: 675514
Conc: 18.03 ng/ml

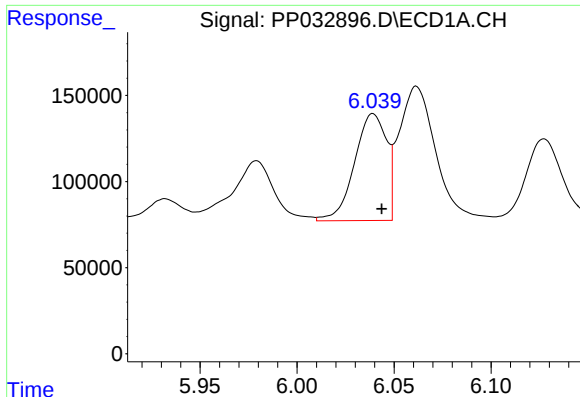


#3 AR-1016-1

R.T.: 6.039 min
Delta R.T.: -0.004 min
Response: 712790
Conc: 438.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

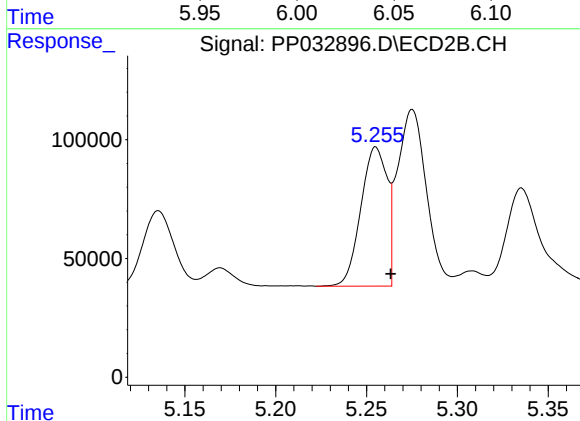


#3 AR-1016-1

R.T.: 5.255 min
Delta R.T.: -0.008 min
Response: 590058
Conc: 434.41 ng/ml

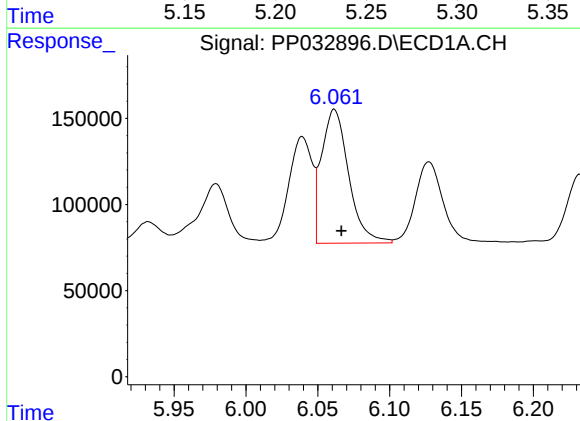


#4 AR-1016-2

R.T.: 6.062 min
Delta R.T.: -0.005 min
Response: 1020886
Conc: 413.15 ng/ml

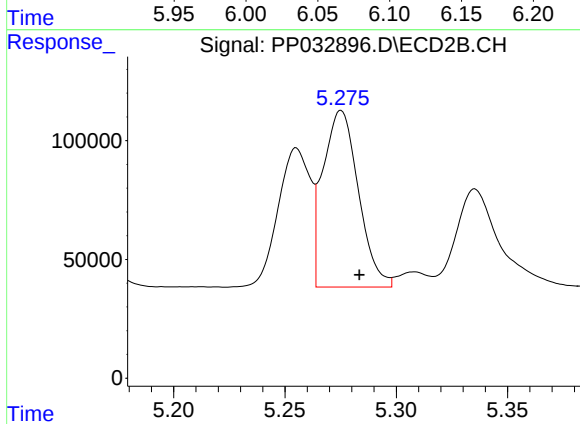

#4 AR-1016-2

R.T.: 5.275 min
Delta R.T.: -0.008 min
Response: 824913
Conc: 406.70 ng/ml

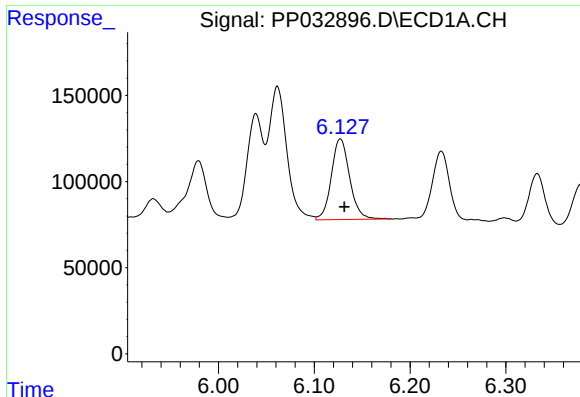


#5 AR-1016-3

R.T.: 6.127 min
Delta R.T.: -0.004 min
Response: 624418
Conc: 420.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

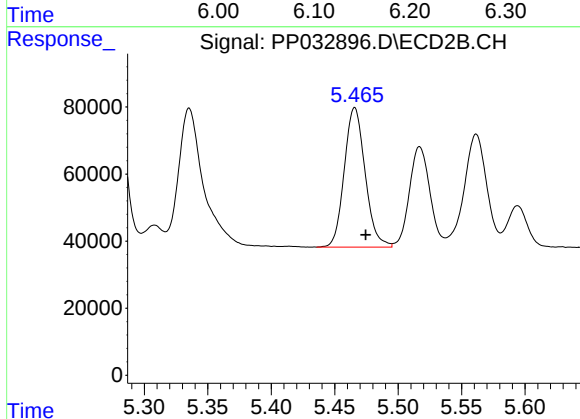


#5 AR-1016-3

R.T.: 5.466 min
Delta R.T.: -0.009 min
Response: 475748
Conc: 435.42 ng/ml

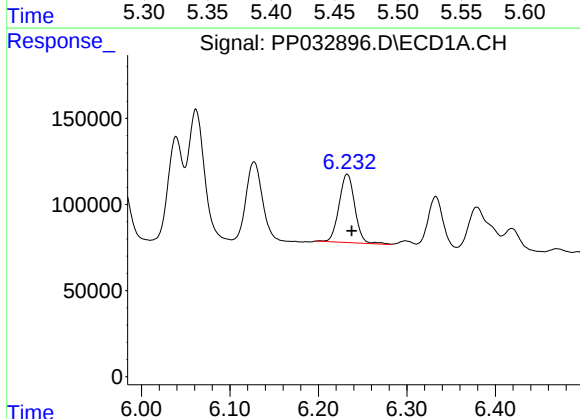


#6 AR-1016-4

R.T.: 6.233 min
Delta R.T.: -0.005 min
Response: 491098
Conc: 394.57 ng/ml

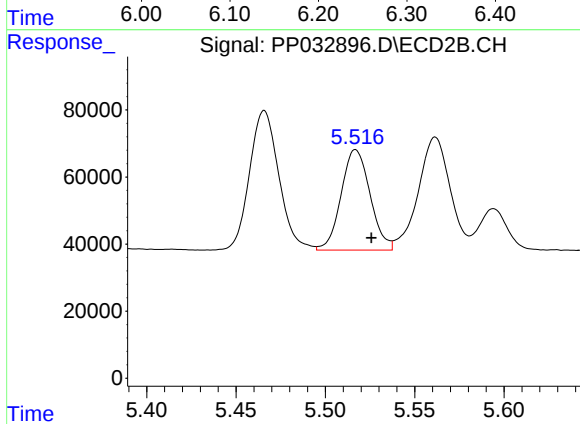

#6 AR-1016-4

R.T.: 5.517 min
Delta R.T.: -0.009 min
Response: 338717
Conc: 418.41 ng/ml

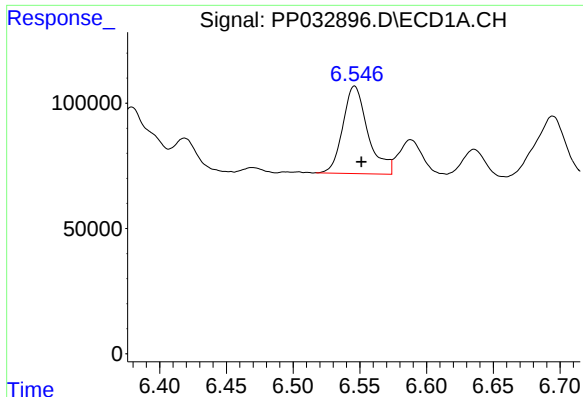


#7 AR-1016-5

R.T.: 6.546 min
Delta R.T.: -0.005 min
Response: 456561
Conc: 402.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

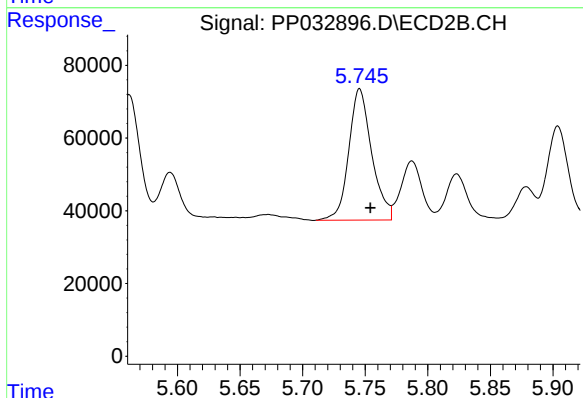


#7 AR-1016-5

R.T.: 5.746 min
Delta R.T.: -0.009 min
Response: 460921
Conc: 427.79 ng/ml

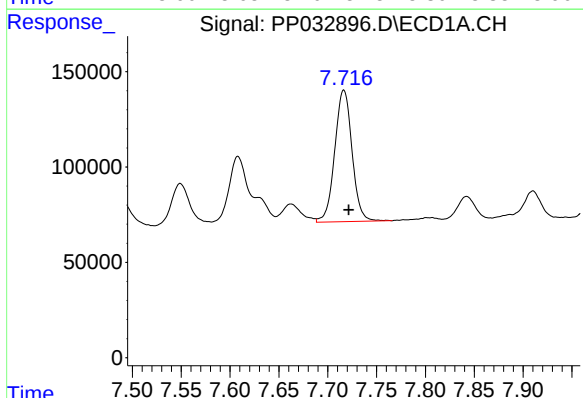


#31 AR-1260-1

R.T.: 7.716 min
Delta R.T.: -0.005 min
Response: 852514
Conc: 447.19 ng/ml

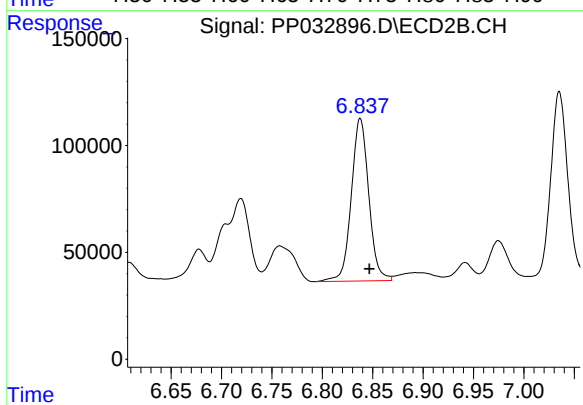

#31 AR-1260-1

R.T.: 6.838 min
Delta R.T.: -0.009 min
Response: 917393
Conc: 480.91 ng/ml

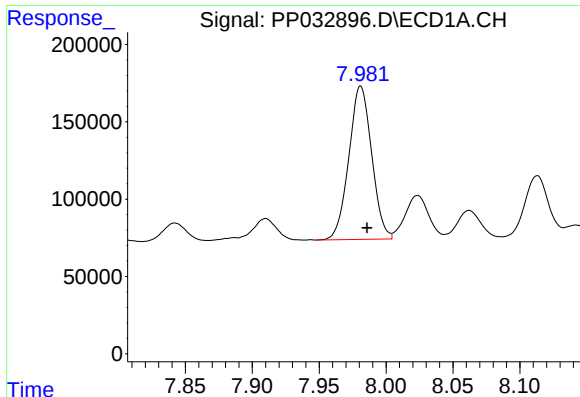


#32 AR-1260-2

R.T.: 7.981 min
Delta R.T.: -0.005 min
Response: 1179700
Conc: 488.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

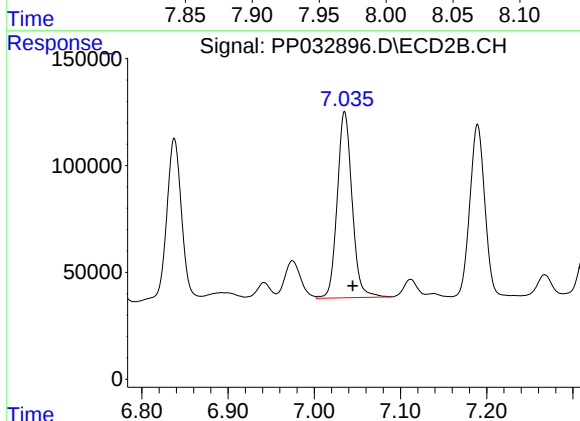


#32 AR-1260-2

R.T.: 7.035 min
Delta R.T.: -0.009 min
Response: 1040751
Conc: 456.70 ng/ml

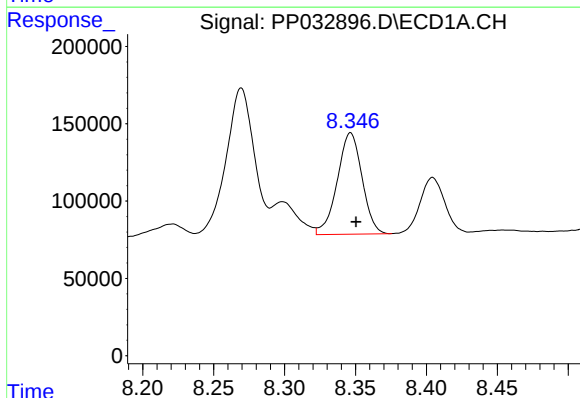


#33 AR-1260-3

R.T.: 8.347 min
Delta R.T.: -0.004 min
Response: 799392
Conc: 396.60 ng/ml

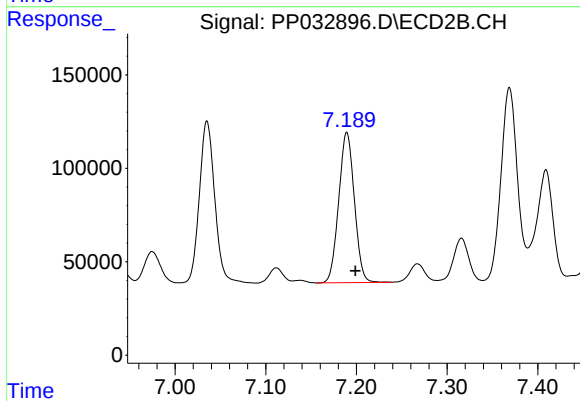

#33 AR-1260-3

R.T.: 7.189 min
Delta R.T.: -0.009 min
Response: 963514
Conc: 440.62 ng/ml

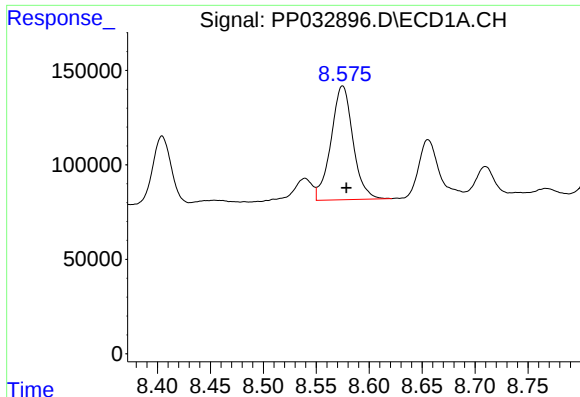


#34 AR-1260-4

R.T.: 8.575 min
Delta R.T.: -0.004 min
Response: 871424
Conc: 422.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-230MS


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:30 AM

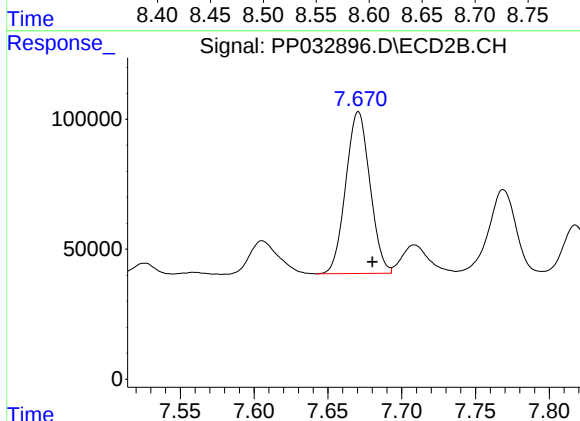


#34 AR-1260-4

R.T.: 7.671 min
Delta R.T.: -0.009 min
Response: 709782
Conc: 388.43 ng/ml

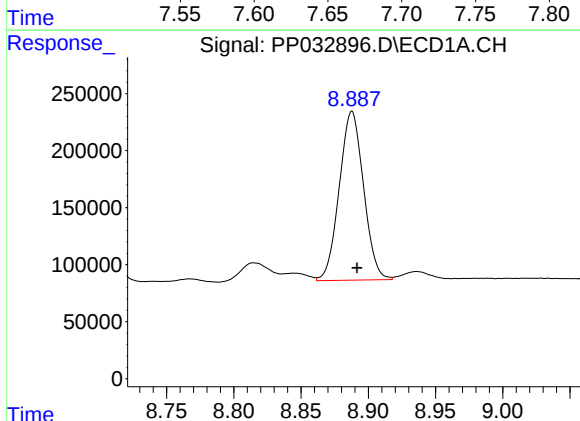

#35 AR-1260-5

R.T.: 8.888 min
Delta R.T.: -0.004 min
Response: 1856721
Conc: 409.88 ng/ml

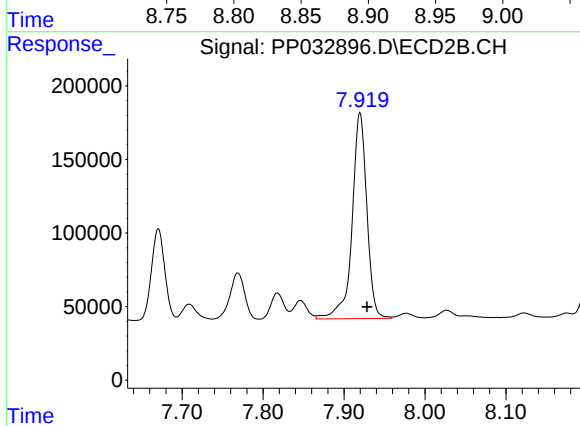

#35 AR-1260-5

R.T.: 7.920 min
Delta R.T.: -0.009 min
Response: 1779020
Conc: 413.56 ng/ml