

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 20:22
 Operator : DD\AJ
 Sample : M1189-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 41108

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:49:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:41:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.739	4.011	1128790	896133	19.435m	19.050m
2) SA Decachlor...	10.585	9.295	1083368	2241608	27.459m	59.836 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 20:22
Operator : DD\AJ
Sample : M1189-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
41108


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:41:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

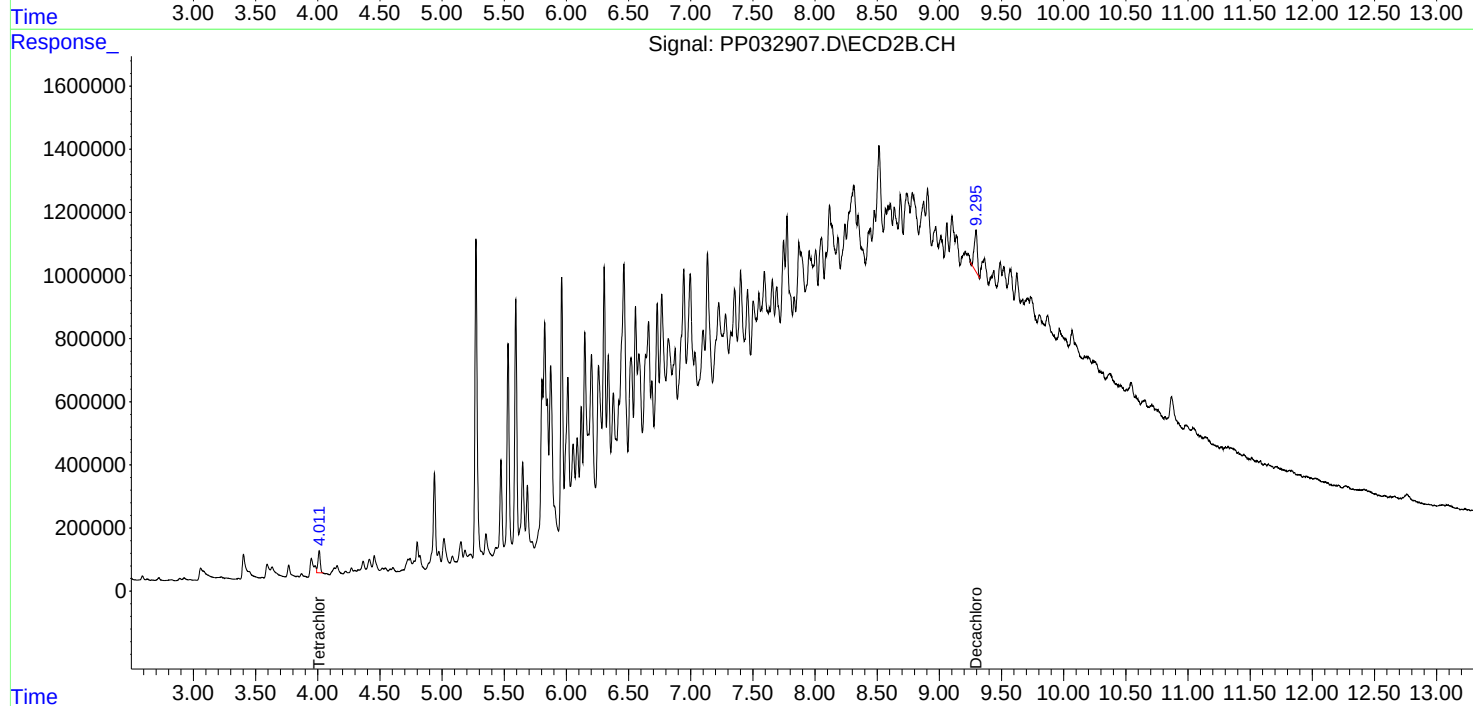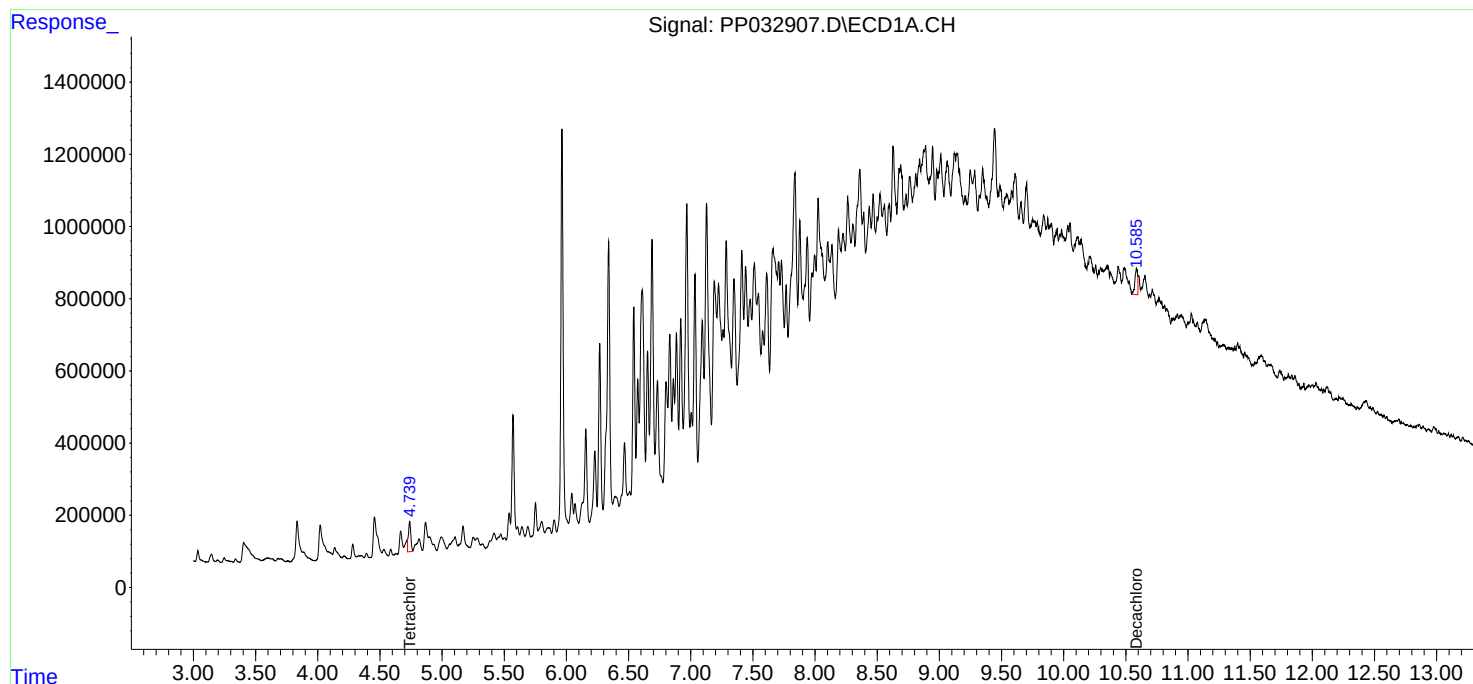

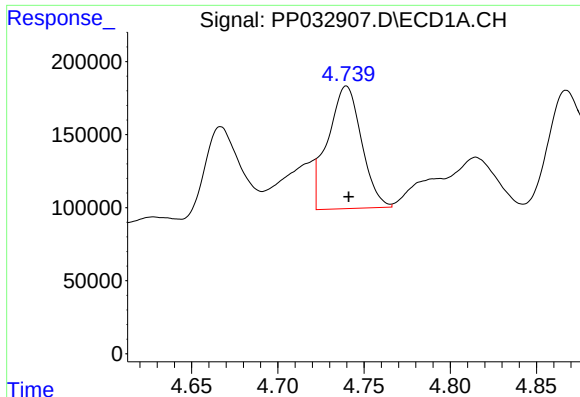


#1 Tetrachloro-m-xylene

R.T.: 4.739 min
Delta R.T.: -0.002 min
Response: 1128790
Conc: 19.43 ng/ml m

Instrument :
ECD_P
ClientSampleId :
41108


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:44 AM

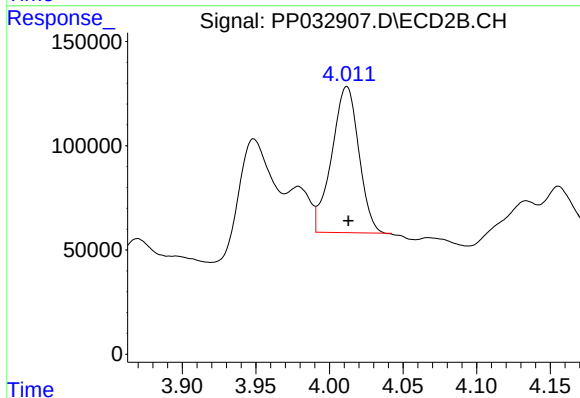


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.001 min
Response: 896133
Conc: 19.05 ng/ml m

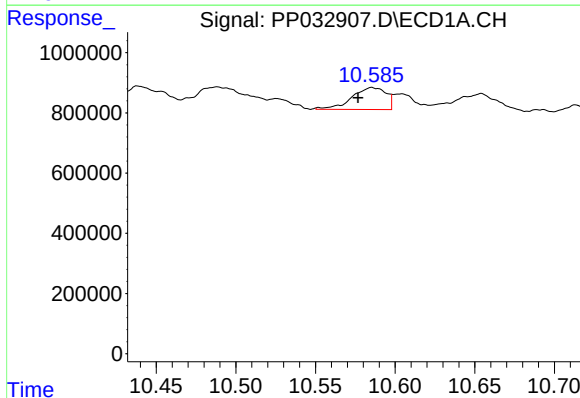

#2 Decachlorobiphenyl

R.T.: 10.585 min
Delta R.T.: 0.008 min
Response: 1083368
Conc: 27.46 ng/ml m

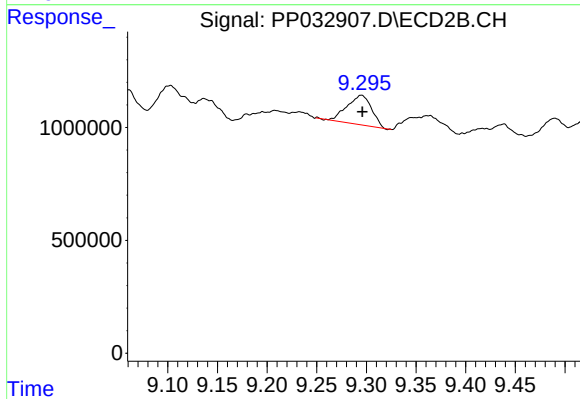

#2 Decachlorobiphenyl

R.T.: 9.295 min
Delta R.T.: 0.000 min
Response: 2241608
Conc: 59.84 ng/ml