

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032909.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 20:56
 Operator : DD\AJ
 Sample : M1189-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 41041

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:49:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:42:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.741	4.014	943044	881715	16.237m	18.744
2) SA Decachlor...	10.590	9.302	1299730	756912	32.943m	20.205 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032909.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 20:56
Operator : DD\AJ
Sample : M1189-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
41041


Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:42:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

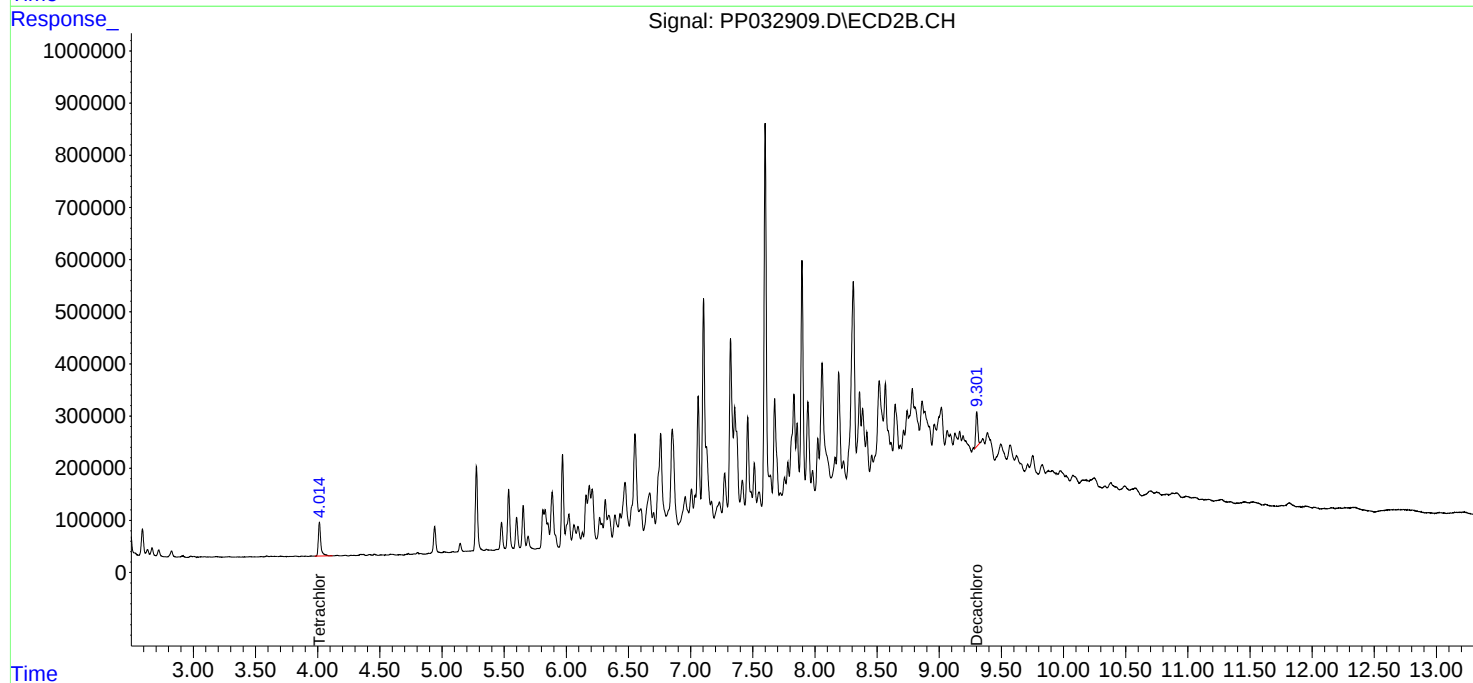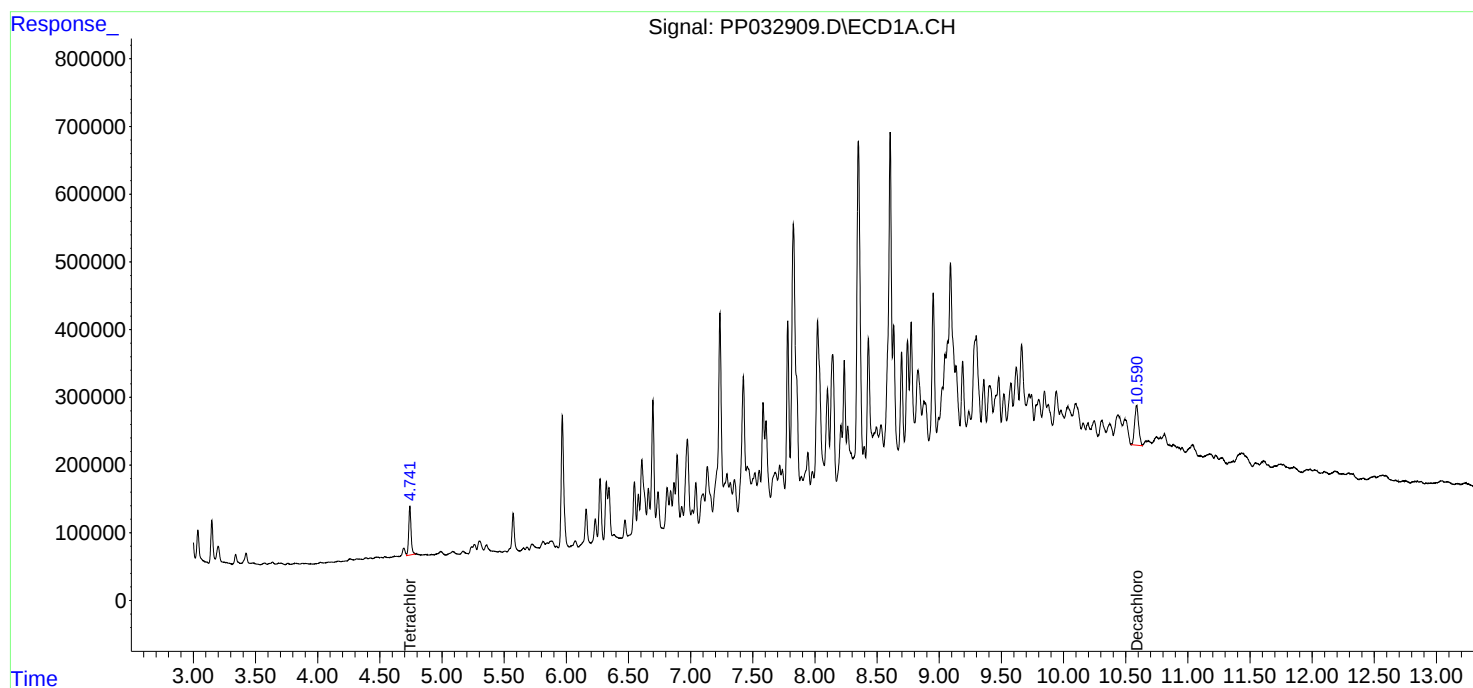

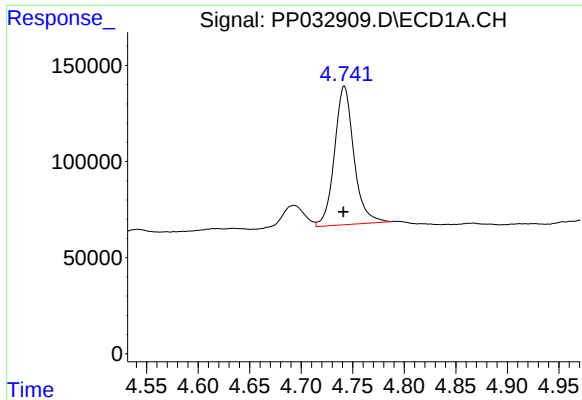

#1 Tetrachloro-m-xylene

R.T.: 4.741 min

Delta R.T.: 0.000 min


Response: 943044

Conc: 16.24 ng/ml m

Instrument :
ECD_P
ClientSampleId :
41041

Manual Integrations
APPROVED

Ankita
1/25/2021 10:49:45 AM

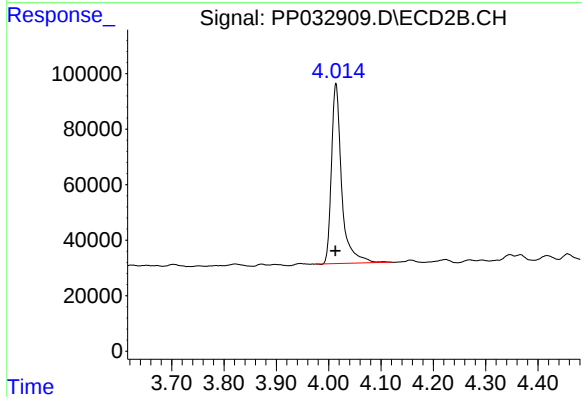


#1 Tetrachloro-m-xylene

R.T.: 4.014 min

Delta R.T.: 0.001 min

Response: 881715

Conc: 18.74 ng/ml

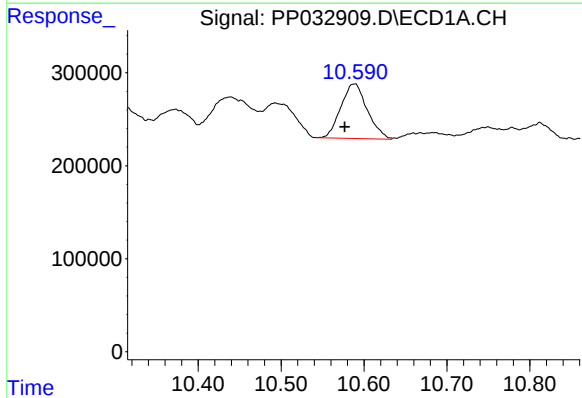


#2 Decachlorobiphenyl

R.T.: 10.590 min

Delta R.T.: 0.013 min

Response: 1299730

Conc: 32.94 ng/ml m

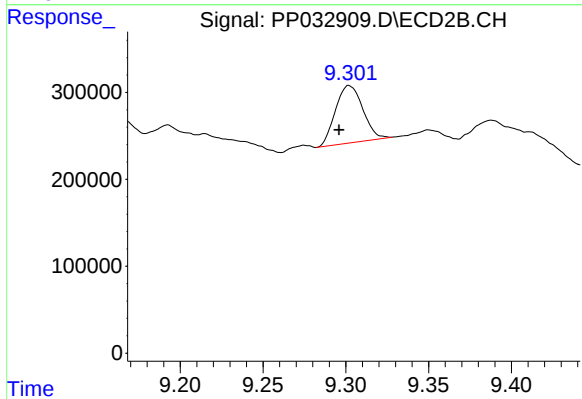

#2 Decachlorobiphenyl

R.T.: 9.302 min

Delta R.T.: 0.006 min

Response: 756912

Conc: 20.20 ng/ml