

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
 Data File : PP032911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 21:30
 Operator : DD\AJ
 Sample : M1189-07 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 41108

Manual Integrations
 APPROVED

Ankita
 1/25/2021 2:34:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:43:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.737	4.005	118230	108818	2.036m	2.313
2) SA Decachlor...	10.563	9.284	79294	215463	2.010m	5.751 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012221\
Data File : PP032911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 21:30
Operator : DD\AJ
Sample : M1189-07 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
41108


Manual Integrations
APPROVED

Ankita
1/25/2021 2:34:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:43:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

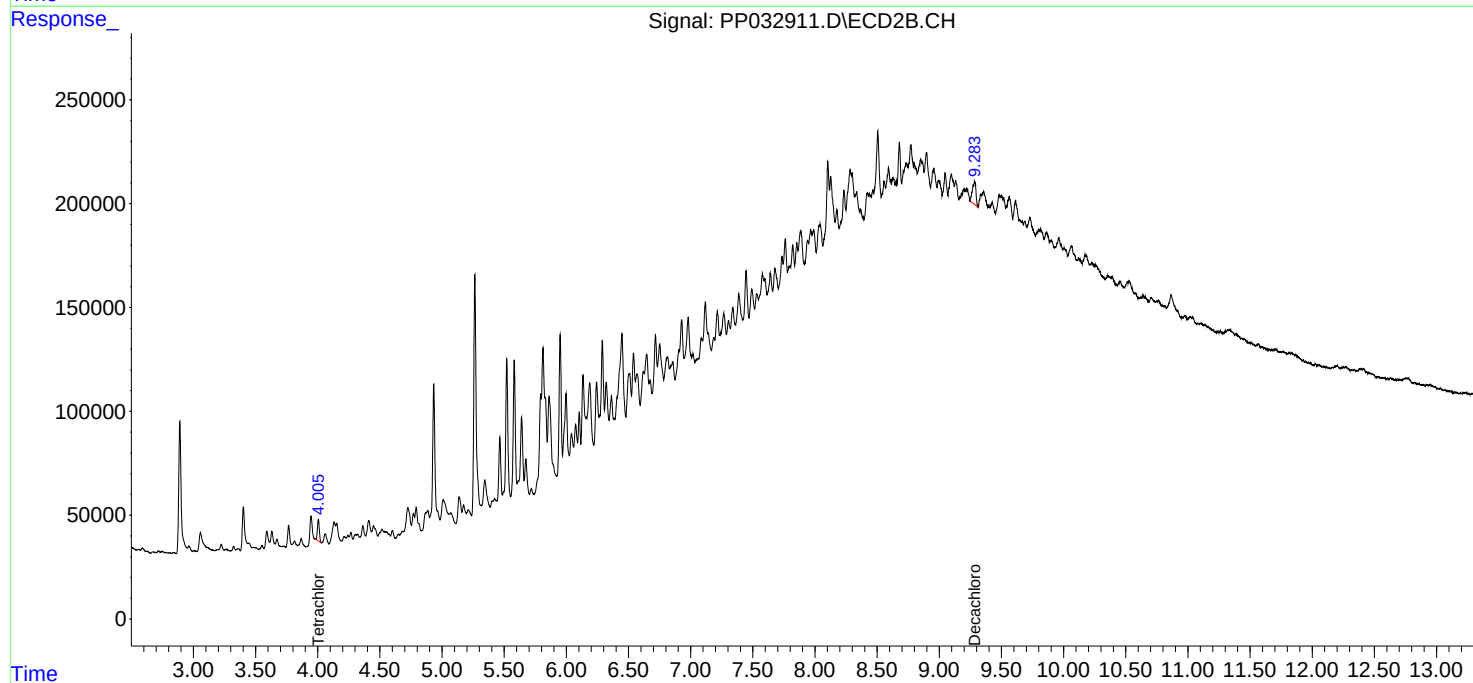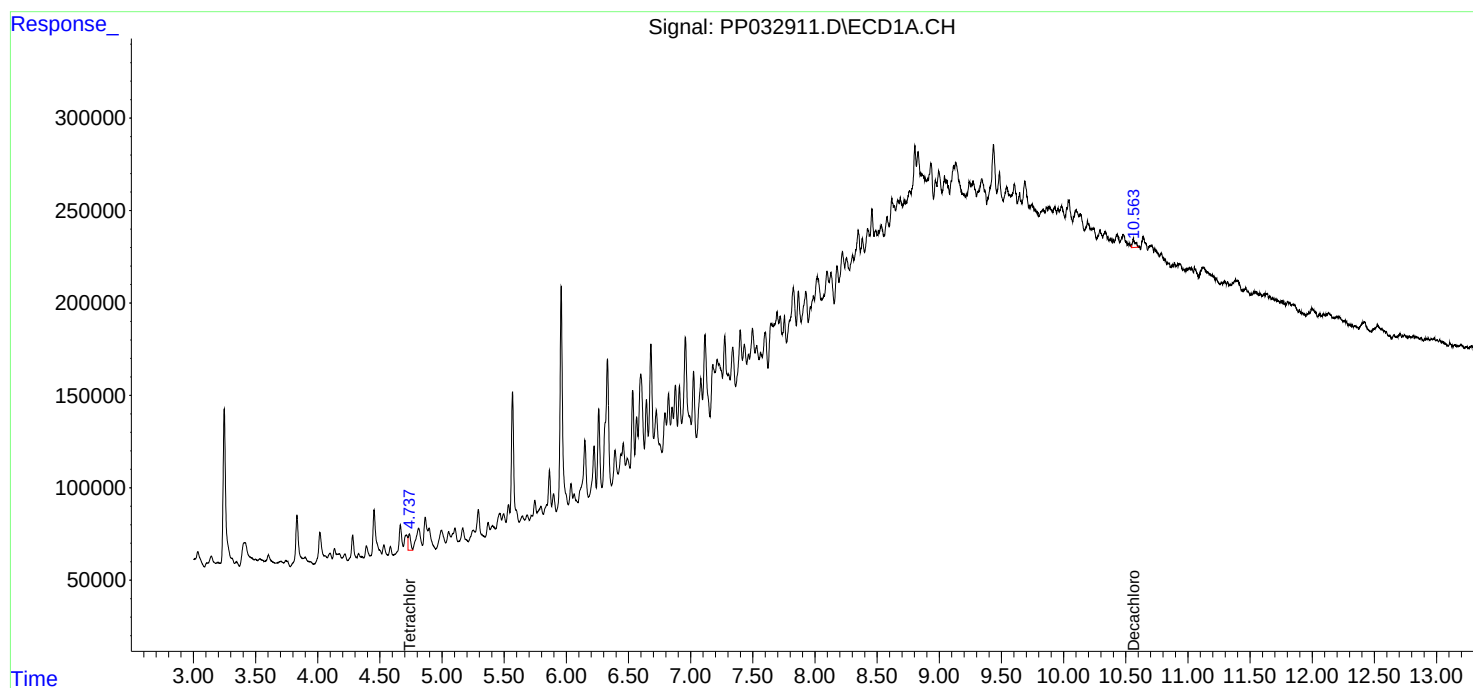

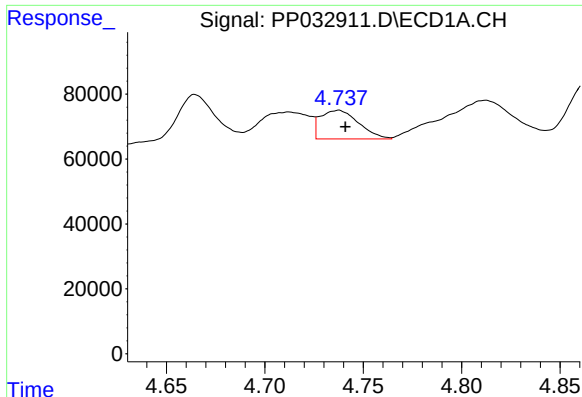


#1 Tetrachloro-m-xylene

R.T.: 4.737 min
Delta R.T.: -0.004 min
Response: 118230
Conc: 2.04 ng/ml m

Instrument :
ECD_P
ClientSampleId :
41108


Manual Integrations
APPROVED

Ankita
1/25/2021 2:34:41 PM

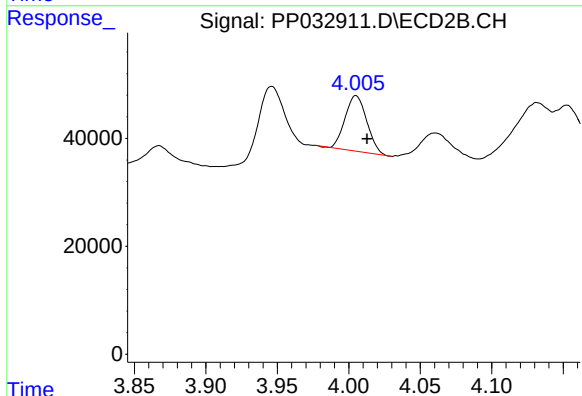


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.008 min
Response: 108818
Conc: 2.31 ng/ml

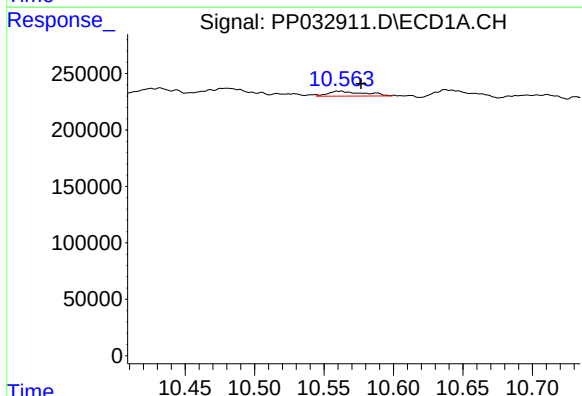

#2 Decachlorobiphenyl

R.T.: 10.563 min
Delta R.T.: -0.014 min
Response: 79294
Conc: 2.01 ng/ml m

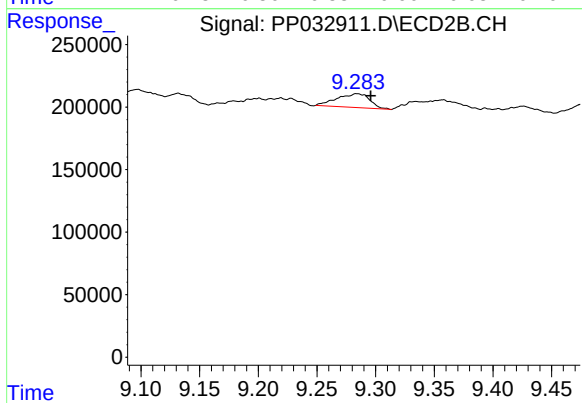

#2 Decachlorobiphenyl

R.T.: 9.284 min
Delta R.T.: -0.012 min
Response: 215463
Conc: 5.75 ng/ml