

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012323\
 Data File : PP054804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 11:26
 Operator : YP\AJ
 Sample : 01236-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NWB-1875

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/24/2023
 Supervised By :Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 15:36:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 18 04:34:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.321	3.636f	666.1E6	656.4E6	362.752m	410.093m
2) SA Decachlor...	10.143f	8.643f	18775435	19083715	13.988m	13.326m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012323\
Data File : PP054804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 11:26
Operator : YP\AJ
Sample : 01236-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NWB-1875


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 15:36:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 18 04:34:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

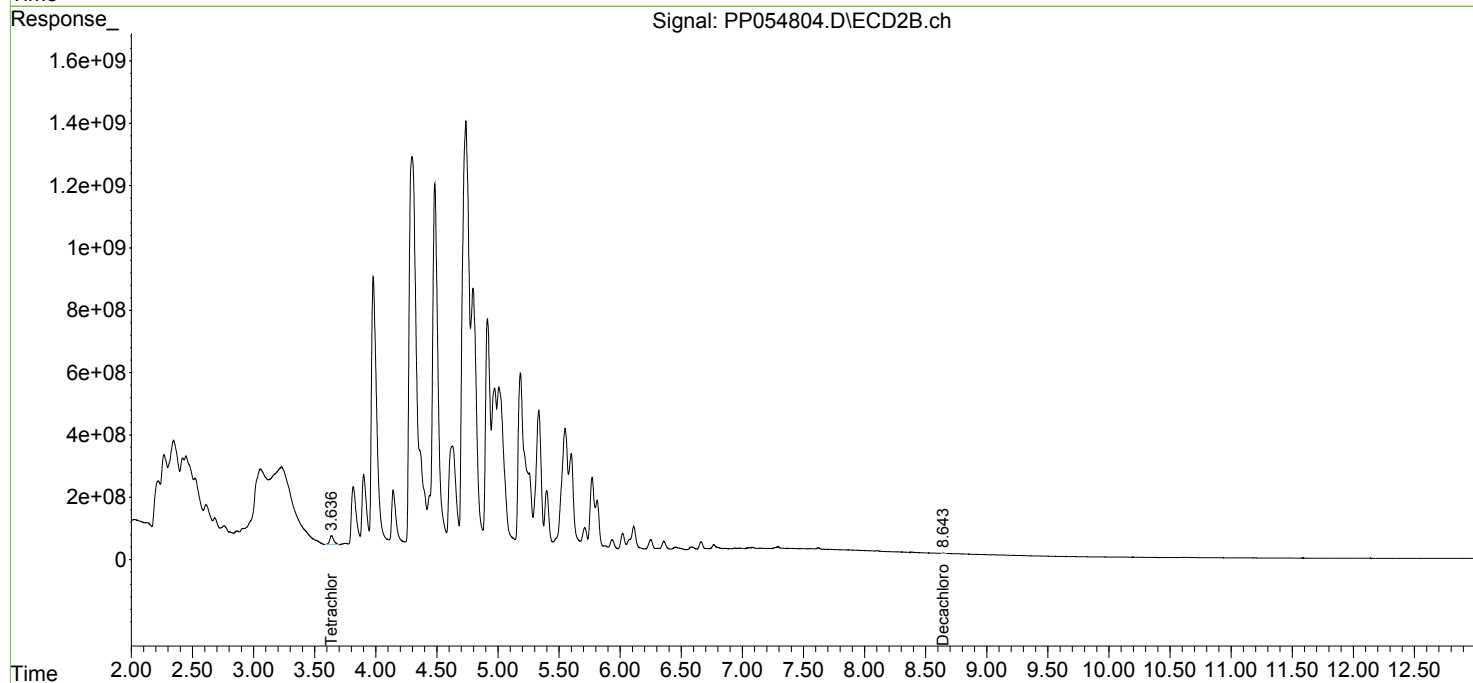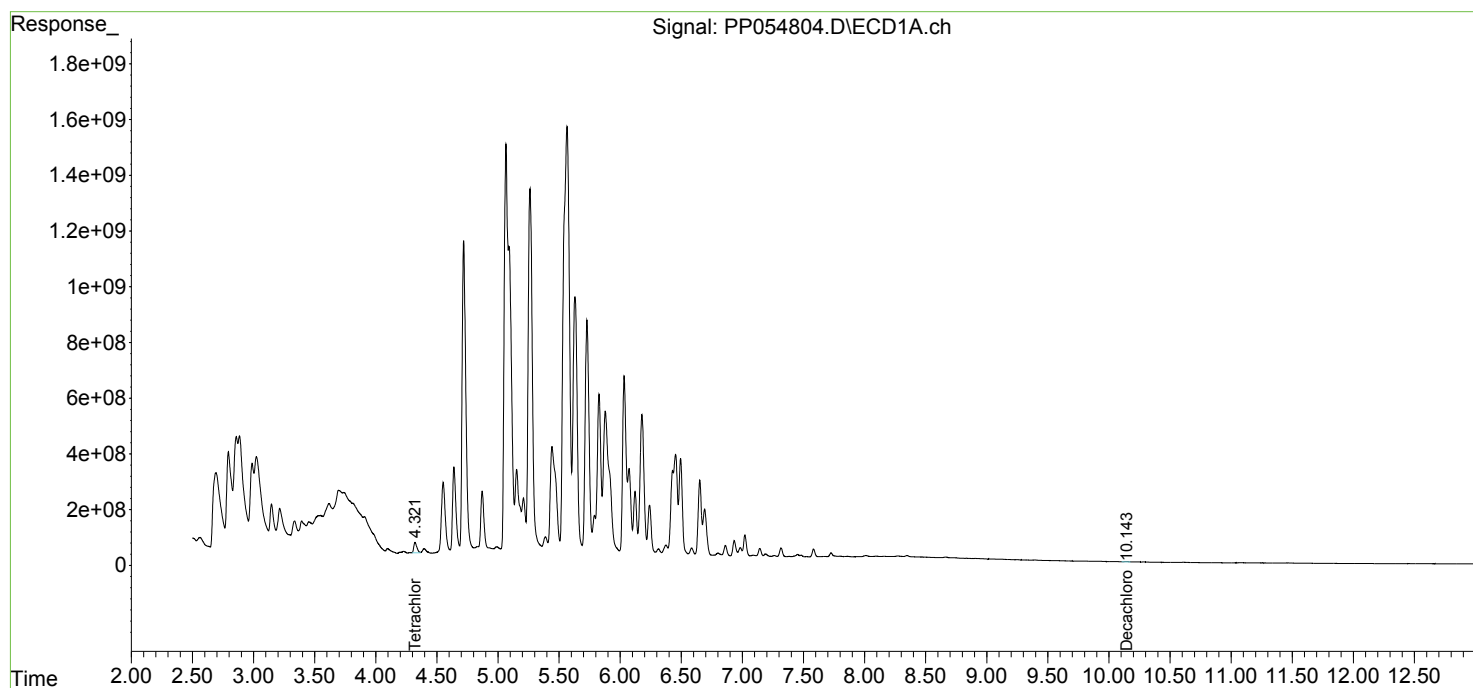

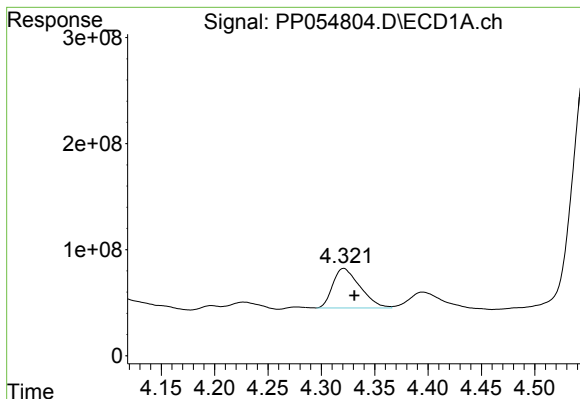


#1 Tetrachloro-m-xylene

R.T.: 4.321 min
Delta R.T.: -0.010 min
Response: 666073612
Conc: 362.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
NWB-1875


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

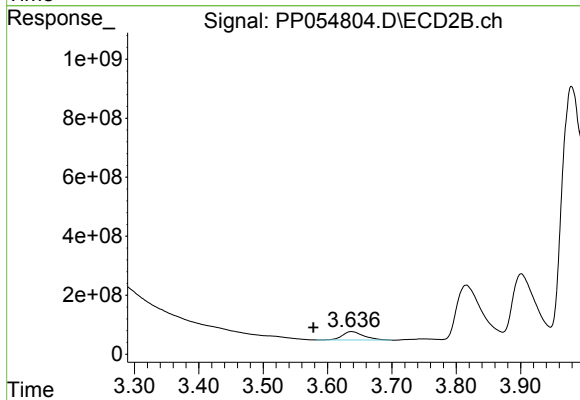


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: 0.058 min
Response: 656436262
Conc: 410.09 ng/ml

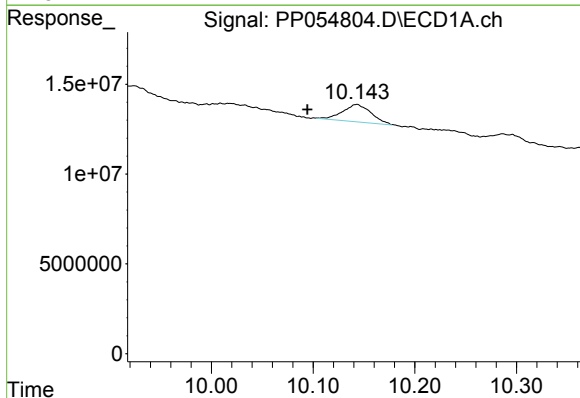

#2 Decachlorobiphenyl

R.T.: 10.143 min
Delta R.T.: 0.049 min
Response: 18775435
Conc: 13.99 ng/ml

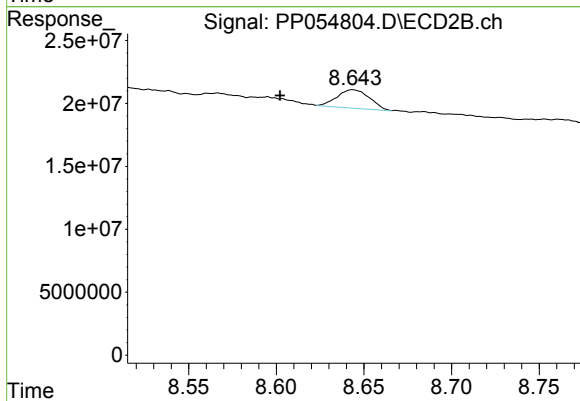

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: 0.041 min
Response: 19083715
Conc: 13.33 ng/ml