

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012323\
 Data File : PP054805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 11:42
 Operator : YP\AJ
 Sample : 01236-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NWB-1770

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/24/2023
 Supervised By :Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 15:36:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 18 04:34:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.333	3.577	16347397	236.6E6	8.903m	147.806m#
2) SA Decachlor...	10.097	8.602	10653020	10061930	7.937m	7.026

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012323\
Data File : PP054805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 11:42
Operator : YP\AJ
Sample : 01236-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NWB-1770


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 01/24/2023
Supervised By : Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 15:36:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 18 04:34:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

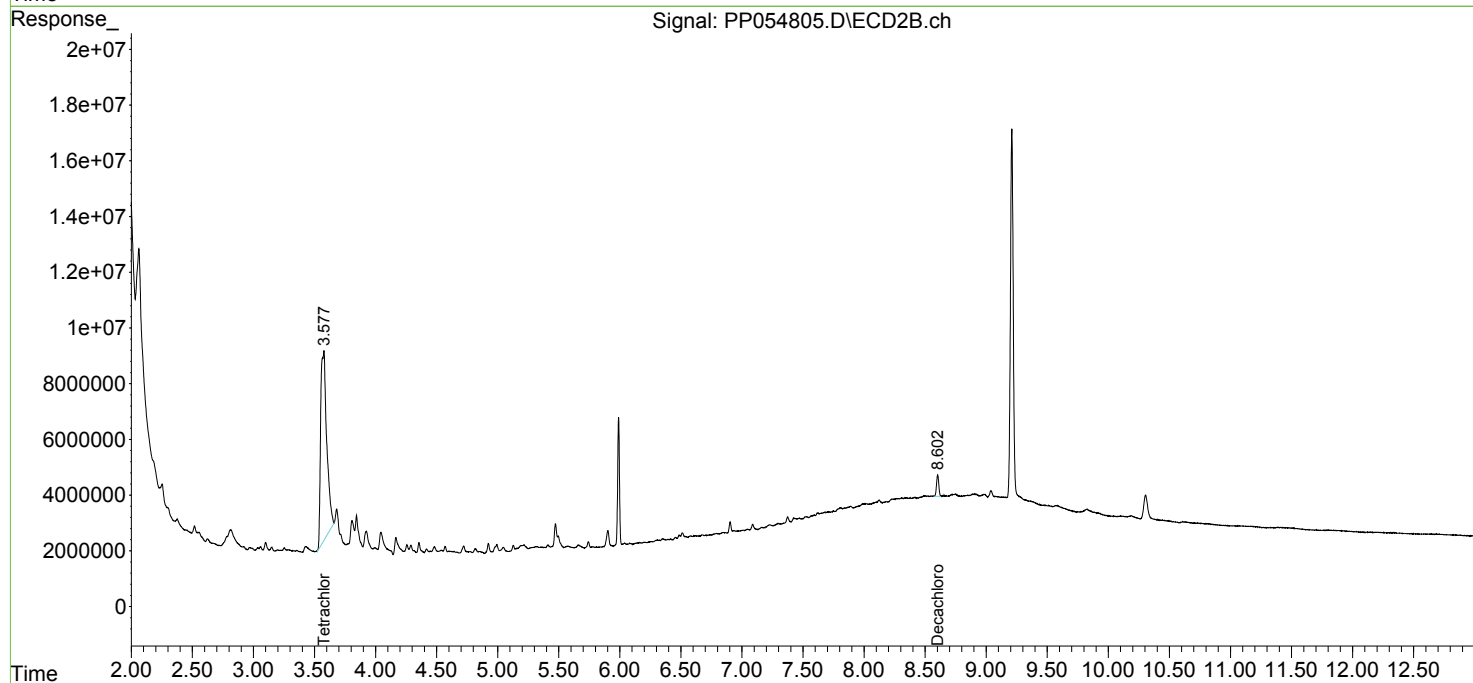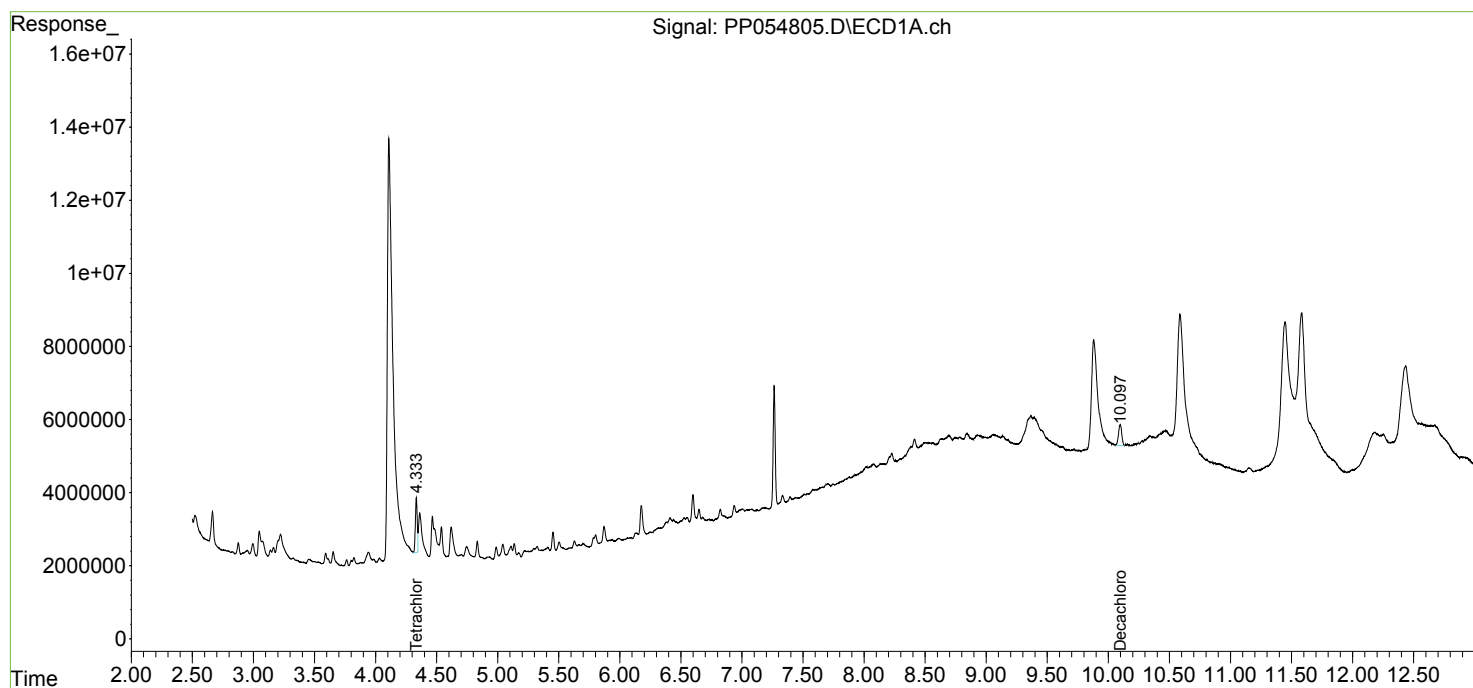

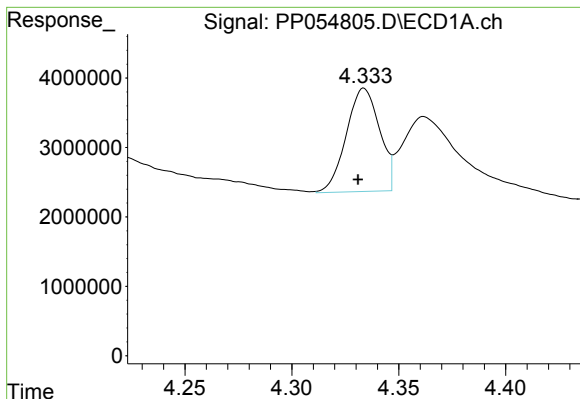


#1 Tetrachloro-m-xylene

R.T.: 4.333 min
Delta R.T.: 0.002 min
Response: 16347397
Conc: 8.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
NWB-1770


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

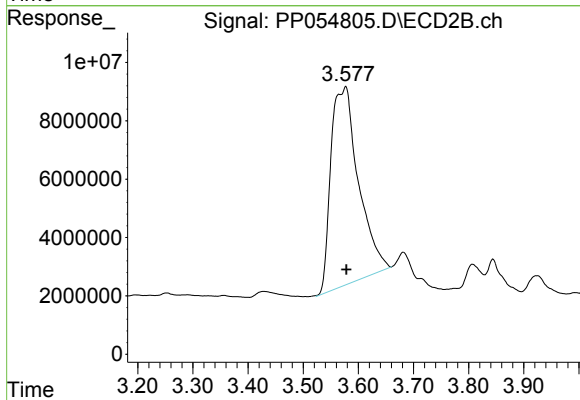


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: -0.001 min
Response: 236593457
Conc: 147.81 ng/ml m

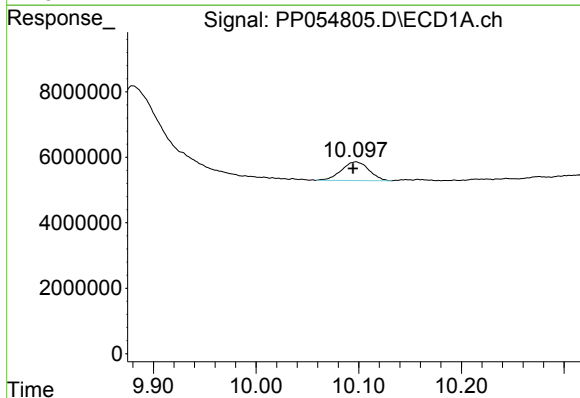

#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: 0.003 min
Response: 10653020
Conc: 7.94 ng/ml m

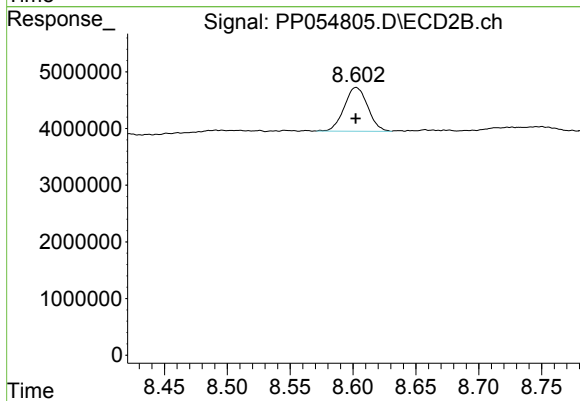

#2 Decachlorobiphenyl

R.T.: 8.602 min
Delta R.T.: 0.000 min
Response: 10061930
Conc: 7.03 ng/ml