

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012422\
 Data File : PP043227.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 1:19
 Operator : AJ\MA
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/25/2022
 Supervised By :mohammad ahmed 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 01:58:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 01:45:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.870	4.035	115455	116823	4.734	4.729
2) SA Decachlor...	10.797	9.366	67593	101211	4.768	5.069
Target Compounds						
26) L6 AR-1254-1	7.080	6.177	31464	74226	43.964	52.345
27) L6 AR-1254-2	7.309	6.336	47533	64531	45.207	52.192
28) L6 AR-1254-3	7.686	6.760	46980	98882	43.682	51.454
29) L6 AR-1254-4	7.981	7.000	32775	55095	46.496	49.838
30) L6 AR-1254-5	8.408	7.430	41649	77972	51.597m	50.476

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012422\
Data File : PP043227.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 1:19
Operator : AJ\MA
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2022
Supervised By :mohammad ahmed 01/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 01:58:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 01:45:00 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

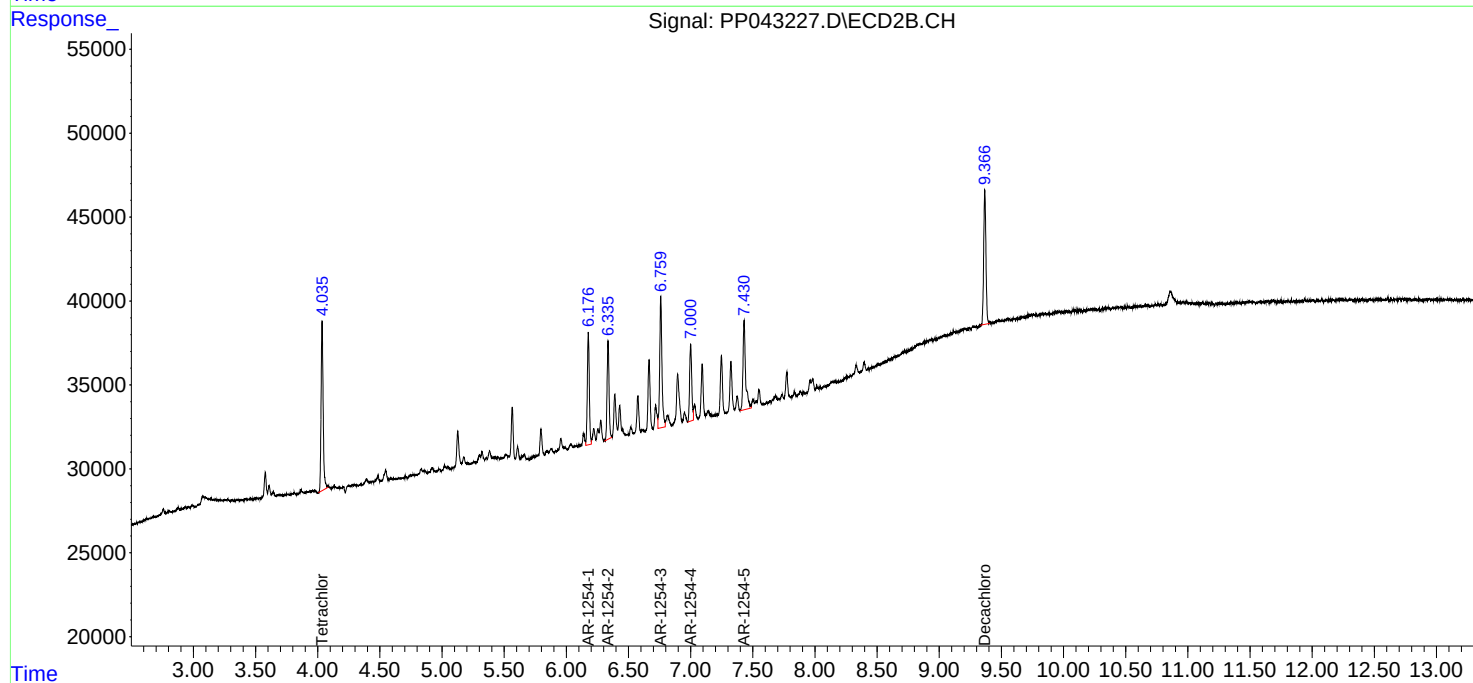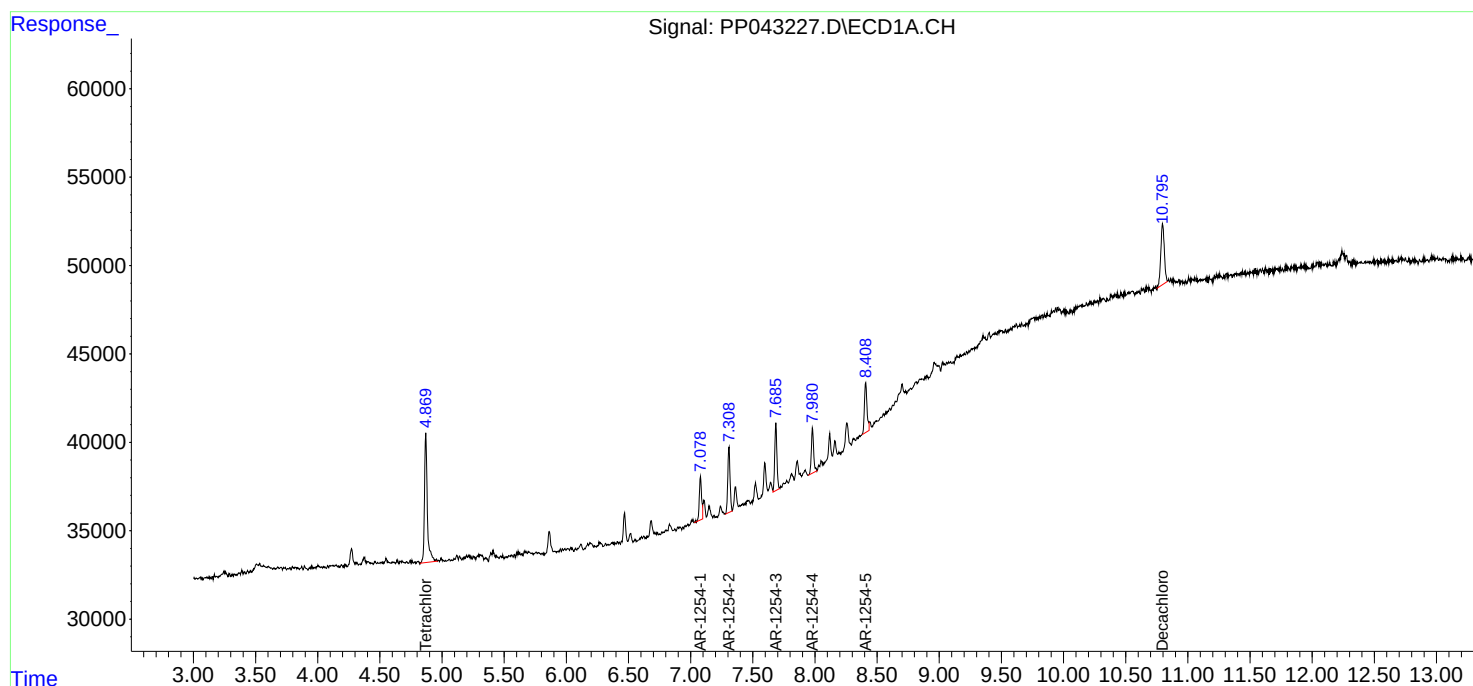

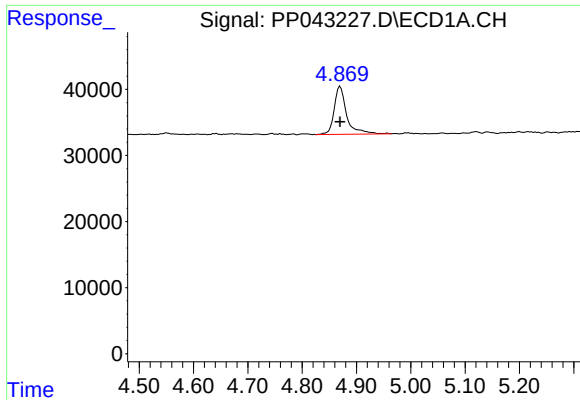


#1 Tetrachloro-m-xylene

R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 115455
Conc: 4.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2022
Supervised By :mohammad ahmed 01/25/2022

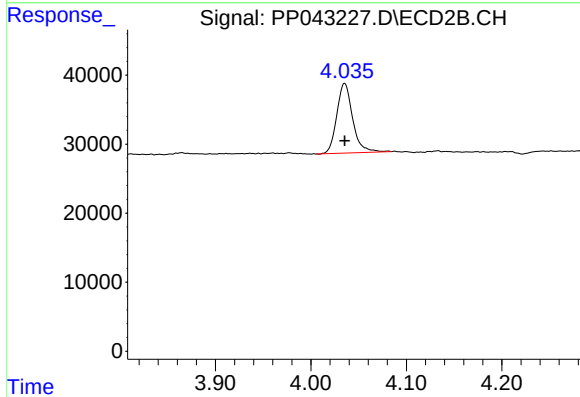


#1 Tetrachloro-m-xylene

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 116823
Conc: 4.73 ng/ml

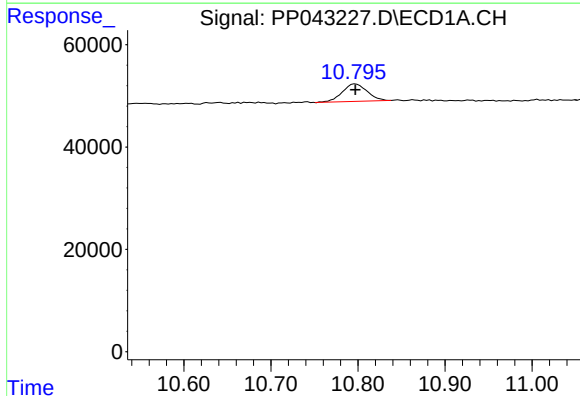


#2 Decachlorobiphenyl

R.T.: 10.797 min
Delta R.T.: 0.000 min
Response: 67593
Conc: 4.77 ng/ml

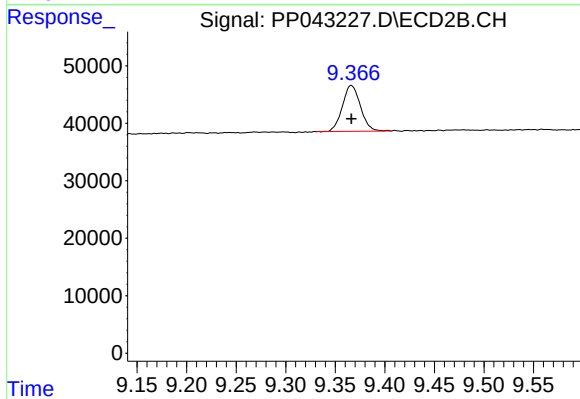

#2 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: 0.000 min
Response: 101211
Conc: 5.07 ng/ml

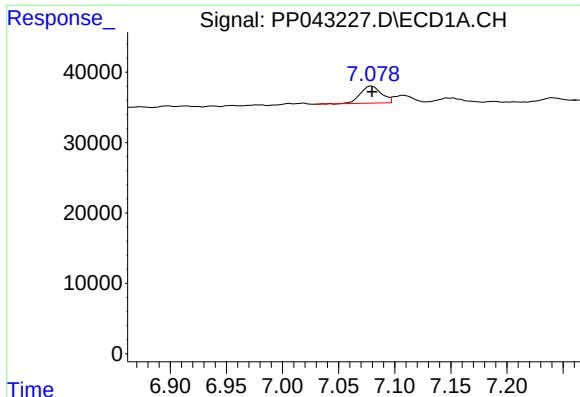


#26 AR-1254-1

R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 31464
Conc: 43.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254\ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2022
Supervised By :mohammad ahmed 01/25/2022

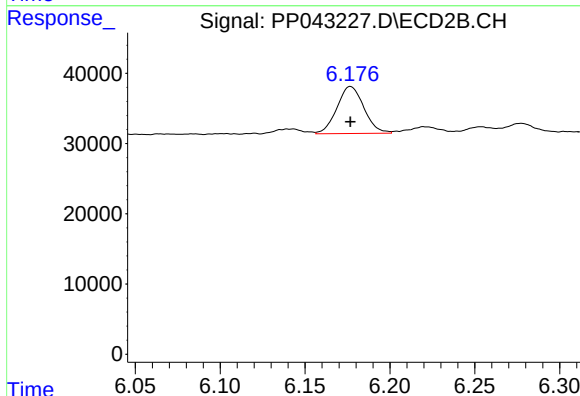


#26 AR-1254-1

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 74226
Conc: 52.35 ng/ml

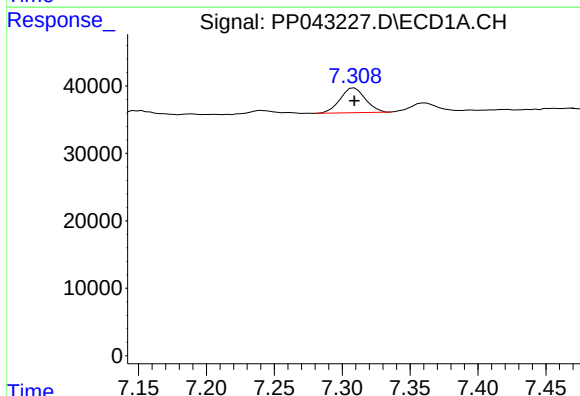


#27 AR-1254-2

R.T.: 7.309 min
Delta R.T.: 0.000 min
Response: 47533
Conc: 45.21 ng/ml

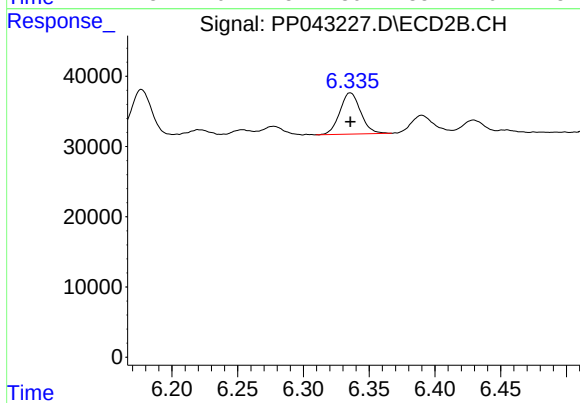

#27 AR-1254-2

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 64531
Conc: 52.19 ng/ml

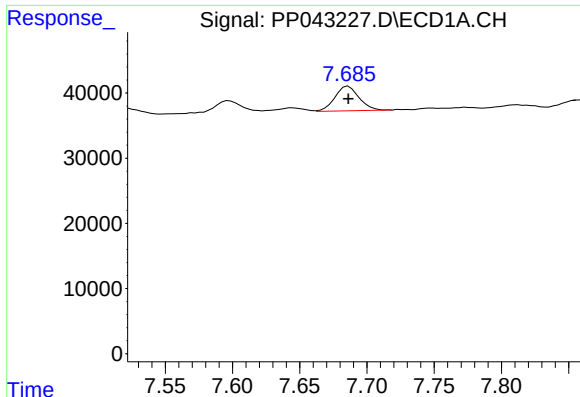


#28 AR-1254-3

R.T.: 7.686 min
Delta R.T.: 0.000 min
Response: 46980
Conc: 43.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2022
Supervised By :mohammad ahmed 01/25/2022

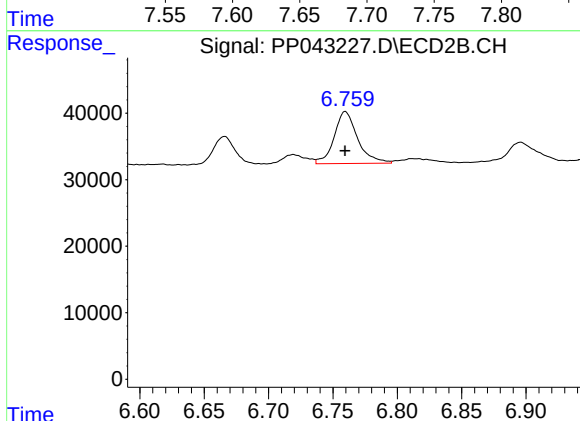


#28 AR-1254-3

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 98882
Conc: 51.45 ng/ml

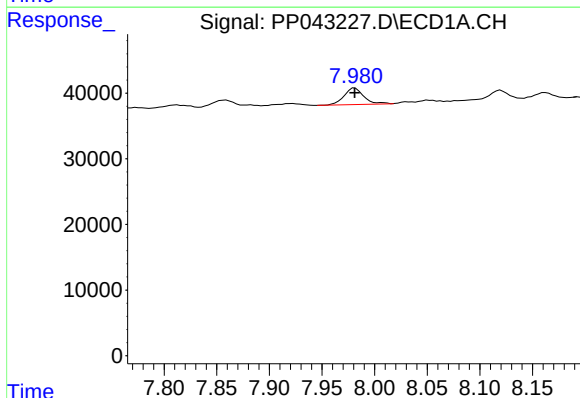


#29 AR-1254-4

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 32775
Conc: 46.50 ng/ml

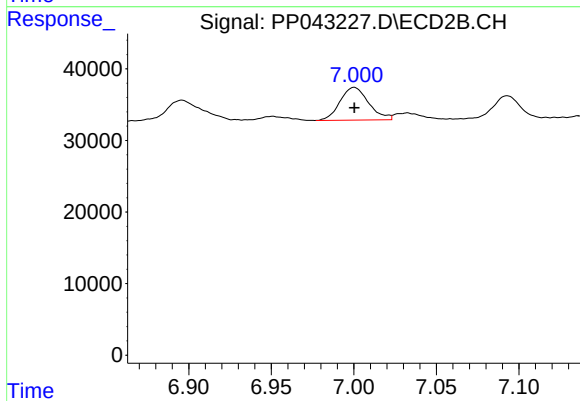

#29 AR-1254-4

R.T.: 7.000 min
Delta R.T.: 0.000 min
Response: 55095
Conc: 49.84 ng/ml

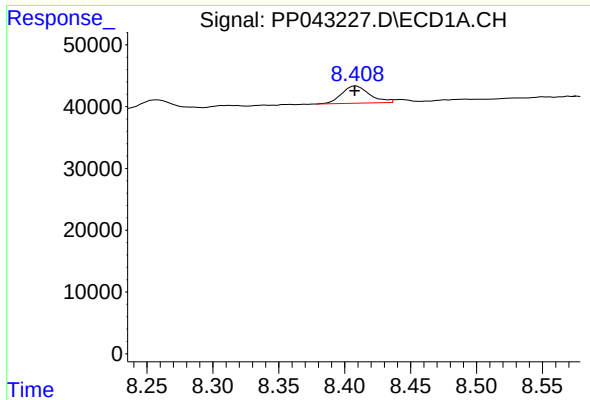


#30 AR-1254-5

R.T.: 8.408 min
Delta R.T.: 0.000 min
Response: 41649
Conc: 51.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254\ICC050

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2022
Supervised By :mohammad ahmed 01/25/2022

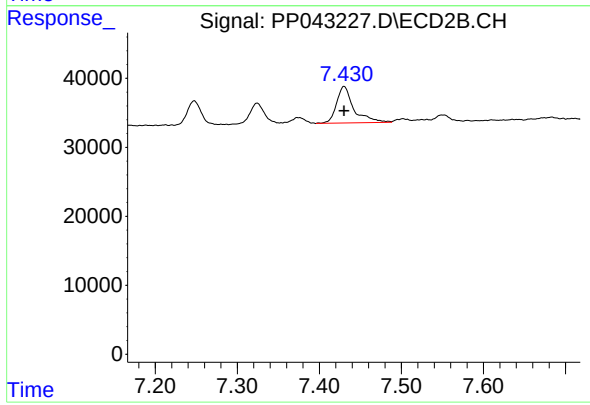

#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 77972
Conc: 50.48 ng/ml