

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012423\
 Data File : PP054842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 01:50
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/24/2023
 Supervised By :Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 02:52:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 02:09:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.578	7838672	6752824	4.560	4.580
2) SA Decachlor...	10.089	8.595	14851740	13048020	4.850	5.223
Target Compounds						
41) L9 AR-1268-1	8.585	7.493	11380033	10738888	46.562	49.754m
42) L9 AR-1268-2	8.679	7.559	11164710	9575863	49.157	49.073
43) L9 AR-1268-3	8.907	7.766	9737128	8530048	48.739	49.661
44) L9 AR-1268-4	9.333	8.054	3555590	3069292	45.267	48.121
45) L9 AR-1268-5	9.749	8.343	29923160	25341341	47.040	48.120

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012423\
Data File : PP054842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 01:50
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 02:52:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 02:09:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

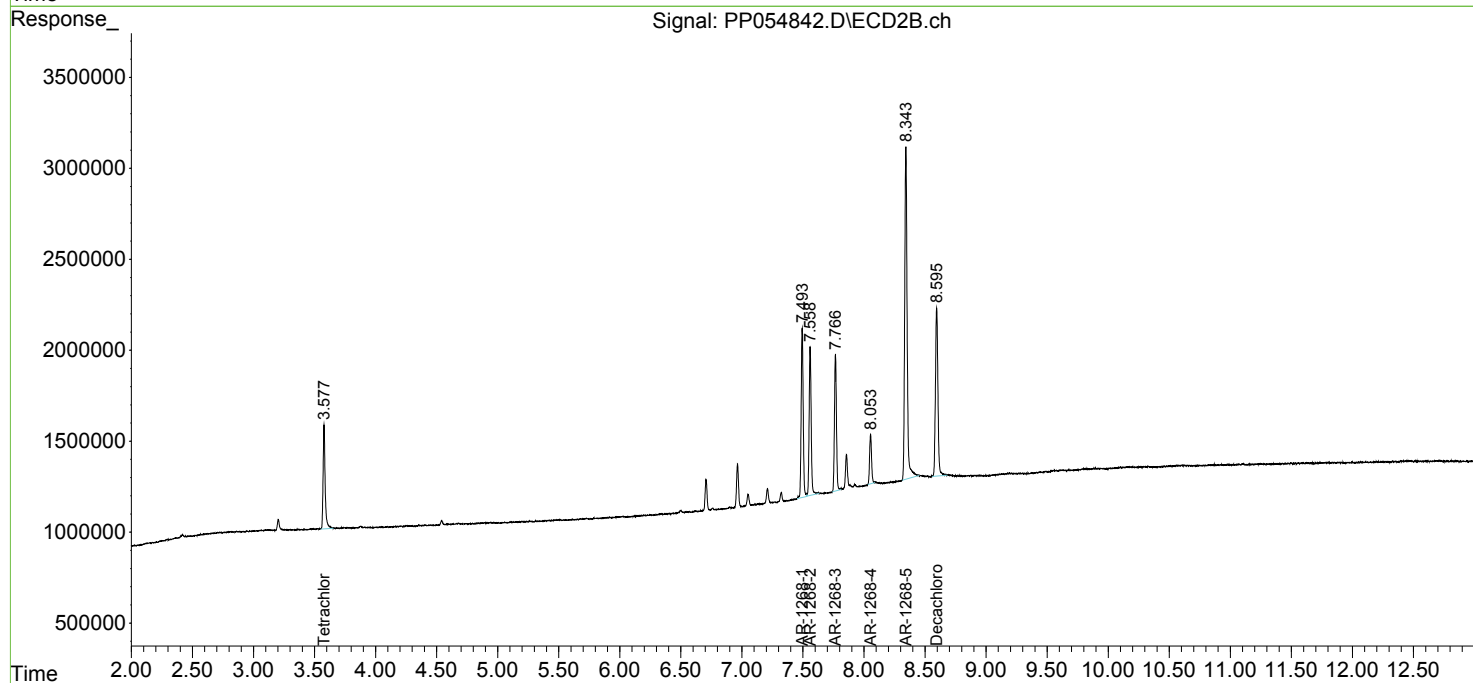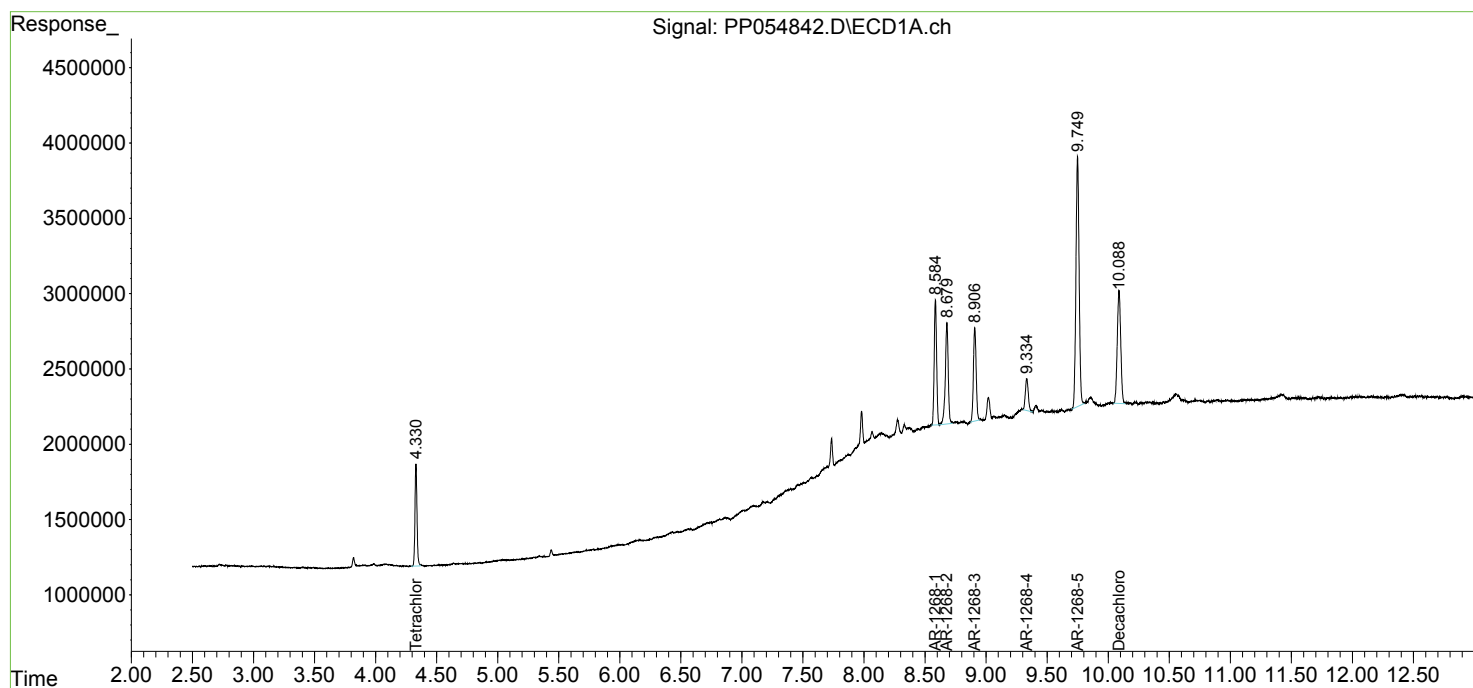

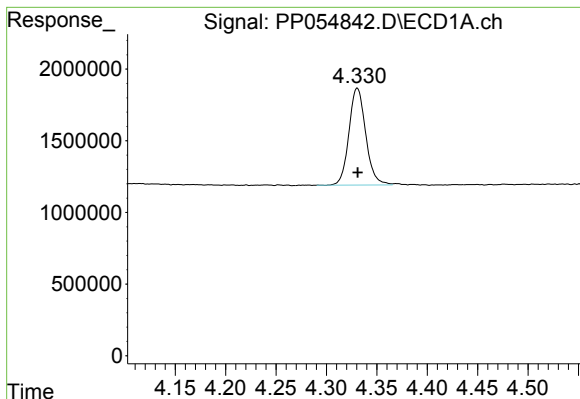


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: 0.000 min
Response: 7838672
Conc: 4.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

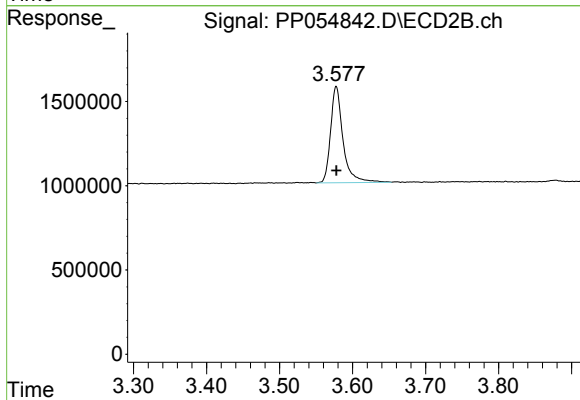


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: 0.000 min
Response: 6752824
Conc: 4.58 ng/ml

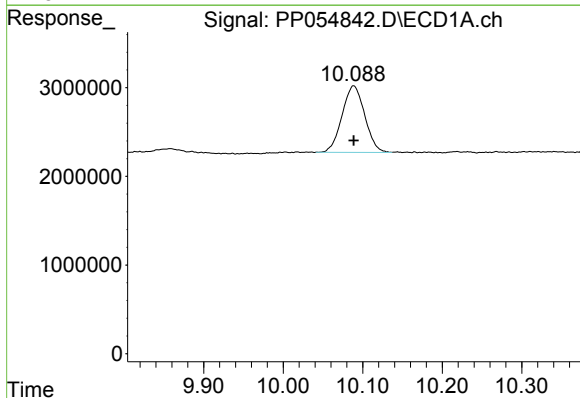


#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: 0.000 min
Response: 14851740
Conc: 4.85 ng/ml

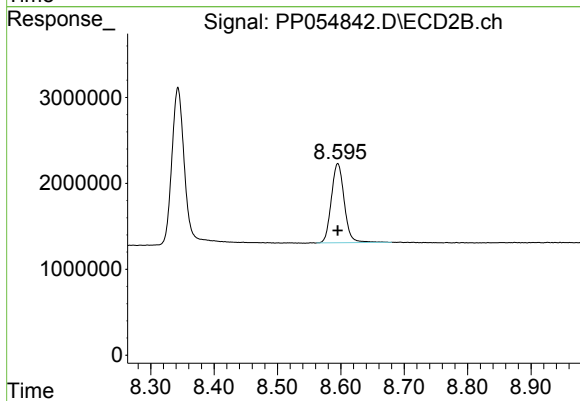

#2 Decachlorobiphenyl

R.T.: 8.595 min
Delta R.T.: 0.000 min
Response: 13048020
Conc: 5.22 ng/ml

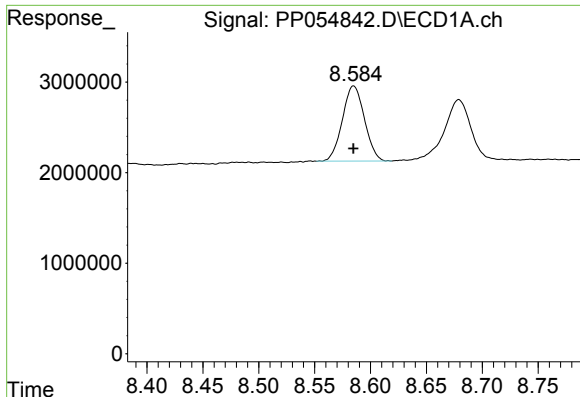


#41 AR-1268-1

R.T.: 8.585 min
Delta R.T.: 0.000 min
Response: 11380033
Conc: 46.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

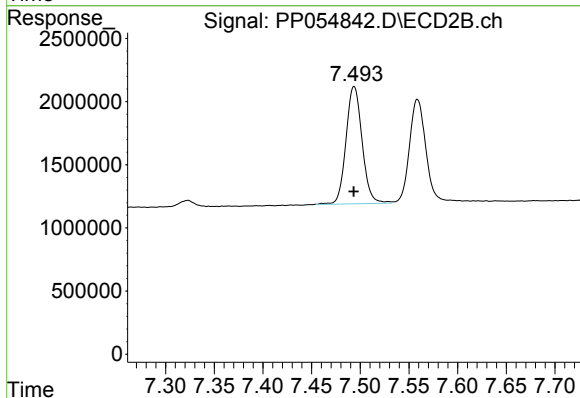


#41 AR-1268-1

R.T.: 7.493 min
Delta R.T.: 0.000 min
Response: 10738888
Conc: 49.75 ng/ml m

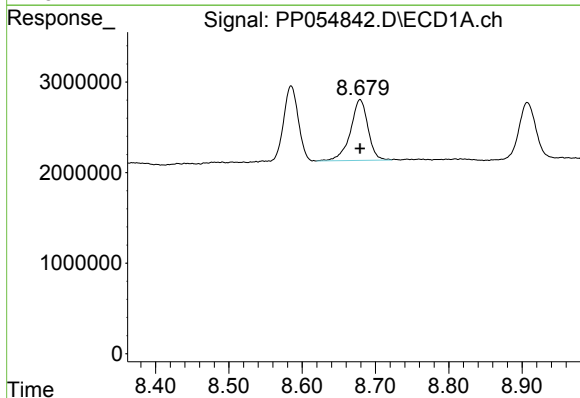


#42 AR-1268-2

R.T.: 8.679 min
Delta R.T.: 0.000 min
Response: 11164710
Conc: 49.16 ng/ml

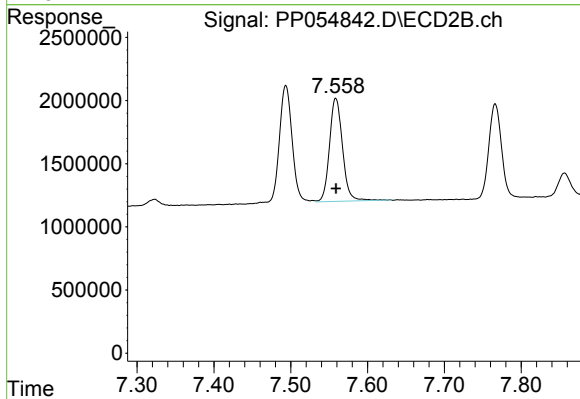

#42 AR-1268-2

R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 9575863
Conc: 49.07 ng/ml

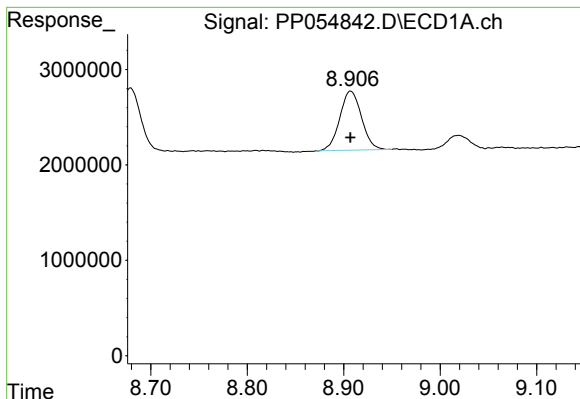


#43 AR-1268-3

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 9737128
Conc: 48.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

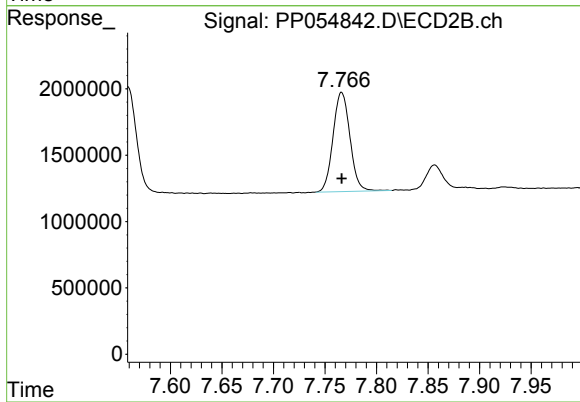


#43 AR-1268-3

R.T.: 7.766 min
Delta R.T.: 0.000 min
Response: 8530048
Conc: 49.66 ng/ml

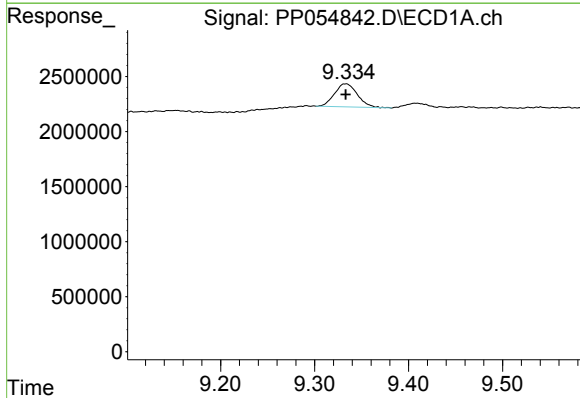


#44 AR-1268-4

R.T.: 9.333 min
Delta R.T.: 0.000 min
Response: 3555590
Conc: 45.27 ng/ml

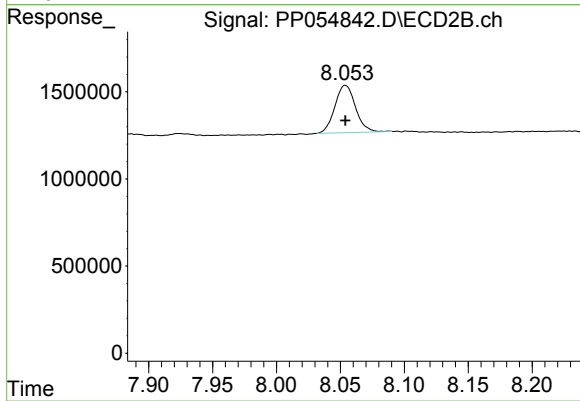

#44 AR-1268-4

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 3069292
Conc: 48.12 ng/ml

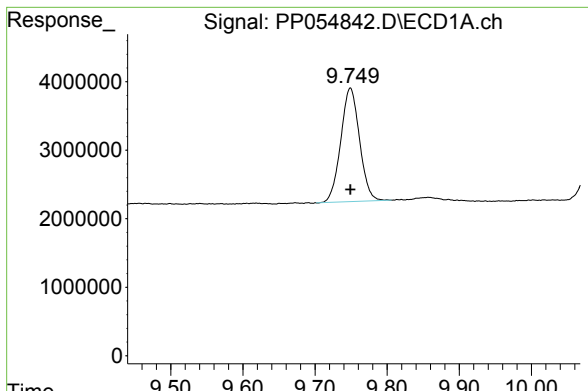


#45 AR-1268-5

R.T.: 9.749 min
Delta R.T.: 0.000 min
Response: 29923160
Conc: 47.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/24/2023
Supervised By :Ankita Jodhani 01/24/2023

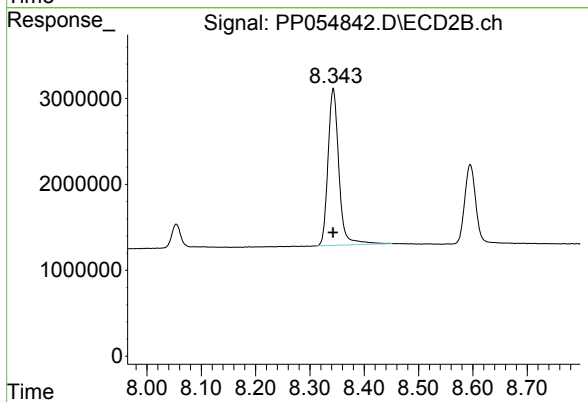

#45 AR-1268-5

R.T.: 8.343 min
Delta R.T.: 0.000 min
Response: 25341341
Conc: 48.12 ng/ml