

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012521\
 Data File : PP032920.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 11:01
 Operator : DD\AJ
 Sample : M1207-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-SF-03-010-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:38:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.737	4.007	973996	843856	16.770	17.939
2) SA Decachlor...	10.569	9.283	785920	674742	19.920	18.011
Target Compounds						
26) L6 AR-1254-1	6.946	6.126	598714	524312	360.485	256.098 #
27) L6 AR-1254-2	7.171	6.280	472217	234266	187.763	133.391 #
28) L6 AR-1254-3	7.547	6.701	360480	268079	133.792	93.344 #
29) L6 AR-1254-4	7.840	6.942	140407	164030	71.280	99.057 #
30) L6 AR-1254-5	8.268	7.367	272923	445281	130.870	184.086 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012521\
Data File : PP032920.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 11:01
Operator : DD\AJ
Sample : M1207-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-010-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:38:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

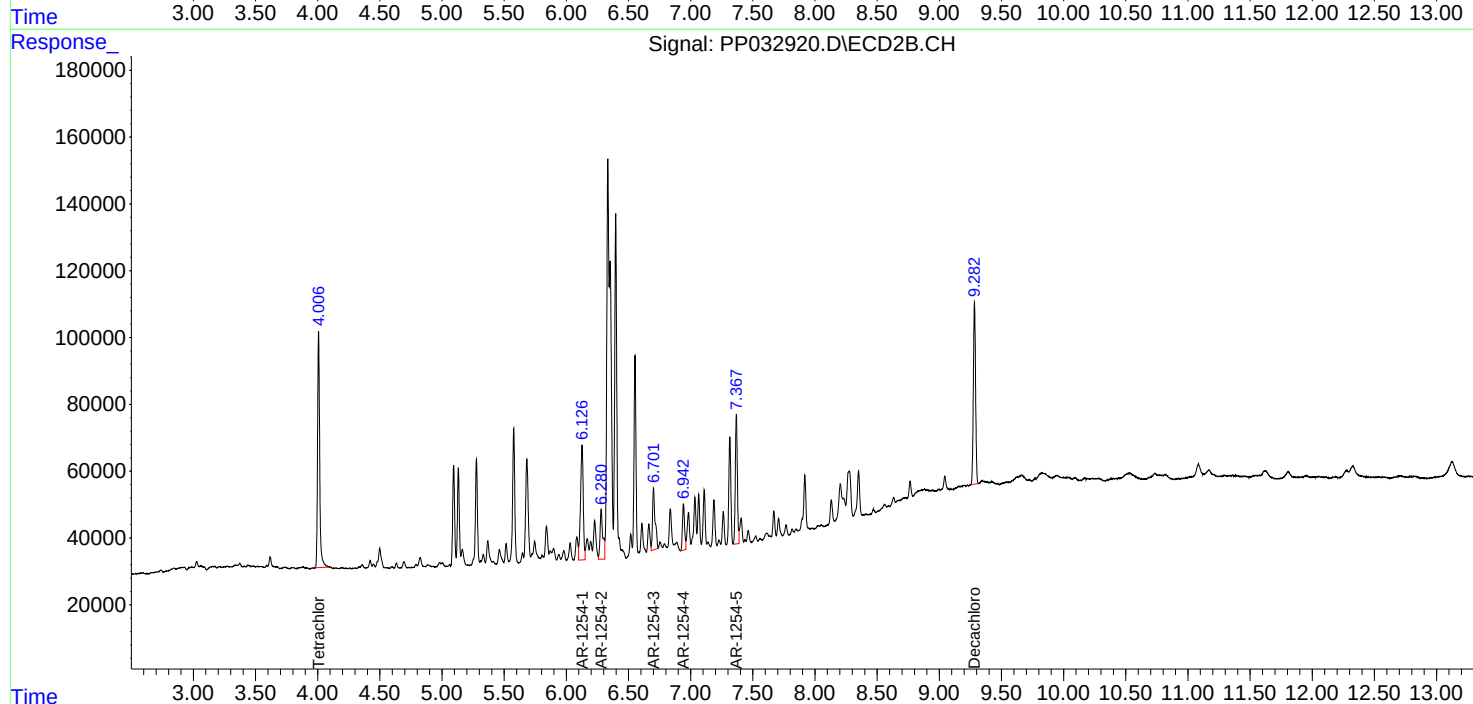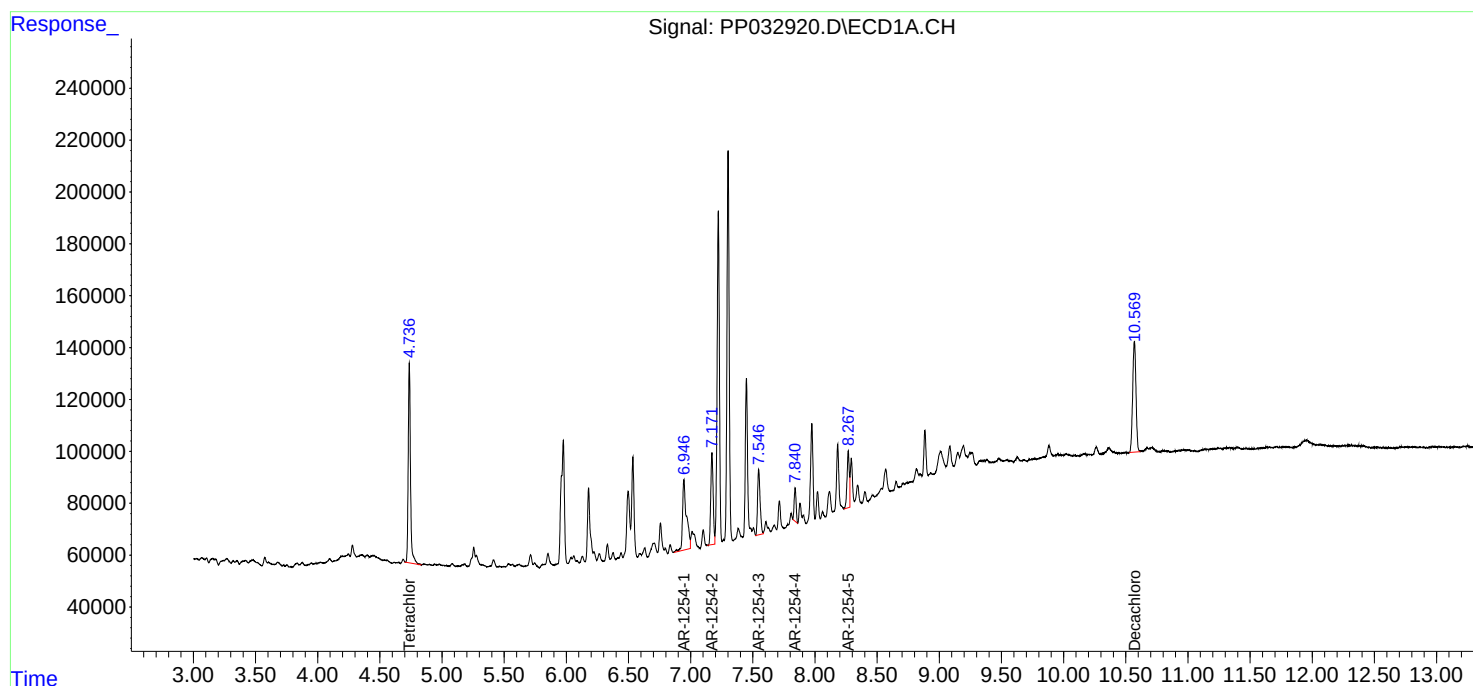


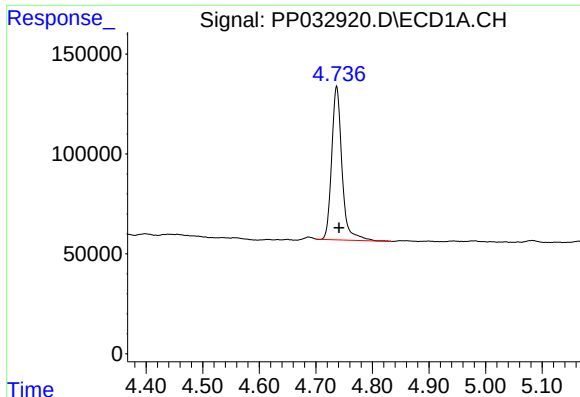

#1 Tetrachloro-m-xylene


R.T.: 4.737 min
Delta R.T.: -0.004 min
Response: 973996
Conc: 16.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-010-B

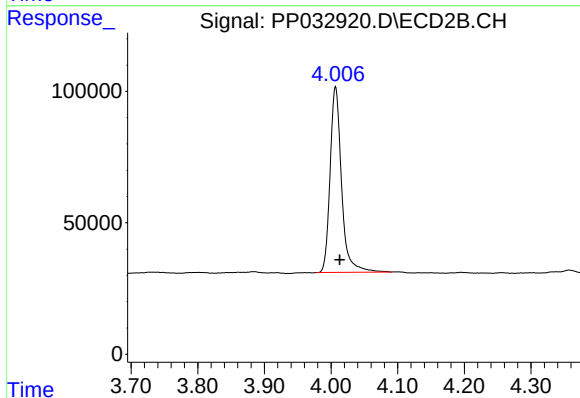


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.006 min
Response: 843856
Conc: 17.94 ng/ml

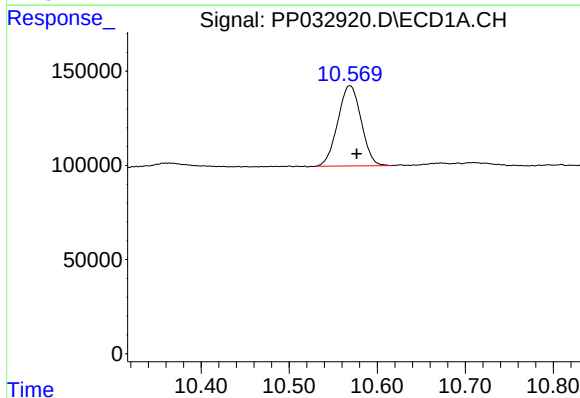


#2 Decachlorobiphenyl

R.T.: 10.569 min
Delta R.T.: -0.008 min
Response: 785920
Conc: 19.92 ng/ml

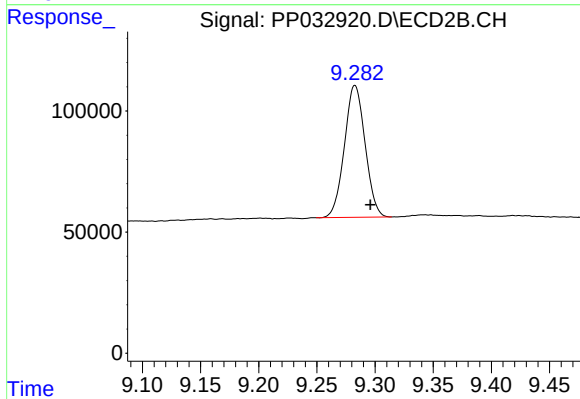

#2 Decachlorobiphenyl


R.T.: 9.283 min
Delta R.T.: -0.013 min
Response: 674742
Conc: 18.01 ng/ml

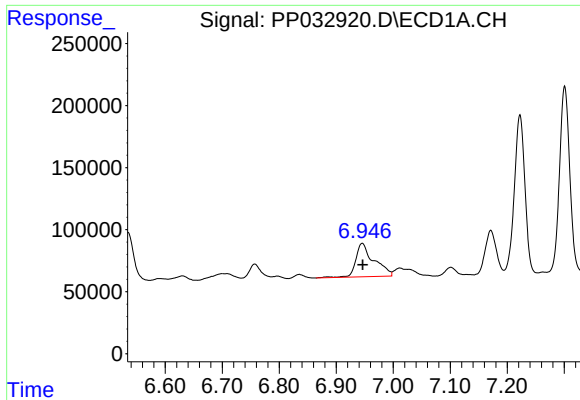

#26 AR-1254-1


R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 598714
Conc: 360.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-010-B

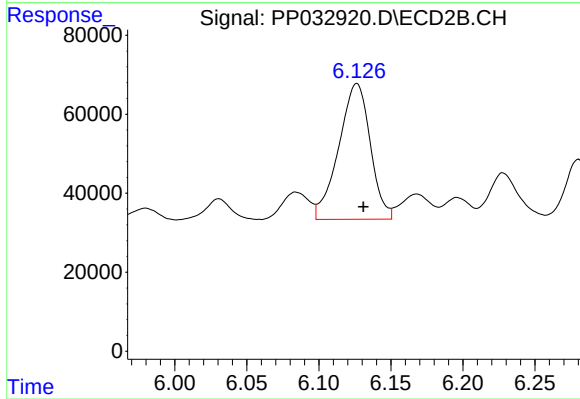


#26 AR-1254-1

R.T.: 6.126 min
Delta R.T.: -0.005 min
Response: 524312
Conc: 256.10 ng/ml

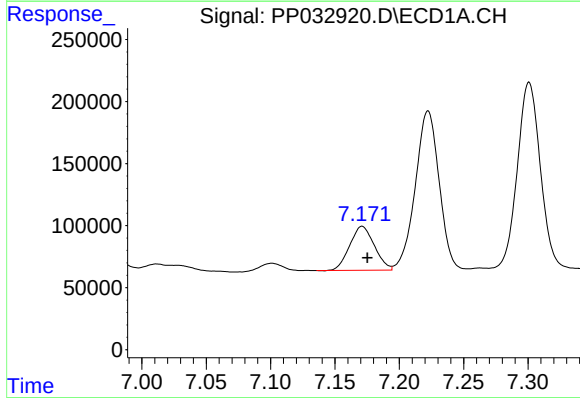


#27 AR-1254-2

R.T.: 7.171 min
Delta R.T.: -0.004 min
Response: 472217
Conc: 187.76 ng/ml

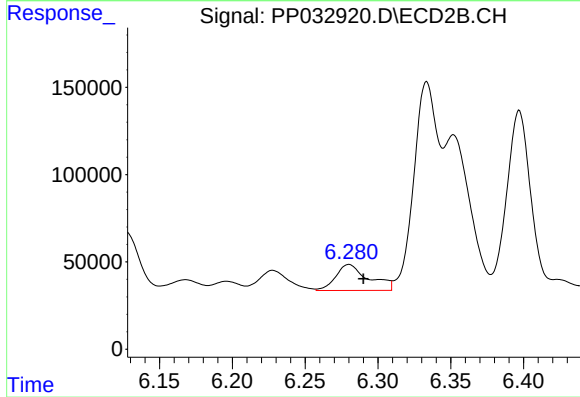

#27 AR-1254-2


R.T.: 6.280 min
Delta R.T.: -0.010 min
Response: 234266
Conc: 133.39 ng/ml

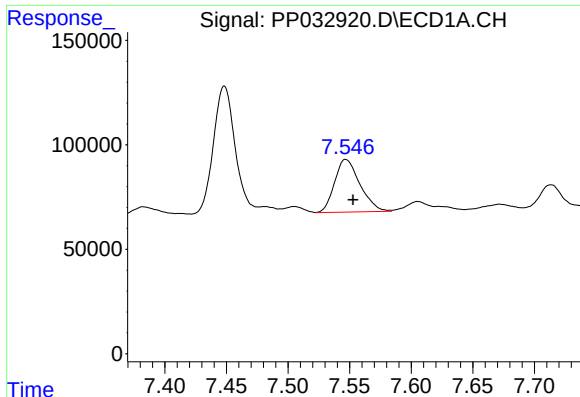

#28 AR-1254-3


R.T.: 7.547 min
Delta R.T.: -0.006 min
Response: 360480
Conc: 133.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-010-B

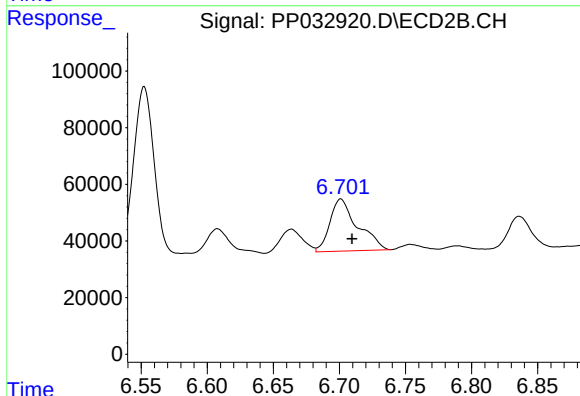


#28 AR-1254-3

R.T.: 6.701 min
Delta R.T.: -0.008 min
Response: 268079
Conc: 93.34 ng/ml

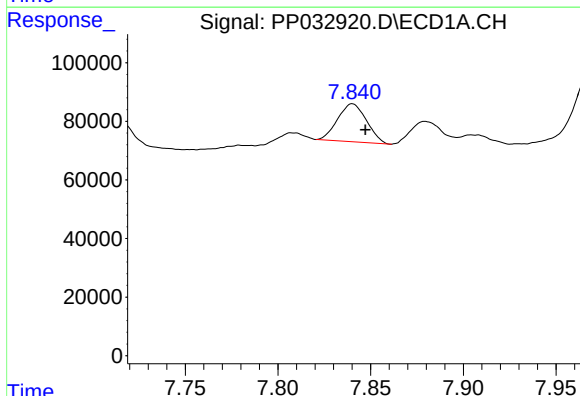


#29 AR-1254-4

R.T.: 7.840 min
Delta R.T.: -0.007 min
Response: 140407
Conc: 71.28 ng/ml

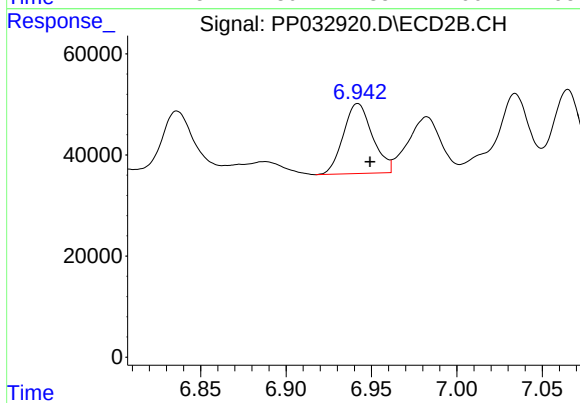

#29 AR-1254-4


R.T.: 6.942 min
Delta R.T.: -0.007 min
Response: 164030
Conc: 99.06 ng/ml

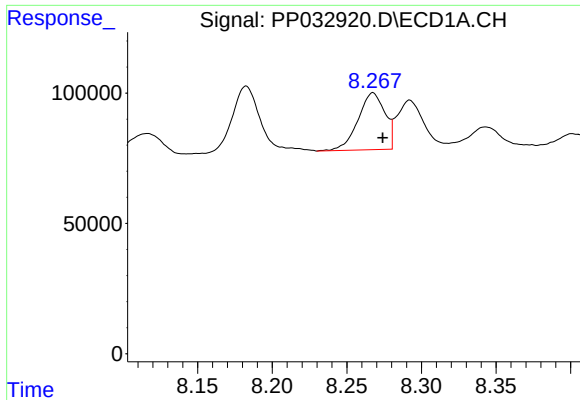

#30 AR-1254-5

R.T.: 8.268 min
Delta R.T.: -0.006 min
Response: 272923
Conc: 130.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-010-B

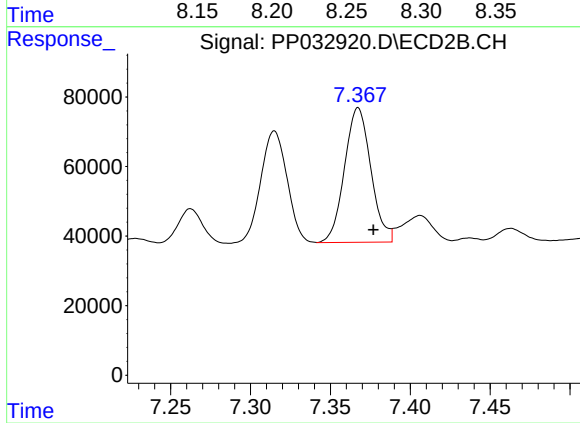

#30 AR-1254-5

R.T.: 7.367 min
Delta R.T.: -0.010 min
Response: 445281
Conc: 184.09 ng/ml