

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012521\
 Data File : PP032921.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 11:18
 Operator : DD\AJ
 Sample : M1208-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-SF-03-011-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:39:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.738	4.007	1084457	961550	18.672	20.441
2) SA Decachlor...	10.571	9.284	842586	729839	21.357	19.482
Target Compounds						
26) L6 AR-1254-1	6.947	6.128	635213	562506	382.461	274.754 #
27) L6 AR-1254-2	7.173	6.281	475252	173564	188.970	98.827 #
28) L6 AR-1254-3	7.548	6.702	353533	272980	131.214	95.050 #
29) L6 AR-1254-4	7.840	6.943	103272	144456	52.427	87.236 #
30) L6 AR-1254-5	8.268	7.368	249119	584333	119.456	241.572 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012521\
Data File : PP032921.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 11:18
Operator : DD\AJ
Sample : M1208-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
FK-SF-03-011-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:39:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

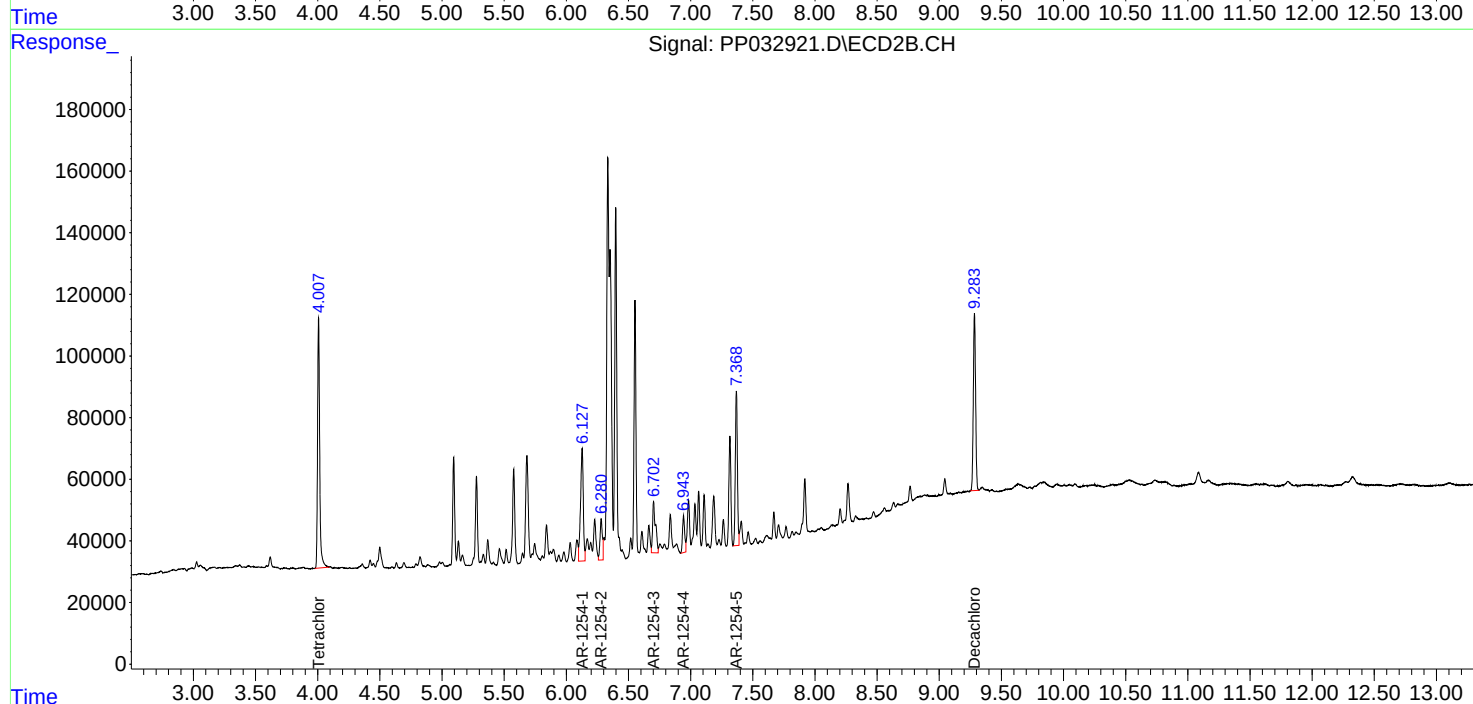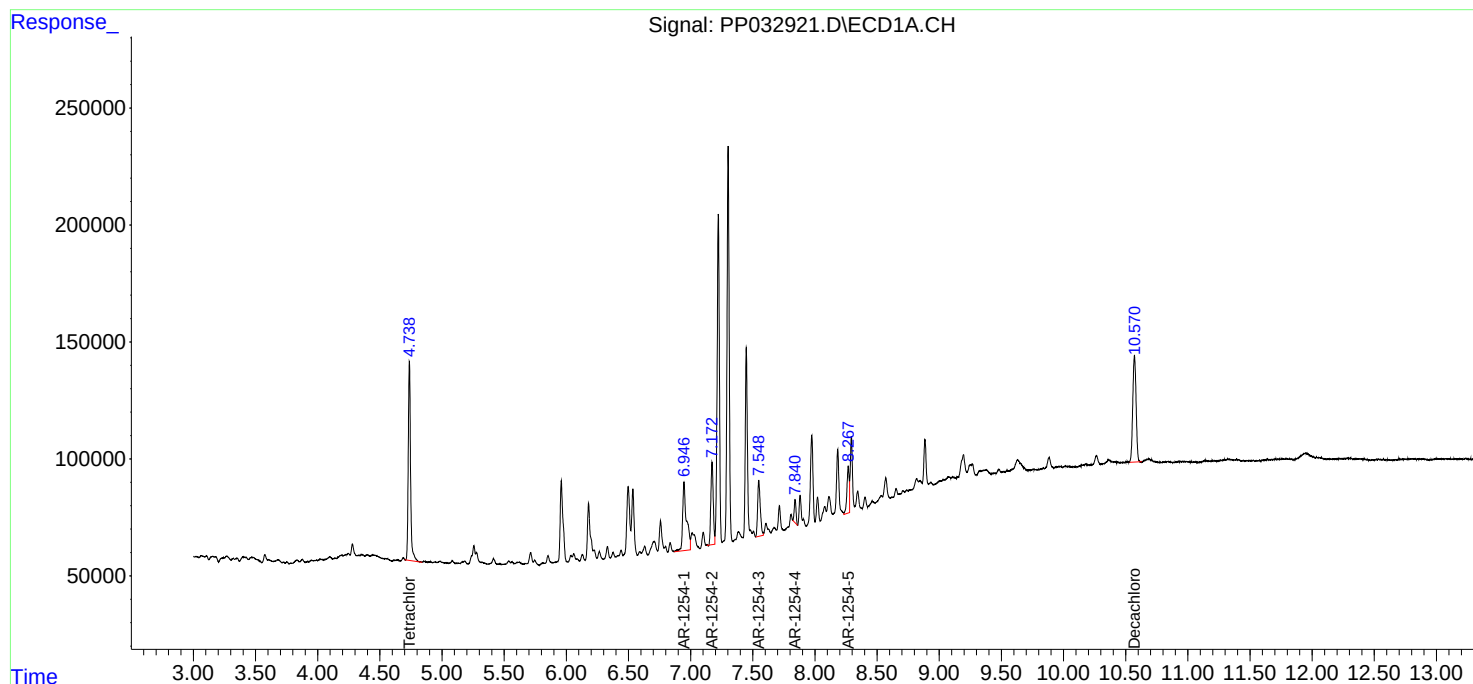


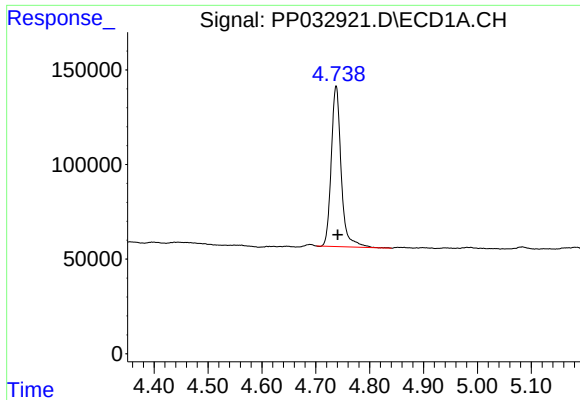

#1 Tetrachloro-m-xylene


R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1084457
Conc: 18.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-A

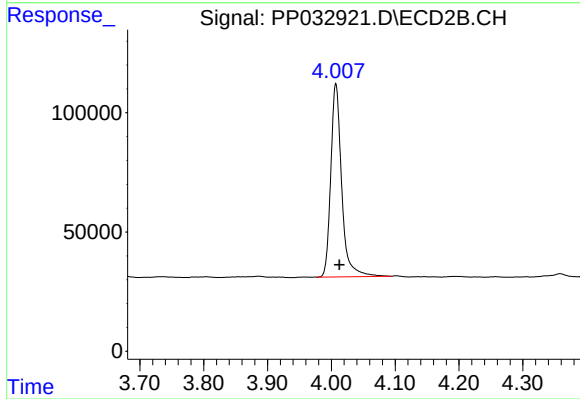


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.006 min
Response: 961550
Conc: 20.44 ng/ml

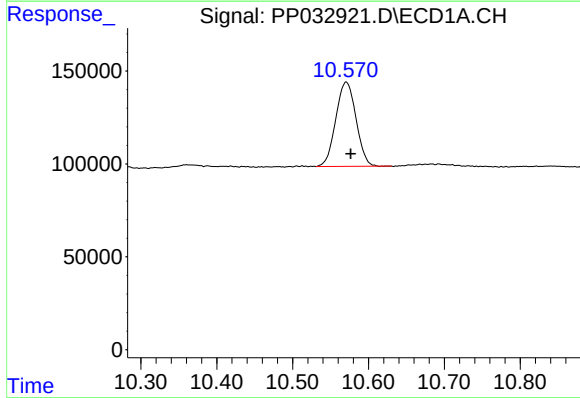


#2 Decachlorobiphenyl

R.T.: 10.571 min
Delta R.T.: -0.006 min
Response: 842586
Conc: 21.36 ng/ml

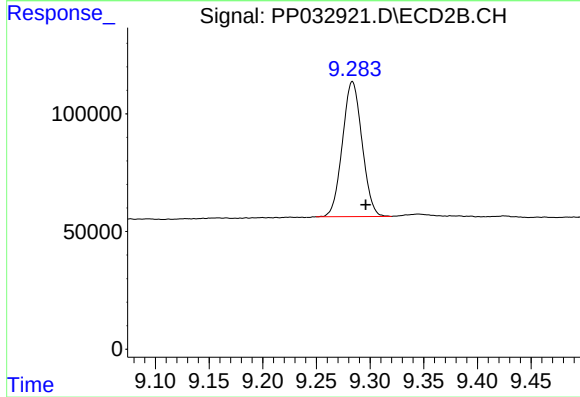

#2 Decachlorobiphenyl


R.T.: 9.284 min
Delta R.T.: -0.012 min
Response: 729839
Conc: 19.48 ng/ml

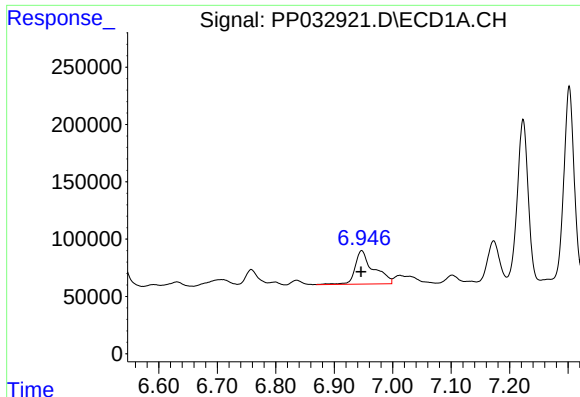

#26 AR-1254-1


R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 635213
Conc: 382.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-A

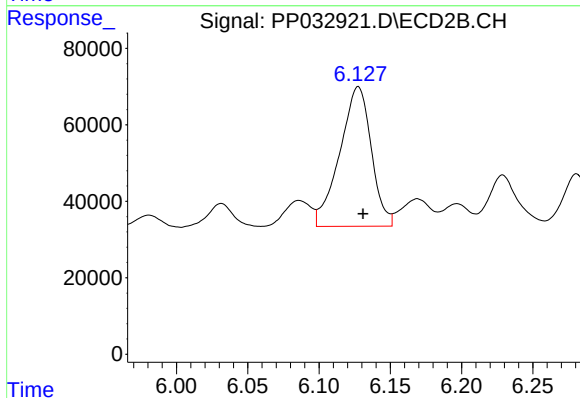


#26 AR-1254-1

R.T.: 6.128 min
Delta R.T.: -0.003 min
Response: 562506
Conc: 274.75 ng/ml

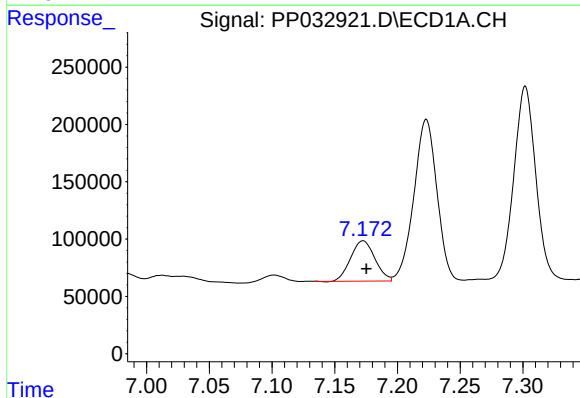


#27 AR-1254-2

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 475252
Conc: 188.97 ng/ml

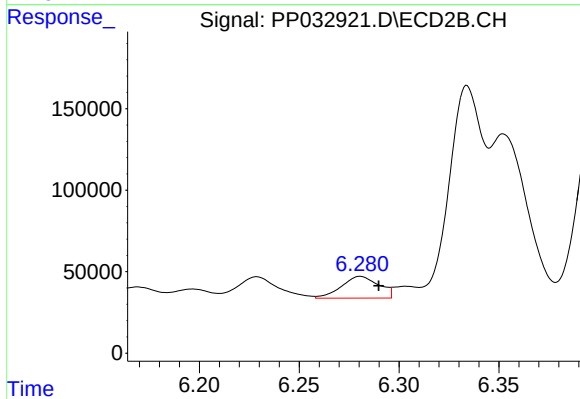

#27 AR-1254-2


R.T.: 6.281 min
Delta R.T.: -0.009 min
Response: 173564
Conc: 98.83 ng/ml

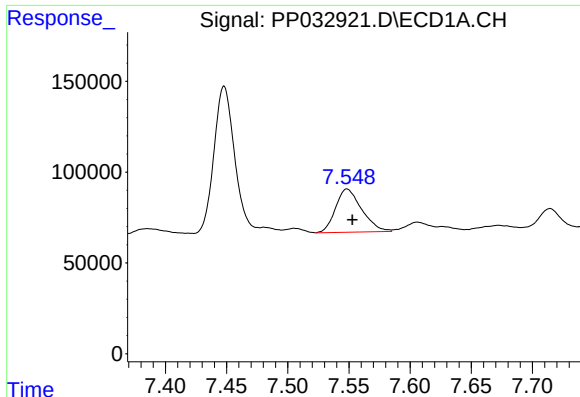

#28 AR-1254-3


R.T.: 7.548 min
Delta R.T.: -0.004 min
Response: 353533
Conc: 131.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-A

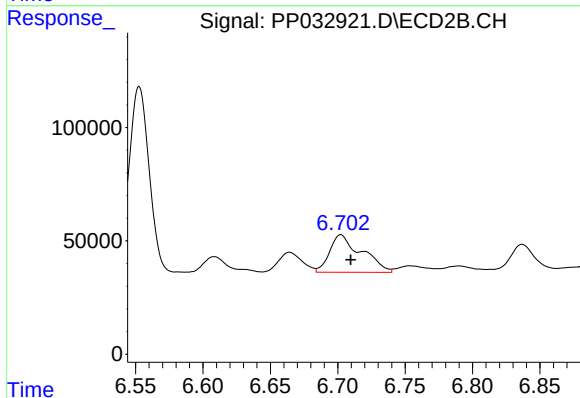


#28 AR-1254-3

R.T.: 6.702 min
Delta R.T.: -0.007 min
Response: 272980
Conc: 95.05 ng/ml

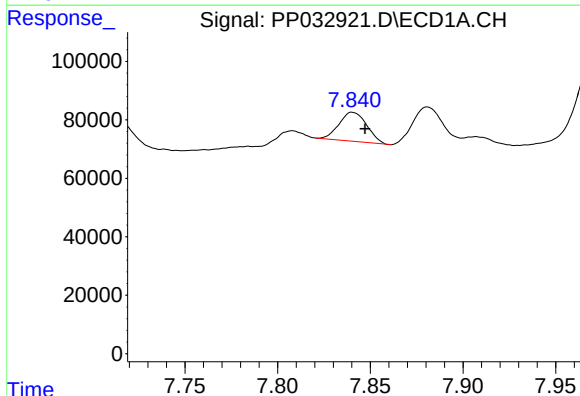


#29 AR-1254-4

R.T.: 7.840 min
Delta R.T.: -0.007 min
Response: 103272
Conc: 52.43 ng/ml

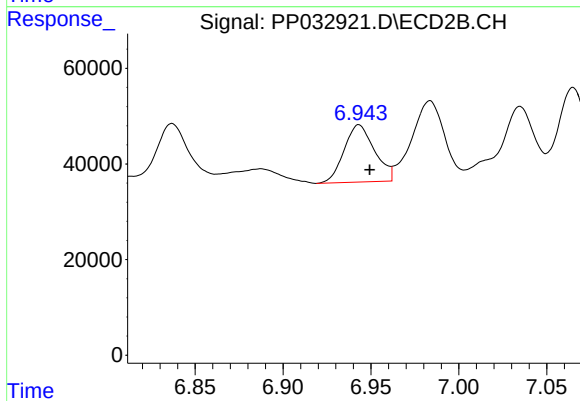

#29 AR-1254-4


R.T.: 6.943 min
Delta R.T.: -0.006 min
Response: 144456
Conc: 87.24 ng/ml

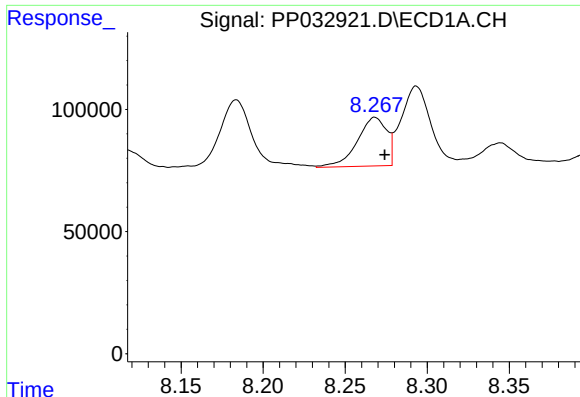

#30 AR-1254-5

R.T.: 8.268 min
Delta R.T.: -0.006 min
Response: 249119
Conc: 119.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-A

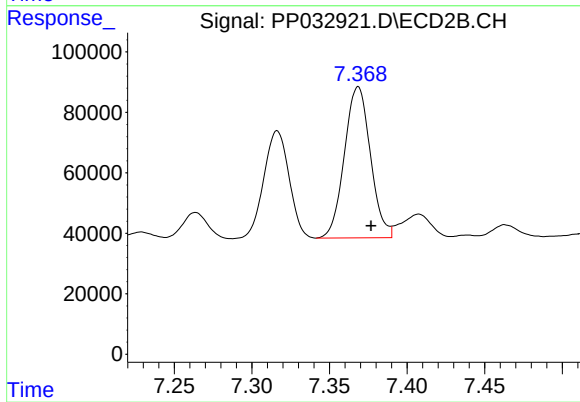

#30 AR-1254-5

R.T.: 7.368 min
Delta R.T.: -0.008 min
Response: 584333
Conc: 241.57 ng/ml