

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012521\
 Data File : PP032922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 11:34
 Operator : DD\AJ
 Sample : M1208-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-SF-03-011-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:39:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.738	4.008	1040689	939452	17.918	19.971
2)	SA Decachlor...	10.570	9.284	813147	715577	20.610	19.101
Target Compounds							
26)	L6 AR-1254-1	6.947	6.128	609865	553890	367.199	270.545 #
27)	L6 AR-1254-2	7.173	6.281	488110	157672	194.082	89.778 #
28)	L6 AR-1254-3	7.549	6.702	318904	148854	118.361	51.830 #
29)	L6 AR-1254-4	7.841	6.944	76500	115968	38.836	70.032 #
30)	L6 AR-1254-5	8.268	7.368	180570	427299	86.586	176.652 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012521\
Data File : PP032922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 11:34
Operator : DD\AJ
Sample : M1208-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:39:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

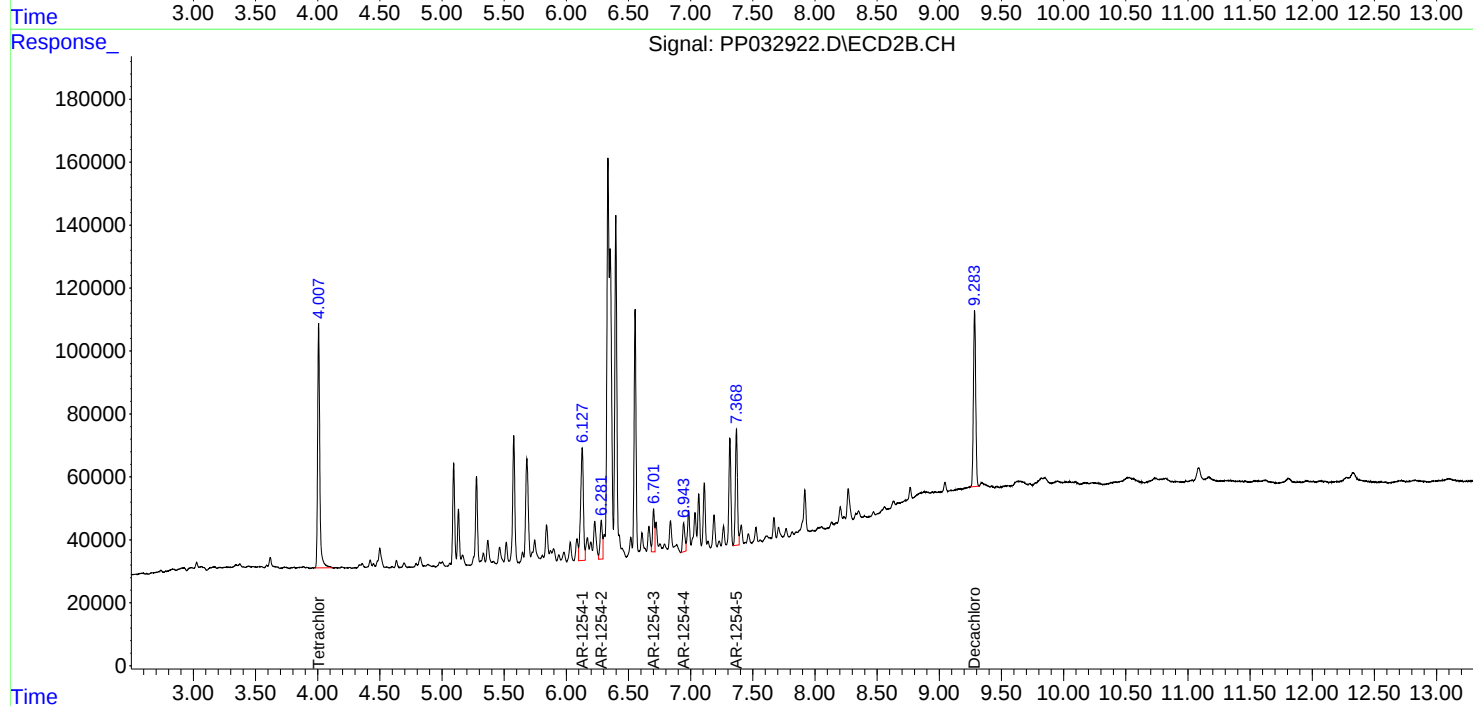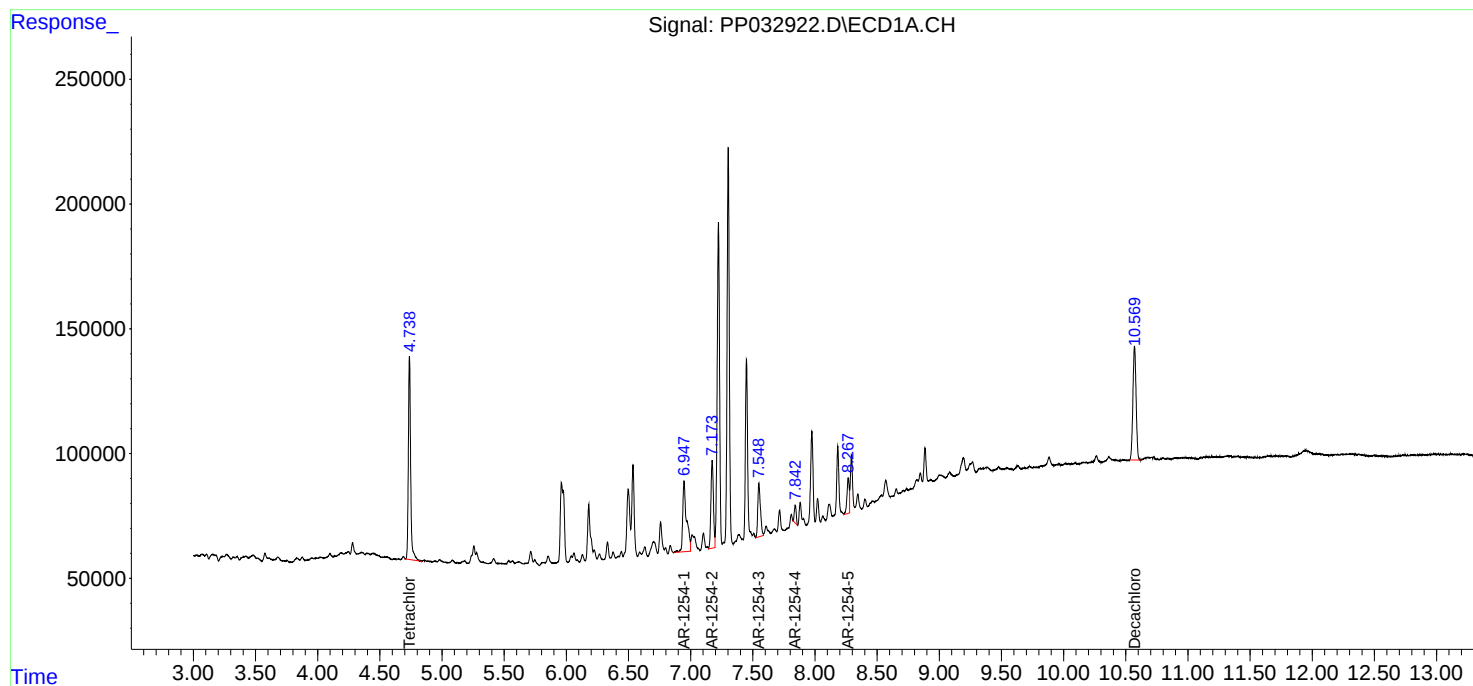


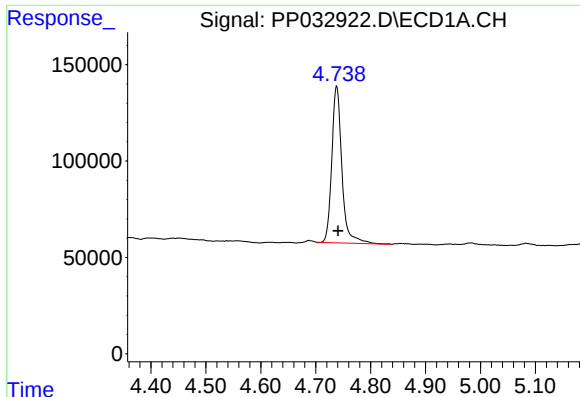

#1 Tetrachloro-m-xylene


R.T.: 4.738 min
Delta R.T.: -0.003 min
Response: 1040689
Conc: 17.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-B

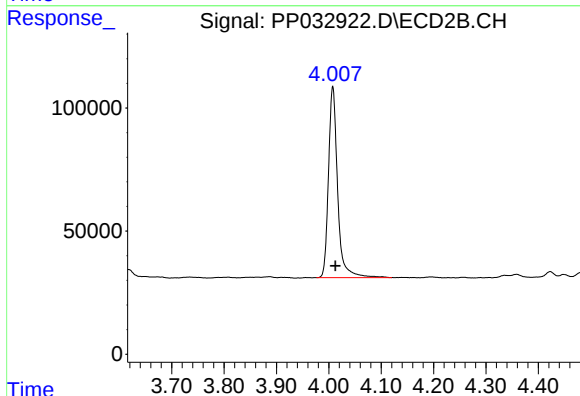


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.005 min
Response: 939452
Conc: 19.97 ng/ml

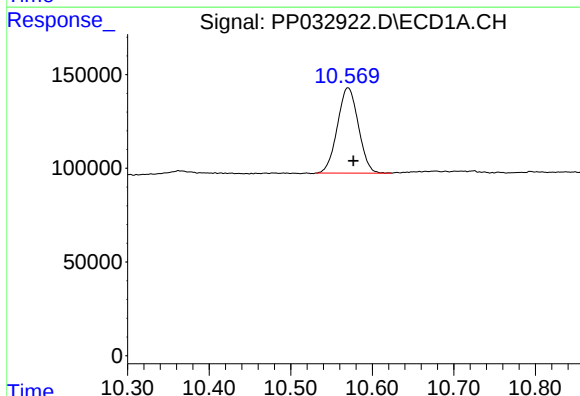


#2 Decachlorobiphenyl

R.T.: 10.570 min
Delta R.T.: -0.007 min
Response: 813147
Conc: 20.61 ng/ml

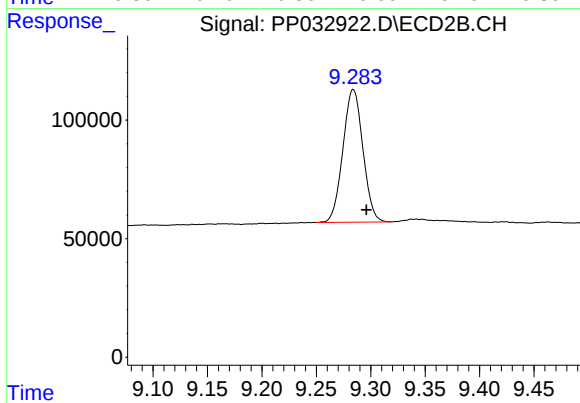

#2 Decachlorobiphenyl


R.T.: 9.284 min
Delta R.T.: -0.012 min
Response: 715577
Conc: 19.10 ng/ml

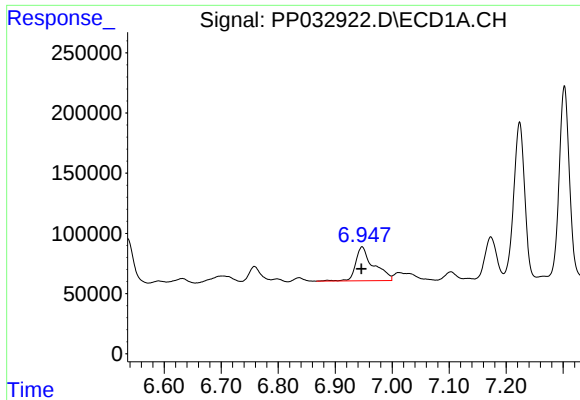

#26 AR-1254-1


R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 609865
Conc: 367.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-B

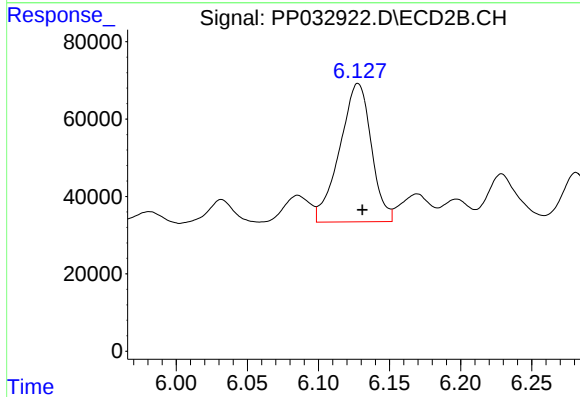


#26 AR-1254-1

R.T.: 6.128 min
Delta R.T.: -0.003 min
Response: 553890
Conc: 270.54 ng/ml

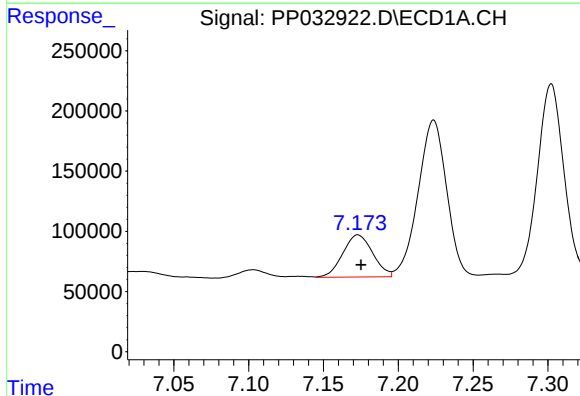


#27 AR-1254-2

R.T.: 7.173 min
Delta R.T.: -0.002 min
Response: 488110
Conc: 194.08 ng/ml

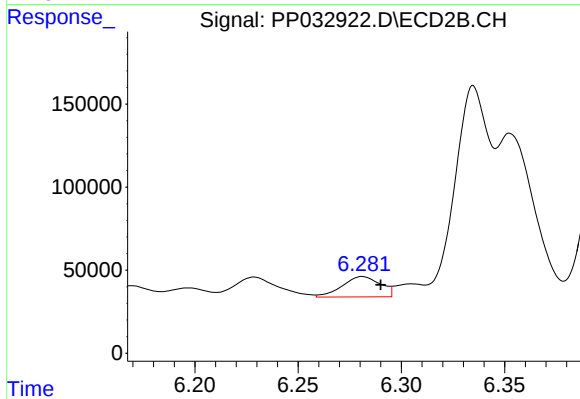

#27 AR-1254-2


R.T.: 6.281 min
Delta R.T.: -0.009 min
Response: 157672
Conc: 89.78 ng/ml

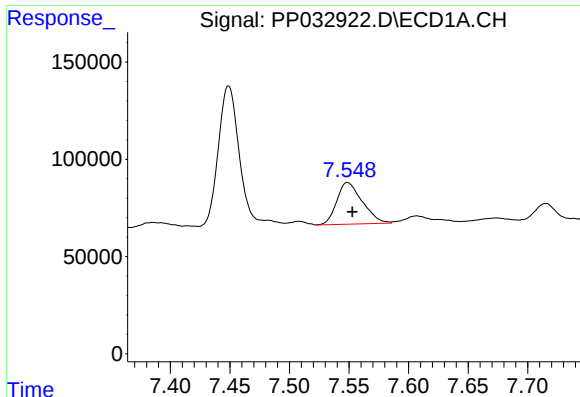

#28 AR-1254-3


R.T.: 7.549 min
Delta R.T.: -0.004 min
Response: 318904
Conc: 118.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-B

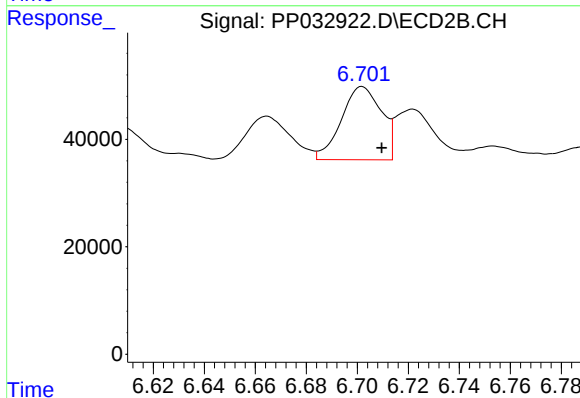


#28 AR-1254-3

R.T.: 6.702 min
Delta R.T.: -0.008 min
Response: 148854
Conc: 51.83 ng/ml

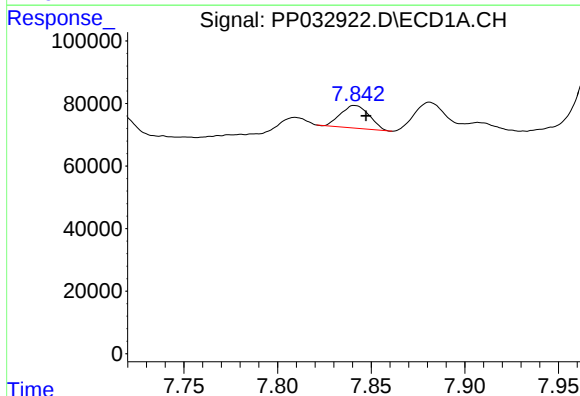


#29 AR-1254-4

R.T.: 7.841 min
Delta R.T.: -0.006 min
Response: 76500
Conc: 38.84 ng/ml

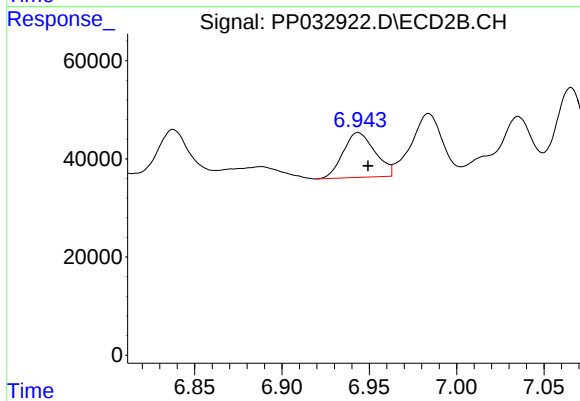

#29 AR-1254-4


R.T.: 6.944 min
Delta R.T.: -0.006 min
Response: 115968
Conc: 70.03 ng/ml

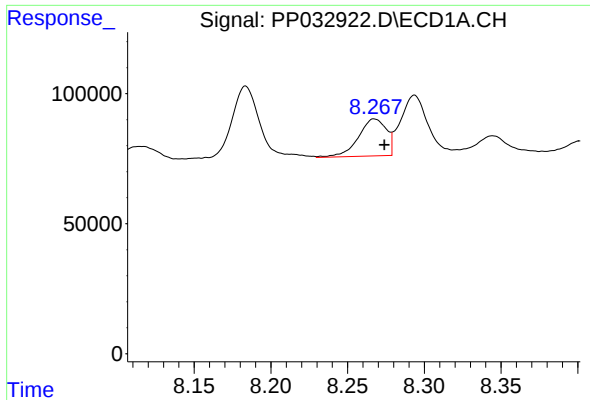

#30 AR-1254-5

R.T.: 8.268 min
Delta R.T.: -0.006 min
Response: 180570
Conc: 86.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-03-011-B

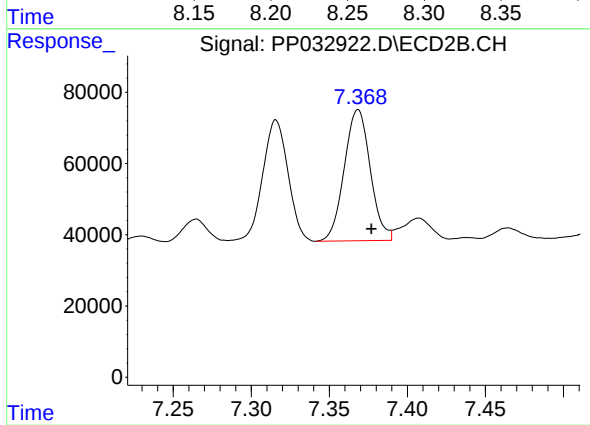

#30 AR-1254-5

R.T.: 7.368 min
Delta R.T.: -0.008 min
Response: 427299
Conc: 176.65 ng/ml