

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
 Data File : PP043244.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 12:36
 Operator : AJ\MA
 Sample : N1240-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2022-9A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:37:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	4.034	41548	45471	1.808	2.041
2) SA Decachlor...	10.791	9.363	40405	39717	2.853	2.130 #
Target Compounds						
20) L4 AR-1242-5	0.000	6.174	0	8137	N.D.	12.727 #
26) L6 AR-1254-1	0.000	6.174	0	8137	N.D.	5.738 #
28) L6 AR-1254-3	0.000	6.759	0	11753	N.D.	6.116 #
29) L6 AR-1254-4	7.979	0.000	3841	0	5.449	N.D. #
30) L6 AR-1254-5	0.000	7.427	0	8226	N.D.	5.325 #
32) L7 AR-1260-2	8.116	0.000	6087	0	7.149	N.D. #
34) L7 AR-1260-4	8.726	0.000	18373	0	24.031	N.D. #
35) L7 AR-1260-5	9.040	0.000	50272	0	38.071	N.D. #
36) L8 AR-1262-1	0.000	7.427	0	8226	N.D.	9.823 #
37) L8 AR-1262-2	9.040	0.000	50272	0	32.707	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
Data File : PP043244.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 12:36
Operator : AJ\MA
Sample : N1240-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:37:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

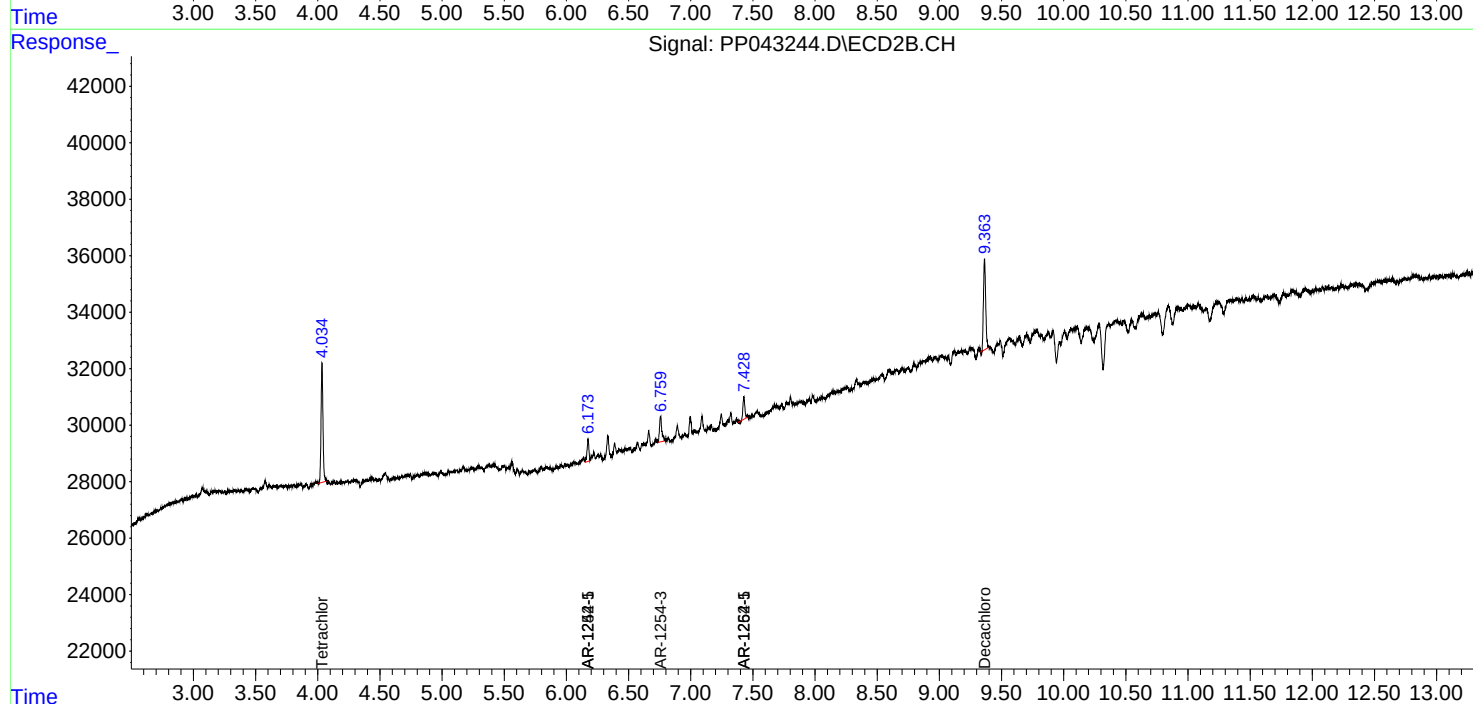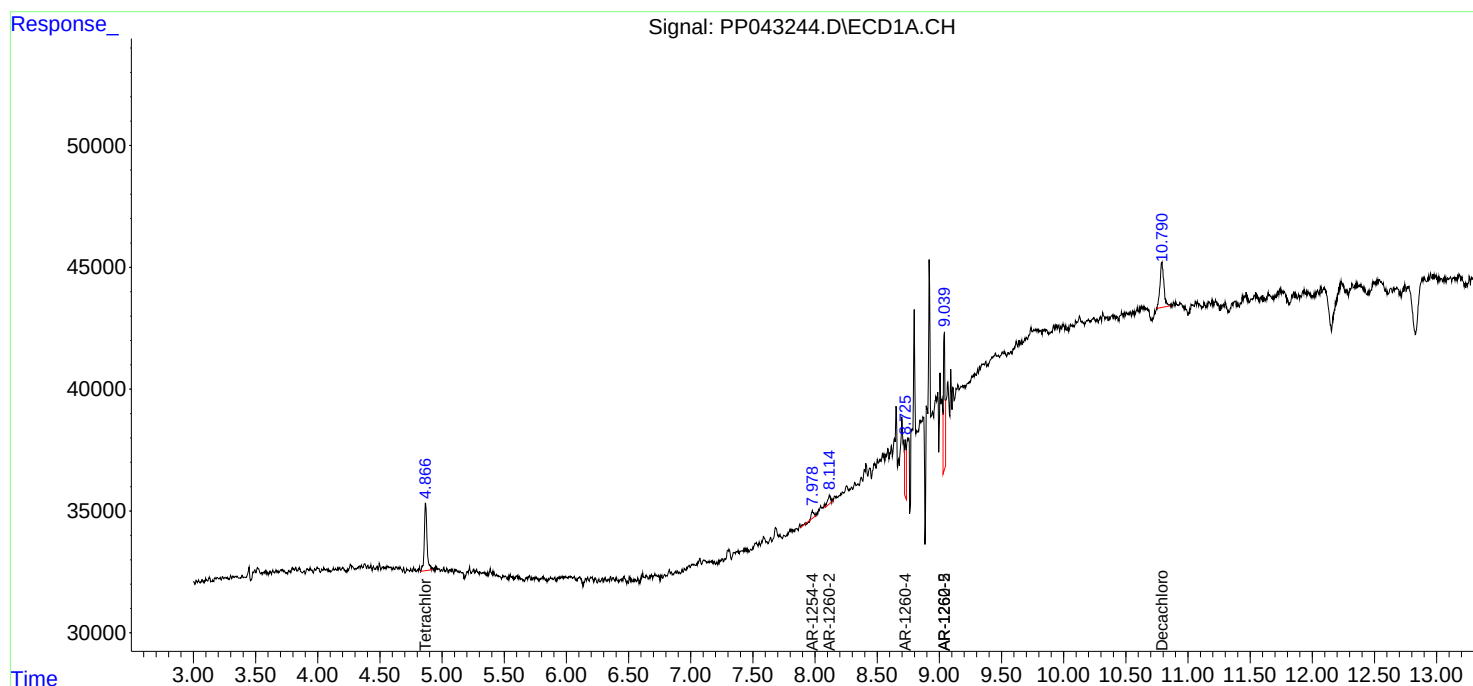


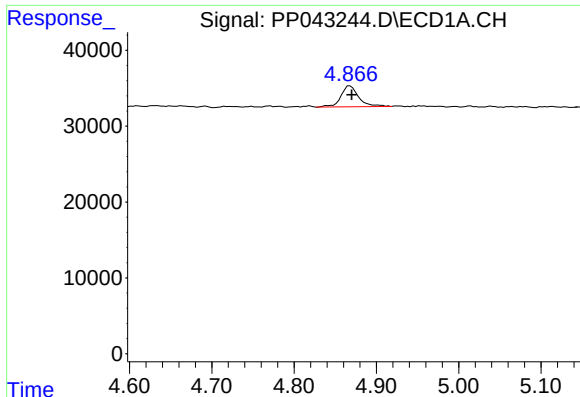

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.002 min
Response: 41548
Conc: 1.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

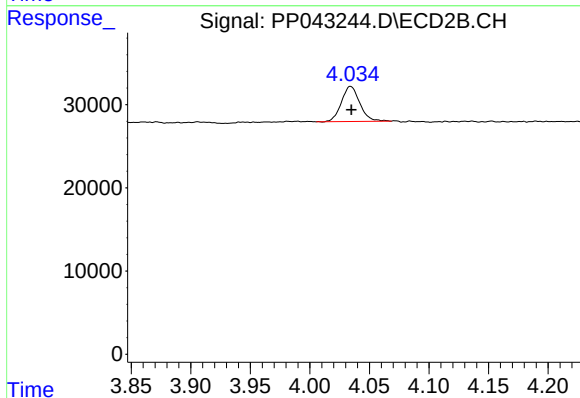


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 45471
Conc: 2.04 ng/ml

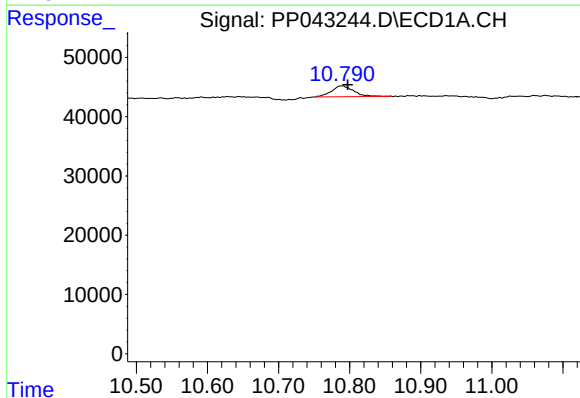


#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: -0.007 min
Response: 40405
Conc: 2.85 ng/ml

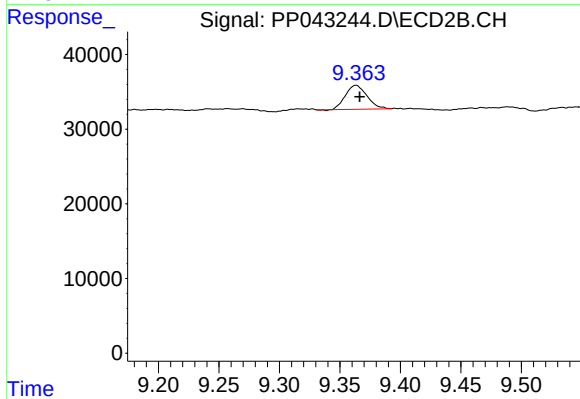

#2 Decachlorobiphenyl


R.T.: 9.363 min
Delta R.T.: -0.003 min
Response: 39717
Conc: 2.13 ng/ml

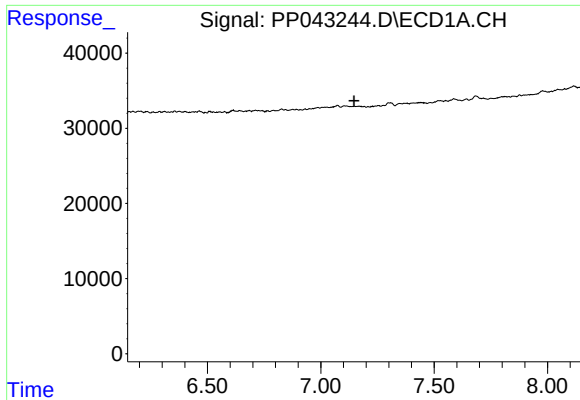

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

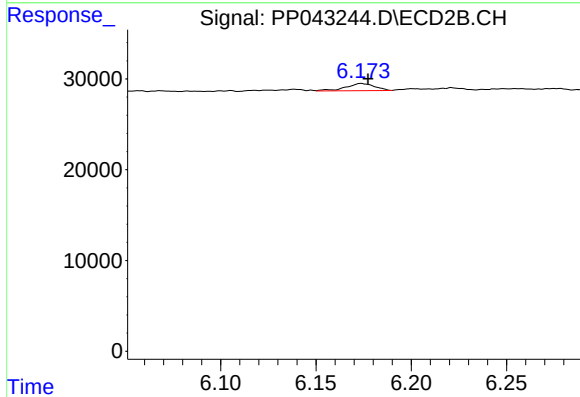


#20 AR-1242-5

R.T.: 6.174 min
Delta R.T.: -0.004 min
Response: 8137
Conc: 12.73 ng/ml

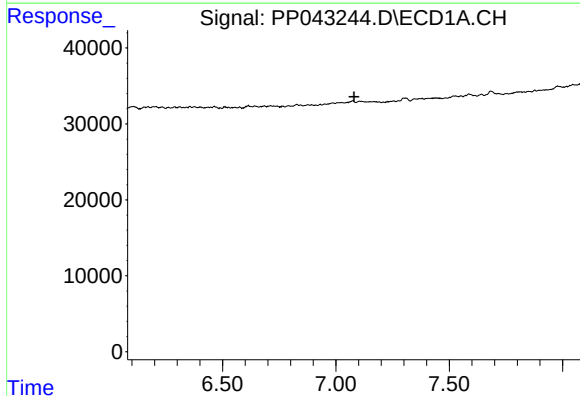


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

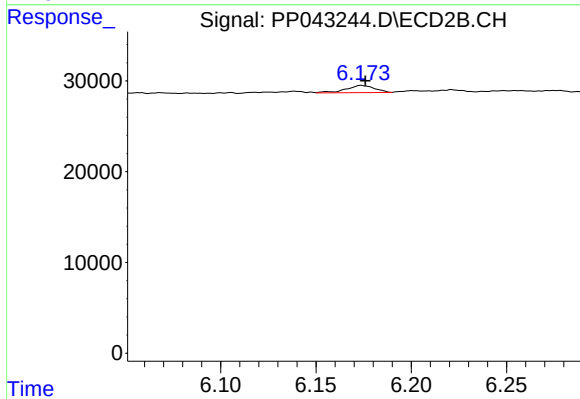

#26 AR-1254-1


R.T.: 6.174 min
Delta R.T.: -0.002 min
Response: 8137
Conc: 5.74 ng/ml

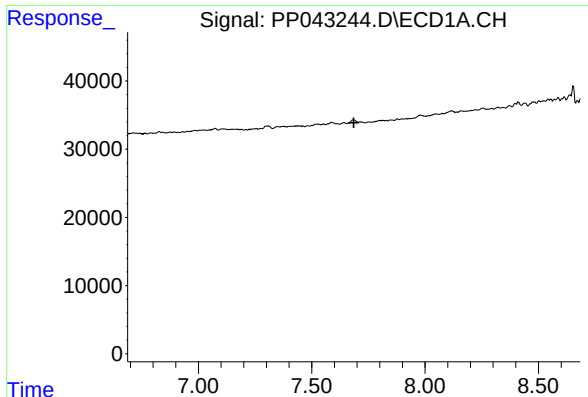

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

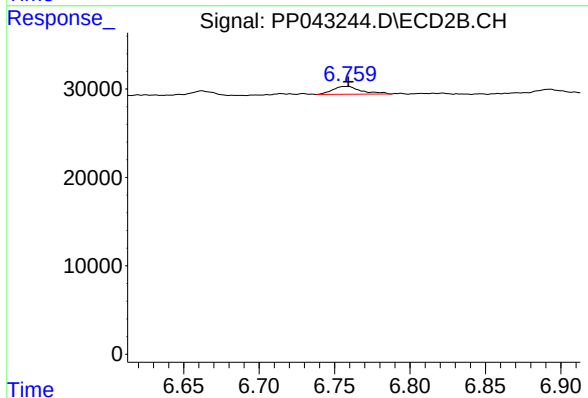


#28 AR-1254-3

R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 11753
Conc: 6.12 ng/ml

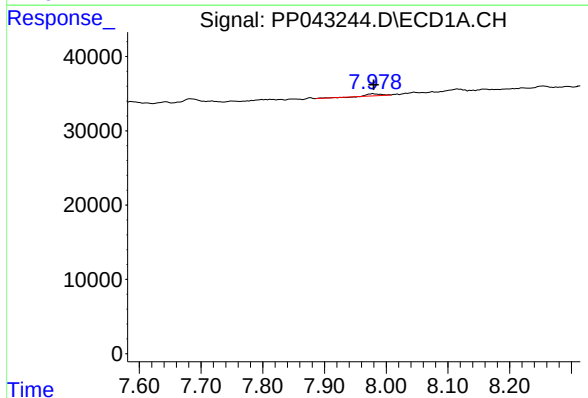


#29 AR-1254-4

R.T.: 7.979 min
Delta R.T.: 0.000 min
Response: 3841
Conc: 5.45 ng/ml

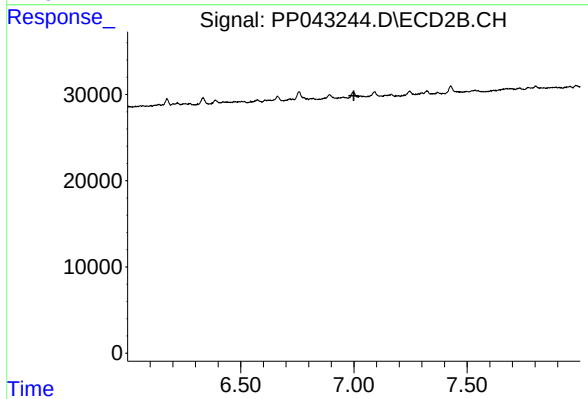

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.000 min
Response: 0
Conc: N.D.

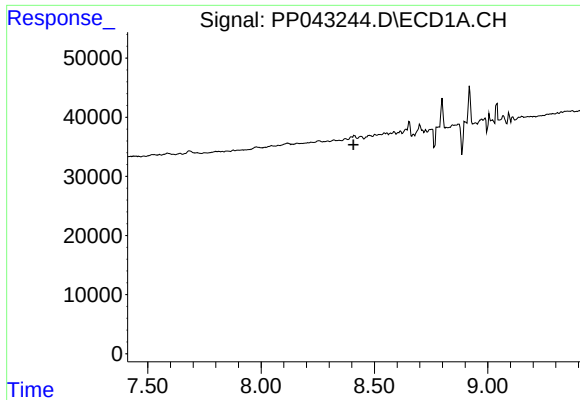

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 8.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

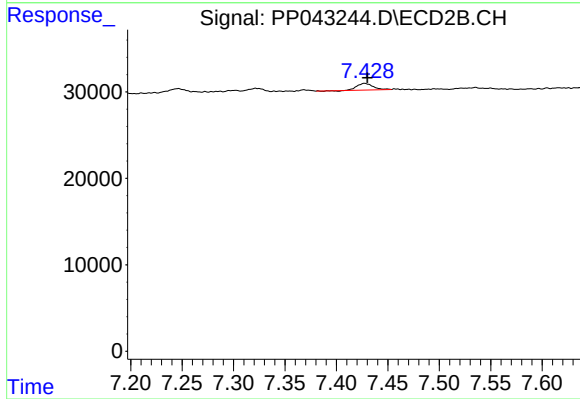


#30 AR-1254-5

R.T.: 7.427 min
Delta R.T.: -0.003 min
Response: 8226
Conc: 5.33 ng/ml

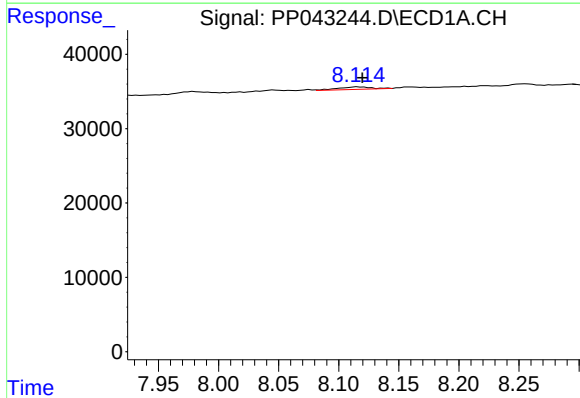


#32 AR-1260-2

R.T.: 8.116 min
Delta R.T.: -0.004 min
Response: 6087
Conc: 7.15 ng/ml

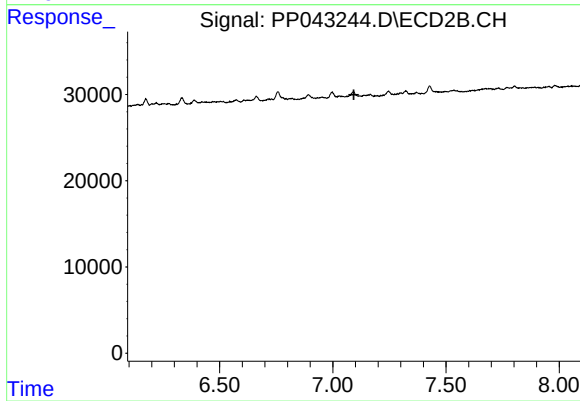

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.093 min
Response: 0
Conc: N.D.

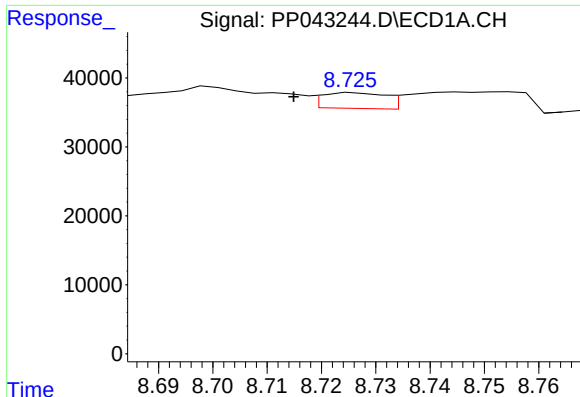

#34 AR-1260-4


R.T.: 8.726 min
Delta R.T.: 0.012 min
Response: 18373
Conc: 24.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

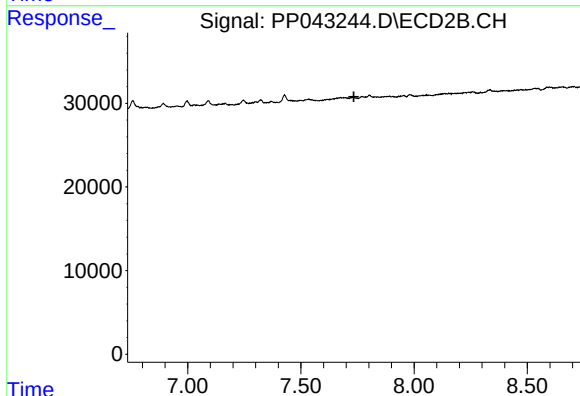


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.734 min
Response: 0
Conc: N.D.

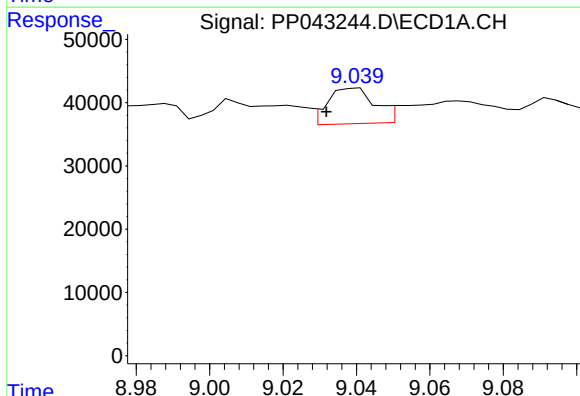


#35 AR-1260-5

R.T.: 9.040 min
Delta R.T.: 0.008 min
Response: 50272
Conc: 38.07 ng/ml

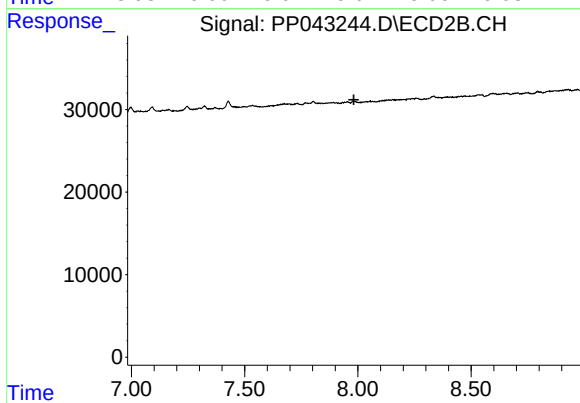

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.982 min
Response: 0
Conc: N.D.

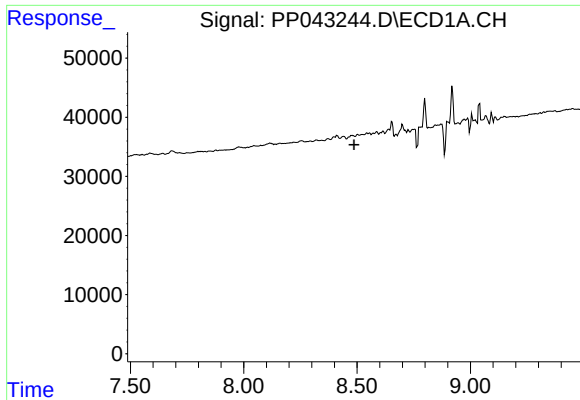

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

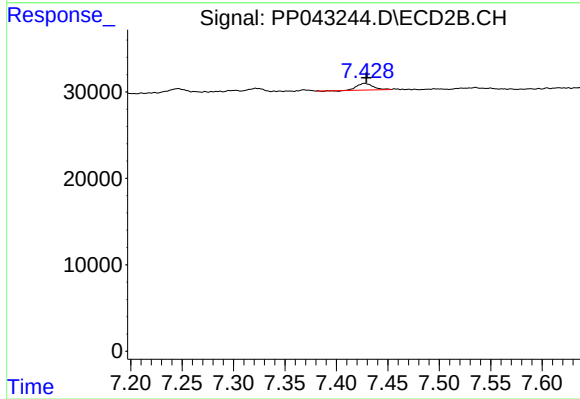


#36 AR-1262-1

R.T.: 7.427 min
Delta R.T.: -0.002 min
Response: 8226
Conc: 9.82 ng/ml

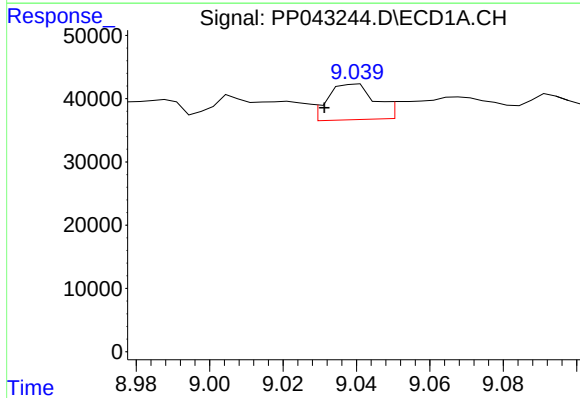

#37 AR-1262-2

R.T.: 9.040 min
Delta R.T.: 0.009 min
Response: 50272
Conc: 32.71 ng/ml

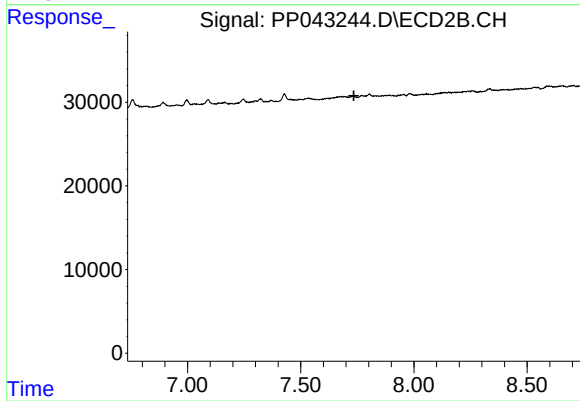

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 7.735 min
Response: 0
Conc: N.D.