

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
 Data File : PP043255.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 16:06
 Operator : AJ\MA
 Sample : N1222-10 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-5B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:39:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.867	4.033	37896	45376	1.649	2.036
2) SA Decachlor...	10.790	9.361	36396	42362	2.570	2.272
Target Compounds						
32) L7 AR-1260-2	8.108	0.000	3228	0	3.791	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
Data File : PP043255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 16:06
Operator : AJ\MA
Sample : N1222-10 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-5B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:39:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

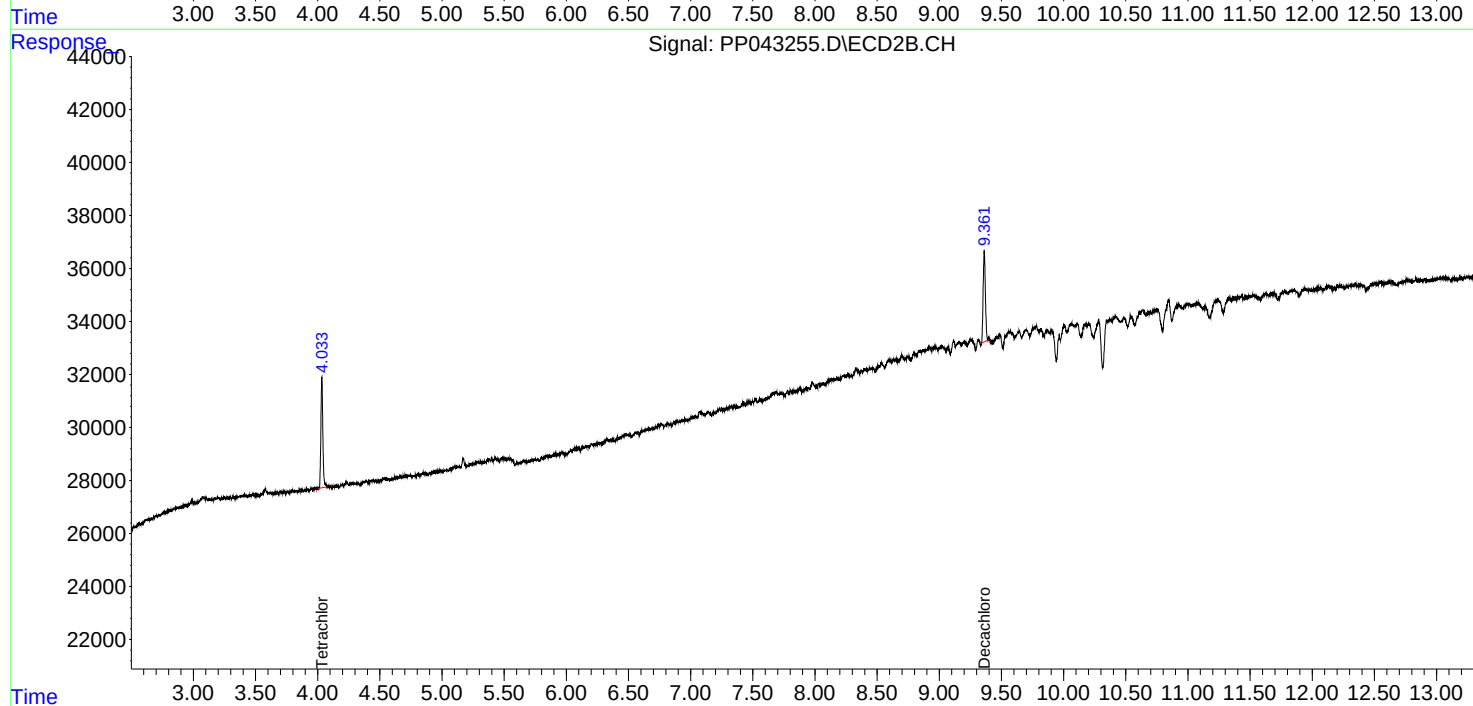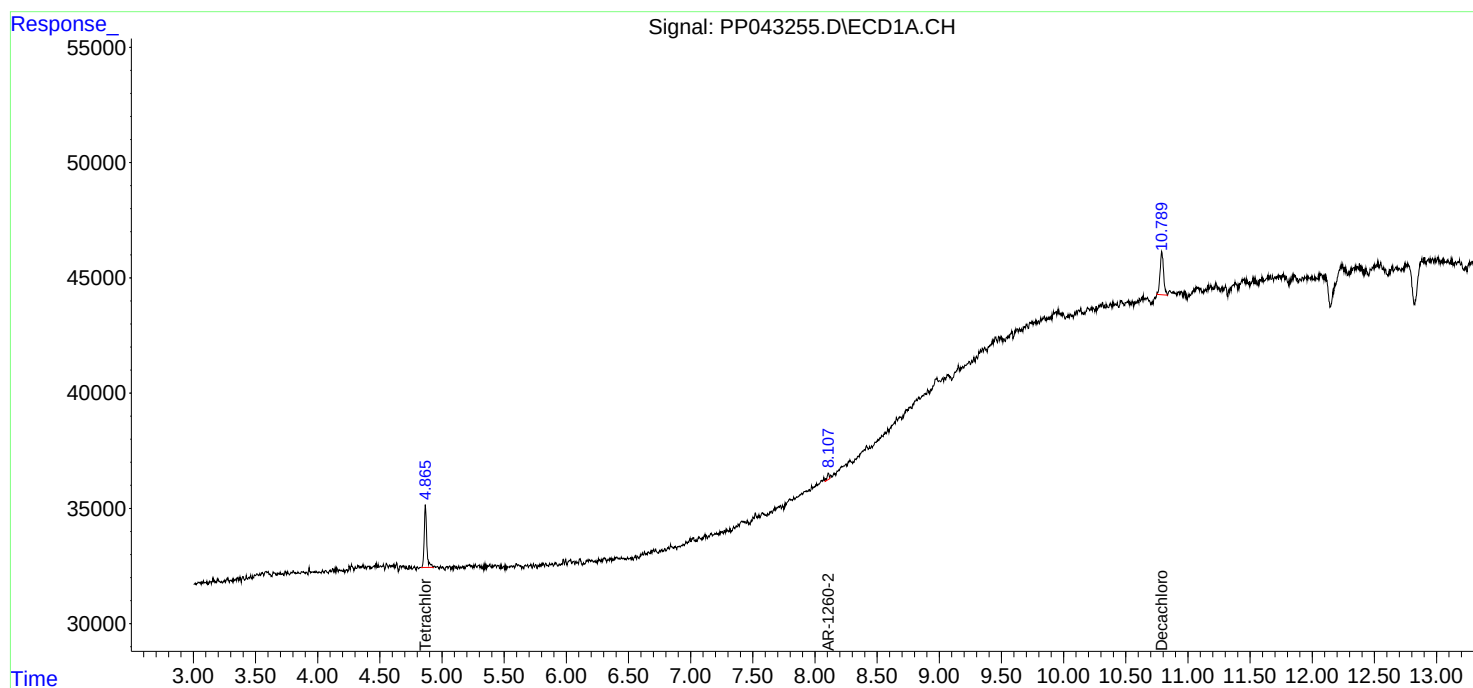


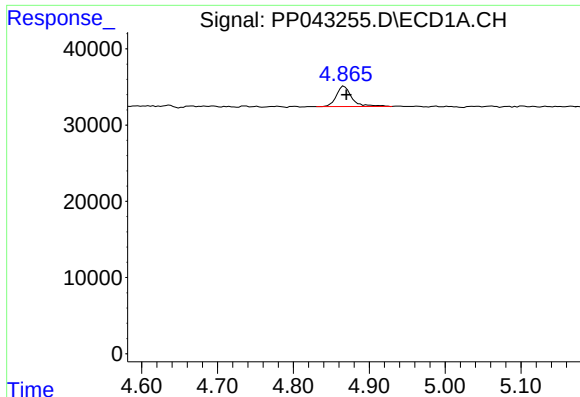

#1 Tetrachloro-m-xylene


R.T.: 4.867 min
Delta R.T.: -0.003 min
Response: 37896
Conc: 1.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-5B

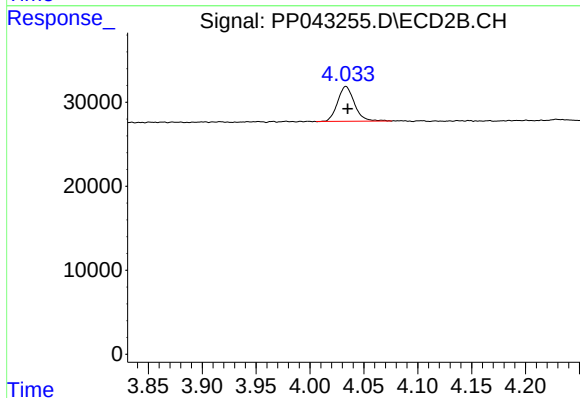


#1 Tetrachloro-m-xylene

R.T.: 4.033 min
Delta R.T.: -0.002 min
Response: 45376
Conc: 2.04 ng/ml

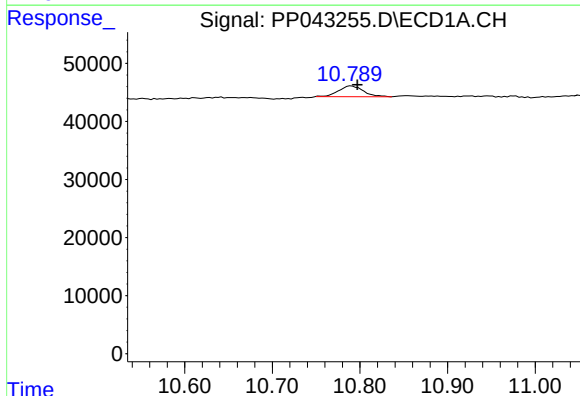


#2 Decachlorobiphenyl

R.T.: 10.790 min
Delta R.T.: -0.007 min
Response: 36396
Conc: 2.57 ng/ml

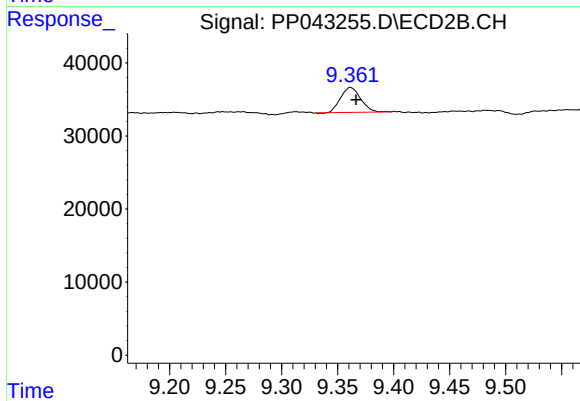

#2 Decachlorobiphenyl


R.T.: 9.361 min
Delta R.T.: -0.005 min
Response: 42362
Conc: 2.27 ng/ml

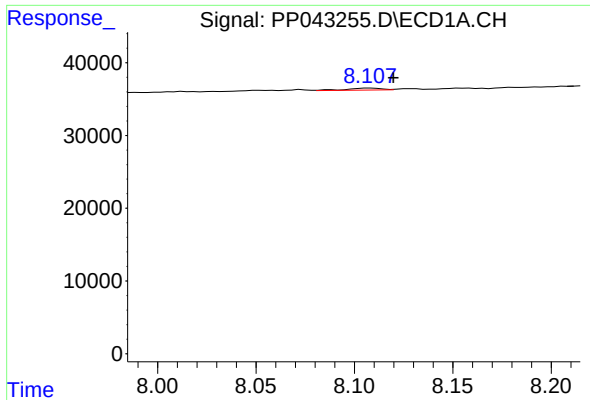

#32 AR-1260-2

R.T.: 8.108 min
Delta R.T.: -0.012 min
Response: 3228
Conc: 3.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-5B

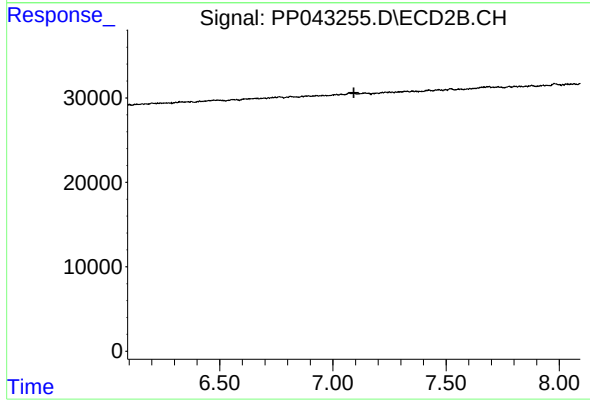

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.093 min
Response: 0
Conc: N.D.