

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
 Data File : PP043257.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 16:39
 Operator : AJ\MA
 Sample : N1222-12 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-6B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:39:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.867	4.034	40725	41010	1.772	1.840
2)	SA Decachlor...	10.791	9.361	36720	41706	2.593	2.237
Target Compounds							
29)	L6 AR-1254-4	7.983	0.000	19535	0	27.714	N.D. #
30)	L6 AR-1254-5	8.408	0.000	2033	0	2.517	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
Data File : PP043257.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 16:39
Operator : AJ\MA
Sample : N1222-12 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-6B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:39:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

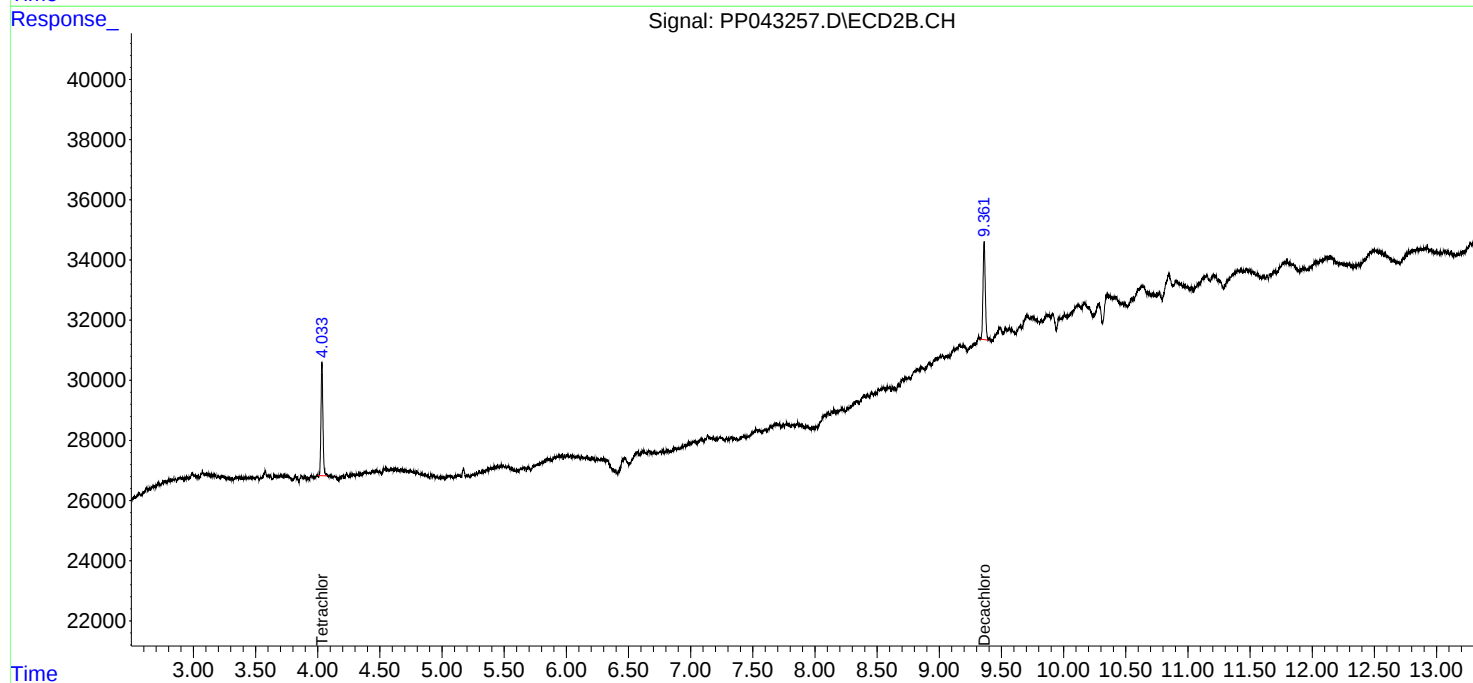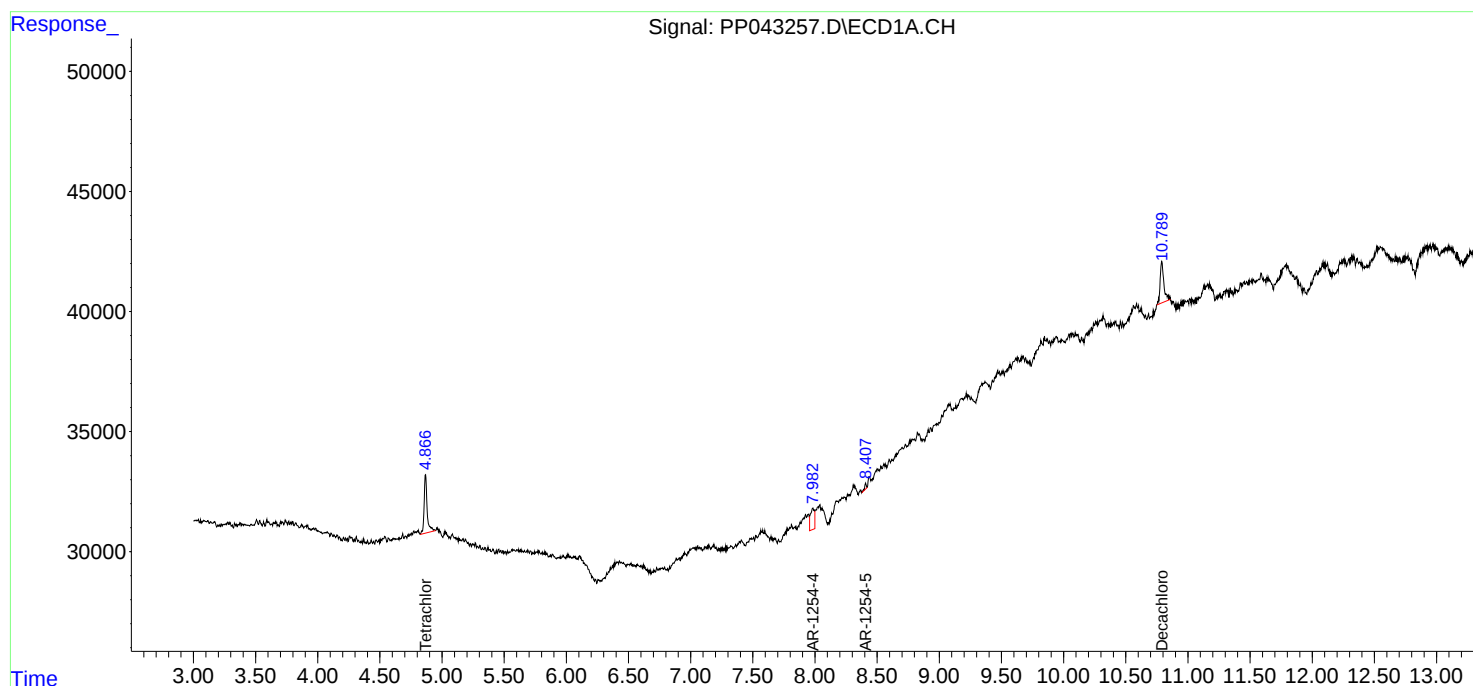


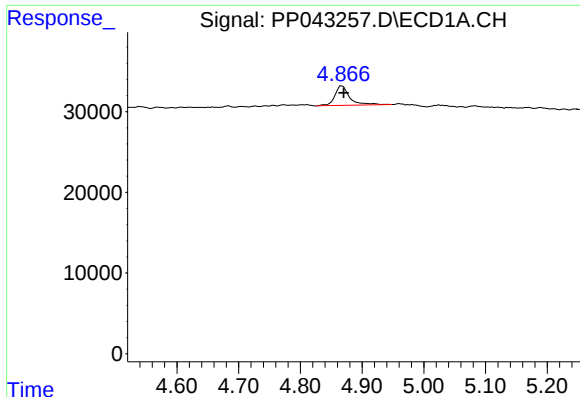

#1 Tetrachloro-m-xylene


R.T.: 4.867 min
Delta R.T.: -0.003 min
Response: 40725
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-6B

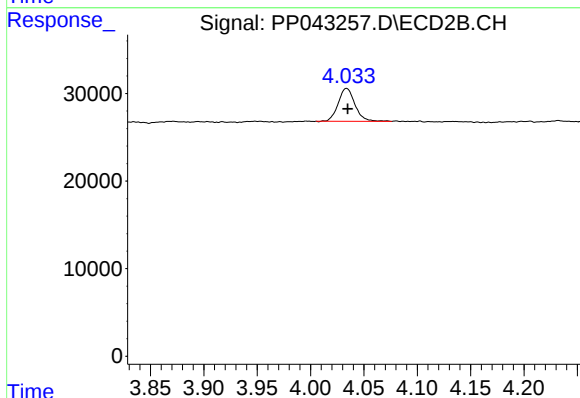


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: -0.001 min
Response: 41010
Conc: 1.84 ng/ml

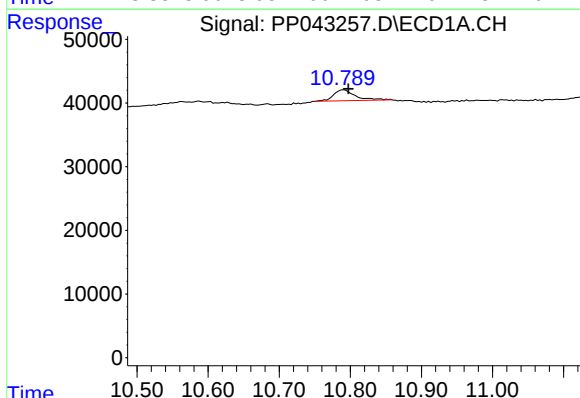


#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: -0.006 min
Response: 36720
Conc: 2.59 ng/ml

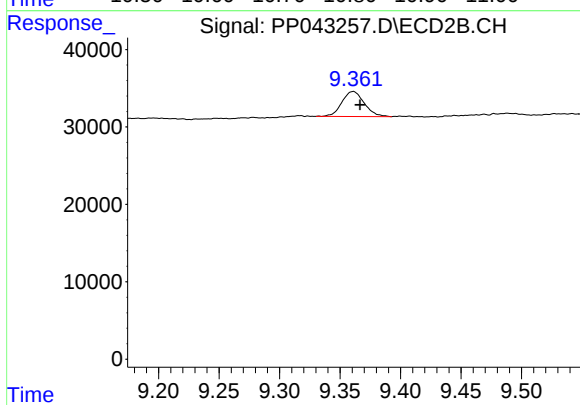

#2 Decachlorobiphenyl


R.T.: 9.361 min
Delta R.T.: -0.005 min
Response: 41706
Conc: 2.24 ng/ml

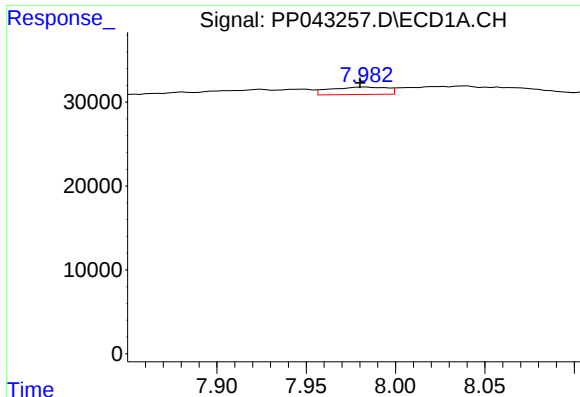

#29 AR-1254-4


R.T.: 7.983 min
Delta R.T.: 0.003 min
Response: 19535
Conc: 27.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-6B

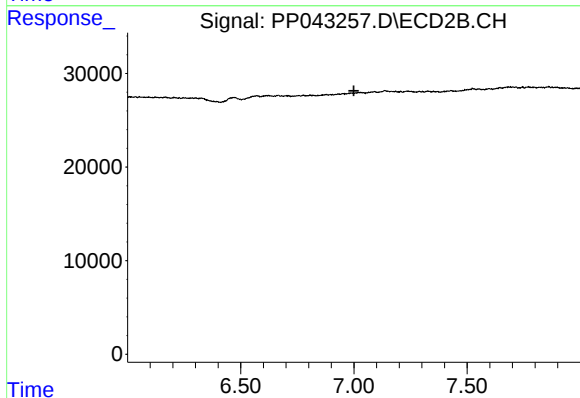


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.000 min
Response: 0
Conc: N.D.

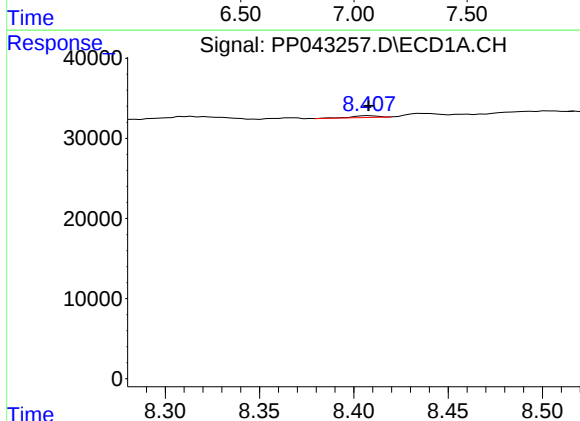

#30 AR-1254-5

R.T.: 8.408 min
Delta R.T.: 0.000 min
Response: 2033
Conc: 2.52 ng/ml

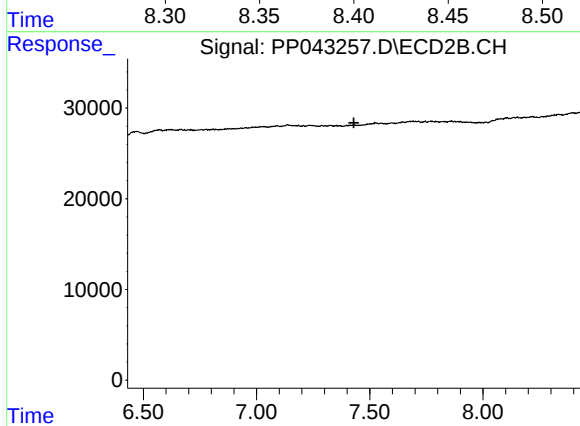

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.