

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
 Data File : PP043260.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 17:29
 Operator : AJ\MA
 Sample : N1222-15 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-8A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:40:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.869	4.034	40710	50601	1.771	2.271 #
2)	SA Decachlor...	10.793	9.363	43510	44501	3.072	2.387
Target Compounds							
33)	L7 AR-1260-3	8.460f	0.000	3622	0	5.493	N.D. #
36)	L8 AR-1262-1	8.460f	0.000	3622	0	3.646	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
Data File : PP043260.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 17:29
Operator : AJ\MA
Sample : N1222-15 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-8A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:40:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

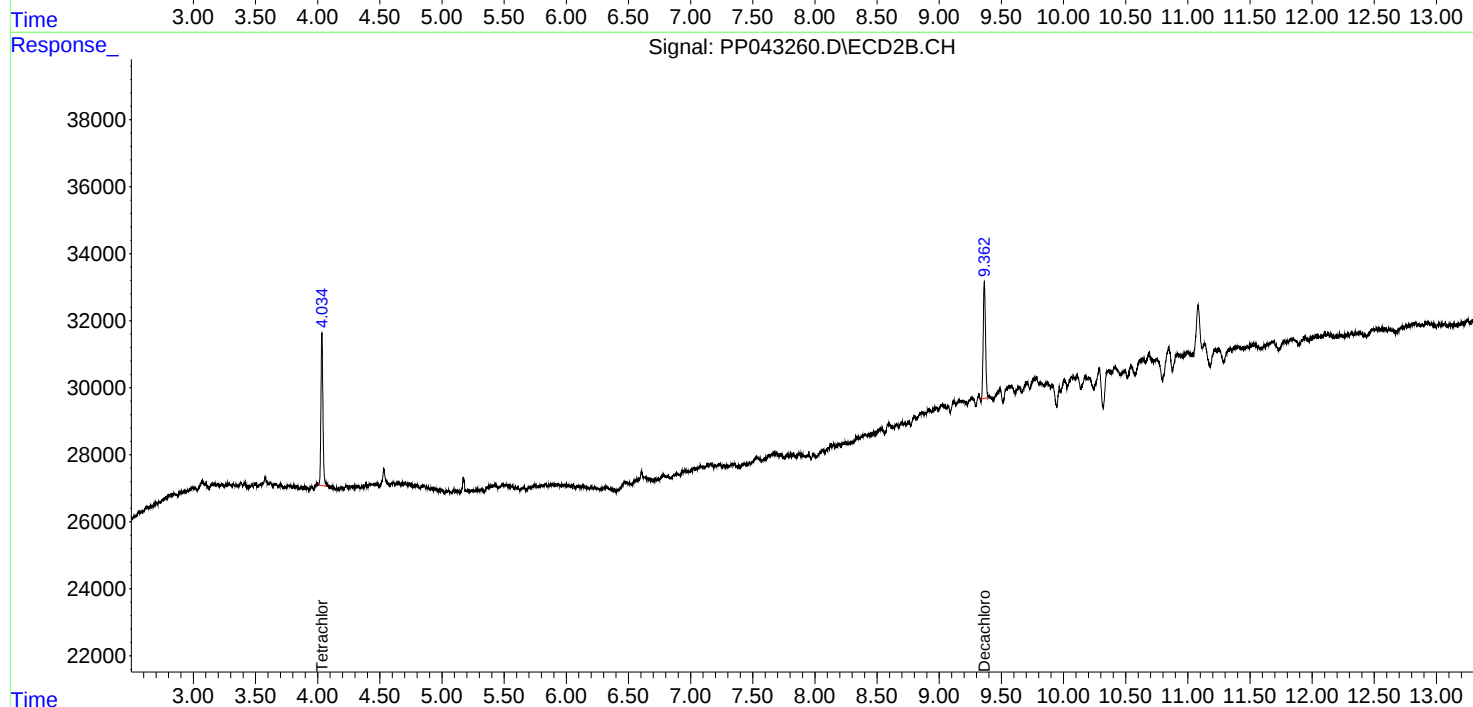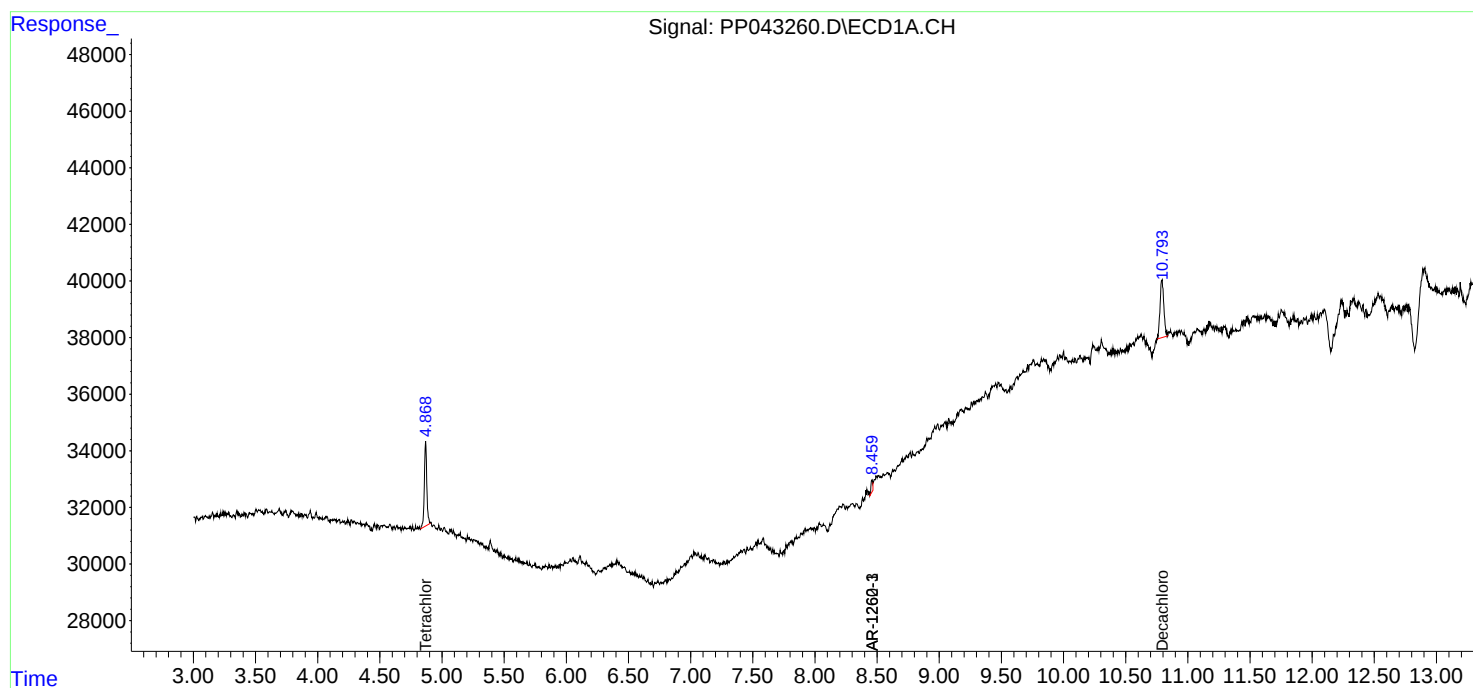


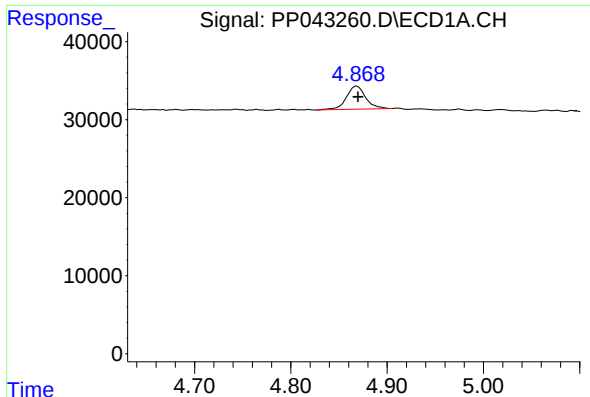

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.001 min
Response: 40710
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-8A

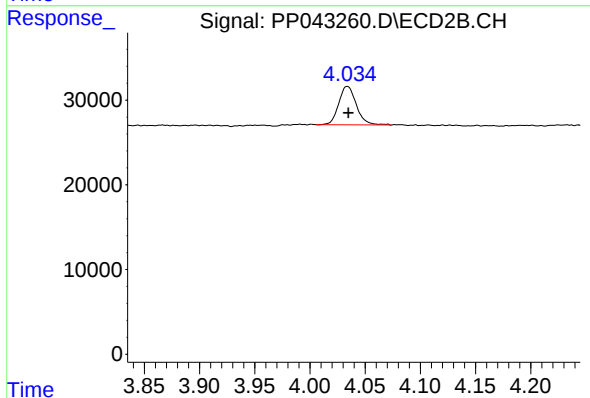


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 50601
Conc: 2.27 ng/ml

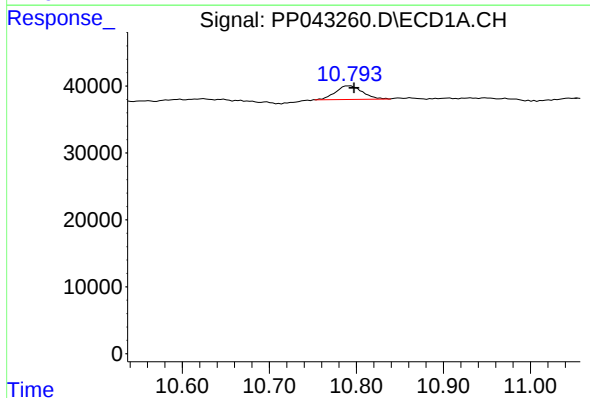


#2 Decachlorobiphenyl

R.T.: 10.793 min
Delta R.T.: -0.004 min
Response: 43510
Conc: 3.07 ng/ml

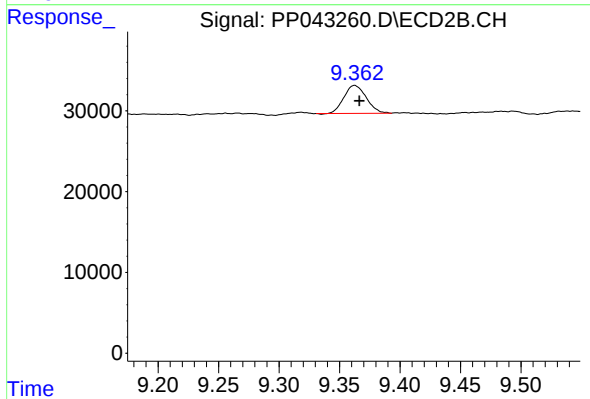

#2 Decachlorobiphenyl


R.T.: 9.363 min
Delta R.T.: -0.004 min
Response: 44501
Conc: 2.39 ng/ml

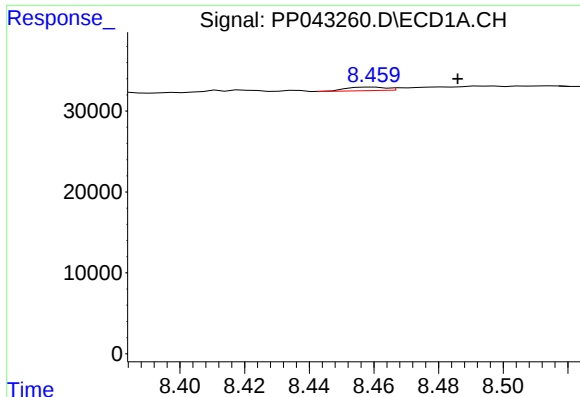

#33 AR-1260-3


R.T.: 8.460 min
Delta R.T.: -0.026 min
Response: 3622
Conc: 5.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-8A

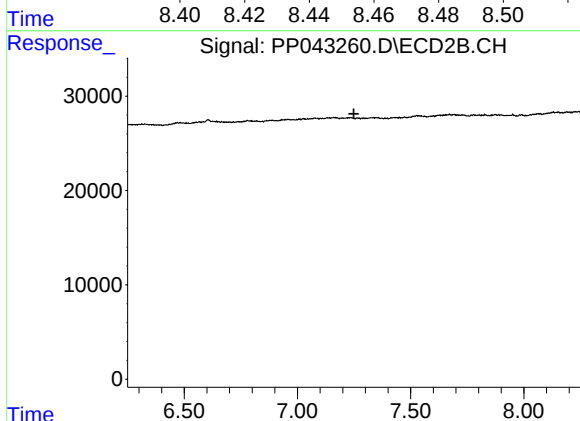


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.250 min
Response: 0
Conc: N.D.

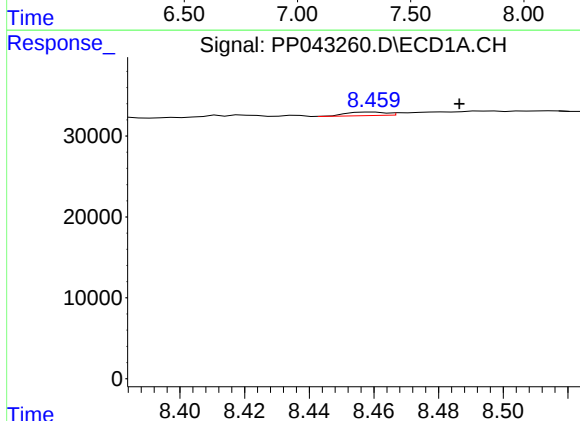

#36 AR-1262-1

R.T.: 8.460 min
Delta R.T.: -0.026 min
Response: 3622
Conc: 3.65 ng/ml

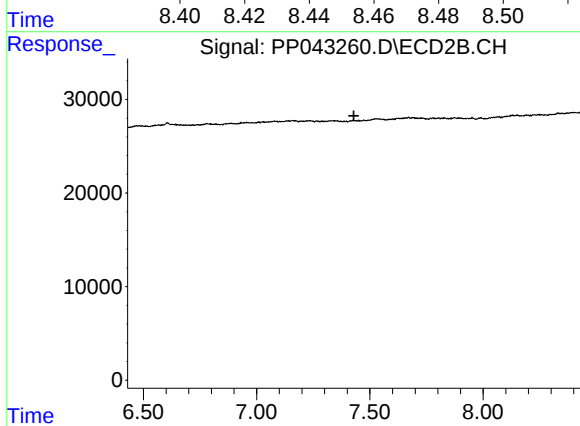

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.429 min
Response: 0
Conc: N.D.