

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
 Data File : PP043244.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 12:36
 Operator : AJ\MA
 Sample : N1240-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2022-9A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:37:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	4.034	41548	45471	1.808	2.041
2) SA Decachlor...	10.791	9.363	40405	39717	2.853	2.130 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
Data File : PP043244.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 12:36
Operator : AJ\MA
Sample : N1240-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:37:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

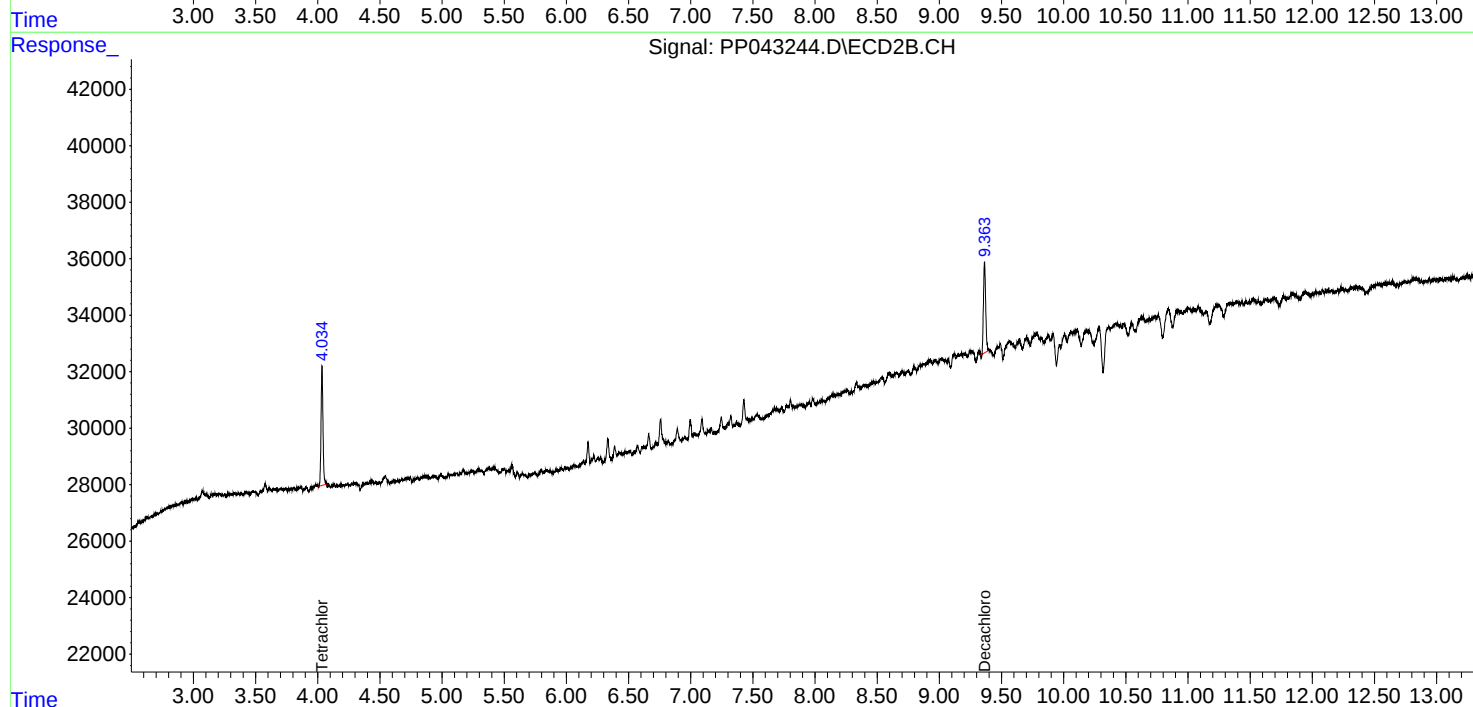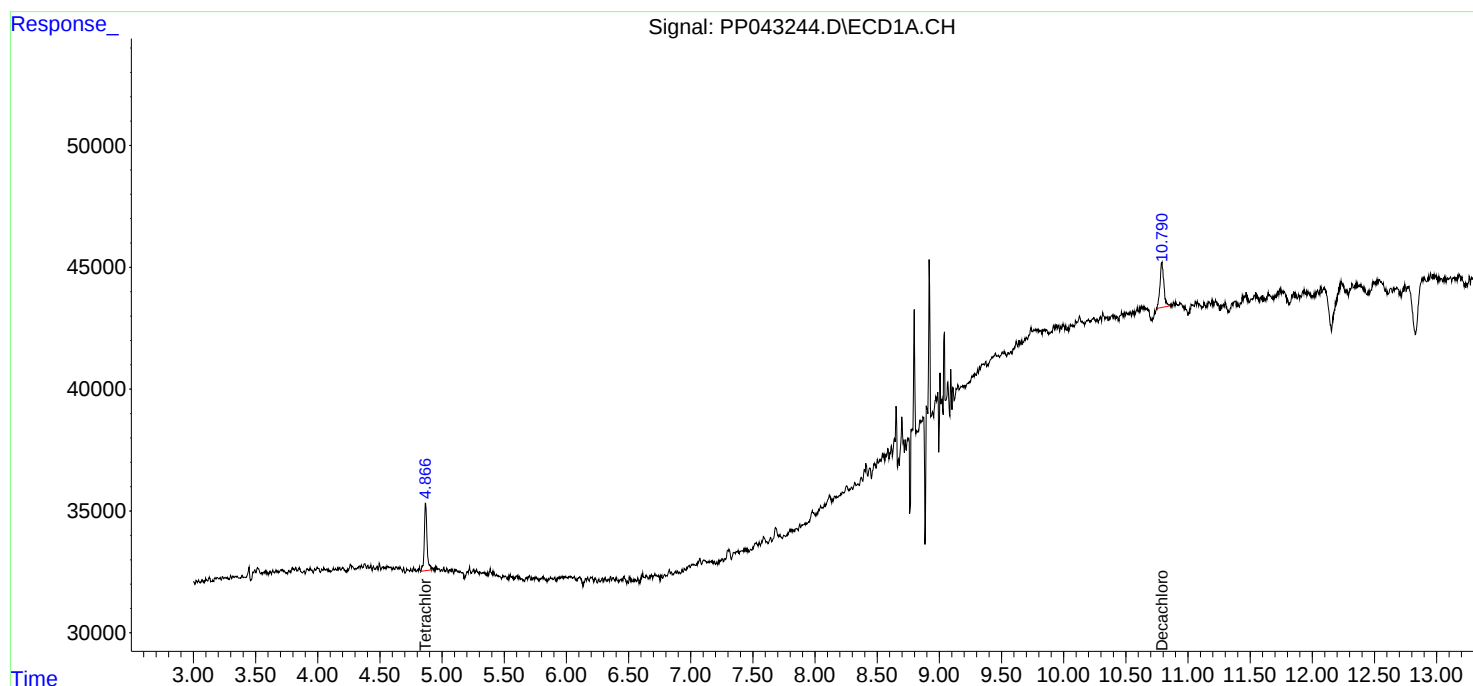


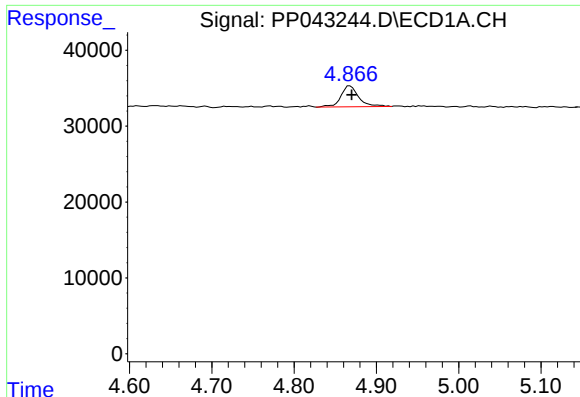

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.002 min
Response: 41548
Conc: 1.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2022-9A

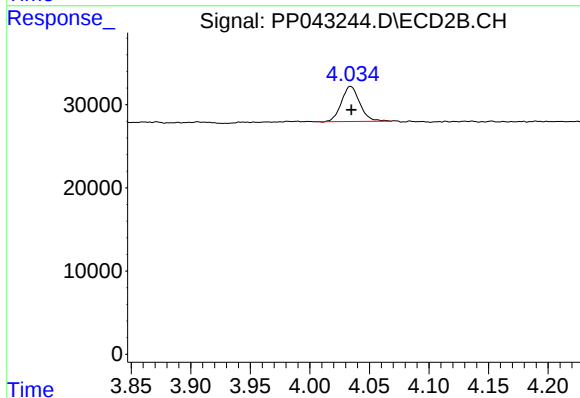


#1 Tetrachloro-m-xylene

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 45471
Conc: 2.04 ng/ml

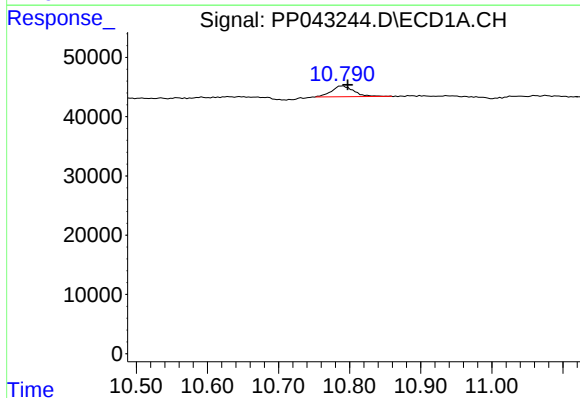

#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: -0.007 min
Response: 40405
Conc: 2.85 ng/ml

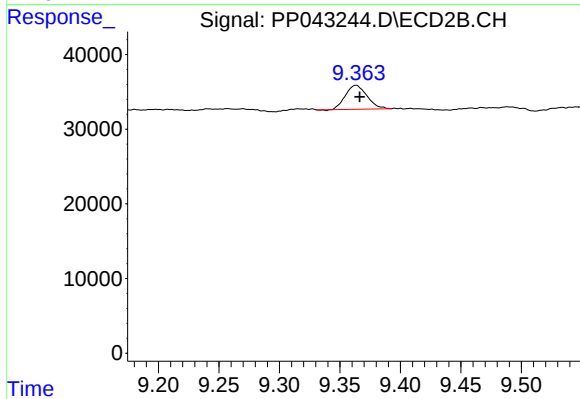

#2 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.003 min
Response: 39717
Conc: 2.13 ng/ml