

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
 Data File : PP043279.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2022 23:12
 Operator : AJ\MA
 Sample : N1241-10 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMA998C-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/26/2022
 Supervised By :Ankita Jodhani 01/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 23:33:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 25 03:09:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	4.035	29919	39814	1.302m	1.787 #
2) SA Decachlor...	10.790	9.363	42002	36786	2.965	1.973 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012522\
Data File : PP043279.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2022 23:12
Operator : AJ\MA
Sample : N1241-10 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMA998C-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/26/2022
Supervised By :Ankita Jodhani 01/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 23:33:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 25 03:09:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

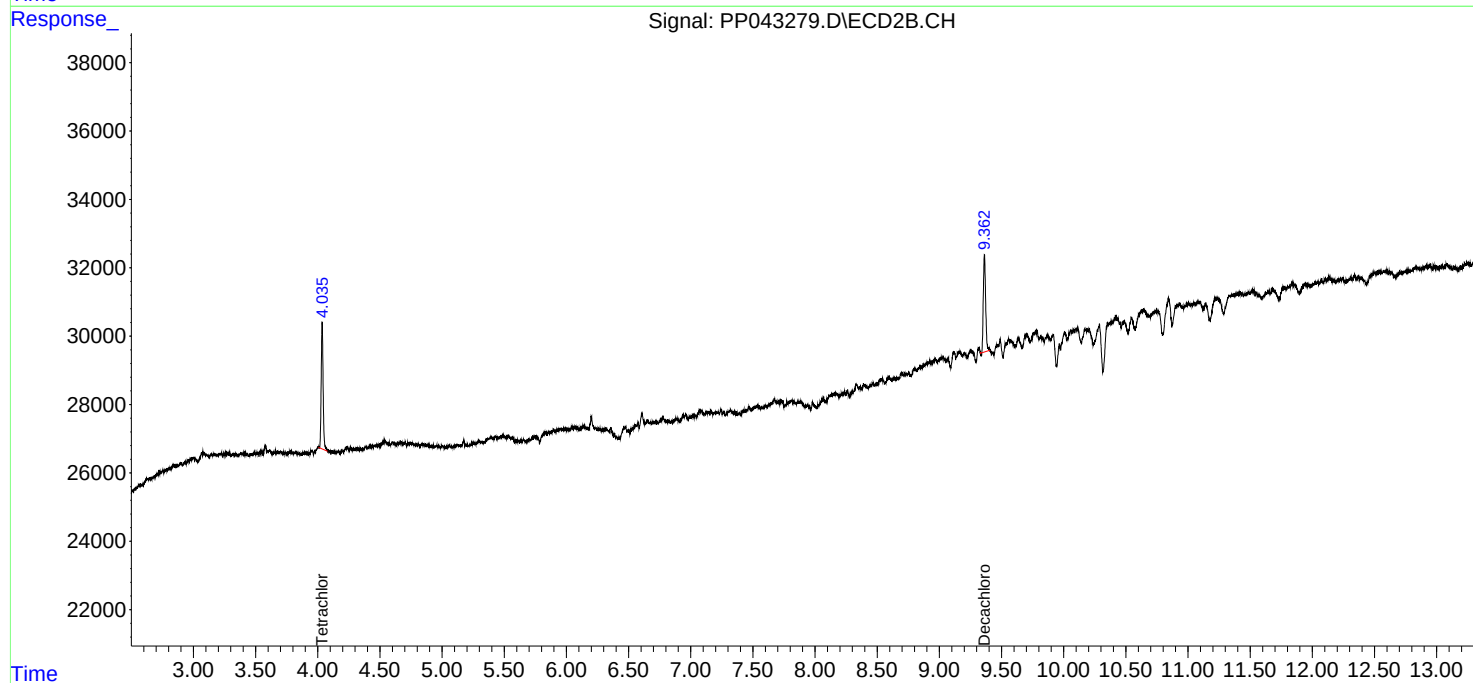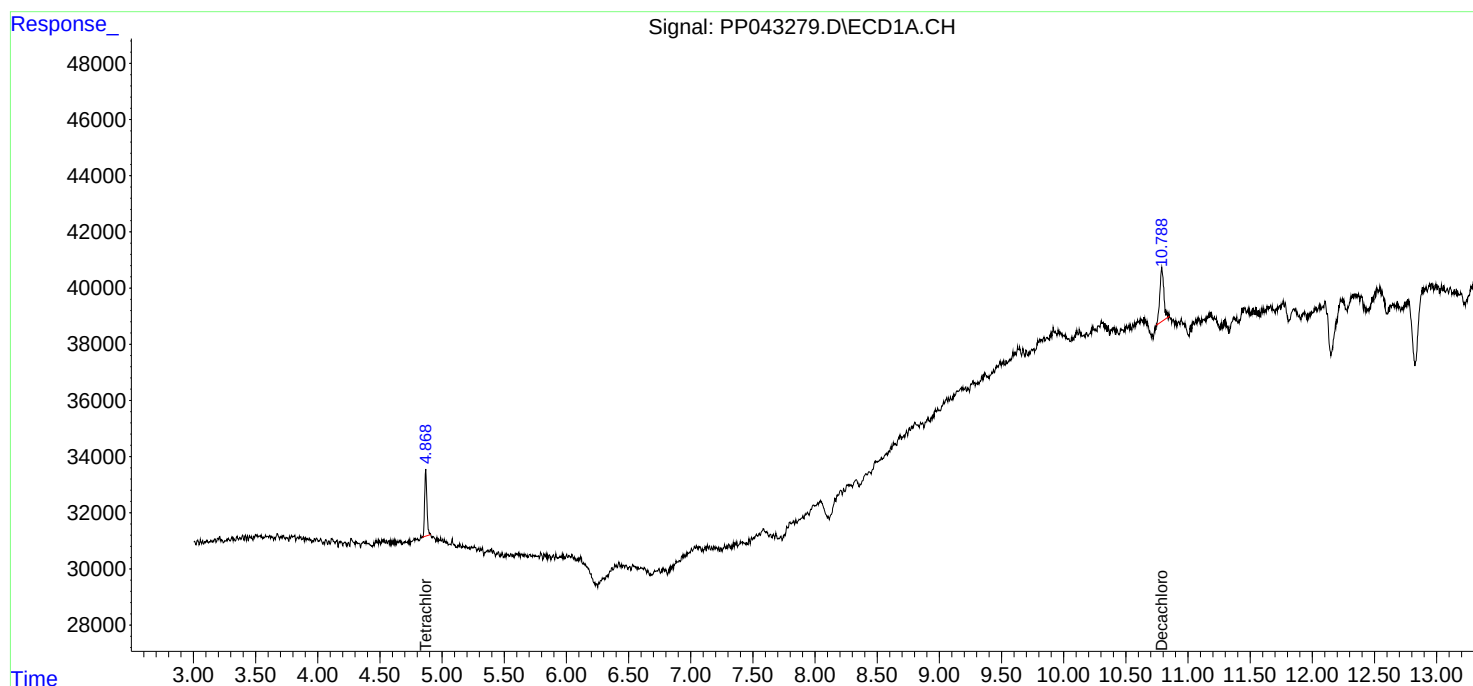

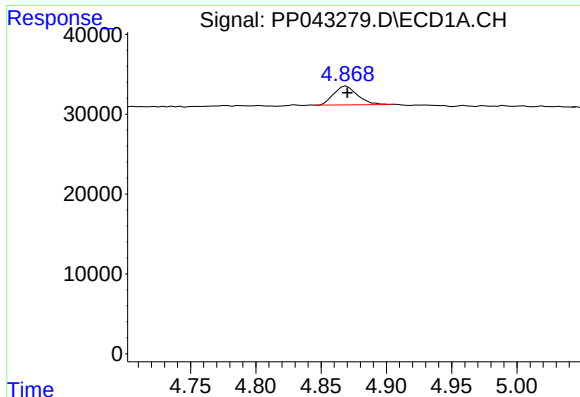

#1 Tetrachloro-m-xylene

R.T.: 4.868 min
Delta R.T.: -0.002 min
Response: 29919
Conc: 1.30 ng/ml

Instrument :

ECD_P


ClientSampleId :

KMA998C-1-2

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 01/26/2022
Supervised By :Ankita Jodhani 01/26/2022

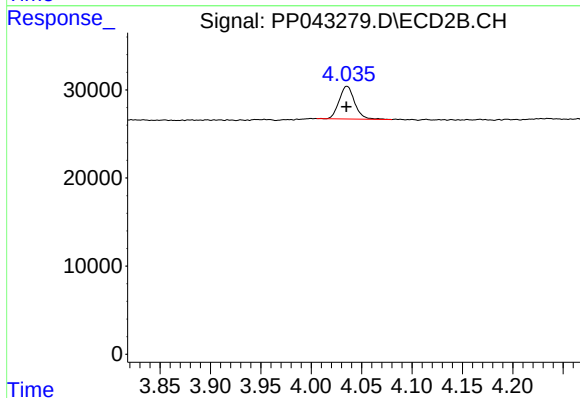


#1 Tetrachloro-m-xylene

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 39814
Conc: 1.79 ng/ml

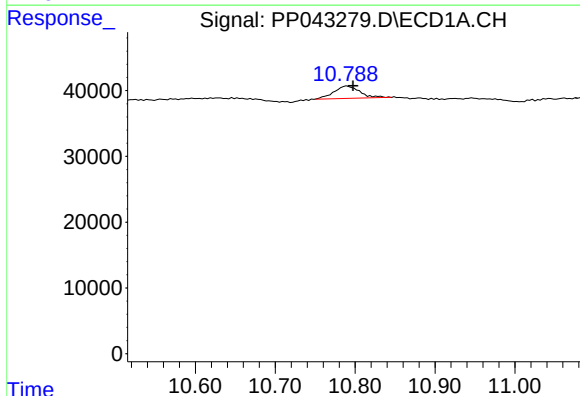

#2 Decachlorobiphenyl

R.T.: 10.790 min
Delta R.T.: -0.008 min
Response: 42002
Conc: 2.97 ng/ml

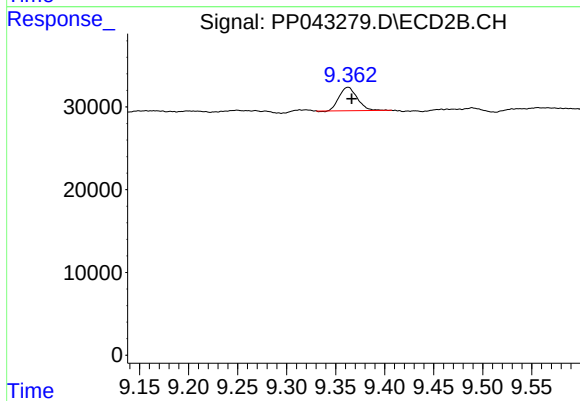

#2 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.004 min
Response: 36786
Conc: 1.97 ng/ml