

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012523\
 Data File : PP054870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 13:43
 Operator : YP\AJ
 Sample : 01243-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TJRC-011923-B4-20-30

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 15:58:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.577	36136532	30818631	20.783	20.529
2) SA Decachlor...	10.086	8.593	32749965	25956416	18.912	19.219

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012523\
Data File : PP054870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 13:43
Operator : YP\AJ
Sample : 01243-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TJRC-011923-B4-20-30

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 15:58:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

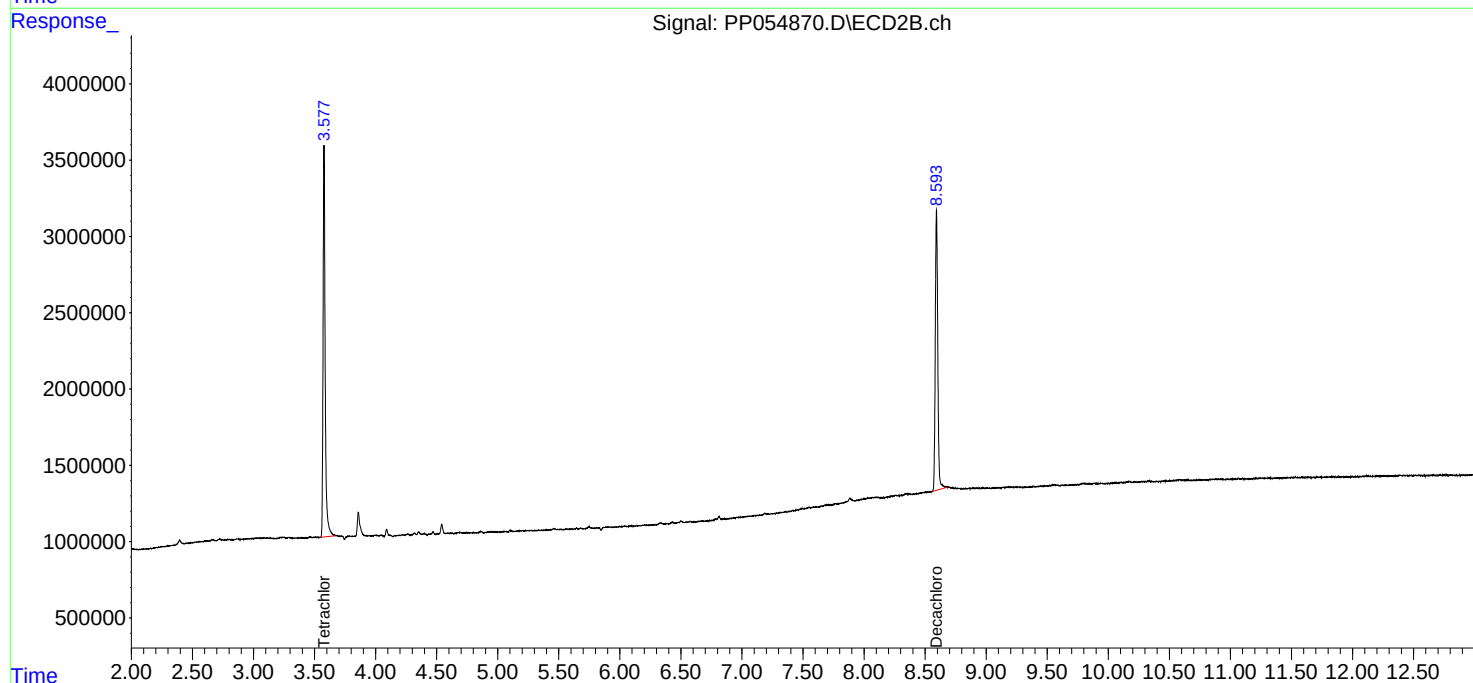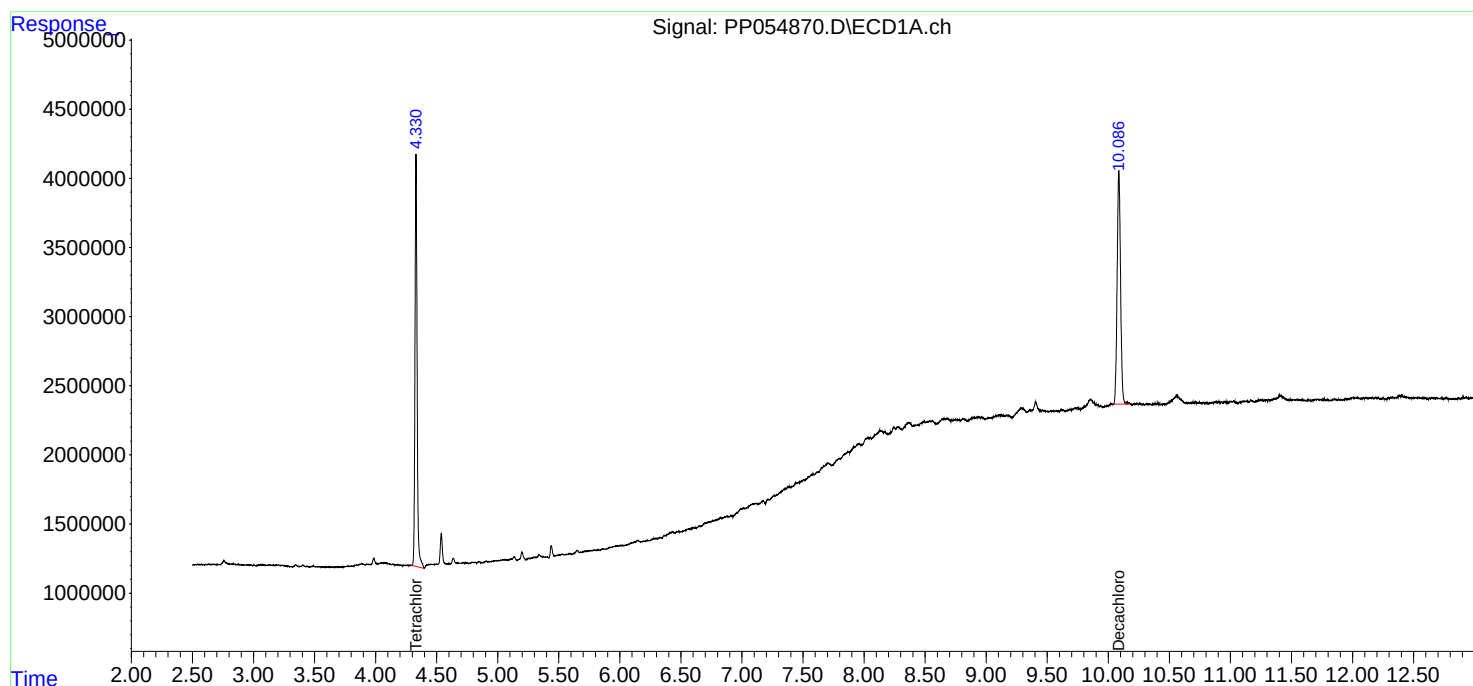


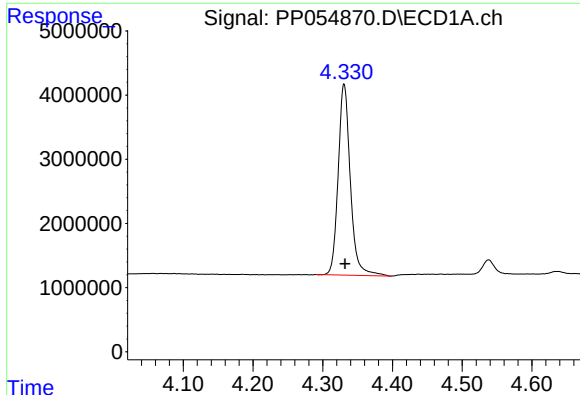

#1 Tetrachloro-m-xylene


R.T.: 4.331 min
Delta R.T.: -0.001 min
Response: 36136532
Conc: 20.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
TJRC-011923-B4-20-30

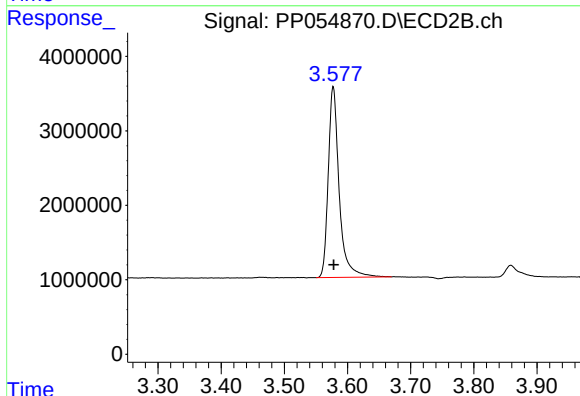


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: 0.000 min
Response: 30818631
Conc: 20.53 ng/ml

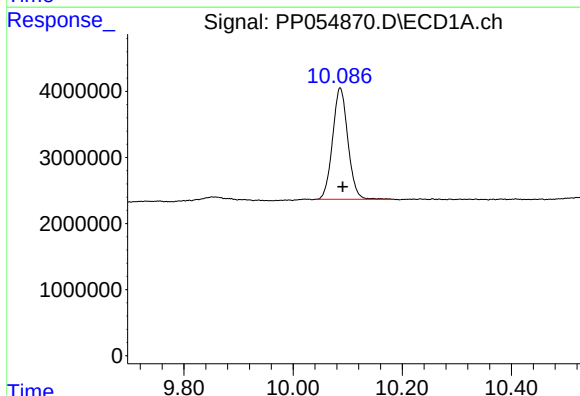

#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: -0.005 min
Response: 32749965
Conc: 18.91 ng/ml

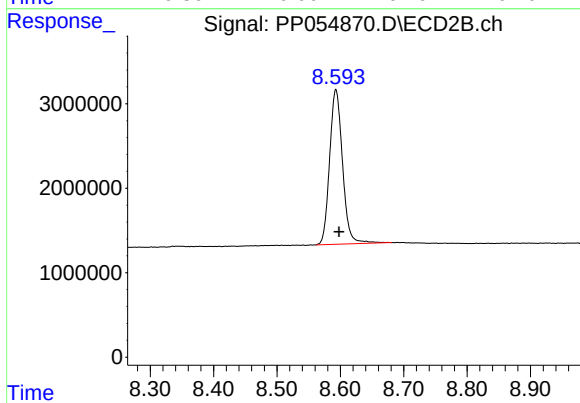

#2 Decachlorobiphenyl

R.T.: 8.593 min
Delta R.T.: -0.005 min
Response: 25956416
Conc: 19.22 ng/ml