

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012523\
 Data File : PP054871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 13:59
 Operator : YP\AJ
 Sample : 01243-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TJRC-011923-B4-30-40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 15:59:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.577	41168079	34521403	23.677	22.996
2) SA Decachlor...	10.086	8.593	36285876	29050048	20.954	21.510

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012523\
Data File : PP054871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 13:59
Operator : YP\AJ
Sample : 01243-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TJRC-011923-B4-30-40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 15:59:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

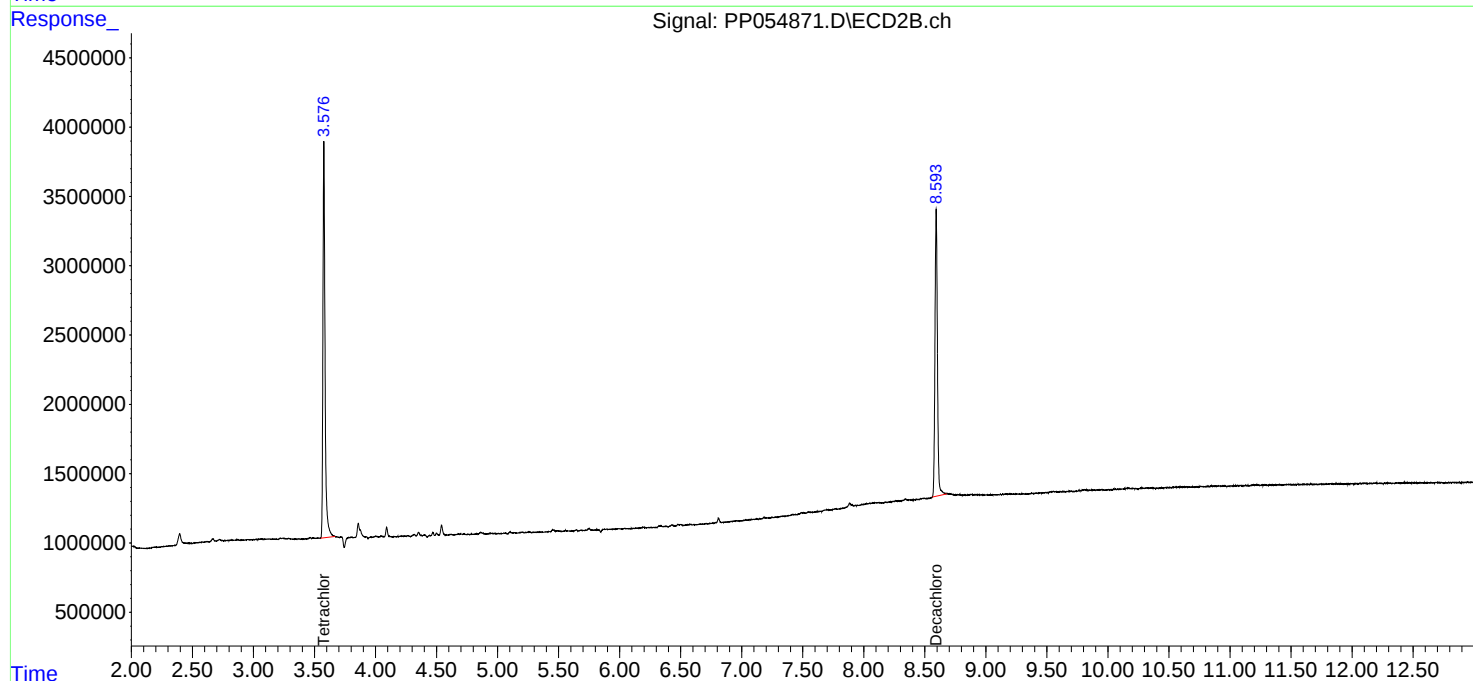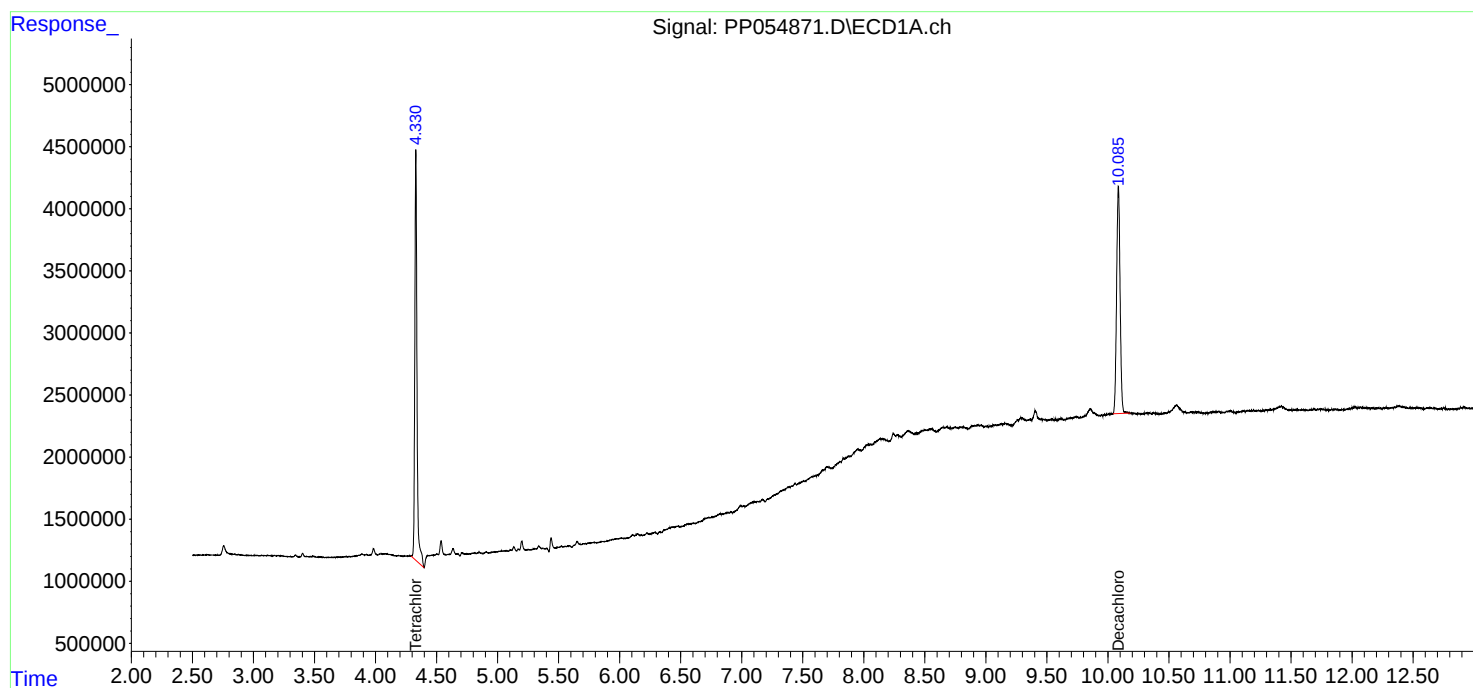


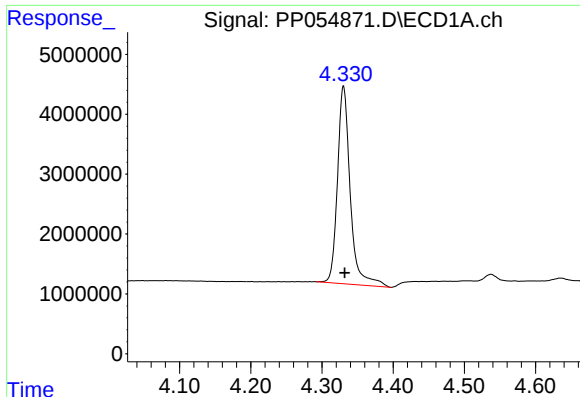

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.002 min
Response: 41168079
Conc: 23.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
TJRC-011923-B4-30-40

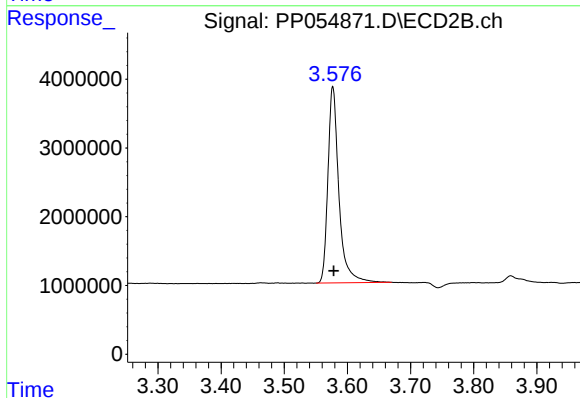


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: -0.001 min
Response: 34521403
Conc: 23.00 ng/ml

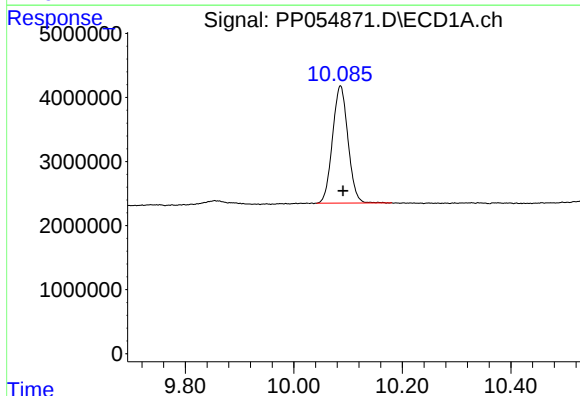

#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: -0.005 min
Response: 36285876
Conc: 20.95 ng/ml

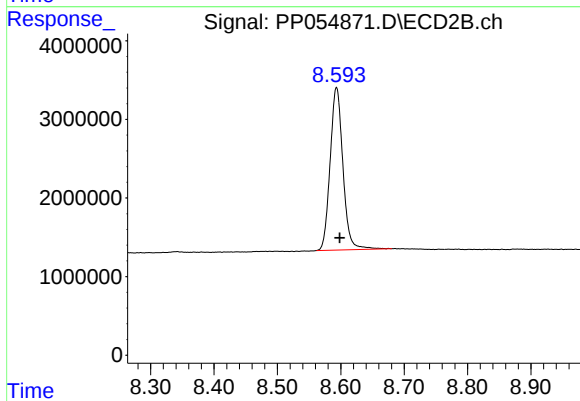

#2 Decachlorobiphenyl

R.T.: 8.593 min
Delta R.T.: -0.005 min
Response: 29050048
Conc: 21.51 ng/ml